

# Fabrication of Low-cost Realistic Three-dimensional Static Kidney Phantom for Ultrasound-guided Biopsy Applications

Firas Fohely<sup>1\*</sup>, Ammar A. Oglat<sup>2</sup>, Khaled Sabarna<sup>1</sup>, Zakaria Shweiki<sup>3</sup>, Bayan Hamoudeh<sup>1</sup>, Rulin Shalaan<sup>1</sup>

<sup>1</sup>Department of Medical Imaging, Faculty of Allied Medical Science, Palestine Ahliya University, Bethlehem, Palestine, <sup>2</sup>Department of Medical Imaging, Faculty of Applied Medical Sciences, The Hashemite University, Zarqa, Jordan, <sup>3</sup>Palestine Radiologic Center, Hebron, Palestine

## Abstract

**Background:** The rapid growth of using ultrasound-guided interventional procedures, including biopsy and drainage, which considered painful procedures, leads to improving the practice cycle of ultrasound-guided procedures. Fabrication of low-cost tissue-mimicking phantoms that serve as a training tool medium for kidney needle biopsy procedures has dramatically overcome the drawbacks associated with these practices, such as reducing the number of miss lesions, medical errors, and recurrence rate as well as these phantoms are widely available and considered a good substitute for cadavers which were not always available and relativity expensive. However, several drawbacks are associated with current kidney phantom models, mainly the short shelf life and the high fabrication cost. **Methods:** This study aims to fabricate a realistic three-dimensional static mature human kidney phantom from low cost and available material for training on ultrasound-guided interventional procedures mainly biopsy test; the material used to fabricate our model is the gelatin-agar mixture. **Results:** This model proved that it is a tissue-mimicking material by measuring their acoustic properties which nearly the same as real human kidney tissue. **Conclusion:** The results of practicing interventional procedures on our phantom model showed good and easy uses for interventional procedures training as well as make it a preferable and economically affordable model.

**Keywords:** Interventional radiology, kidney, phantom, renal biopsy, ultrasound

## INTRODUCTION

Ultrasound-guided needle biopsy is a medical procedure used to explore more about lesions and masses and detect their properties. Ultrasound guidance procedures, including fine needle aspirations, percutaneous biopsy, or catheter insertion, are considered as commonly used practices. Many practices involving needle guides are associated with ultrasound.<sup>[1]</sup>

The majority of radiologists, once they well practice the technique, tend to perform interventional techniques “freehand.” Ultrasonic guidance procedures are considered a hard technique to practice. The first attempt at detecting needles in soft tissue and eventually guiding them into lesions are associated with considerable anxiety and frustration, especially for most trainee radiologists.<sup>[2]</sup>

Phantoms are anthropomorphic that fabricated to represent a defined anatomical structure. They are designed to use in

medical research, training, and quality assurance. Phantom could be made from different materials with different geometric and technical properties based on their application. Alssabbagh *et al.* fabricated a three-dimensional (3D) thyroid gland phantom that could mimic computed tomography (CT) characteristics of real tissue.<sup>[3]</sup> Opik *et al.* have developed a high fidelity anthropomorphically shaped physical phantom to simulate the liver tissue, which uses with the robotic surgical system organs.<sup>[4]</sup>

For biopsy test purposes, an ideal phantom should simulate the structural and physiological properties of human tissue and minimize the sideways movement of the needle. Tissue-mimicking phantoms that precisely represent the

**Address for correspondence:** Dr. Firas Fohely,  
Department of Medical Imaging, Faculty of Allied Medical Science, Palestine  
Ahliya University, Bethlehem 1041, Palestine.  
E-mail: [firmas@paluniv.edu.ps](mailto:firmas@paluniv.edu.ps)

Received: 14-12-2020 Revised: 07-04-2021 Accepted: 19-04-2021 Available Online: 27-12-2021

### Access this article online

#### Quick Response Code:



**Website:**  
[www.jmuonline.org](http://www.jmuonline.org)

**DOI:**  
10.4103/JMU.JMU\_181\_20

This is an open access journal, and articles are distributed under the terms of the Creative Commons Attribution-NonCommercial-ShareAlike 4.0 License, which allows others to remix, tweak, and build upon the work non-commercially, as long as appropriate credit is given and the new creations are licensed under the identical terms.

**For reprints contact:** [WKHLRPMedknow\\_reprints@wolterskluwer.com](mailto:WKHLRPMedknow_reprints@wolterskluwer.com)

**How to cite this article:** Fohely F, Oglat AA, Sabarna K, Shweiki Z, Hamoudeh B, Shalaan R. Fabrication of low-cost realistic three-dimensional static kidney phantom for ultrasound-guided biopsy applications. *J Med Ultrasound* 2022;30:36-40.

properties of human organs tissue are playing a major role in safety practicing and verification of new imaging procedures.<sup>[5]</sup>

The wide use of ultrasound-guided interventional procedures, including biopsy and drainage, which considered painful procedures has pushed toward improving the efficiency of the training and the practicing cycle of ultrasound-guided procedures, beginner as medical students and trainees usually used cadaver for practicing ultrasound-guided interventional procedures or by training on real patients. However, practicing these procedures on patients by student and beginner physicians lead to many serious medical errors that could be painful and lethal, so it is not recommended to practicing such procedures on patients.<sup>[6]</sup>

Today's challenge in kidney needle biopsy training is basically designing a low-cost tissue-mimicking phantom, which can be used more than once to serve as a training tool and practice medium for kidney needle biopsy procedures. Several drawbacks are associated with current kidney phantom models, mainly the short shelf life of these models and the high fabrication cost.

Therefore, this study aims to fabricate a realistic 3D mature static human kidney phantom from low cost and available material; basically, the gelatin-agar mixture, which according to previous studies in the same field, greatly simulates the real kidney tissues.<sup>[7]</sup> The phantom designed can be used frequently (more than one time). It will be basically used to improve the quality assurance of kidney needle biopsy procedures under ultrasound as well as make it easy for students and trainees practicing the biopsy test widely possible instead of using pricy commercial training phantoms available today.

## MATERIALS AND METHODS

### Initial sample preparation

Initially, three samples were prepared and tested under ultrasound to develop the final mixture for phantom fabrication. All three samples were basically consisting of a gelatin-agar mixture but with different concentrations. For the first sample, a 30 g of dry weight gelatin powder (Sigma Aldrich) and 5 g of starch powder were used to prepare the sample; both powders were dissolved in 500 ml of distilled water and boiled to 75°C. The mixture was left to cool down at the normal room temperature and then stored in the fridge under 4°C for 24 h. The second sample consisted of 30 g of dry weight gelatin powder and 9.0 g of dry weight agar powder (Sigma Aldrich) and 5 g of starch. All the materials dissolved in 500 ml of distilled water and heated to 75°C. The mixture was left to cool down at the normal room temperature and then stored in the fridge under 4°C for 24 h.

While for the third sample, 30 g of dry weight gelatin powder and 9.0 g of dry weight agar powder (Sigma Aldrich) were dissolved in 500 ml distilled water and heated to 75°C. The mixture was left to cool down at the normal room

temperature and then stored in the refrigerator under 4°C for 24 h [Table 1].

The three samples were tested under ultrasound, to investigate their acoustic properties to determine which sample perfectly simulates the real kidney tissue most under ultrasound. The samples were tested by a 3.5 MHz Convex probe at a scanning angle of 90°. Sensor CASSY-2 from Leybold was used to measure the speed of sound, sound attenuation, and thermal diffusivity; Table 2 shows the values of these measurements for the three samples compared to the value of the same measurements of the real kidney tissue under ultrasound.

Referring to Table 2, it was obvious that the speed of sound, attenuation, and the thermal diffusivity (speed of sound: 1553 m/s, attenuation: 0.47 dB/cm/MHz, and thermal diffusivity: 0.132 mm<sup>2</sup>/s) of sample 3 were the closest value of these measurements of the real kidney tissue under ultrasound (speed of sound: 1546 m/s, attenuation: 0.58 dB/cm/MHz, and thermal diffusivity: 0.141 mm<sup>2</sup>/s). It is obvious from Table 2 that sample 3 is the sample that mostly has the same acoustic properties as the real renal tissue and thus is considered the sample that best among others to simulate the real kidney tissue under ultrasound; for this reason, sample 3 chosen for the final fabrication of our phantom.

### Fabrication of kidney phantom

#### Designing of 3D kidney mold

For the designing of mature kidney mold, a 3D anthropomorphic kidney with the adrenal gland model made from fiberglass was used to manufacture the kidney phantom shape [Figure 1]. A 1500 ml elastic-plastic container chosen to pour the mold solution; the container was fixed at the center bottom of retort stands; then the 3D kidney model was hanged with the stand using rope, taking into account that the kidney model is adjusted to be at the center of the container with the same distance from all sides [Figure 2].

The mold solution was primarily made of agarose powder (C<sub>24</sub>H<sub>38</sub>O<sub>19</sub>)—(Sigma Aldrich). 20 g of dry weighted agarose powder was dissolved in 1500 ml of distilled water. The solution was mixed properly and then heated to 80°C; it was left to cool down for room temperature, then it smoothly poured into the plastic container that contains the kidney model. The container was stored at room temperature (22°C ± 2°C). After 48 h, the mold became solid and flexible; it was ready to eject the 3D kidney anthropomorphic from the mold; the mold's internal lumen of the mold took the same shape, size, and dimension as the kidney anthropomorphic. Figure 3 shows the removal of the kidney anthropomorphic from the mold. After the anthropomorphic has been removed, the mold was ready, the tissue-mimicking solution was prepared in the same concentration, and properties as sample 3, a red dye was added to the solution to make the solution color more realistic. The mold was fixed on a stable flat board. Then, the solution was poured into the mold simultaneously then stored steadily in the refrigerator (4°C) for 48 h. After 48 h, the mold was moved out from the refrigerator, the mold was incised, and the kidney

**Table 1: Summarization of the composition of all samples**

Sample	Material	Mass (gram)			
Sample one	Gelatin	30g			
	Starch	5g			
Sample two	Gelatin	30g	Dissolved in 500 ml of distilled water	Heated to 75°C	Stored at 4°C for 24 h
	Agar	9g			
	Starch	5g			
Sample three	Gelatin	30g			
	Agar	9g			

**Table 2: The acoustic properties of gelatin-agar-starch samples and compare them with the acoustic properties of the real kidney tissue**

Property	Sample 1	Sample 2	Sample 3	Real - kidney tissue*
Speed of sound (m/s)	1956±21	1882±10	1553±15	1546
Attenuation (dB/cm/MHz)	0.31±0.05	0.36±0.05	0.47±0.05	0.58
Thermal diffusivity (mm <sup>2</sup> /s)	0.220±0.006	0.237±0.004	0.132±0.006	0.141

\*According to Insana<sup>[8]</sup> and Feldman<sup>[9]</sup>



**Figure 1:** The three-dimensional anthropomorphic kidney model

phantom was gently pulled out. Figure 4 shows the final kidney phantom as it is ejected from the mold.

Renal depth in a mature human was estimated by Xue *et al.*, 2017 using a new formula. Renal depths were determined using CT by measuring the distance between the skin and the anterior as well as the posterior surface of the kidneys at the level of the renal hilum. The left kidney depth was found to be  $6.82 \pm 0.65$  cm, while the right kidney depth was  $7.03 \pm 0.6$  cm.<sup>[10]</sup> The renal depth was taken into account. To make the biopsy practicing more similar to the real renal tissue, the kidney phantom was placed into a gelatin medium at a depth of 7.32 cm from the surface [Figure 5].

## RESULTS

### Characterization of tissue-phantom model

To produce a kidney tissue mimic material, a mature 3D-kidney model was used to design the kidney mold. Then, the tissue-mimicking solution was poured into the mold and



**Figure 2:** The preparation steps of pouring the mold material

kept in the refrigerator (4°C) for 48 h. After 48 h, the mold has moved out from the fridge. Then, the mold was incised; it was obvious that the tissue-mimicking phantom took the realistic shape and diameter of the 3D Kidney model.

### Phantom evaluation under ultrasound


The final phantom was fabricated and tested under ultrasound, a CHISON Doppler ultrasound machine used for this purpose with a 3.5 MHz Convex probe and scanning angle 90°. Figure 6a shows a sagittal image of the final kidney phantom under ultrasound, while Figure 6b shows an axial image of the kidney phantom. Figure 6c shows the Trucut biopsy needle (16-gauge needle) while inserted (45°) in the kidney by the radiologist.

## DISCUSSION

Recently, interventional radiology procedures including biopsy and drainage have been considered preferable and minimally invasive procedures since they are more comfortable for the



**Figure 3:** Removal of kidney model from the anthropomorphic

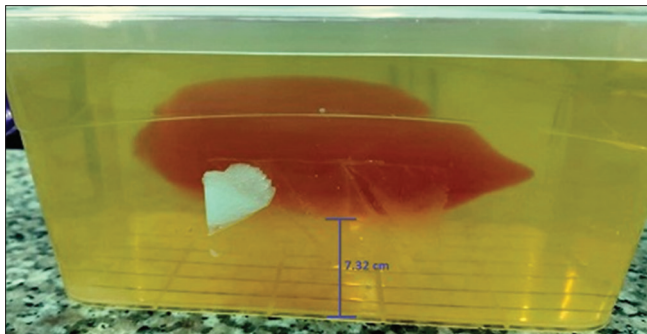

**Figure 5:** Kidney phantom place in gelatin medium in 7.32 cm depth to simulate real renal depth


patients and have less chance for infections and lower cost compared to other procedures such as surgery.<sup>[11]</sup>

For interventional procedures, high training will lead to good practicing and high performance, which minimizes the pain and medical errors that may associate with these procedures, such as biopsy when it is applied to patients. Realistic phantoms improved and maintained physicians' skills, which in turn improve the performance and dramatically minimize the missed lesion and enhance the success of biopsy procedures.<sup>[12]</sup> This makes realistic phantoms that precisely simulate real tissue anatomy and properties an important tool for training and practicing not only for residents but also for medical students.<sup>[13]</sup>

There are a variety of versions and types of training phantoms for educational and training purposes in medicine. However, the vast majority of these phantoms are comparably costly and include many defects in anatomical structure and have a relatively short life span.<sup>[14]</sup> In some recent studies, they were basically used nonwater-soluble material for phantom fabrication, including Acrylonitrile-butadiene-styrene<sup>[15]</sup> and some other acute oral toxic material such as Polyvinyl alcohol.<sup>[16]</sup> Some other studies presented models that can withstand till 3 months after manufacturing. They did not show signs of deterioration by preserving them in standard conditions.<sup>[17]</sup>



**Figure 4:** Final kidney phantom after it has ejected from the mold

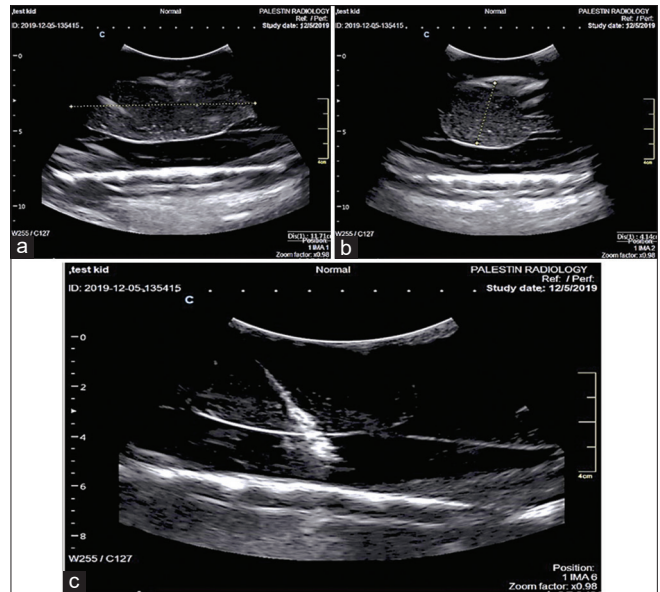

**Figure 6:** From the left; (a) Shows sagittal image of the final kidney phantom under ultrasound. (b) Shows an axial image of the kidney phantom with the kidney diameter obvious. (c) Shows the Trucut biopsy needle (16-gauge needle) while inserted (45o) in the kidney by the radiologist

In this study, a 3D-realistic kidney phantom made up of relatively low-cost material including gelatin and agar powder was proposed. This model has major advantages; it allows the use of a wide different low-cost, nontoxic, biocompatible materials, and water-soluble material was used to fabricate our phantom. These materials are mimicking human kidney tissues. One unit of this presenting model costs 70 USD, which makes it quite affordable and available for a wide range of educational institutions as well as students and physicians compared to the standard model cost, which starts from 4442 USD according to True Phantom Solution-2020.

The ultrasound images of the kidney phantom of our presented model, as shown in Figure 6a and b, show that the kidney appears clearly and realistic. However, it slightly shortage the internal structure. The kidney medium does not appear similar to the appearance of the real human kidney as various materials were used for fabrication. This is because the surrounding tissue of the human kidney has higher attenuation than the kidney itself, while for the phantom, it is the opposite.<sup>[18]</sup> The results showed that our phantom model is quite realistic and tissue-mimicking under ultrasound and easy to practicing and

training compare to the traditional models. Our proposed model allows creating a low-cost phantom, which can be a good substitute for the expensive commercial training phantoms available today.

## CONCLUSION

This study was presented an economically affordable, realistic static kidney phantom; this phantom appears realistic in ultrasound imaging and has good elasticity. The acoustic properties of our tissue-mimicking material used for phantom fabrication, including speed of sound, attenuation, and thermal diffusivity, were measured and showed a perfect fit of the acoustic properties of the gelatin-agar materials that were used with the acoustic properties of the real human kidney tissue as presented in Table 2. The phantom was tested under ultrasound and appeared clearly with their dimension, as shown in Figure 6a and b. Moreover, it was also tested by radiologists under ultrasound while inserting a Trucut biopsy needle, as shown in Figure 6c.

Our low-cost gelatin phantoms model provides several advantages over other simple models, primary skills including flexible probe positioning, and easy needle placement due to the flat surface of the model enhances practicing learning and provides a convenient way to practice invasive procedures before performing them on live patients.

In addition, our model's main advantage is the ability to use it multiple times. Practicing needle placement on the model can leave some marks and scratch on the gelatin. A proposed technique to increase the shelf life of our model, in particular, is microwaving the model for 7–10 s which will be enough to remove all marks and scratch from the model and reuse it again.

The results of practicing interventional procedures on our phantom model show good and easy uses for interventional procedures training as well as make it a preferable and economically affordable model. The results also provide good feedback for future improvement.

## Acknowledgment

The authors would like to sincerely thank all the parties that collaborate in this work, and the authors also address special thanks for Mr. Muntaser Ahmad for his assistance in collecting all the necessary materials used in this study.

## Financial support and sponsorship

Nil.

## Conflicts of interest

There are no conflicts of interest.

## REFERENCES

- Zhao L, Gong Y, Wang J, Dawlett M, Huo L, Caraway NP, *et al.* Ultrasound-guided fine-needle aspiration biopsy of thyroid bed lesions from patients with thyroidectomy for thyroid carcinomas. *Cancer Cytopathol* 2013;121:101-7. [doi: 10.1002/cncy.21202].
- Nicholson RA, Crofton M. Training phantom for ultrasound guided biopsy. *Br J Radiol* 1997;70:192-4.
- Alssabbagh M, Tajuddin AA, Abdulmanap M, Zainon R. Evaluation of 3D printing materials for fabrication of a novel multi-functional 3D thyroid phantom for medical dosimetry and image quality. *Radiat Phys Chem* 2017;8:1005-18. [doi: 10.1016/j.radphyschem.2017.02.009].
- Opik R, Hunt A, Ristolainen A, Aubin PM, Kruusmaa M. Development of High Fidelity Liver and Kidney Phantom Organs for Use with Robotic Surgical Systems. In Proceedings of the IEEE RAS and EMBS International Conference on Biomedical Robotics and Biomechanics; 2012.
- Farrer AI, Odéen H, de Bever J, Coats B, Parker DL, Payne A, *et al.* Characterization and evaluation of tissue-mimicking gelatin phantoms for use with MRgFUS. *J Ther Ultrasound* 2015;3:9.
- Kim YH. Ultrasound phantoms to protect patients from novices. *Korean J Pain* 2016;29:73-7.
- Novaes AK, Dalamura R, Menon T, Pazeli JM, Bastos MG. Homemade ultrasound phantom for simulation of hydronephrosis. *J Bras Nefrol* 2018;40:206-8.
- Insana MF, Hall TS, Fishback JL. Identifying acoustic scattering sources in normal renal parenchyma from the anisotropy in acoustic properties. *Ultrasound Med Biol* 1991;17:613-26.
- Feldman MK, Katal S, Blackwood MS. US artifacts. *Radiographics* 2009;29:1179-89.
- Xue J, Deng H, Jia X, Wang Y, Lu X, Ding X, *et al.* Establishing a new formula for estimating renal depth in a Chinese adult population. *Medicine (Baltimore)* 2017;96:e5940.
- Bragg K, VanBalen N, Cook N. Home study program. Future trends in minimally invasive surgery. *AORN J* 2005;82:1005-18.
- Harvey JA, Moran RE, Hamer MM, DeAngelis GA, Omary RA. Evaluation of a turkey-breast phantom for teaching freehand, US-guided core-needle breast biopsy. *Acad Radiol* 1997;4:565-9.
- Liberman L, Benton CL, Dershaw DD, Abramson AF, LaTrenta LR, Morris EA. Learning curve for stereotactic breast biopsy: How many cases are enough? *Am J Roentgenol* 2001;176:721-7.
- Madsen EL, Zagzebski JA, Banjavie RA, Jutila RE. Tissue mimicking materials for ultrasound phantoms. *Med Phys* 1978;5:391-4.
- Mashiko T, Otani K, Kawano R, Konno T, Kaneko N, Ito Y, *et al.* Development of three-dimensional hollow elastic model for cerebral aneurysm clipping simulation enabling rapid and low cost prototyping. *World Neurosurg* 2015;83:351-61.
- Turney BW. A new model with an anatomically accurate human renal collecting system for training in fluoroscopy-guided percutaneous nephrolithotomy access. *J Endourol* 2014;28:360-3.
- Yasukawa K, Kunisue T, Tsuta K, Shikinami Y, Kondo T. An Ultrasound Phantom with Long-Term Stability Using a New Biomimic Soft Gel Material. In Proceedings-IEEE Ultrasonics Symposium; 2007. [doi: 10.1109/ULTSYM.2007.629].
- Hunt A, Ristolainen A, Ross P, Öpik R, Krumme A, Kruusmaa M. Low cost anatomically realistic renal biopsy phantoms for interventional radiology trainees. *Eur J Radiol* 2013;82:594-600.