

Croat Med J. 2014;55:537-41
doi: 10.3325/cmj.2014.55.537

Y-chromosomal haplotyping of single sperm cells isolated from semen mixtures – a successful identification of three perpetrators in a multi-suspect sexual assault case

Aim To obtain individual Y-short tandem repeat (STR) profiles in a multi-suspect sexual assault case.

Methods We used laser cut microdissection to capture the single sperm cell in the multi-contributor semen sample, combined with the low volume polymerase chain reaction (LV-PCR) method to genotype the single sperm cell profiles using the Yfiler® kit. Consensus DNA profiles were generated from 5 replicate experiments.

Results Ninety-four parallel LV-PCRs were performed and 41 reactions (44%) produced Y-STR profiles with more than nine loci. Three individual Y-STR profiles were successfully obtained.

Conclusion The three Y haplotype units matched three known perpetrators' genotypes. Our results showed that single sperm cells Y-STR analysis was a powerful method for analyzing multi-donor semen mixture sample.

Lei Feng^{1,2}, Cheng Xu³,
Xianhai Zeng⁴, Huaicai
Zhang⁵, Fan Yang³,
Wanshui Li^{1,2}, Zheng Tu^{1,2},
Caixia Li^{1,2}, Lan Hu^{1,2}

¹Institute of Forensic Science,
Ministry of Public Security, Beijing,
People's Republic of China

²Key Laboratory of Forensic
Genetics, Ministry of Public
Security, Beijing, People's Republic
of China

³Chinese People's Public Security
University, Beijing, People's
Republic of China

⁴Forensic Technology Division,
Public Security Bureau of Fujian
Province, Fuzhou, People's Republic
of China

⁵Institute of Criminal Science and
Technology, Public Security Bureau
of Hangzhou City, Hangzhou,
People's Republic of China

Received: May 23, 2014

Accepted: October 21, 2014

Correspondence to:

Lan Hu
Institute of Forensic Science,
Ministry of Public Security
Beijing, 100038, China
13911162826@139.com

Multi-suspect sexual assault is a crime frequently encountered by forensic scientists. Current standard procedures, including preferential lysis, are incapable to separate the sperm DNA of different donors. In this way, a mixture profile is often obtained, which can only be used for exclusion rather than identification. Another method to isolate single cells from mixtures that has been successfully used in the forensic community is laser cut microdissection (LCM) (1-5). However, by means of this method it is still challenging to get the autosome short tandem repeat (STR) profile for semen mixtures with more than two contributors. This is because of the random assortment of chromosomes in meiosis (6). An alternative strategy to analyze male DNA is Y-STR analysis. In our laboratory, we previously established LCM system and low volume polymerase chain reaction (LV-PCR) platform for biological mixture analysis (7). Here, we developed a method of single sperm cells Y-STR analysis combining LCM and LV-PCR, which was successfully used in a sexual assault case.

Case background

In May 2012, a drunken woman was sexually assaulted in a hotel room and a video recording indicated three men as suspects. No other evidence but a vaginal swab was collected from the victim. Using preferential lysis method to separate the sperm cells, the sperm DNA was purified by a commercial kit. We got a mixed DNA profile of more than two contributors, by which it was difficult to exclude or identify suspects. The victim's vaginal swab was the key evidence, so we re-analyzed this sample by LCM platform to genotype the perpetrators' DNA for forensic analysis. The analysis was focused on genotyping the Y-STR of single sperm cells.

MATERIALS AND METHODS

Sample collection

A single-source semen sample was collected on tissue paper from one healthy volunteer, who had given informed consent. Three perpetrators' semen samples were also collected on tissue paper. The victim's vaginal swab had been collected previously by local police. All the samples were air dried overnight and stored at room temperature (25°C) until needed.

Routine DNA detection

Standard "in-tube" DNA amplification was performed to verify the result of single sperm assay. The single

source semen sample and three perpetrators' sperm samples were treated with MagAttract® DNA Mini M48 kit (Qiagen, Hilden, Germany) to extract genome DNA according to the manufacturer's guidelines. The equivalent of 1 ng DNA was amplified using the AmpFISTRs Yfiler® kit (Applied Biosystems, Foster City, CA, USA).

The case swab sample was treated with preferential lysis method to separate sperm cells and epithelial cells. The sperm cells DNA was extracted with MagAttract® DNA Mini M48 kit and 1 ng DNA was amplified with AmpFISTRs Yfiler® kit.

Single sperm separation with LCM

Step 1 – slide preparation. The tissue paper with volunteer's semen (0.5 cm²) or swab sperm specimens were placed in 500 µL ddH₂O and incubated for 60 minutes at 37°C in a shaking metal bath. After centrifugation and removal of the supernatant, the cell pellets were resuspended in 30 µL ddH₂O and smeared onto a UV-sterilized polyethylene naphthalate membrane slide (Carl Zeiss Ltd, Jena, Germany). The slide was air dried at room temperature.

Step 2 – sperm isolation and lysis. Sperm isolation was performed with a PALM MicroBeam instrument (Carl Zeiss Ltd) as reported previously (8). Each sperm cell was captured onto one AG480F AmpliGrid® slide reaction site (Advantix AG, Munich, Germany). Ninety-two assays were performed for single source sample and 94 assays for case sperm samples.

For cell lysis, 0.75 µL lysis buffer (0.1 mg/mL proteinase K, 4 mM DTT) was added to each reaction site and sealed with 5 µL mineral oil (Advantix AG). Cells were lysed at 56°C for 2 hours and boiled for 10 minutes on an AmpliSpeed Cycler (Advantix AG).

PCR and electrophoresis

LV-PCR was performed with AG480F AmpliGrid slide on AmpliSpeed Cycler. The PCR mixture contained 3.7 µL PCR Reaction Mix, 2.0 µL Primer Mix, 0.2 µL 25 mM MgCl₂, and 4 U AmpliTaq Gold DNA Polymerase. An aliquot of the mixture (0.75 µL) was added to each reaction site after cell lysis. Control DNA 9947A (Applied Biosystems, 0.1 ng/mL) was used as positive control, and no DNA template was used as negative control. PCR conditions were as follows: preincubation at 95°C for 15 minutes; 34 cycles of denaturation at 94°C for 1 minute, annealing at 61°C for 1.25

minutes, and extension at 72°C for 1.25 minutes; followed by a final elongation step at 60°C for 1 hour. For the single source semen sample and three perpetrators' sperm samples, PCR was amplified according to the AmpFISTRs Yfiler® kit guidelines.

All the PCR products (including 1.5 µL PCR product and 5 µL sealing oil) were denatured in 10 µL loading buffer, which was composed of HI-DI™ formamide and LIZ™-500 size standard mixture (Applied Biosystems) in a proportion of 500:1 (volume in volume). For the single source semen sample and three perpetrators' sperm samples, 1 µL amplified DNA was denatured in 10 µL of loading buffer. DNA was separated by capillary electrophoresis using an ABI 3500xl Genetic Analyzer (Applied Biosystems). The peak detection threshold was set at 50 RFU, and the data analysis was performed using GeneMapper™ ID X (Applied Biosystems) software.

RESULTS

DNA profiling of single source semen specimens

To assess the single sperm Y-STR analysis method, a volunteer's sperm sample was examined. Single sperm cell was captured onto one site of the slice using LCM (Figure 1) and genotyped using Y-STR with LV-PCR method. To overcome the random allelic drop-ins, replicate analyses were performed (9). In total, 92 parallel LV-PCRs were performed. Considering that half of the sperm cells contain an X chromosome instead of a Y chromosome, only half of the reactions should yield successful profiles. The actual proportion of Y-STR profiles with more than nine geno-

typed loci was 48% (44 of 92). Ten complete allelic profiles and 23 acceptable profiles (13-15 loci) were obtained (Table 1). According to Gill's guidelines (10), an allele can only be confirmed when two or more independent PCR reactions obtain duplicate results. We combined the best five results, which were all complete allelic profiles, to obtain a consecutive genotype (Supplementary Table 1) and the consensus genotype was identical with the known profile.

TABLE 1. DNA genotyping results of the single source semen sample

No. of genotyped loci	No. of tests	Call rate (%)
16	10	10.9
13-15	23	25.0
9-12	11	12.0
0-8	48	52.1
Sum of test	92	100

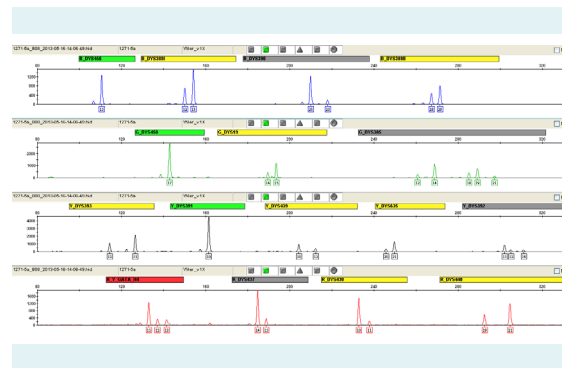


FIGURE 2. Mixed Y-STR profile of the vaginal swab obtained by the routine method.

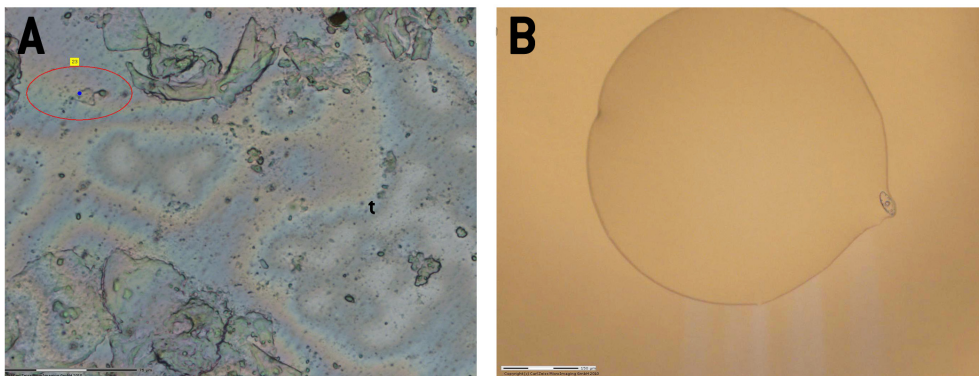


FIGURE 1. Sperm micrograph (10×40). (A) One sperm cell was chosen with PALM MicroBeam instrument (Carl Zeiss Ltd) and (B) captured and placed on the reaction site.

Casework sample analysis

The vaginal swab contained the victim's epithelial cells and three perpetrators' sperm cells. Routine preferential lysis DNA analysis yielded a mixed Y-STR profile generated from multiple contributors (Figure 2). Single sperm assay was performed. Ninety-four independent reactions were performed using Yfiler Kit. Two complete allelic profiles and 20 acceptable profiles (13-15 loci) were obtained. Forty-one reactions (44%) produced valid Y-STR profiles of more than nine loci. Twenty-five, ten, and six valid profiles were obtained respectively for the perpetrator A, B, and C (Table 2). According to Gill's guidelines, we obtained three distinct Y haplotype units (Supplementary Tables 2-4, Figure 3), which corresponded to three perpetrators' genotypes. This result served as supportive evidence for the case.

DISCUSSION

This study successfully obtained three individual Y-STR profiles in a multi-suspect sexual assault case. Multi-

ple-contributors sperm mixtures in sexual assault cases are challenging to analyze, since they always generate mixed DNA profiles or a profile that only represents the major contributor (11). In the case reported here, the mixed profile was very difficult to interpret as it included three persons' profiles. Until now, no effective method could distinguish sperm cells originating from different men, although cells containing Y chromosomes (male cells) can easily be distinguished from female cells by labeling the X and Y chromosomes with fluorescence in situ hybridization (FISH) (12). In multi-rapist cases, when valid autosomal STR information cannot be obtained from semen mixtures, Y-STR information can be used to trace the paternal line and implicate a perpetrator (13), and it can also be used to exclude a person that does not match.

In our case testing, 44% of the assays yielded valid profiles (more than nine loci), indicating that we must capture dozens of sperm cells to perform LV-PCR for one Y-STR profile. The consensus profile was used for comparison with the perpetrators' profile. For the mixed sperm sample, the testing number of the three profiles was different. We assumed that this was mainly due to the different number of sperm cells of the three donors in the semen mixture. The other possible reason may be the random sperm selection process. Our future work will focus on investigating more effective procedures to differentiate the X type sperm and Y type sperm, such as FISH.

TABLE 2. DNA genotyping results of the 41 reactions that produced valid Y-STR profiles (9-16 loci) in the case sample

No. of genotyped loci	No. of tests for Perpetrator A	No. of tests for Perpetrator B	No. of tests for Perpetrator C	Call rate (%)
16	1	0	1	4.9
13-15	14	3	3	48.8
9-12	10	7	2	46.3
Sum of test	25	10	6	

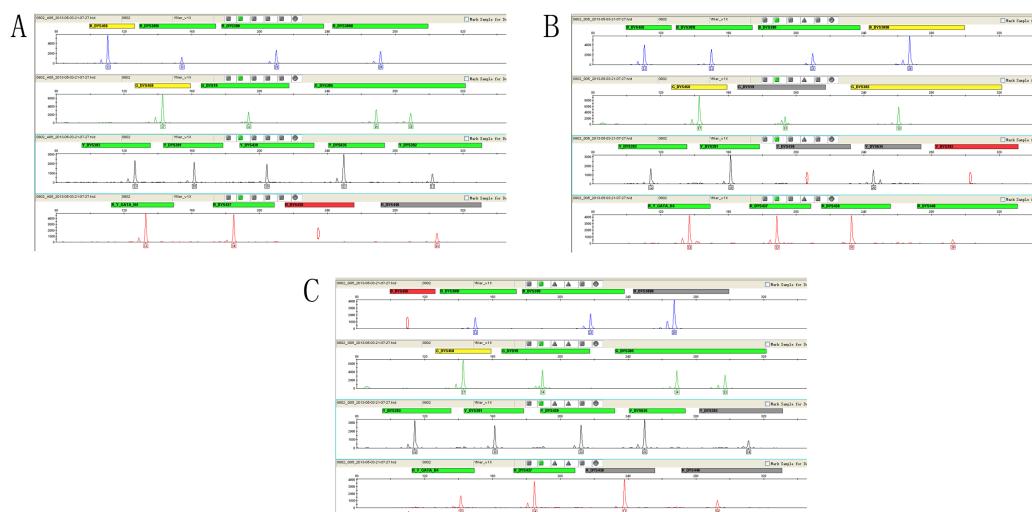


FIGURE 3. Y-STR electropherograms of the three perpetrators (A-C) derived from the casework sample. The red circle indicates allele dropout.

Acknowledgments We thank the volunteer who contributed a semen sample for genetic analysis.

Funding This study was supported by the grant of Science and Technology Special Program, Ministry of Public Security of China (NO.2014GABJC040).

Ethical approval The study was approved by Ethics Committee of Institute of Forensic Science of China.

Declaration of authorship LF designed the experiments, collected, and analyzed the data, and wrote the manuscript. CX and FY performed the experiments. XHZ and H CZ performed sample collection. WSL, ZT, and CXL designed the experiments. LH was the head of the research program and designed the experiments.

Competing interests All authors have completed the Unified Competing Interest form at www.icmje.org/coi_disclosure.pdf (available on request from the corresponding author) and declare: no support from any organization for the submitted work; no financial relationships with any organizations that might have an interest in the submitted work in the previous 3 years; no other relationships or activities that could appear to have influenced the submitted work.

References

- Budimlija ZM, Popiolek D, Fogt F, Prinz M. Forensic applications of laser capture microdissection: use in DNA-based parentage testing and platform validation. *Croat Med J.* 2005;46:549-55. [Medline:16100757](#)
- Di Martino D, Staiti N, Simone A, Todaro P. Laser microdissection and DNA typing of cells from single hair follicles. *Forensic Sci Int.* 2004;146:S155-7. [Medline:15639565](#) [doi:10.1016/j.forsciint.2004.09.047](#)
- Elliott K, Lambert C, Burroughes TR, Gill P. Use of laser microdissection greatly improves the recovery of DNA from sperm on microscope slides. *Forensic Sci Int.* 2003;137:28-36. [Medline:14550610](#) [doi:10.1016/S0379-0738\(03\)00267-6](#)
- Vandewoestyne M, Deforce D. Laser capture microdissection in forensic research: a review. *Int J Legal Med.* 2010;124:513-21. [Medline:20680318](#) [doi:10.1007/s00414-010-0499-4](#)
- Vandewoestyne M, Van Hoofstat D, Van Nieuwerburgh F, Deforce D. Suspension fluorescence in situ hybridization (S-FISH) combined with automatic detection and laser microdissection for STR profiling of male cells in male/female mixtures. *Int J Legal Med.* 2009;123:441-7. [Medline:19319556](#) [doi:10.1007/s00414-009-0341-z](#)
- Lucy D, Curran JM, Pirie AA, Gill P. The probability of achieving full allelic representation for LCN-STR profiling of haploid cells. *Sci Justice.* 2007;47:168-71. [Medline:18229758](#) [doi:10.1016/j.scijus.2007.10.001](#)
- Li C, Qi B, Ji A, Xu X, Hu L. The combination of single cell micromanipulation with LV-PCR system and its application in forensic science. *Forensic Sci Int.* 2009;2:516-7.
- Cai-xia Li, Han JP, Ren WY, Ji AQ, Xu XL, Hu L. DNA profiling of spermatozoa by laser capture microdissection and low volume-PCR. *Plos One.* 2011;6:e22316-7. [Medline:21853031](#) [doi:10.1371/journal.pone.0022316](#)
- Budowle B, van Daal A. Validity of low copy number typing and applications to forensic science. *Croat Med J.* 2009;50:207-17. [Medline:19480017](#) [doi:10.3325/cmj.2009.50.207](#)
- Gill P, Whitaker J, Flaxman C, Brown N, Buckleton J. An investigation of the rigor of interpretation rules for STRs derived from less than 100 pg of DNA. *Forensic Sci Int.* 2000;112:17-40. [Medline:10882828](#) [doi:10.1016/S0379-0738\(00\)00158-4](#)
- Anoruo B, van Oorschot R, Mitchell J, Howells D. Isolating cells from non-sperm cellular mixtures using the PALM microlaser micro dissection system. *Forensic Sci Int.* 2007;173:93-6. [Medline:17459628](#) [doi:10.1016/j.forsciint.2007.01.031](#)
- Murray C, McAlister C, Elliott K. Use of fluorescence in situ hybridisation and laser microdissection to isolate male non-sperm cells in cases of sexual assault. *Int Congr Ser.* 2006;1288:622-4. [doi:10.1016/j.ics.2005.09.109](#)
- Ballantyne KNKV, Wollstein A, Choi Y, Zuniga SB, Ralf A. A new future of forensic Y-chromosome analysis: rapidly mutating Y-STRs for differentiating male relatives and paternal lineages. *Forensic Sci Int Genet.* 2012;6:208-18. [Medline:21612995](#) [doi:10.1016/j.fsigen.2011.04.017](#)