

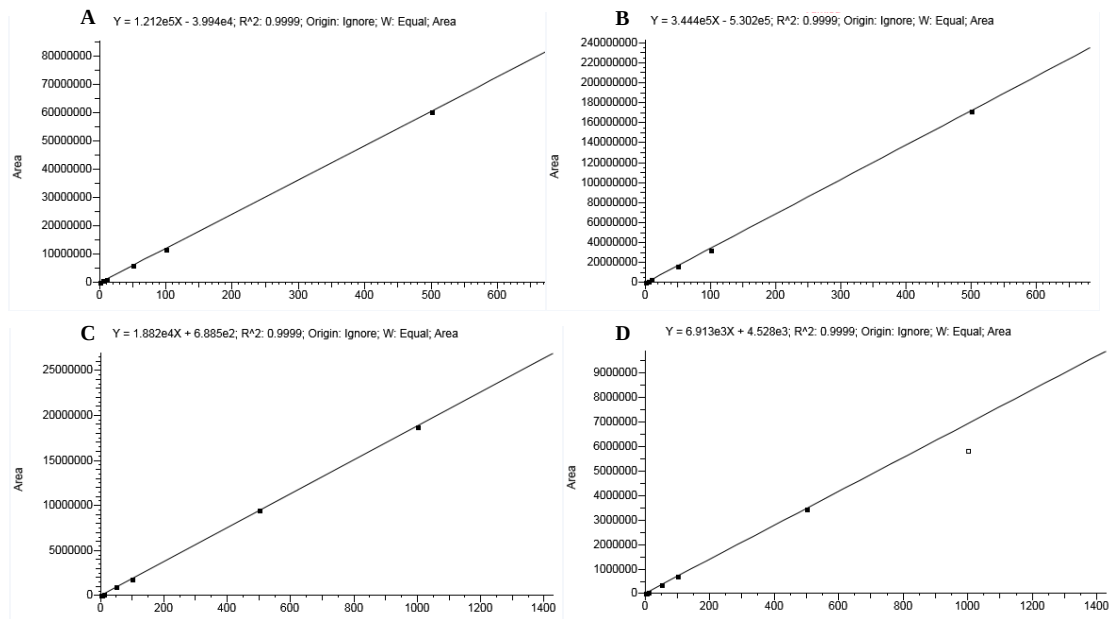


Fig. S1 Calibration curves for IAA, ZR, GA₃ and ABA standards obtained from HPLC-MS/MS analysis. a: IAA; b: ZR; c: GA₃; d: ABA.