

Complication incidence of two implant systems up to six years: a comparison between internal and external connection implants

Sung-Wook Chae¹, Young-Sung Kim^{1,2}, Yong-Moo Lee³, Won-Kyung Kim¹, Young-Kyoo Lee¹, Su-Hwan Kim^{1,2,*}

¹Department of Periodontics, Asan Medical Center, Seoul, Korea

²Department of Dentistry, University of Ulsan College of Medicine, Seoul, Korea

³Department of Periodontology, Dental Research Institute, Seoul National University School of Dentistry, Seoul, Korea

Purpose: This study was conducted to compare the cumulative survival rates (CSRs) and the incidence of postloading complications (PLCs) between a bone-level internal connection system (ICS-BL) and an external connection system (ECS).

Methods: The medical records of patients treated with either a ICS-BL or ECS between 2007 and 2010 at Asan Medical Center were reviewed. PLCs were divided into two categories: biological and technical. Biological complications included > 4 mm of probing pocket depth, thread exposure in radiographs, and soft tissue complications, whereas technical complications included chipping of the veneering material, fracture of the implant, fracture of the crown, loosening or fracture of the abutment or screw, loss of retention, and loss of access hole filling material. CSRs were determined by a life-table analysis and compared using the log-rank chi-square test. The incidence of PLC was compared with the Pearson chi-squared test.

Results: A total of 2,651 implants in 1,074 patients (1,167 ICS-BLs in 551 patients and 1,484 ECSs in 523 patients) were analyzed. The average observation periods were 3.4 years for the ICS-BLs and 3.1 years for the ECSs. The six-year CSR of all implants was 96.1% (94.9% for the ICS-BLs and 97.1% for the ECSs, $P=0.619$). Soft tissue complications were more frequent with the ECSs ($P=0.005$) and loosening or fracture of the abutment or screw occurred more frequently with the ICS-BLs ($P<0.001$).

Conclusions: Within the limitations of this study, the ICS-BL was more prone to technical complications while the ECS was more vulnerable to biological complications.

Keywords: Dental implant-abutment design, Dental implants, Retrospective studies, Survival rate.

INTRODUCTION

After the concept of osseointegration was introduced by Brånemark et al. [1], the indications for dental implants were expanded from fully edentulous to partially edentulous cases and a high long-term success/survival rate was demonstrated [2,3]. Despite the general reliability of implantation techniques, it is not always possible to perform a restoration without any complications. In the literature, the complications arising from implants have been categorized into two types: technical and biological [4-9]. The general category of technical complications refers to any mechanical damage of the implants, implant components, and suprastructures, whereas biological complications are disturbances in implant function that affect the supporting peri-implant tissues [8]. According to previous studies [4-7,9], the

pISSN 2093-2278
eISSN 2093-2286



JPIS >
Journal of Periodontal
& Implant Science

Research Article

J Periodontal Implant Sci 2015;45:23-29
<http://dx.doi.org/10.5051/jpis.2015.45.1.23>

Received: Nov. 10, 2014

Accepted: Dec. 31, 2014

*Correspondence:

Su-Hwan Kim

Department of Periodontics, Asan Medical Center,
88 Olympic-ro 43-gil, Songpa-gu, Seoul 138-736,
Korea

E-mail: shkimperio@amc.seoul.kr

Tel: +82-2-3010-5797

Fax: +82-2-3010-6967

This is an Open Access article distributed under the terms of the Creative Commons Attribution Non-Commercial License (<http://creativecommons.org/licenses/by-nc/3.0/>).

overall survival rate of implants ranges from 94.5% to 97.2%. However, the incidence of biological and technical complications has varied widely as implant systems have changed over time.

Implant systems can generally be classified as either external connection systems (ECSs) or internal connection systems (ICSs) according to the type of fixture or abutment connection. ICS can be subdivided into bone-level systems (ICS-BL) and transmucosal systems. ECSs are characterized by an external hexagon and have served well over the years. The external hexagon was developed to facilitate the insertion of components such as abutments and impression copings, rather than to provide an antirotational ability [6] and therefore, external systems exhibit weakness due to micromovements of the abutments under a high occlusal load due to their limited hexagonal height [5]. ICSs typically have a tapered conical connection and are popular for their mechanically stable and self-locking interface [9]. It has been shown that the conical internal connection transfers stress from the abutment apically to a greater extent and, as a result, reduces stress on the crestal bone in comparison with external connections [10]. However, fractures may occur in the coronal portion of some ICS-BL fixtures under a high occlusal load [11].

Abundant long-term clinical data regarding ECSs are available. Most technical complications are well-reported, and it is known that the fixtures in ECSs can experience breakage of the abutment screw instead of undergoing fixture fracture, with potentially catastrophic results [10,12]. In contrast, few long-term clinical data have been reported for ICSs, and the mechanical advantages of ICSs have been assessed based on *in vitro* studies. Moreover, recent studies have challenged the mechanical stability of ICSs and have shown that increased axial displacement occurs in ICSs as tightening torque and loading cycles increase [13–15].

Although abundant studies have investigated survival rates and/or complication incidences, no comparative studies of different implant/abutment connection systems have been performed. As a consequence, survival rates and the incidence of complications according to the type of implant/abutment connection can only be indirectly compared in systematic reviews [4,16]. Therefore, the present study was conducted to retrospectively compare the survival rates and the incidence of post-loading complications in two implant systems—one an ICS-BL and the other an ECS—installed in one institution.

MATERIALS AND METHODS

This study was a retrospective analysis of the cumulative survival rates (CSRs) and the incidence of complications in two implant systems—one ICS-BL (ASTRA Tech Implant System EV, Dentsply Implants, Mölndal, Sweden) and one ECS (Brånemark Implant System, Nobel Biocare, Göteborg, Sweden)—and was approved by the Institutional Review Board at Asan Medical Center (S2012-2211-0001). A total of 2,651 implants in 1,074 patients were reviewed, including all types of implant prostheses, such as fixed partial or full-arch restorations, hybrid-type restorations and overdentures. All the patients were treated in the Department of Dentistry, Asan Medical Center in

Seoul, South Korea between January 2007 and December 2010.

A thorough and complete review of the medical records of the enrolled patients was performed and all data were inserted into spreadsheets (Microsoft Excel 2007, Microsoft Inc., Redmond, WA, USA). The collected data included the implant system (ASTRA Tech or Brånemark), the position of the fixture, the diameter and length of the fixture, the date of fixture installation, the date of prosthesis delivery, the date of the last visit, the type of prosthesis (fixed partial, fixed full-arch, hybrid, or overdenture), the type of crown retention (screw, cement, or screw-cement), the type of superstructure (gold, metal-ceramic, or all ceramic), the date of fixture removal due to failure (if any), the probing depth around the implant crown, thread exposure in follow-up radiographic images taken after at least three months of loading, soft tissue complications, chipping of the veneering material, fracture of the implant, fracture of the implant crown, loosening or fracture of the abutment or screw, loss of retention, and loss of access hole filling material. Thread exposure in radiographic images was defined as marginal bone loss involving more than two threads exposed in an ECS or extending beyond the microthread region in an ICS-BL [4,17]. A soft tissue complication was considered to be present if records indicated signs of inflammation, bleeding on probing, suppuration, hyperplasia, or dehiscence in the peri-implant mucosa. Among the complications recorded, probing pocket depth > 4 mm, thread exposure in follow-up radiographic images, and soft tissue complications were considered to be biological complications, whereas chipping of the veneering material, fracture of the implant, fracture of the implant crown, loosening or fracture of the abutment or screw, loss of retention, and loss of access hole filling material were considered to be technical complications.

The observation period of an implant was defined as the time interval from the day of prosthesis delivery to the day of the last visit in a patient's medical record. Survival was defined as the condition of an implant remaining *in situ* with or without modifications, while failure was defined as the condition of an implant that had to be removed [18]. CSRs were calculated using time-table survival probabilities and the log-rank chi-square test was used to compare the survival rates between the two implant systems. The incidence of biological and technical complications between the two systems was compared with the Pearson chi-square test. The statistical analysis was carried out with IBM SPSS Statistics ver. 22.0 (IBM Co., Armonk, NY, USA), and *P*-values < 0.05 were considered to indicate statistical significance.

RESULTS

The characteristics of the subjects according to the type of implant that was placed are presented in Tables 1 and 2. A total of 1,074 patients aged between 14 and 92 years (mean, 53.1 ± 13.5 years) at the time of fixture installation, of whom 484 were female, were enrolled in the study. A total of 2,651 implants (1,167 ICS-BLs and 1,484 ECSs) were placed in the 1,074 patients (551 ICS-BLs and

Table 1. Demographics of the enrolled patients (n = 1,074).

Demographic	ECS			ICS-BL			Overall		
	Male	Female	Subtotal	Male	Female	Subtotal	Male	Female	Total
No. of patients	284	239	523	306	245	551	590	484	1,074
Age (year)									
≤29	13	8	21	22	29	51	35	37	72
30–39	20	15	35	32	33	65	52	48	100
40–59	156	129	285	179	119	298	335	248	583
60–79	88	82	170	69	64	133	157	146	303
≥80	7	5	12	4	0	4	11	5	16
Mean±SD	55±13	57±12	56±13	51±13	50±14	50±13	53±13	53±14	53±14

ECS: external connection implant system, ICS-BL: bone-level internal connection implant system, SD: standard deviation.

523 ECSs), with an approximate average of 2.47 implants per patient. A total of 653 ICS-BL implants (56.0%) and 727 ECS implants (49.0%) were inserted in the maxillae, while 659 ICS-BL implants (56.5%) and 836 ECS implants (56.3%) were placed in the molar region. The average observation periods for the ICS-BL and ECS were 3.4 years (range, 0.1–6.2 years) and 3.1 years (range, 0.1–6.0 years), respectively. More than half of the superstructures were fixed partial prostheses of screw-retained gold crowns with resin veneering.

Cumulative survival rate

The overall CSR after six years was 96.1%. No statistically significant difference between the two systems was observed, although the CSR for the ICS-BL (94.9%) was lower than that for the ECS (97.1%) (Table 3). Both systems showed similar pattern of failure occurrence, in which more than half of failures occurred in the first year of loading. The ICS-BLs mostly failed in the molar region, whereas the failure rate of the ECSs did not significantly vary depending on the position of the implant. Moreover, higher failure rates were observed in the ICS-BLs in the mandibular molar region and in the ECSs in the maxillary anterior region ($P < 0.05$) (Fig. 1).

Complication incidence

Fig. 2 shows the incidence of complications in the two implant systems. Biological complications (2.1%–10.4%) were more frequent than technical complications (0.1%–6.9%). Of all the complications investigated, soft tissue complications had the highest incidence (8.1% in the ICS-BLs and 10.4% in the ECSs), followed by loosening or fracture of the abutment or screw (6.9% and 3.2%, respectively), probing pocket depth > 4 mm (4.0% and 4.3%, respectively), and chipping of the veneering material (3.5% and 3.0%, respectively), while the incidence of other complications was less than 3.0%. Fractures of the implant or crown occurred very rarely. Regardless of statistical significance, the ECSs tended to show more biological complications while the ICS-BLs were more prone to technical complication. Moreover, soft tissue complications were more frequent in the ECSs ($P = 0.005$) and loosening or fracture of

the abutment or screw occurred more frequently in the ICS-BLs ($P < 0.001$).

DISCUSSION

The present study compared the CSRs and the incidence of complications in two different implant systems. Since most commercially available implant systems yield a satisfactory outcome in terms of osseointegration, postloading complications are of primary importance for the long-term success of an implant. In order to ensure the usefulness of our data in future systematic reviews or meta-analyses, the functional complications of implants were categorized according to Misch and Wang's criteria [8]. Previous studies of implant complications have either involved one system with a small number of subjects or several systems with a relatively large number of subjects. Analyses of one system with a small number of subjects may present in-depth information on the system studied, but are not more generally relevant due to their small sample sizes. Meanwhile, the extant studies on several systems with a large number of subjects were conducted using a multicenter design, in which the collected data are often heterogeneous. In the present study, more than 500 subjects with more than 1,000 implants for each system were enrolled, and all procedures were performed in the same center. These considerations increase the relevance of the present study.

The six-year CSRs were 94.9% for the ICS-BL and 97.1% for the ECS. These CSRs correspond to those reported in previous studies [4,19]. Although ECSs had a higher CSR than ICS-BLs, the difference was not statistically significant. This result should be interpreted with caution because the incidence of failure of the ICS-BLs was higher through the second year to the sixth year compared to that of the ECSs. The more frequent failure in the ICS-BLs was partly associated with fractures of the fixture. Previous studies have shown an incidence of fracture of 0.7% for ICS-BLs and 0.18% for ECSs [20,21]. Cha et al. [11] also reported that 11 of 136 implants were removed due to implant fracture within five years. For a proper and accurate comparison of the two systems, long-term CSRs of

Table 2. Characteristics of the implants investigated in this study (n = 2,651).

Variable	ECS			ICS-BL			Overall		
	Male	Female	Subtotal	Male	Female	Subtotal	Male	Female	Total
Implant position									
Maxilla									
Anterior	69	45	114	98	86	184	167	131	298 (11.2)
Premolar	147	110	257	86	84	170	233	194	427 (16.1)
Molar	196	160	356	188	111	299	384	271	655 (24.7)
Mandible									
Anterior	63	32	95	31	34	65	94	66	160 (6.0)
Premolar	98	84	182	30	59	89	128	143	271 (10.2)
Molar	255	225	480	196	164	360	451	389	840 (31.7)
Subtotal	828	656	1,484	629	538	1,167	1,457	1,194	2,651 (100)
Observation period (year)									
<1	183	140	323	125	110	235	308	250	558 (21.0)
1–2	205	190	395	105	102	207	310	292	602 (22.7)
2–3	122	122	244	128	122	250	250	244	494 (18.6)
3–4	168	142	310	176	132	308	344	274	618 (23.3)
4–5	110	100	210	90	56	146	200	156	356 (13.4)
5–6	1	1	2	14	7	21	15	8	23 (0.9)
Subtotal	789	695	1,484	638	529	1,167	1,427	1,224	2,651 (100)
Type of retention									
Screw	729	594	1,323	384	370	754	1,113	964	2,077 (78.3)
Cement	57	25	82	111	116	227	168	141	309 (11.7)
Screw-cement	40	39	79	117	69	186	157	108	265 (10.0)
Subtotal	826	658	1,484	612	555	1,167	1,438	1,213	2,651 (100)
Type of prosthesis									
Fixed partial	694	583	1,277	586	507	1,093	1,280	1,090	2,370 (89.4)
Fixed full-arch	15	10	25	11	5	16	26	15	41 (1.5)
Hybrid	17	9	26	11	4	15	28	13	41 (1.5)
Overdenture	99	57	156	21	22	43	120	79	199 (7.5)
Subtotal	825	659	1,484	629	538	1,167	1,454	1,197	2,651 (100)
Superstructure									
Gold-resin	627	488	1,115	561	488	1,049	1,188	976	2,164 (81.6)
Metal-ceramic	196	164	360	42	36	78	238	200	438 (16.5)
All ceramic	2	7	9	26	14	40	28	21	49 (1.8)
Subtotal	825	659	1,484	629	538	1,167	1,454	1,197	2,651 (100)

ECS: external connection implant system, ICS-BL: bone-level internal connection implant system.

more than 10 years should be examined.

Previous studies comparing these two systems focused on technical complications [4,22] and no studies have compared biological complications in these systems. In the present study, both categories of complications were simultaneously investigated and compared. Soft tissue complications, which fall into the category of biological complications, were the most frequent complication.

However, it is possible that the incidence of soft tissue complications was underestimated, since bleeding on probing or soft tissue enlargement/dehiscence around the implant can often be observed in daily practice. Unfortunately, no previous studies have evaluated the incidence of soft tissue complications. The second most frequent complication was loosening or fracture of the abutment or screw, which falls into the category of technical complications.

Table 3. Life-table analysis of the cumulative survival rates of the two implant systems.

Period (year)	Overall					ICS-BL					ECS				
	Initial	Withdrawn	Failed	SR	CSR	Initial	Withdrawn	Failed	SR	CSR	Initial	Withdrawn	Failed	SR	CSR
0-1	2,651	527	31	0.997	0.987	1,167	222	13	0.996	0.988	1,484	305	18	0.998	0.987
1-2	2,093	596	6	0.997	0.984	932	203	4	0.995	0.983	1,161	393	2	0.998	0.985
2-3	1,491	489	5	0.996	0.980	725	247	3	0.995	0.978	766	242	2	0.997	0.982
3-4	997	611	7	0.990	0.970	475	305	3	0.991	0.969	522	306	4	0.989	0.971
4-5	379	354	2	0.990	0.961	167	144	2	0.979	0.949	212	210	0	1.000	0.971
5-6	23	23	0	1.000	0.961	21	21	0	1.000	0.949	2	2	0	1.000	0.971

There was no statistically significant difference in CSR between the two systems according to the log-rank test ($P=0.619$).

SR: survival rate, CSR: cumulative survival rate, ECS: external connection implant system, ICS-BL: bone-level internal connection implant system.

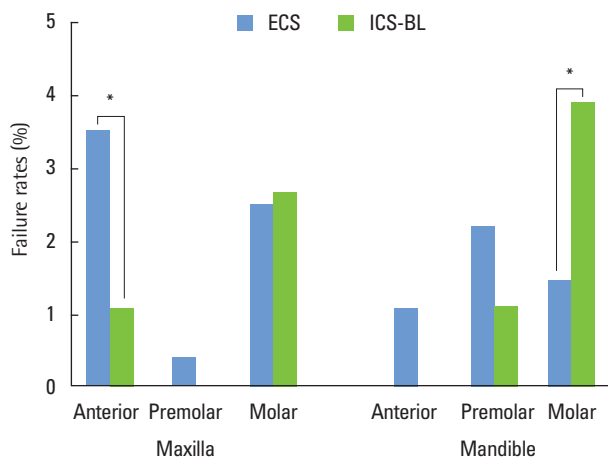


Figure 1. Failure rates according to the position of the implants. The ECSs failed most often in the maxillary anterior region while the ICS-BLs failed most often in the mandibular molar area. ECS: external connection implant system, ICS-BL: bone-level internal connection implant system. $*P<0.05$.

Loosening or fracture of the abutment or screw also included a broad range of situations, which may contribute to its high incidence. Other studies have reported a 5% and 9% occurrence of screw loosening [20,23], which are comparable to our results. It was noteworthy that soft tissue complications were more frequent in the ECS and loosening or fracture of the abutment or screw occurred more frequently in the ICS-BL. Moreover, regardless of statistical significance, the ECS tended to show higher incidences of biological complications, while the ICS-BL was more prone to technical complications.

Recent systematic reviews have reported that the cumulative complication rate of >2 mm of bone loss in implants was 5.2% [20], and two other systemic reviews have shown marginal bone loss rates of 2.6% and 5.7% [21,23]. In the present study, thread exposure in radiographs was used as a parameter indicating marginal bone loss and had an incidence of 2.1% and 2.5% for the ICS-BLs and ECSs, respectively. The low incidence compared to those found in the previous reviews may reflect the loose definition of thread exposure in radiographs. However, the loose definition was suffi-

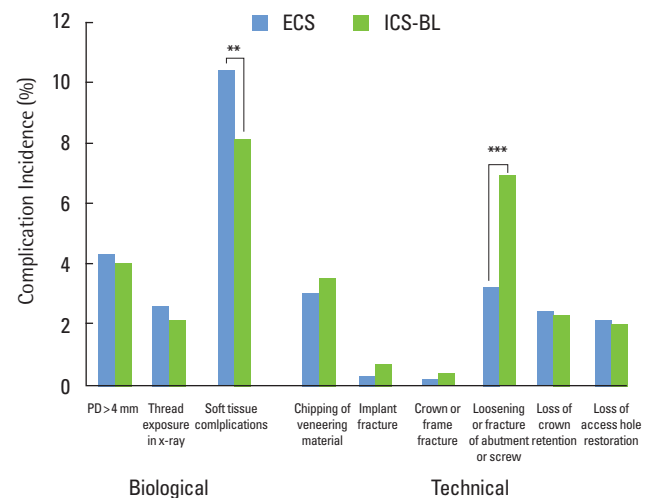


Figure 2. Complication incidence in the two implant systems. Soft tissue complications, belonging to the category of biological complications, occurred more often in the ECSs, while loosening or fracture of the abutment or screw was more frequent in the ICS-BLs. PD: periodontal debridement, ECS: external connection implant system, ICS-BL: bone-level internal connection implant system. $**P<0.01$. $***P<0.001$.

cient to compare the incidences between the two systems because the dimensions of the microthread region in the ICS-BL were similar to those from the platform to the second thread in the ECS.

The higher incidence of soft tissue complications in the ECSs could partly be explained by the effect of platform-switching [24], which was employed in the ICS-BL. In platform-switched systems, some additional thickness in the horizontal soft tissue component might contribute to reducing crestal bone loss resulting from the reformation of biologic width and the microgap. However, another comparative study between platform-matching and platform-switching systems showed minimal marginal bone-level changes with no difference between the implant systems [25]. Taking these studies into account, we suggest that soft tissue complications such as signs of inflammation, bleeding on probing, and suppuration on peri-implant mucosa may be associated with the stability of peri-implant soft tissues rather than that of peri-implant marginal bone level, and that

the ICS-BL can stabilize adjacent soft tissues more than the ECS can. However, further studies are required because other factors, including the emergence profile of the crown and the location of the crown margin in a cement-retained crown, can affect the condition of peri-implant soft tissue.

The frequency of loosening or fracture of the abutment or screw has been reported to be 12% and 19% [17,20], but was much lower in the present study (6.9% in the ICS-BLs and 3.2% in the ECSs). The relatively short follow-up period and the use of a single implant system for each connection type may play a role in these low complication rates. Moreover, in the present study, loosening or fracture of the abutment or screw occurred more often in the ICS-BLs. No previous study has directly compared the occurrence of this complication between the two systems. In recent publications, conflicting results have been reported: more screw loosening has been observed in ECSs, while more axial displacement and a decrease of loosening torque have been reported in ICS-BLs [15,16,26]. Another study conducted in our institution also reported a 25.7% rate of abutment screw loosening in single ICS-BL implant restorations up to five years [11]. Maeda et al. [10] demonstrated that the thinner lateral wall at the coronal part of an ICS fixture was related to fixture tearing or fracture. Furthermore, the ICS-BLs showed a faster CSR decrease than did the ECSs over time, which may be another indication that the coronal portion of fixtures in the ICS-BL is relatively weak.

In conclusion, within the limitations of this retrospective study, the ICS-BLs were more prone to technical complications while the ECSs were more vulnerable to biological complications. For this reason, the ICS-BL may be more suitable for restoring anterior regions experiencing esthetic challenges, whereas the ECS may be preferred in posterior regions under a high occlusal load.

CONFLICT OF INTEREST

No potential conflict of interest relevant to this article was reported.

ACKNOWLEDGEMENTS

This research was supported by Basic Science Research Program through the National Research Foundation of Korea (NRF) funded by the Ministry of Science, ICT, and Future Planning (NRF-2013 R1A1A2011974).

ORCID

Sung-Wook Chae <http://orcid.org/0000-0002-7122-9692>
 Young-Sung Kim <http://orcid.org/0000-0003-2674-3649>
 Yong-Moo Lee <http://orcid.org/0000-0002-5619-3847>
 Won-Kyung Kim <http://orcid.org/0000-0003-2557-1646>
 Young-Kyoo Lee <http://orcid.org/0000-0001-7065-282X>
 Su-Hwan Kim <http://orcid.org/0000-0002-3431-453X>

REFERENCES

1. Brånemark PI, Adell R, Breine U, Hansson BO, Lindström J, Ohlsson A. Intra-osseous anchorage of dental prostheses. I. Experimental studies. *Scand J Plast Reconstr Surg* 1969;3:81-100.
2. Astrand P, Ahlqvist J, Gunne J, Nilson H. Implant treatment of patients with edentulous jaws: a 20-year follow-up. *Clin Implant Dent Relat Res* 2008;10:207-17.
3. Lekholm U, Grondahl K, Jemt T. Outcome of oral implant treatment in partially edentulous jaws followed 20 years in clinical function. *Clin Implant Dent Relat Res* 2006;8:178-86.
4. Astrand P, Engquist B, Dahlgren S, Grondahl K, Engquist E, Feldmann H. Astra Tech and Brånemark system implants: a 5-year prospective study of marginal bone reactions. *Clin Oral Implants Res* 2004;15:413-20.
5. Becker W, Becker BE. Replacement of maxillary and mandibular molars with single endosseous implant restorations: a retrospective study. *J Prosthet Dent* 1995;74:51-5.
6. Brånemark PI, Zarb GA, Albrektsson T. *Tissue-Integrated prostheses: osseointegration in clinical dentistry*. Chicago, IL: Quintessence Publishing Co.; 1985.
7. Finger IM, Castellon P, Block M, Elian N. The evolution of external and internal implant/abutment connections. *Pract Proced Aesthet Dent* 2003;15:625-32.
8. Misch K, Wang HL. *Implant surgery complications: etiology and treatment*. *Implant Dent* 2008;17:159-68.
9. Sutter F, Weber HP, Sorensen J, Belser UC. The new restorative concept of the ITI dental implant system: design and engineering. *Int J Periodontics Restorative Dent* 1993;13:409-31.
10. Maeda Y, Satoh T, Sogo M. In vitro differences of stress concentrations for internal and external hex implant-abutment connections: a short communication. *J Oral Rehabil* 2006;33:75-8.
11. Cha HS, Kim YS, Jeon JH, Lee JH. Cumulative survival rate and complication rates of single-tooth implant; focused on the coronal fracture of fixture in the internal connection implant. *J Oral Rehabil* 2013;40:595-602.
12. Binon PP, McHugh MJ. The effect of eliminating implant/abutment rotational misfit on screw joint stability. *Int J Prosthodont* 1996;9:511-9.
13. Dailey B, Jordan L, Blind O, Tavernier B. Axial displacement of abutments into implants and implant replicas, with the tapered conescrew internal connection, as a function of tightening torque. *Int J Oral Maxillofac Implants* 2009;24:251-6.
14. Kim KS, Lim YJ, Kim MJ, Kwon HB, Yang JH, Lee JB, et al. Variation in the total lengths of abutment/implant assemblies generated with a function of applied tightening torque in external and internal implant-abutment connection. *Clin Oral Implants Res* 2011;22:834-9.
15. Lee JH, Kim DG, Park CJ, Cho LR. Axial displacements in external and internal implant-abutment connection. *Clin Oral Implants Res* 2014;25:e83-9.
16. Gracis S, Michalakakis K, Vigolo P, Vult von Steyern P, Zwahlen M,

- Sailer I. Internal vs. external connections for abutments/reconstructions: a systematic review. *Clin Oral Implants Res* 2012;23 Suppl 6:202-16.
17. Papaspyridakos P, Chen CJ, Chuang SK, Weber HP, Gallucci GO. A systematic review of biologic and technical complications with fixed implant rehabilitations for edentulous patients. *Int J Oral Maxillofac Implants* 2012;27:102-10.
 18. Buser D, von Arx T, ten Bruggenkate C, Weingart D. Basic surgical principles with ITI implants. *Clin Oral Implants Res* 2000;11 Suppl 1:59-68.
 19. van Steenberghe D, De Mars G, Quirynen M, Jacobs R, Naert I. A prospective split-mouth comparative study of two screw-shaped self-tapping pure titanium implant systems. *Clin Oral Implants Res* 2000;11:202-9.
 20. Jung RE, Zembic A, Pjetursson BE, Zwahlen M, Thoma DS. Systematic review of the survival rate and the incidence of biological, technical, and aesthetic complications of single crowns on implants reported in longitudinal studies with a mean follow-up of 5 years. *Clin Oral Implants Res* 2012;23 Suppl 6:2-21.
 21. Romeo E, Storelli S. Systematic review of the survival rate and the biological, technical, and aesthetic complications of fixed dental prostheses with cantilevers on implants reported in longitudinal studies with a mean of 5 years follow-up. *Clin Oral Implants Res* 2012;23 Suppl 6:39-49.
 22. Koo KT, Lee EJ, Kim JY, Seol YJ, Han JS, Kim TI, et al. The effect of internal versus external abutment connection modes on crestal bone changes around dental implants: a radiographic analysis. *J Periodontol* 2012;83:1104-9.
 23. Pjetursson BE, Thoma D, Jung R, Zwahlen M, Zembic A. A systematic review of the survival and complication rates of implant-supported fixed dental prostheses (FDPs) after a mean observation period of at least 5 years. *Clin Oral Implants Res* 2012;23 Suppl 6: 22-38.
 24. Lazzara RJ, Porter SS. Platform switching: a new concept in implant dentistry for controlling postrestorative crestal bone levels. *Int J Periodontics Restorative Dent* 2006;26:9-17.
 25. Astrand P, Engquist B, Dahlgren S, Engquist E, Feldmann H, Grondahl K. Astra Tech and Brånemark System implants: a prospective 5-year comparative study. Results after one year. *Clin Implant Dent Relat Res* 1999;1:17-26.
 26. Squier RS, Psoter WJ, Taylor TD. Removal torques of conical, tapered implant abutments: the effects of anodization and reduction of surface area. *Int J Oral Maxillofac Implants* 2002;17:24-7.