

ORAL PRESENTATION

Open Access

# Quantitative molecular imaging of angiogenesis-targeted fluorinated nanoparticles: new approaches for B<sub>1</sub>-mapping compensation for <sup>19</sup>F-MRI

Matthew J Goette<sup>1\*</sup>, Anne H Schmieder<sup>1</sup>, Todd A Williams<sup>1</sup>, John S Allen<sup>1</sup>, Jochen Keupp<sup>2</sup>, Gregory M Lanza<sup>1</sup>, Samuel A Wickline<sup>1</sup>, Shelton D Caruthers<sup>1</sup>

From 16th Annual SCMR Scientific Sessions  
San Francisco, CA, USA. 31 January - 3 February 2013

## Background

Quantitative MR molecular imaging allows for the detection of targeted contrast agents to diagnose disease states and monitor response to therapy, such as anti-angiogenic therapy in atherosclerosis and cancer with  $\alpha_v\beta_3$ -integrin targeted perfluorocarbon (PFC) nanoparticles. Recently, <sup>19</sup>F MR using a <sup>19</sup>F/<sup>1</sup>H dual-tuned RF coil has been utilized to directly image and quantify the fluorinated core of these PFC nanoparticle (NP) emulsions. However, low concentrations of these fluorine agents in the body, in conjunction with varying RF coil sensitivity profiles (B<sub>1</sub>-field inhomogeneities) raise obstacles to accurate quantification. This study presents a strategy to more accurately quantify the sparse <sup>19</sup>F signal from PFC NP emulsions with a <sup>1</sup>H image-based Actual Flip-angle Imaging (AFI) B<sub>1</sub>-mapping correction to the <sup>19</sup>F and <sup>1</sup>H images.

## Methods

New Zealand White Rabbits (2 kg) were implanted with a VX2 adenocarcinoma tumor (2-3 cm) in the hind leg. Angiogenesis imaging was performed 2 weeks post implantation, under ketamine/xylazine anesthesia. An  $\alpha_v\beta_3$ -integrin targeted perfluoro-octyl bromide (PFOB) nanoparticle emulsion was prepared, and injected intravenously 3 hours before imaging. MR data were acquired on a 3T clinical whole-body scanner (Achieva, Philips Healthcare) with a dual <sup>19</sup>F/<sup>1</sup>H spectrometer system and a dual-tuned transmit/receive single loop surface RF coil (7×12 cm). A simultaneous <sup>19</sup>F/<sup>1</sup>H gradient echo (GRE)

imaging sequence was used with: <sup>19</sup>F offset frequency on the center of the PFOB CF<sub>2</sub> peak, 15 4-mm slices, 140 mm FOV, 48<sup>3</sup> matrix,  $\alpha = 60^\circ$ , TE/TR = 2.2/8.5 ms, 21 min scan time. The B<sub>1</sub> field was mapped using an AFI sequence with matching geometry. Using the flip angle map and a model of the GRE signal, a spatially-dependent calibration mask was calculated in MATLAB (MathWorks) and used to compensate the <sup>1</sup>H and <sup>19</sup>F signal intensities for the GRE sequence.


## Results

PFC NP targeted the tumor neovasculature, and provided localized <sup>19</sup>F signal as expected. Figure 1 displays the uncorrected (top) and corrected (bottom) <sup>1</sup>H images with the <sup>19</sup>F signal superimposed, using the AFI (middle) B<sub>1</sub>-mapping correction technique. After correction, the <sup>1</sup>H signal intensity profile as a function of distance from the surface coil (located at right) is improved. After the same correction to the <sup>19</sup>F signal, the measured concentration of nanoparticles when compared to a standard was  $10.2 \pm 1.0 \text{ mM}_{19\text{F}}$ , versus  $9.0 \pm 2.2 \text{ mM}_{19\text{F}}$  before correction.

## Conclusions

An image-based B<sub>1</sub>-mapping correction acquired with <sup>1</sup>H can be used to correct signal intensities for <sup>19</sup>F and <sup>1</sup>H images of angiogenesis in an *in vivo* rabbit model. The correction results in a more homogeneous <sup>1</sup>H image of the anatomy and facilitates accurate measurement of bound  $\alpha_v\beta_3$ -integrin targeted nanoparticles with <sup>19</sup>F imaging.

<sup>1</sup>School of Medicine, Washington University in St. Louis, St. Louis, MO, USA  
Full list of author information is available at the end of the article

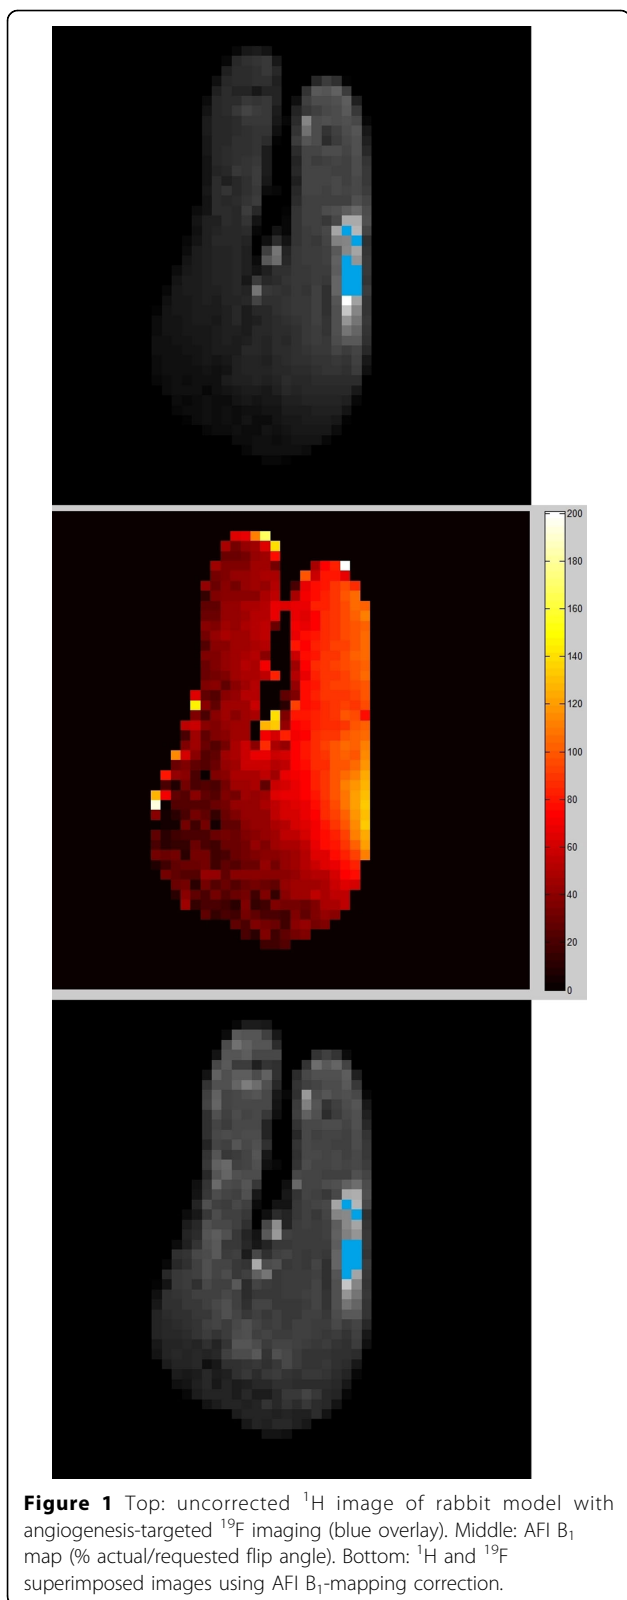

## Funding

AHA 11PRE7530046; NIH R01 HL073646.

## Author details

<sup>1</sup>School of Medicine, Washington University in St. Louis, St. Louis, MO, USA.

<sup>2</sup>Philips Research Europe, Hamburg, Germany.

Published: 30 January 2013

doi:10.1186/1532-429X-15-S1-O83

**Cite this article as:** Goette *et al.*: Quantitative molecular imaging of angiogenesis-targeted fluorinated nanoparticles: new approaches for  $B_1$ -mapping compensation for  $^{19}\text{F}$ -MRI. *Journal of Cardiovascular Magnetic Resonance* 2013 15(Suppl 1):O83.

Submit your next manuscript to BioMed Central and take full advantage of:

- Convenient online submission
- Thorough peer review
- No space constraints or color figure charges
- Immediate publication on acceptance
- Inclusion in PubMed, CAS, Scopus and Google Scholar
- Research which is freely available for redistribution

Submit your manuscript at  
[www.biomedcentral.com/submit](http://www.biomedcentral.com/submit)

