

POSTER PRESENTATION

Open Access

Multi-echo single-shot EPI for hyperpolarized ^{13}C cardiac metabolic imaging of small animals

Andreas Sigfridsson^{1*}, Kilian Weiss¹, Lukas Wissmann¹, Julia Busch¹, Marcin Krajewski¹, Darach O h-Ici^{2,3}, Michael Batel⁴, Georgios Batsios¹, Sebastian Kozerke¹

From 16th Annual SCMR Scientific Sessions
San Francisco, CA, USA. 31 January - 3 February 2013

Background

Cardiac metabolic imaging based on hyperpolarized ^{13}C -labeled pyruvate shows great potential for assessing the metabolic changes that the heart undergoes during ischemia [1]. Rodent animal models offer unique opportunities to study ischemic processes, however, methods based on spectral-spatial excitation [2] of the individual metabolites is challenging due to the large minimal slice thickness that can be achieved with available gradient systems. A thick slice introduces both signal dephasing over the slice and errors due to partial volume effects.

In this work, we explore multi-echo measurements using single-shot echo-planar imaging (EPI) readouts for thin slice dynamic cardiac metabolic imaging of small animals.

Methods

Healthy female Wistar rats (200g) were scanned in a 9.4T horizontal bore Bruker MRI system. A home-built multi-sample dissolution DNP system was used to hyperpolarize pyruvate [3]. During image acquisition, 2ml 45mM ^{13}C -labeled hyperpolarized pyruvate was injected in the tail

vein. The pulse sequence consisted of 7 echoes separated by 383us, each triggered to 80ms after the R-wave of the ECG. With an RR-interval of ~180ms, a temporal resolution of ~1.3s was obtained. For each image, a 4mm short axis slice was excited with a flip angle of 8 degrees, and a 60x60mm² FOV was read out using a single-shot EPI-readout with a matrix of 30x30. Images for each metabolite were then reconstructed and separated into lactate, pyruvate hydrate, alanine, pyruvate and bicarbonate using a multi-point Dixon technique [4,5]. The reconstruction included correction of EPI gradient delays, B0 offset, chemical shift displacement and separation.

Results

Images for the metabolites are shown in Figure 1. Time curves for the metabolites in two segments of the myocardium are shown in Figure 2.

Conclusions

By using the multi-echo technique, the requirements on the gradient system performance are relaxed. In contrast





Figure 1 Metabolic images of pyruvate (left), lactate (center) and bicarbonate (right) as a sum over the signal bolus. Signal loss in the posterior wall of the heart is due to the sensitivity of the surface coil lying on the chest of the rat. The thin slice excitation reduces the impact of dephasing due to magnetic field inhomogeneities across the slice as well as partial volume effects. The result is a higher effective in-plane resolution.

¹Biomedical Engineering, ETH Zurich, Zurich, Switzerland
Full list of author information is available at the end of the article

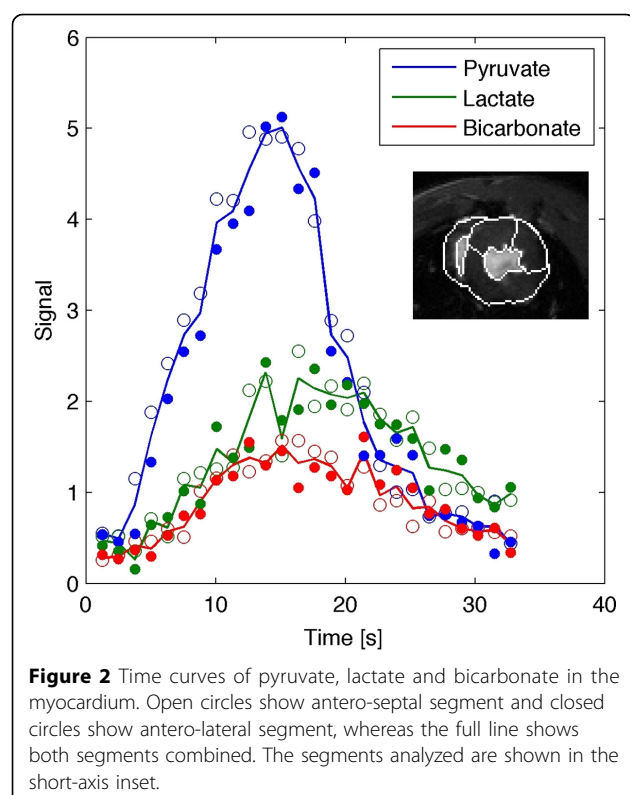

to using a spectral-spatial excitation, a simple slice excitation can be used that allows for thinner slices. This is especially important in small animal imaging. Due to the thin slices, the dephasing and partial volume effects are significantly reduced, and the effective in-plane resolution is improved. This is especially important in separating the signal from pyruvate between myocardium and blood pool when using kinetic modeling. The high in-plane resolution is of importance for metabolic imaging after selective occlusion of one coronary artery, and for studies of the metabolic changes that the heart undergoes under controlled experiments in small animals.

Funding

Marie Curie Intra European Fellowship.
Swiss National Science Foundation.

Author details

¹Biomedical Engineering, ETH Zurich, Zurich, Switzerland. ²Congenital Heart Disease and Pediatric Cardiology, Deutsches Herzzentrum Berlin, Berlin, Germany. ³Imaging Sciences and Biomedical Engineering, King's College London, London, UK. ⁴Physical Chemistry, ETH Zurich, Zurich, Switzerland.

Published: 30 January 2013

References

1. Schroeder, et al. *Circulation* 2011, **124**:1580-1594.
2. Cunningham, et al. *JMR* 2008, **193**:139-146.
3. Batel, et al. *JMR* 2012, **214**:166-174.

4. Reeder, et al. *MRM* 2003, **51**:35-45.
5. Wiesinger, et al. *MRM* 2012, **68**:8-16.

doi:10.1186/1532-429X-15-S1-P217

Cite this article as: Sigfridsson et al.: Multi-echo single-shot EPI for hyperpolarized ¹³C cardiac metabolic imaging of small animals. *Journal of Cardiovascular Magnetic Resonance* 2013 **15**(Suppl 1):P217.

Submit your next manuscript to BioMed Central and take full advantage of:

- Convenient online submission
- Thorough peer review
- No space constraints or color figure charges
- Immediate publication on acceptance
- Inclusion in PubMed, CAS, Scopus and Google Scholar
- Research which is freely available for redistribution

Submit your manuscript at
www.biomedcentral.com/submit

