



CORRECTION

Correction to: Clinical Performance of Samfilcon A Contact Lenses in Intensive Digital Device Users: A Multicenter, Prospective Clinical Study

Ömür Ö. Uçakhan · Emrullah Taşındı · Ebru Toker · Ferda Çiftçi ·
Sevda Aydın Kurna · Mutlu Acar · Ferah Özçelik · Ali Rıza Cenk Çelebi ·
Hatice Elvin Yıldız · Yonca Aydın Akova · Emine Sibel Öncü ·
Zeynep Özbek · Zerrin Tuncer · Sibel Kocabeyoğlu · Burak Şeker ·
Deniz Kaya · Maxime Barakat
Published online: October 22, 2021
© The Author(s) 2021

Correction to: Ophthalmol Ther
<https://doi.org/10.1007/s40123-021-00389-4>

The original article can be found online at <https://doi.org/10.1007/s40123-021-00389-4>.

Ö. Ö. Uçakhan
Department of Ophthalmology, Ankara University
School of Medicine, Ankara, Turkey

E. Taşındı
Department of Ophthalmology, İstanbul Okan
University Faculty of Medicine, İstanbul, Turkey

E. Toker
Department of Ophthalmology, Marmara University
Pendik Training and Research Hospital, İstanbul,
Turkey

F. Çiftçi
Department of Ophthalmology, Batıgöz Altunizade
Hospital, İstanbul, Turkey

S. A. Kurna
Department of Ophthalmology, Fatih Sultan
Mehmet Training and Research Hospital, İstanbul,
Turkey

M. Acar
Department of Ophthalmology, Dışkapı Yıldırım
Beyazıt Training and Research Hospital, Ankara,
Turkey

F. Özçelik
Department of Ophthalmology, Prof Dr Reşat Belger
Beyoğlu Training and Research Hospital, İstanbul,
Turkey

A. R. C. Çelebi
Department of Ophthalmology, Acıbadem Atakent
Hospital, İstanbul, Turkey

H. E. Yıldız
Department of Ophthalmology, Haydarpaşa
Numune Training and Research Hospital, İstanbul,
Turkey

Y. A. Akova
Department of Ophthalmology, Bayındır
Kavaklıdere Hospital, Ankara, Turkey

E. S. Öncü
Department of Ophthalmology, Birinci Eye
Hospital, İstanbul, Turkey

Z. Özbek
Department of Ophthalmology, 9 Eylül University
Hospital, İzmir, Turkey

Figure 3 in the original version of this article has been replaced, the figure should have appeared as shown below.

The original article has been corrected.

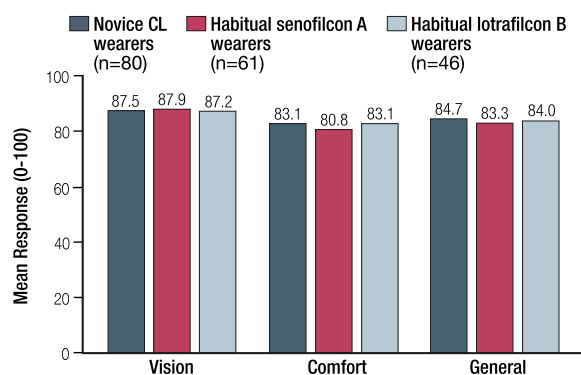


Fig. 3 Patient satisfaction with samfilcon A lenses: comfort, visual quality and in general (4-week assessment). *CL* contact lens. Likert Scale (0–100) 100–81: excellent; 80–61: very good; 60–41: good; 40–21: fair; 20–0: poor

OPEN ACCESS

This article is licensed under a Creative Commons Attribution-NonCommercial 4.0 International License, which permits any non-commercial use, sharing, adaptation, distribution and reproduction in any medium or format, as long as you give appropriate credit to the original author(s) and the source, provide a link to the Creative Commons licence, and indicate if changes were made. The images or other third party material in this article are included in the article's Creative Commons licence, unless indicated otherwise in a credit line to the material. If material is not included in the article's Creative Commons licence and your intended use is not permitted by statutory regulation or exceeds the permitted use, you will need to obtain permission directly from the copyright holder. To view a copy of this licence, visit <http://creativecommons.org/licenses/by-nc/4.0/>.

Z. Tuncer

Department of Ophthalmology, Göz Vakfı
Bayrampaşa Eye Hospital, Istanbul, Turkey

S. Kocabeyoğlu

Department of Ophthalmology, Hacettepe University
Faculty of Medicine, Ankara, Turkey

B. Şeker (✉) · D. Kaya

Bausch + Lomb, Istanbul, Turkey
e-mail: burak.seker@bausch.com

M. Barakat

Bausch Health, Laval, QC, Canada