

Methodology

Open Access

Signal stability of Cy3 and Cy5 on antibody microarrays

Qiang Gu*, Thamil Mani Sivanandam and Caroline Aehyun Kim

Address: Department of Neurobiology and Anatomy, Wake Forest University School of Medicine, Medical Center Boulevard, Winston-Salem, North Carolina 27157, USA

Email: Qiang Gu* - qgu@wfubmc.edu; Thamil Mani Sivanandam - tsivan@wfubmc.edu; Caroline Aehyun Kim - ckim@wfubmc.edu

* Corresponding author

Published: 11 October 2006

Received: 22 June 2006

Proteome Science 2006, 4:21 doi:10.1186/1477-5956-4-21

Accepted: 11 October 2006

This article is available from: <http://www.proteomesci.com/content/4/1/21>

© 2006 Gu et al; licensee BioMed Central Ltd.

This is an Open Access article distributed under the terms of the Creative Commons Attribution License (<http://creativecommons.org/licenses/by/2.0>), which permits unrestricted use, distribution, and reproduction in any medium, provided the original work is properly cited.

Abstract

Background: The antibody microarray technique is a newly emerging proteomics tool for differential protein expression analyses that uses fluorescent dyes Cy 3 and Cy 5. Environmental factors, such as light exposure, can affect the signal intensity of fluorescent dyes on microarray slides thus, it is logical to scan microarray slides immediately after the final wash and drying processes. However, no research data are available concerning time-dependent changes of fluorescent signals on antibody microarray slides to this date. In the present study, microarray slides were preserved at -20°C after regular microarray experiments and were rescanned at day 10, 20 and 30 to evaluate change in signal intensity.

Results: Fluorescent intensities of microarray spots were detected using a confocal laser scanner after the experiment at day 0, and re-examined at day 10, 20 and 30, respectively. Fluorescent intensities of rescanned microarray spots did not show significant changes when compared with those scanned immediately after standard microarray experiments.

Conclusion: Microarray slides can be preserved and rescanned multiple times using a confocal laser scanner over a period of days or weeks.

Background

Antibody microarray analyses of protein expression levels represent a new trend of cutting-edge proteomics research [1-6], and have been increasingly utilized in studies of normal and pathological conditions [7-22]. The technique has several distinct advantages. First, compared to the cDNA microarray analysis, antibody microarrays detect differential gene expression at the protein level. Although cDNA microarray analyses have generated a large database concerning gene expression patterns, most of these studies have focused on gene expression at the mRNA level only, with the assumption that the relative mRNA levels represent the relative levels of proteins. Since there is often a poor correlation between mRNA levels and

protein levels [23-28], this assumption may not be true for many of the genes. Second, the antibody microarray technique is more sensitive compared to gel electrophoreses. With microarray technology, protein levels can be detected in the low pg/ml range. This allows the measurement of the expression of both small and large molecular weight proteins simultaneously, regardless of their isoelectric points. In addition, some protein extraction buffers used for antibody microarray experiments contain non-denaturing detergents in order to keep the proteins in their native state. While gel electrophoreses usually separate denatured proteins for expression analyses, antibody microarrays can measure relative abundance of naïve undenatured proteins.

The vast majority of antibody microarray experiments conducted so far used the fluorescent dyes Cy3 and Cy5 for protein labelling. In general, fluorescent dyes are sensitive to light exposure as well as other environmental factors such as water, high temperature, alkali, and alcohol. Recent evidence indicates that even ozone levels in the laboratory atmosphere could affect fluorescent dyes on microarrays [29]. In order to avoid or to minimize the effects of these risk factors, it is appropriate to scan microarray slides instantly upon finishing the final wash and drying processes without unnecessary delays. However, no data are currently available concerning time-dependent changes of fluorescent signals on antibody microarray slides. Furthermore, the published research on repeated scans of antibody or protein microarrays is scant. Although repeated scans of cDNA microarrays have been conducted [30-35], it is not known whether amine-coupled fluorescent dyes on antibody/protein microarrays behave in the same way as those nucleotide-coupled fluorescent dyes on cDNA microarrays. In addition, previous studies conducted multiple scans of cDNA microarrays sequentially, usually within minutes. Therefore, it is also unknown whether prolonged intervals between scans in the range of days or weeks could modify the signal intensity of fluorescent dyes on antibody or protein microarrays. Furthermore, previous rescan studies were conducted using different laser power levels or photomultiplier tube (PMT) gains rather than using a consistent setting of the laser power and PMT. It is expected that different settings of the laser power and PMT generated different signal intensities. Whether the same setting of the laser power and PMT can generate consistent intensity outcome over time has not been demonstrated. Using a confocal laser scanner to minimize photo-bleaching effects, we scanned microarrays slides at day 0, 10, 20 and 30, respectively. After regular antibody microarray experiments, the microarray slides were stored in a laboratory freezer at -20°C . Fluorescent intensities of microarray spots at these time points were then quantified and compared. Our results indicate no significant changes in intensities of both Cy3 and Cy5 signals over the examined period.

Results and discussion

Clontech™ antibody microarrays were used in this study, which had 1024 microarray spots on each slide. Among them, 6 spots were printed with fluorescence-labeled albumin and served as positive controls, whereas 4 spots were printed with non-labeled albumin and served as negative controls. For all microarray slides, the negative control spots had similar intensities as those of background signals. These 10 control spots were not included in the final microarray spot analyses. The remaining 1014 spots on each microarray slide were followed up throughout the entire length of the study. In order to keep the same exper-

imental condition, the following steps were taken: when a storage vial containing the microarray slide was taken out of the freezer, it was kept at room temperature for 30 minutes; and to keep the scan condition consistent, the same strength of the laser power (100%) and PMT (65%) were used for all scans of the microarray slides. No spot on the microarray slides was saturated using these settings of the laser power and PMT, so that unchanged intensities of microarray spots due to saturation could be excluded in the present study.

For each microarray spot, the signal intensity was measured 4 times, at day 0 (I_0), day 10 (I_{10}), day 20 (I_{20}), and day 30 (I_{30}), respectively. Because I_0 of each microarray spot had a different value, we set I_0 as the reference, and calculated the ratio of I_{10}/I_0 , I_{20}/I_0 , and I_{30}/I_0 , respectively, for each of the 1014 spots on the microarray slide. If the fluorescent signals on a microarray slide decrease over time, the ratio value of I_{10}/I_0 , I_{20}/I_0 , and I_{30}/I_0 should become smaller and smaller. Fourteen slides were examined for Cy3 and for Cy5, respectively.

Figure 1 shows an example of Cy3 signals on a microarray slide at day 0, 10, 20, and 30, respectively. There was no apparent decrease of Cy3 signal intensities.

Quantitative analyses of all Cy3 spots (summarized in Table 1) further suggest that there was no statistically significant change in intensities of Cy3 signals over the examined time frame ($p > 0.05$, ANOVA).

Figure 2 shows an example of Cy5 signals on a microarray slide at day 0, 10, 20, and 30, respectively. Like the case of Cy3, there was no apparent decrease of Cy5 signal intensities. Quantitative analyses of all Cy5 spots (summarized in Table 2) also suggest that there was no statistically significant change in intensities of Cy5 signals over the examined time frame ($p > 0.05$, ANOVA).

Microarray spot signal intensities can span a broad range from 0 to 65536 ($= 2^{16}$). To examine whether microarray spots with different intensities behave differently over time, we divided the microarray spots into three groups according to their intensities: 1) lower range when I_0 was lower than 20000, 2) middle range when I_0 was between 20000 and 40000, and 3) higher range when I_0 was higher than 40000, and calculated spot intensities in each group of the Cy3-labeled ($N = 14$ slides) and in each group of the Cy5-labeled ($N = 14$ slides) at day 0, 10, 20, and 30, respectively. Quantitative analyses did not show statistically significant changes in intensities over the examined time frame regardless of their intensities. ($p > 0.05$, ANOVA).

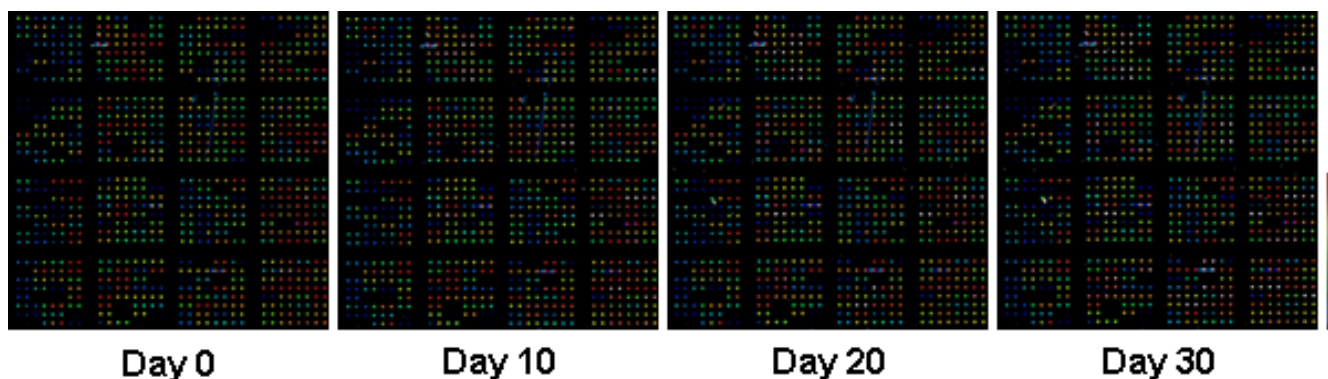


Figure 1
 Examples of Cy3 signals on a microarray slide scanned at day 0, 10, 20, and 30, respectively. At day 0, the spot intensities on this slide range from 261 to 46409, with an average background intensity of 366 versus an average intensity of 488 for the 4 negative control spots. The scale bar on the right indicates color-coded signal intensities.

These results suggest that Cy3 and Cy5 signals on antibody microarrays are stable when the microarray slides are stored in an airtight slide vial at -20°C. These results are crucial to guide contemporary proteomics research involving microarrays. For instance, occasionally microarray slides could not be scanned soon after the experiment due to time restraints. If this is inevitable, microarray slides could be stored and scanned at a later time. Oftentimes, it is determined that signals of some proteins on microarray slides were too strong (e.g. saturated) after data analysis has been done. In such cases, a rescan of microarray slides is usually desirable with a reduced setting of the laser power and/or PMT, so that signal intensities of these pro-

teins become non-saturated and suitable for data analyses.

The signal intensities of microarray spots did not show a significant decrease after repeated scans, suggesting that the employed settings of the laser power and PMT were adequate for multiple scans. We used a confocal microarray scanner in our study, which, due to the confocal nature of the laser beam, kept the bleaching effect of the laser light minimal. However, whether a non-confocal microarray scanner could achieve similar results as a confocal scanner remains to be determined. Also, we tested only Cy3 and Cy5 dyes in the present study. It is possible

Table 1: Summary of ratio comparisons of Cy3 spots.

Slide Number	$\overline{I_{10}/I_0}$	$\overline{I_{20}/I_0}$	$\overline{I_{30}/I_0}$
1	1.037 ± 0.004	1.086 ± 0.005	1.157 ± 0.006
2	1.008 ± 0.017	1.047 ± 0.004	1.087 ± 0.004
3	0.986 ± 0.003	1.025 ± 0.003	1.006 ± 0.002
4	1.021 ± 0.002	1.093 ± 0.002	0.988 ± 0.002
5	0.973 ± 0.007	1.006 ± 0.008	1.071 ± 0.009
6	1.044 ± 0.006	1.121 ± 0.007	1.104 ± 0.007
7	0.991 ± 0.008	0.990 ± 0.003	0.990 ± 0.003
8	0.982 ± 0.003	0.929 ± 0.003	0.948 ± 0.003
9	1.039 ± 0.004	1.051 ± 0.004	1.060 ± 0.004
10	1.055 ± 0.004	1.064 ± 0.006	1.001 ± 0.004
11	1.084 ± 0.009	1.142 ± 0.004	1.075 ± 0.004
12	1.066 ± 0.003	1.117 ± 0.012	1.026 ± 0.003
13	1.135 ± 0.007	1.138 ± 0.006	1.083 ± 0.021
14	0.985 ± 0.004	1.101 ± 0.003	1.114 ± 0.014
Average	1.029 ± 0.013	1.065 ± 0.018	1.051 ± 0.017

Each of the 1014 microarray spot was examined at day 0, 10, 20, and 30, respectively, and its intensities (I_0 , I_{10} , I_{20} , and I_{30}) were measured. Then, the ratios of I_{10}/I_0 , I_{20}/I_0 , and I_{30}/I_0 for each microarray spot were generated. The average ratios of all 1014 spots on each individual slide at day 10 (I_{10}/I_0), day 20 (I_{20}/I_0), and day 30 (I_{30}/I_0) as well as the averaged value of all slides at day 10, 20 and 30 are shown (mean ± SEM).

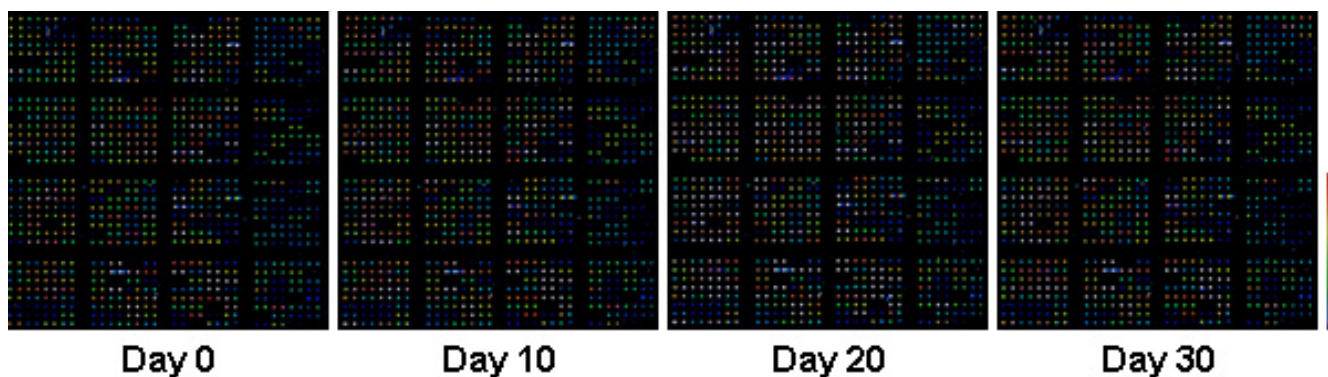


Figure 2
 Examples of Cy5 signals on a microarray slide scanned at day 0, 10, 20, and 30, respectively. At day 0, the spot intensities on this slide range from 592 to 58229, with an average background intensity of 2504 versus an average intensity of 2512 for the 4 negative control spots. The scale bar on the right indicates color-coded signal intensities.

that other fluorescent dyes may show similar results as those of Cy3 and Cy5.

In theory, the fluorescent signal on microarray slides should either remain the same or decrease in intensity but is not expected to increase over time. However, we had a few slides that displayed higher intensities at a later scanning time point when compared to the intensities acquired immediately after the drying procedure. Two possibilities may be accountable for this phenomenon. Such event could be attributed to the instability of the laser power and/or PMT of the microarray scanner. Another potential source of error may be due to incomplete drying of a microarray slide after the final centrifuga-

tion. Any remaining fluid in the slide holder may evaporate and keep the microarray slide humid. The moisture on microarray spots is reduced over time, which leads to a stronger fluorescent signal.

In the present study we employed antibody microarray slides from Clontech Laboratories Inc. (Mountain View, California) for the following reasons: The Clontech™ antibody microarrays detect a wide variety of cytosolic, membrane-bound, and nuclear proteins. Over 500 proteins can be examined in a single experiment. As part of the antibody microarray development, all antibodies have been extensively tested to verify their specificity. Each is raised against a known protein. Antibodies that display a

Table 2: Summary of ratio comparisons of Cy5 spots.

Slide Number	$\overline{I_{10}/I_0}$	$\overline{I_{20}/I_0}$	$\overline{I_{30}/I_0}$
1	1.115 ± 0.013	1.102 ± 0.013	1.054 ± 0.013
2	1.139 ± 0.005	1.162 ± 0.007	1.141 ± 0.006
3	1.103 ± 0.006	1.185 ± 0.006	0.999 ± 0.072
4	1.150 ± 0.022	1.153 ± 0.020	1.053 ± 0.012
5	1.054 ± 0.007	1.133 ± 0.008	1.180 ± 0.009
6	1.170 ± 0.007	1.220 ± 0.008	1.191 ± 0.008
7	1.120 ± 0.006	1.093 ± 0.006	1.070 ± 0.012
8	0.999 ± 0.011	0.970 ± 0.003	1.010 ± 0.082
9	1.030 ± 0.004	0.978 ± 0.004	0.943 ± 0.004
10	1.055 ± 0.006	1.005 ± 0.007	1.054 ± 0.009
11	0.959 ± 0.005	0.957 ± 0.037	0.868 ± 0.003
12	0.902 ± 0.002	0.844 ± 0.002	0.814 ± 0.003
13	1.080 ± 0.006	0.996 ± 0.006	1.025 ± 0.007
14	0.932 ± 0.002	0.797 ± 0.003	0.828 ± 0.003
Average	1.058 ± 0.024	1.042 ± 0.037	1.016 ± 0.034

Each of the 1014 microarray spot was examined at day 0, 10, 20, and 30, respectively, and its intensities (I_0 , I_{10} , I_{20} , and I_{30}) were measured. Then, the ratios of I_{10}/I_0 , I_{20}/I_0 , and I_{30}/I_0 for each microarray spot were generated. The average ratios of all 1014 spots on each individual slide at day 10 (I_{10}/I_0), day 20 (I_{20}/I_0), and day 30 (I_{30}/I_0) as well as the averaged value of all slides at day 10, 20 and 30 are shown (mean ± SEM).

poor specific signal or a high level of cross-reactivity were excluded from the antibody microarrays. In addition, all antibodies were checked for the linearity of signal that can be obtained, a necessary step to ensure accurate quantification. Antibodies that show non-linear binding kinetics were also excluded from the antibody microarrays. Each antibody is double printed side-by-side on the microarray slide to provide an additional internal control. The antibody microarrays are produced on standard 75 × 25 × 1 mm glass slides, an open platform that is compatible with commercially available scanners commonly used for DNA microarrays. Thus, the Clontech™ antibody microarrays represent the most comprehensive antibody microarrays to this date. Since the coupling of cyanine dyes (N-hydroxysuccinimide-esters) to proteins is universal through amines, our results should be applicable to other types of antibody or protein microarrays as well.

A recent study showed that ozone levels in the laboratory atmosphere could adversely affect intensities of fluorescent dyes such as Cy5 and Alexa 647 on DNA microarrays [29]. The fact that fluorescent intensities did not show significant decrease at day 10, 20, and 30 when compared to those at day 0 suggests that the ozone level in our laboratory is not a critical component in our antibody microarray experiments.

Based on our experience we summarize the key issues to maintain the stability of fluorescent signals on microarray slides as follows: 1) to dry the microarray slides thoroughly, 2) to keep them under a dry condition, 3) to store them in a freezer (e.g. -20°C), and 4) to minimize light exposure.

Conclusion

Microarray spot signals are more stable than previously thought if microarray slides are stored at -20°C in an air-tight slide vial. Microarray slides can be preserved and rescanned multiple times using a confocal laser scanner over a period of days or weeks.

Methods

Proteins extracted from visual cortex of young and adult mice were used in this study. The use of animals and the experimental procedures involving animals were approved by the Animal Care and Use Committee of Wake Forest University Health Sciences (Protocol number A03-045). All animals were euthanized with an overdose of pentobarbital (150 mg/kg body-weight). A conventional two-color dye-swap protocol was used for antibody microarray experiments [11,17,18,20,21]. In brief, proteins were extracted using a protein extraction buffer (Clontech, Mountain View, California), which contained non-denaturing detergents. Tissue samples were homogenized with alumina (0.5 g/100 mg tissue) and extraction

buffer (2 ml/100 mg tissue). The suspension was centrifuged at 10,000 × g for 30 minutes at 4°C. The supernatant was collected and its protein concentration was measured using a Protein Assay Kit (Pierce, Rockford, Illinois). The protein concentration was diluted to 1.1 mg/ml by adding an appropriate volume of the extraction buffer. The monoamine reactive dyes Cy3 and Cy5 (Amersham, Piscataway, New Jersey) were dissolved in 110 µl extraction buffers, respectively. 50 µl dye solutions and 450 µl protein solutions were mixed to generate 4 samples: Adult-Cy3, Young-Cy3, Adult-Cy5, and Young-Cy5. After 90 minutes of incubation on ice, the labeling process was stopped by adding 4 µl of 1 M ethanolamine. After protein labeling, unbound dyes were removed by gel filtration using disposable PD-10 desalting columns (Amersham). Each column was equilibrated with 3 × 5 ml desalting buffer (Clontech) before adding a protein sample, which was eluted by applying 2 ml desalting buffer. The protein concentration in each sample was determined using the Pierce Protein Assay Kit.

Two antibody microarray incubation solutions were made with the following compositions: (1) 5 ml incubation buffer (Clontech), 25 µg of the Adult-Cy3 protein sample, and 25 µg of the Young-Cy5 protein sample, and (2) 5 ml incubation buffer, 25 µg of the Adult-Cy5 protein sample, and 25 µg of the Young-Cy3 protein sample. After 30 minutes incubation at room temperature with gentle rocking, the antibody microarray slides (Clontech) were washed with seven different wash buffers (Clontech) at 5 minutes each, dried by centrifugation (1,000 × g) in a swing bucket rotor at room temperature for 25 minutes, and scanned using a confocal microarray scanner (ScanArray Gx) with a pixel resolution of 5 µm. The excitation wavelength and the emission filter wavelength for Cy3 and Cy5 were preset by the scanner's manufacturer (Perkin-Elmer, Shelton, Connecticut) at 543 nm/570 nm (excitation/emission) and 633 nm/670 nm (excitation/emission), respectively. After each scan, the microarray slide was put in a dry and air-tight plastic vial, and stored in a -20°C freezer until the next scan. Fluorescent signals of microarray spots were quantified using ScanArray Express (Perkin-Elmer). The mean intensity of the fluorescent signal within each microarray spot as well as the mean background intensity immediately surrounding the microarray spot was determined. The intensity of a microarray spot is defined as the value of the spot mean intensity minus the background mean intensity. Analysis of variance (ANOVA) was applied to test statistic significance of signal intensities at different time points, using signal intensities of the microarray spots as dependent variables and the microarray spots (1014) and time points (4) as independent variables.

Competing interests

The author(s) declare that they have no competing interests.

Authors' contributions

QG planned the experiments, participated in the experiments and data analyses, and wrote the manuscript. TMS participated in the microarray experiments and conducted data analyses. CK participated in data analyses.

Acknowledgements

This work was supported by a grant from NIH (EY14892). We thank Veena Nagendrappa for writing Excel macros which were utilized in our data analyses.

References

- Haab BB: **Methods and applications of antibody microarrays in cancer research.** *Proteomics* 2003, **3**:2116-2122.
- Barry R, Soloviev M: **Quantitative protein profiling using antibody arrays.** *Proteomics* 2004, **4**:3717-3726.
- Perlee L, Christiansen J, Dondero R, Grimwade B, Lejinine S, Mullenix M, Shao W, Sorette M, Tchernev V, Patel D, Kingsmore S: **Development and standardization of multiplexed antibody microarrays for use in quantitative proteomics.** *Proteome Sci* 2004, **2**:9.
- Wingren C, Borrebaeck CA: **High-throughput proteomics using antibody microarrays.** *Expert Rev Proteomics* 2004, **1**:355-364.
- Angenendt P: **Progress in protein and antibody microarray technology.** *Drug Discov Today* 2005, **10**:503-511.
- Eckel-Passow JE, Hoering A, Therneau TM, Ghobrial I: **Experimental design and analysis of antibody microarrays: applying methods from cDNA arrays.** *Cancer Res* 2005, **65**:2985-2989.
- Belov L, de la Vega O, dos Remedios CG, Mulligan SP, Christopherson R: **Immunophenotyping of leukemias using a cluster of differentiation antibody microarray.** *Cancer Res* 2001, **61**:4483-4489.
- Belov L, Huang P, Barber N, Mulligan SP, Christopherson R: **Identification of repertoires of surface antigens on leukemias using an antibody microarray.** *Proteomics* 2003, **3**:2147-2154.
- Knezevic V, Leethanakul C, Bichsel VE, Worth JM, Prabhu VV, Gutkind JS, Liotta LA, Munson PJ, Petricoin EF 3rd, Krizman DB: **Proteomic profiling of the cancer microenvironment by antibody arrays.** *Proteomics* 2001, **1**:1271-1278.
- Lin Y, Huang R, Santanam N, Liu YG, Parthasarathy S, Huang RP: **Profiling of human cytokines in healthy individuals with vitamin E supplementation by antibody array.** *Cancer Lett* 2002, **187**:17-24.
- Anderson K, Potter A, Baban D, Davies KE: **Protein expression changes in spinal muscular atrophy revealed with a novel antibody array technology.** *Brain* 2003, **126**:2052-2064.
- Miller JC, Zhou H, Kwekel J, Cavallo R, Burke J, Butler EB, The BS, Haab BB: **Antibody microarray profiling of human prostate cancer sera: antibody screening and identification of potential biomarkers.** *Proteomics* 2003, **3**:56-63.
- De Ceuninck F, Dassencourt L, Anract P: **The inflammatory side of human chondrocytes unveiled by antibody microarrays.** *Biochem Biophys Res Commun* 2004, **323**:960-969.
- Hudelist G, Pacher-Zavisin M, Singer CF, Holper T, Kubista E, Schreiber M, Manavi M, Bilban M, Czerwenka K: **Use of high-throughput protein array for profiling of differentially expressed proteins in normal and malignant breast tissue.** *Breast Cancer Res Treat* 2004, **86**:281-291.
- Turtinen LW, Prall DN, Bremer LA, Nauss RE, Hartsel SC: **Antibody array-generated profiles of cytokine release from THP-1 leukemic monocytes exposed to different amphotericin B formulations.** *Antimicrob Agents Chemother* 2004, **48**:396-403.
- Abdo M, Irving B, Hudson P, Zola H: **Development of a cluster of differentiation antibody-based protein microarray.** *J Immunol Methods* 2005, **305**:3-9.
- Andersson O, Kozlowski M, Garachtchenko T, Nikoloff C, Lew N, Litman DJ, Chaga G: **Determination of relative protein abundance by internally normalized ratio algorithm with antibody arrays.** *J Proteome Res* 2005, **4**:758-767.
- Bartling B, Hofmann HS, Boettger T, Hansen G, Burdach S, Silber RE, Simm A: **Comparative application of antibody and gene array for expression profiling in human squamous cell lung carcinoma.** *Lung Cancer* 2005, **49**:145-154.
- Gao WM, Kuick R, Orzechowski RP, Misek DE, Qiu J, Greenberg AK, Rom WN, Brenner DE, Omenn GS, Haab BB, Hanash SM: **Distinctive serum protein profiles involving abundant proteins in lung cancer patients based upon antibody microarray analysis.** *BMC Cancer* 2005, **5**:110.
- Mathur P, Kaga S, Zhan L, Das DK, Maulik N: **Potential candidates for ischemic preconditioning-associated vascular growth pathways revealed by antibody array.** *Am J Physiol Heart Circ Physiol* 2005, **288**:H3006-H3010.
- Mathur P, Kaga S, Zhan L, Das DK, Maulik N: **Antibody-array technique reveals overexpression of important DNA-repair proteins during cardiac ischemic preconditioning.** *J Mol Cell Cardiol* 2005, **38**:99-102.
- Watanabe M, Guo W, Zou S, Sugiyo S, Dubner R, Ren K: **Antibody array analysis of peripheral and blood cytokine levels in rats after masseter inflammation.** *Neurosci Lett* 2005, **382**:128-133.
- Anderson L, Seilhamer J: **A comparison of selected mRNA and protein abundances in human liver.** *Electrophoresis* 1997, **18**:533-537.
- Gygi SP, Rochon Y, Franzosa BR, Aebersold R: **Correlation between protein and mRNA abundance in yeast.** *Mol Cell Biol* 1999, **19**:1720-1730.
- Ideker T, Thorsson V, Ranish TA, Christmas R, Buhler J, Eng JK, Bumgarner R, Goodlett DR, Aebersold R, Hood L: **Integrated genomic and proteomic analyses of a systematically perturbed metabolic network.** *Science* 2001, **292**:929-934.
- Chen G, Gharib TG, Huang C-C, Taylor JMG, Misek DE, Kardias SLR, Giordano TJ, Iannettoni MD, Orringer MB, Hanash SM, Beer DG: **Discordant protein and mRNA expression in lung adenocarcinomas.** *Mol Cell Proteomics* 2002, **1**:304-313.
- Lee PS, Shaw LB, Choe LH, Mehra A, Hatzimanikatis V, Lee KH: **Insights into the relation between mRNA and protein expression patterns: II. Experimental observations in Escherichia coli.** *Biotechnol Bioeng* 2003, **84**:834-841.
- Tian Q, Stepaniants SB, Mao M, Weng L, Feetham MC, Doyle MJ, Yi EC, Dai H, Thorsson V, Eng J, Goodlett D, Berger JP, Gunter B, Linsley PS, Stoughton RB, Aebersold R, Collins SJ, Hanlon WA, Hood LE: **Integrated genomic and proteomic analyses of gene expression in mammalian cells.** *Mol Cell Proteomics* 2004, **3**:960-969.
- Fare TL, Coffey EM, Dai H, He YD, Kessler DA, Kilian KA, Koch JE, LeProust E, Marton MJ, Meyer MR, Stoughton RB, Tokiwa GY, Wang Y: **Effects of atmospheric ozone on microarray data quality.** *Anal Chem* 2003, **75**:4672-4675.
- Romualdi C, Trevisan S, Celegato B, Costa G, Lanfranchi G: **Improved detection of differentially expressed genes in microarray experiments through multiple scanning and image integration.** *Nucleic Acids Res* 2003, **31**:e149.
- Garcia de la Nava J, van Hijum S, Trelles O: **Saturation and quantization reduction in microarray experiments using two scans at different sensitivities.** *Stat Appl Genet Mol Biol* 2004, **3**:Article11.
- Lyng H, Badiie A, Svendsrud DH, Hovig E, Myklebost O, Stokke T: **Profound influence of microarray scanner characteristics on gene expression ratios: analysis and procedure for correction.** *BMC Genomics* 2004, **5**:10.
- Khondoker MR, Glasbey CA, Worton BJ: **Statistical estimation of gene expression using multiple laser scans of microarrays.** *Bioinformatics* 2006, **22**:215-219.
- Piepho HP, Keller B, Hoecker N, Hochholdinger F: **Combining signals from spotted cDNA microarrays obtained at different scanning intensities.** *Bioinformatics* 2006, **22**:802-807.
- Skibbe DS, Wang X, Zhao X, Borsuk LA, Nettleton D, Schnable PS: **Scanning microarrays at multiple intensities enhances discovery of differentially expressed genes.** *Bioinformatics* 2006, **22**:1863-1870.