

Design and development of safe gait prosthetic knee joint in India

Veerendra K. Shandilya¹, Lata D. Parmar², Ashwinikumar V. Shandilya³

¹Sumandeep Vidyapeeth, Piparia, Waghodia, Vadodara, Gujarat, ²College of Physiotherapy, Sumandeep Vidyapeeth, Piparia, Waghodia, Vadodara, Gujarat, ³Rehabs Clinic, Opp. Baroda High School, Vadodara, Gujarat, India

ABSTRACT

Context: The prosthetic technology in recent years has grown by leap and bounds. The most advanced gadgets like microprocessors are available worldwide at exorbitant costs. Developing countries have issues with terrain, access to services, and cost. The new design of the prosthetic knee joint was planned to develop a cost-effective, sturdy, and easy to fit a universal system. **Methods and Material:** This exploratory design was undertaken to develop a prototype. The design was further developed and tested for its materialistic properties. Pilot study assessing functions using this joint is also underway. **Results and Conclusion:** The novelty of this knee joint is that locking and unlocking are made simple such that it can be done by the transfemoral amputee at will, with ease, on the spot, independent of the terrain he/she is traversing. The awareness of such a prosthetic joint is vital for family physicians.

Keywords: Gait analysis, microprocessor, a prosthetic knee joint, single-axis knee joint, transfemoral amputee

Introduction

The prosthetic technology in recent years has grown by leap and bounds. The most advanced prosthesis incorporates advanced gadgets like microprocessors^[1-11] which are available at exorbitant costs. India is a developing country and the Indian Government endeavors to provide the aids and appliances to the disabled at the minimum costs.^[12] Although the government has floated several schemes for the welfare of the disabled, these schemes are not enough. Moreover, these schemes are fraught with terms and conditions which make it very difficult for the patients to avail of the benefits.

There are grossly two types of lower limb prostheses endoskeletal and exoskeletal. Since, endoskeletal prosthetic components are

modular, interchangeable, and easy to align anytime they are widely accepted. Most endoskeletal knee joints available in India are imported and are thus expensive.

As most institutions in India were fitting exoskeletal prostheses to all transfemoral amputation (TFA) using wooden shin attached to a constant friction wooden knee block, which is carved and assembled to the transfemoral socket (technically has a pivotable joint with a backstop at 180°). The fitting of the knee joint assembly has an elastic strap fixed on the anterior aspect of the knee assembly as an extension assist to those TFA who would prefer to walk with a free knee gait. This knee assembly also has a manual locking mechanism like a door latch which would slide down the shin to lock and maintain full knee extension of the prosthetic knee. This would help in the initial weight bearing learning and gait training of the TFA with above-knee (AK) prosthesis. The locking mechanism always added security to the TFA while using their prosthesis and to overcome the fear to stumble.

Address for correspondence: Dr. Lata D. Parmar, College of Physiotherapy, Sumandeep Vidyapeeth, Piparia, Waghodia, Vadodara, Gujarat, India.
E-mail: principal.physiotherapy@sumandeepvidyapeethdu.edu.in

Received: 08-08-2020

Revised: 06-10-2020

Accepted: 07-10-2020

Published: 30-11-2020

Access this article online

Quick Response Code:



Website:
www.jfmipc.com

DOI:
10.4103/jfmipc.jfmipc_1616_20

This is an open access journal, and articles are distributed under the terms of the Creative Commons Attribution-NonCommercial-ShareAlike 4.0 License, which allows others to remix, tweak, and build upon the work non-commercially, as long as appropriate credit is given and the new creations are licensed under the identical terms.

For reprints contact: WKHLRPMedknow_reprints@wolterskluwer.com

How to cite this article: Shandilya VK, Parmar LD, Shandilya AV. Design and development of safe gait prosthetic knee joint in India. J Family Med Prim Care 2020;9:5588-91.

The most common and economical prostheses in India is the “Jaipur foot”^[4] prostheses which has an exoskeletal system with a pair of an orthotic drop lock externally fitted for all its prostheses and which requires both hands to lock and unlock the knee joint. All amputees fitted with Jaipur foot prostheses, therefore, walk with a stiff/locked knee, the reason being that the amputee wants to have the stability to negotiate on all terrains.^[13]

In brief, knee joints of AK prosthesis are used for the stance phase for load-bearing stability and to have swing phase control. In recent years, worldwide, we have many kinds of knee joints developed providing control either with the use of hydraulic fluid mechanisms or pneumatic control mechanisms.^[1,3-7,9,11] For the consumer, choice of knee joint and selection of knee joint is becoming problematic.

The single axis, constant friction artificial knee joints, power not needed in the passive endoskeletal prosthesis like OFM 2 of Medi, Endolite, Otto Bock, and Ossur, available today in India do not provide the amputee the freedom to lock or unlock at will. He has to take the help of a prosthetist to lock or unlock it or select the knee joint accordingly.

The new endoskeletal prosthetic knee joint (SAFE GAIT) was thus planned and designed with the main objective that

1. It will eliminate the services of a prosthetist to lock or unlock the prosthetic knee joint for TFA.
2. The locking and unlocking mechanism of the knee joint will be simple and easy to operate
3. The amputee should be able to walk with a free knee at will.

Procedure

Design considerations for Safe Gait Prosthetic Knee Joint

Stainless steel material was chosen for the manufacture of the knee joint due to the following reasons:

1. Titanium is costly and would take the cost too high.
2. Stainless steel would make knee joint rust-proof (free of corrosion) and durable.
3. An investment casting has been done on the joint to make it cost-effective manufacturing.
4. Since there are no standard tests on knee joint testing available in the country, the prototype was manufactured with Stainless Steel 304, and a compression load test was done at the Energy Research Development Agency (ERDA) – an authentic autonomous body in the field of testing.

Technical features

- The knee axis is behind (posterior) for stability
- Extension assist is done with an elastic cord which is easily interchangeable and tension can be adjusted for the swing phase.
- The lock mechanism works with a spring-loaded plunger, when the knob is shifted; it immediately locks the knee (in full extension)

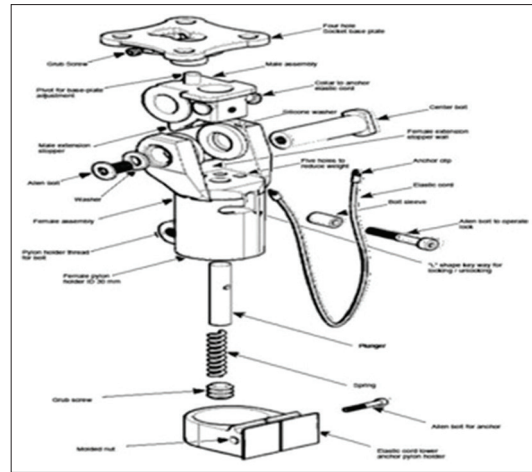


Figure 1: Various components of safe gait prosthetic knee joint



Figure 2: Assembly drawing of safe gait prosthetic knee joint



Figure 3: Final look of safe gait prosthetic knee joint

- Load Limit - 120 kg, UNB 12.9
- Knee Flexion Range – 125° (approx)
- Height (Knee center – upper edge) – 22 m
- Optional height (Knee center with special coupling) -12 mm
- Universal socket assembly features (which could be fitted to any prosthetic component manufacturer’s assembly system)- 30 mm pylon tube fitting.

Description

Figures 1 and 2: The upper end or top end of the joint has a universal four-bolt baseplate which has a groove to accommodate

the pin (part of the male component) with both sides grub screw so that desired rotation of the knee joint while assembling with socket could be achieved.

The middle/male component of the knee joint has an inbuilt pin which anchors on the base plate on the top. It has a look like that of a bobbin with an extension to be functioning as a stop. It also has two built-in pins on both sides in the front like a flat head rivet, this is to anchor the elastic cord which would help in extension (swing phase motion) the hole in the center of the male component acts as the hinge to the center bolt.

The center bolt is in conjunction with the female component which is machined with a spherical shape on one side, which settles in the spherical shaped groove of the female component (for firm anchor). The center bolt also has fine threading on the other end to get itself locked. There are silicon and metal washers that mimic free motion as a hinge. Overall, the male rests on the female body which has a flat surface like a wall on the rear side which makes the 180° stop. The bottom part of the female component is a double locking pipe holder for a 30 mm tube which is now universally used.

It also has a small tube in the center which acts like a barrel for the inserted plunger (which is inserted in the small hollow shank which is parallel to the 30 mm inner diameter tube clamp, the center body replicates a pipe within a pipe) where the inner pipe has respective threading for grub screw at the bottom to hold the spring-loaded plunger in its desired position, once the plunger is up it would lock the joint restricting/lock the male component in 180°.

To control the plunger movement there is an Alan bolt which is tightened in the middle shaft of the plunger pin, which passes through the L-shaped keyhole on the outer front part of the female body this controls the locking and unlocking of the joint. The operating Alan bolt has a soft sleeve that gives grip for easy operation by the amputee. The elastic cord for extension assist is like any other prosthetic knee joint universally available. The manufactured joints are as shown in Figure 3.

Discussion

Amputee functional level and their prosthetic components are classified universally as K levels^[3]

- K0 – Non-ambulatory (cannot walk at all),
- K1 – Transfer activity (wheelchair to bed/commode seat),
- K2 – Household ambulatory (can walk only on even surface predominantly indoor),
- K3 – Community ambulatory (can walk outdoor on uneven surfaces/staircase/ramps etc.),
- K4 – High activity level ambulatory (sports, recreational activity).

In India, no prosthetic components have been categorized. Besides, soft sleeves are not manufactured and hence only a hard

socket system with an EVA foam liner is fitted and distributed in the camps free of cost.

Prosthetic knee joints are categorized from K2 to K4 levels which meet the demands of stability and mobility during the gait cycle, also during activities like the stand to sit. Apart from closely resembling the biological knee, ideally, a knee prosthesis should not exceed the size and the weight of the missing limb.^[3]

There are three major groups in which the TFA prosthesis have been classified, viz. passive, damping, and powered. No power is needed in the passive prosthesis while damping need power for variable damping and powered prosthetic knees can perform positive knee work^[1-3,5-10]

The safe gait knee joint stands out giving the TFA ease to lock unlock at will and without anyone's assistance. This is possible because of the "plunger mechanism with a control knob" used. The operation of locking unlocking is possible with a very slight pressure of a single finger of the hand on the control knob.

In free knee gait mode, shortfalls are also applicable to this newly designed joint i.e., it is not capable of adapting to the changing speed during gait. Mechanical stance control (although the knee axis is kept posterior for stability) may still be unreliable, this increases the risk of stumbling in free knee joint ambulation.

Ideally, there is a protocol for a TFA to reach a stage where he can be fitted to a permanent prosthesis. Besides, following this he needs to undertake physiotherapy sessions of gait training, strengthening, balance, etc., apart from other education about donning, doffing, etc., However, most fittings of prostheses in India are done during camps, therefore, there may be minimal time given for gait training and very seldom under a qualified physical therapist.

In camp, on fitting prosthesis on the first day, the amputee is struggling to gain the confidence of stability, while standing and the easy locking mechanism is desired as only then will he attempt to ambulate with the prosthesis. The "safe gait" joint provides the locking mechanism with ease and at will thus providing initial confidence of stability required by TFA.

Conclusion

The novelty of this "prosthetic knee joint" is that it can be locked and unlocked by the patient himself on the spot depending on the terrain he is traversing, without having to go to the professional. This feature is hoped to help the amputee to negotiate even uneven terrain and crowded situations with confidence, apart from being economical and available at a very low cost. The awareness of such a prosthetic joint is vital for family physicians.

The pilot study comparing this novel knee joint to other imported knee joints available is completed and found to be satisfactorily compatible (under publication).

Financial support and sponsorship

Nil.

Conflicts of interest

There are no conflicts of interest.

References

1. Kannenberg A, Zacharias B, Pröbsting E. Benefits of microprocessor-controlled prosthetic knees to limited community ambulators: Systematic review. *J Rehabil Res Dev* 2014;51:1469-96.
2. Creylman V, Knippels I, Janssen P, Biesbrouck E, Lechler K, Peeraer L. Assessment of transfemoral amputees using a passive microprocessor-controlled knee versus an active powered microprocessor-controlled knee for level walking. *Biomed Eng Online* 2016;15(Suppl 3):142.
3. Berke GM, Buell N, Ferguson J, Gailey R, Hafner B, Hubbard S, Willingham L. *Transfemoral Amputation: The Basic and Beyond*. Prosthetics Research Study; 2008.
4. Kaufman KR, Frittoli S, Frigo CA. Gait asymmetry of transfemoral amputees using mechanical and microprocessor-controlled prosthetic knees. *Clin Biomech* 2012;27:460-5.
5. Chin T, Machida K, Sawamura S, Shiba R, Oyabu H, Nagakura Y, *et al.* Comparison of different microprocessor controlled knee joints on the energy consumption during walking in trans-femoral amputees: Intelligent knee prosthesis (IP) versus C-leg. *Prosthet Orthot Int* 2006;30:73-80.
6. Sapin E, Goujon H, de Almeida F, Fodé P, Lavaste F. Functional gait analysis of transfemoral amputees using Hydracadence® knee joints compared with other single axis prosthetic knees with hydraulic swing. *International symposium of the analysis of 3D human movement*, Valenciennes, France 2006.
7. Kaufman KR, Levine JA, Brey RH, McCrady SK, Padgett DJ, Joyner MJ. Energy expenditure and activity of transfemoral amputees using mechanical and microprocessor-controlled prosthetic knees. *Arch Phys Med Rehabil* 2008;89:1380-5.
8. Webster JB, Poorman CE, Cifu DX. Department of veterans affairs amputation system of care: 5 years of accomplishments and outcomes. *J Rehabil Res Dev* 2014;51:vii-xvi.
9. Bai X, Ewins D, Crocombe AD, Xu W. A biomechanical assessment of hydraulic ankle-foot devices with and without micro-processor control during slope ambulation in trans-femoral amputees. *PLoS One* 2018;13:e0205093.
10. Arun S, Marbaniang B, Borgohain B, Kanagaraj S. Rehabilitation evaluation of the newly developed polymeric based passive polycentric knee joint. *Disabil Rehabil Assist Technol* 2019:1-7. doi: 10.1080/17483107.2019.1621955.
11. Kadhim FM, Chiad JS, Takhakh AM. Design and manufacturing knee joint for smart transfemoral prosthetic. *InIOP Conference Series: Materials Science and Engineering*, International Conference on Materials Engineering and Science 2018 (Vol. 454).
12. Scheme of Assistance to Disabled Persons for Purchase/Fitting of Aids/Appliances (ADIP Scheme). Govt. of India Ministry of Social Justice and Empowerment, Shastri Bhavan, New Delhi. 1st April, 2014
13. Mahida H, Mahida D. Jaipur foot: an attempt to replicate Jaipur model in surat city.