



Evaluation of the marginal and internal gaps of three different dental prostheses: comparison of the silicone replica technique and three-dimensional superimposition analysis

Jin-Young Park¹, So-Yeon Bae², Jae-Jun Lee², Ji-Hwan Kim², Hae-Young Kim^{2,3}, Woong-Chul Kim^{2*}

¹Institute for Health Science, Korea University, Seoul, Republic of Korea

²Department of Dental Laboratory Science and Engineering, College of Health Science, Korea University, Seoul, Republic of Korea

³Department of Public Health Sciences, Graduate School & BK21+ Program in Public Health Sciences, Korea University, Seoul, Republic of Korea

PURPOSE. The purposes of this study were to evaluate the marginal and internal gaps, and the potential clinical applications of three different methods of dental prostheses fabrication, and to compare the prostheses prepared using the silicone replica technique (SRT) and those prepared using the three-dimensional superimposition analysis (3DSA). **MATERIALS AND METHODS.** Five Pekkton, lithium disilicate, and zirconia crowns were each manufactured and tested using both the SRT and the two-dimensional section of the 3DSA. The data were analyzed with the nonparametric version of a two-way analysis of variance using rank-transformed values and the Tukey's post-hoc test ($\alpha = .05$). **RESULTS.** Significant differences were observed between the fabrication methods in the marginal gap ($P < .010$), deep chamfer ($P < .001$), axial wall ($P < .001$), and occlusal area ($P < .001$). A significant difference in the occlusal area was found between the two measurement methods ($P < .030$), whereas no significant differences were found in the marginal gap ($P > .350$), deep chamfer ($P > .719$), and axial wall ($P > .150$). As the 3DSA method is three-dimensional, it allows for the measurement of arbitrary points. **CONCLUSION.** All of the three fabrication methods are valid for measuring clinical objectives because they produced prostheses within the clinically acceptable range. Furthermore, a three-dimensional superimposition analysis verification method such as the silicone replica technique is also applicable in clinical settings. [J Adv Prosthodont 2017;9:159-69]

KEYWORDS: Silicone replica technique; Three-dimensional superimposition analysis; CAD/CAM, Polyetherketoneketone; Marginal and internal gap

Corresponding author:
Woong-Chul Kim
Department of Dental Laboratory Science and Engineering, College of Health Science, Korea University, #377 Hana Science Hall, 145 Anam-ro (1-2, Anam-dong 5-ga), Seongbuk-gu, Seoul 02841, Republic of Korea
Tel. +82232905665; e-mail, kuc2842@korea.ac.kr
Received July 25, 2016 / Last Revision December 23, 2016 / Accepted March 21, 2017

© 2017 The Korean Academy of Prosthodontics
This is an Open Access article distributed under the terms of the Creative Commons Attribution Non-Commercial License (<http://creativecommons.org/licenses/by-nc/3.0>) which permits unrestricted non-commercial use, distribution, and reproduction in any medium, provided the original work is properly cited.

This study was supported by the Korea University Grant (K1600741).

INTRODUCTION

Dental prostheses can replace lost or damaged teeth. Thus, they should be manufactured using aesthetically acceptable, durable, precise, and biocompatible dental materials in order to replicate the function of natural teeth as closely as possible.¹

Dental ceramic has well-established efficacy in its use as the material for dental prostheses.² It was developed to satisfy the aesthetic expectations of patients and has been widely applied.³ Zirconium dioxide (zirconia) ceramic material is comparable in color with natural teeth and has a flexural strength of 900 - 1200 MPa, which is comparable with

that of metal.⁴ Lithium disilicate ceramic material has better transparency than zirconia.⁵ In addition, it has excellent properties such as biocompatibility, chemical stability, and mechanical strength.⁶ Furthermore, veneers, inlays, prostheses in the form of crowns, and three-unit anterior fixed partial dentures have been utilized as dental prostheses.⁷ Lithium disilicate ceramic materials produced by the computer-aided design/manufacturing (CAD/CAM) technique and zirconium dioxide ceramic materials have volume shrinkage rates of 0.25% and 22 - 25%, respectively, during sintering.⁸⁻¹⁰ Therefore, these two materials may negatively affect the fit of a dental prosthesis owing to shrinkage in pre-sintered blanks during the sintering process.⁷ In contrast to ceramics, Polyetherketoneketone (PEKK), a new material in the dental field, does not exhibit shrinkage. Furthermore, PEKK exhibits highly biocompatible characteristics that are desirable in the medical industry. For these reasons, PEKK has been utilized as the primary transplantation material, adequately replacing titanium, a material that was used for a considerable length of time in orthopedic applications.¹¹⁻¹⁴

Fuhrmann *et al.*¹¹ reported that PEKK can provide a solid production in the manufacturing of crowns and fixed dental prostheses (FDPs). In particular, crystalline PEKK is utilized for crowns and FDPs, while amorphous PEKK is used for removable prostheses. Crystalline PEKK and amorphous PEKK are resistant to chemical wear, have high mechanical resistance and tensile and flexural strengths, can withstand high temperatures (melt temperature, 300°C) and have high-quality characteristics of good dimension stability.^{11,15} In addition, according to Stawarczyk *et al.*,¹⁶ PEKK is biocompatible, and in contrast to metal restorations, it has an appearance similar to that of natural teeth. It can also be easily formed with a simple dental bur. However, considering its aesthetic qualities, PEKK has low transparency and a grayish pigmentation when compared with natural teeth (or dental ceramics), and cannot be processed in an overall shape.¹⁶ Therefore, it is predominantly manufactured within a framework.

The complexity associated with the manufacture of dental prostheses has led to the development of the CAD/CAM technology that can eliminate errors in temporary elements during the traditional manufacturing process of dental prostheses.¹⁷ CAD/CAM not only is efficient, but also has standardized repeated accuracy.² Furthermore, CAD/CAM systems have revolutionized manufacturing processes in the dental industry, enabling the rapid production of simple prostheses.¹⁸ In a study by Rudolph *et al.*,¹⁷ the utilization of oral scanners was found to eliminate the error incurred during the operative course of the impression and plaster model. A CAD/CAM system with an oral scanner has also been reported to be associated with valid and prompt manufacturing.²

The accuracy of the milling process is largely affected by the axis of the milling machine, and the current milling machines are distributed as 3-, 4-, and 5-axis milling machines.¹⁹ While 3-axis milling has a short production time and simple operation, there is a limit in milling the inner

surface of the tooth restoration, which is a free-form curved surface as there is no rotating shaft.¹⁹ Therefore, a 4-axis milling machine with three axis added to the rotation axis and a 5-axis milling machine with two rotation axes were developed.¹⁹

According to Bosch *et al.*,² the 5-axis milling machine has better accuracy than a 4-axis milling machine. However, using a 4-axis milling machine is cheaper than using a 5-axis milling machine, reducing the cost of the prosthesis.²⁰ In addition, the digital simulated process has been reported to reduce the process time and manufacturing waste; thus, 4-axis milling is a practical method for creating free-form surfaces.²⁰ The number of the milling axis is not necessarily proportional to the level of accuracy, but it has a wider impact on accuracy digitization, data processing, and production processes.

The accurate manufacturing of dental prostheses is important for long-term clinical applications.²¹ Accuracy and precision between abutment teeth and dental prostheses are required in the manufacturing process of dental prosthesis. Inaccurately manufactured dental prostheses can lead to secondary caries, marginal microleakage, periodontal inflammation, periodontal lesion, plaque accumulation, and nonsurgical endodontic treatment.^{7,21,22} Therefore, manufacturing dental prostheses with an accurate margin is important. The silicone replica technique (SRT) has been frequently utilized owing to its ability to measure the fitness of a dental prosthesis without causing damage.^{23,24} However, numerous studies have failed to validate the accuracy of measurements using the SRT. Studies investigating the accuracy of two-dimensional (2-D) sections of three-dimensional (3-D) superimposition analysis (3DSA) are relatively rare. Therefore, the purposes of this study were to (1) evaluate the marginal and internal gaps in three types of dental prostheses (subtractive manufacturing systems using a lithium disilicate crown [LC], zirconia crown [ZC], or PEKK crown [PC]) and (2) to compare between the measurements obtained from using the SRT (control group) and those obtained from using the 2-D sections of the 3DSA method (test group). The null hypothesis tested was that the marginal and internal gaps do not significantly differ among the three groups or between the two measurement methods.

MATERIALS AND METHODS

An acrylic model (AG-3 ZPVK 16 [maxillary right first molar]; Frasco GmbH, Tettngang, Germany) with abutment teeth was used. Therefore, the maxillary right first molars were prepared with a 360° 1.0-mm deep chamfer. The occlusal reductions ranged from 1.5 - 2.0 mm.²⁵ The master model was created with silicone (Deguform, DeguDent GmbH, Hanau, Germany) by pouring polymethyl methacrylate (PMMA; JT, Lang Dental Mfg. Co. Inc., Wheeling, IL, USA),²⁶ which has a reflective index within the range of a natural tooth, into the maxillary buccal flange of the replicated silicone.

A RST-CEREC file was obtained using Omnicam (CEREC

Omniscam, Sirona Dental System GmbH, Bensheim, Germany) with the master model. According to the manufacturer's instructions, we designed the clinical crown with CEREC inLab software (Sirona Dental System GmbH) with the RST-CEREC file. Before the crowns were designed, the following design parameters were set: spacer value, 30 μm ; occlusal thickness, 1.5 mm; and axial thickness, 0.8 mm. With the designed file, each pre-sintered LC (IPS e.max CAD, Ivoclar Vivadent AG, Schaan, Liechtenstein) and pre-sintered ZC (Sirona inCoris TZI, Sirona Dental Systems GmbH) was milled five times, under one file, with a four-axial milling machine (inLab MC XL, Sirona Dental System GmbH).² The IPS object refill putty pin was fixed to the inner surface of the pre-sintered LC. Five LCs were produced based on the sintering manual provided by the manufacturer with a dental ceramic furnace (Programat P310, Ivoclar Vivadent). Five ZCs were created with a specific furnace (Sirona inFire HTC, Sirona Dental Systems GmbH) based on the sintering manual provided by the manufacturer.

The master model was replicated with light-body silicone (Aquasil Ultra XLV Regular Set, Dentsply Caulk, Milford, DE) and heavy-body silicone (Aquasil Ultra Rigid Regular Set, Dentsply Caulk) to obtain an impression (ISO 4823:2000).²⁷ The study model was created by inserting a type IV stone (Dentona esthetic-base gold, Dentona AG, Dortmund, Germany) in the replicated impression. The study model was scanned using a noncontact blue light scanner (Identica, Medit Co. Ltd., Seoul, Korea). The obtained file had a 30 μm space (cervical, side, and occlusal cement gaps), and the cement film thickness theoretically required a space of 20 - 40 μm .²⁸ The Delcam PowerSHAPE Pro

(Delcam Plc, Birmingham, UK) was used to generate the standard triangulated language (STL) file and design the framework for a 0.5-mm-thick maxillary right first molar.

With the generated STL file, the PEKK framework was milled five times with a four-axial milling machine (Cendres+Métaux SA, Biel-Bienne, Switzerland). With the milled Pekkton framework, five PCs were created by framing the external form of the crown with a microhybrid resin composite (Gradia Direct; GC Corporation, Tokyo, Japan), according to the manufacturer's instructions (Fig. 1).

After creating five samples for each group, the SRT method was used to measure the marginal and internal gaps of each crown. Light-body silicone (Aquasil Ultra XLV Regular Set, Dentsply Caulk) was placed into a dental silicone gun (MixPac, Dentsply Caulk) with a 1:1 mixture of base and catalyst. The silicone was injected between the internal region of the crown and the model through an impression tip that was applied with finger pressure and an Instron universal testing machine (Instron 3345 Tester, Instron, Norwood, MA, USA), which was tested at 50 N. After 5 minutes, the crown and model were separated and the heavy-body silicone (Aquasil Ultra Rigid Regular Set, Dentsply Caulk) was placed into the same gun and injected into a round-shaped tray before embedding the replicated light-body silicone. To measure as a fixed part, two epoxy models were created by inserting epoxy (Modralit 3K, Dreve Dentamid GmbH, Unna, Germany) after replicating the master model. A customized jig was manufactured for one epoxy model cut in a buccolingual direction, while the other model was cut in a mesiodistal direction. The silicone replica was cut on these jigs with a razor blade (Fig. 2A). To

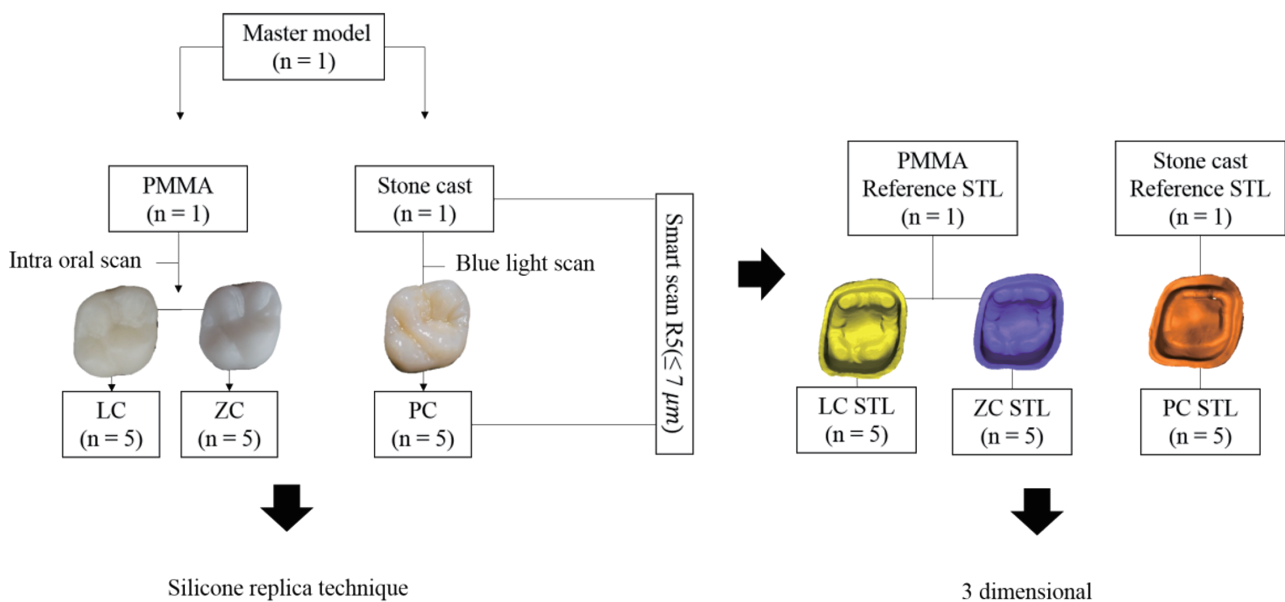


Fig. 1. Study design flowchart. PMMA, polymethyl methacrylate; LC, lithium disilicate crown; PC, Pekkton crown; STL, standard template library; ZC, zirconia crown.

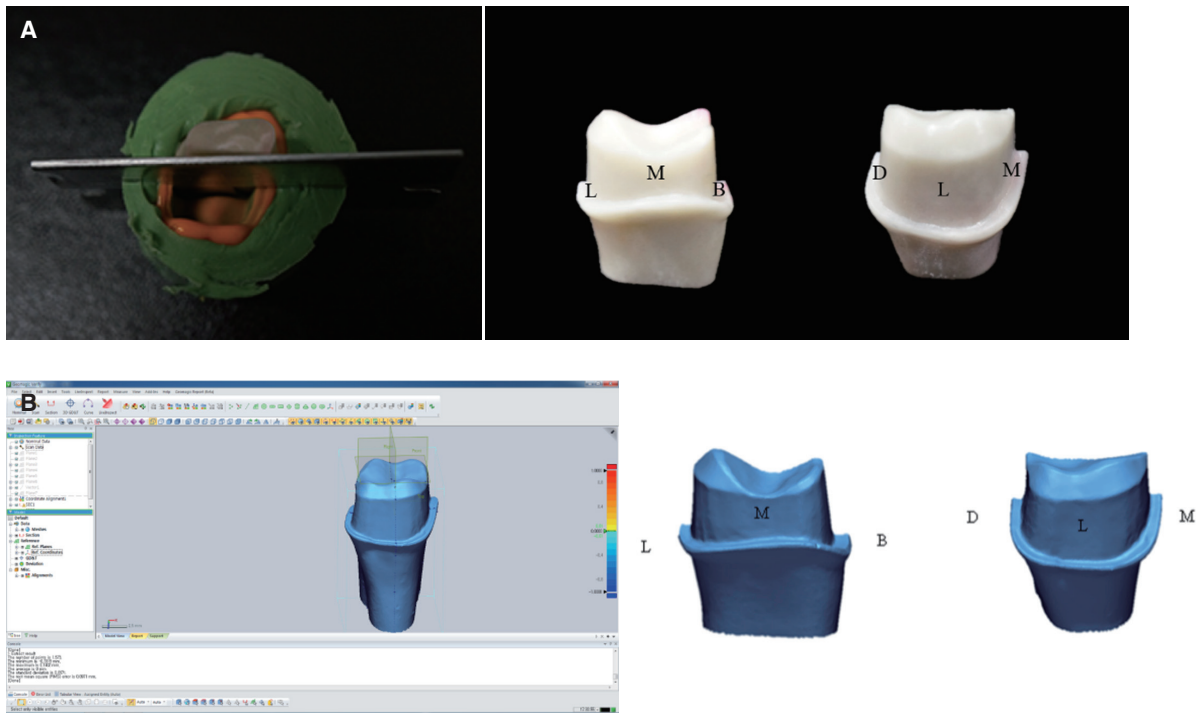


Fig. 2. Cutting regions for measurements. (A) Jig for the silicone replica technique: By the insertion of a jig for the silicone replica technique, the region was cut with the side to be measured with a constant blade in order to measure the same point, (B) Two-dimensional section of the three-dimensional superimposition analysis: the cut was made in the buccolingual and mesiodistal directions.

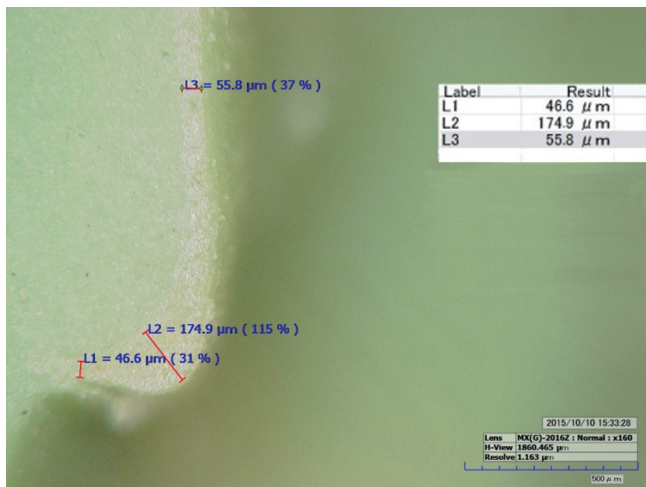


Fig. 3. Digital microscope image of the silicone replica technique (160 \times magnification).

measure the space between the model and the crown in the light-body silicone replica,^{25,29} the silicone replica was observed under a digital microscope (KH-7700, Hirox, Tokyo, Japan) at 160 \times magnification (Fig. 3). The measuring point of the marginal and internal gaps (16 points) was then determined (Fig. 4). One experienced dental technician was involved in the measurement. As it involves a potential bias such as

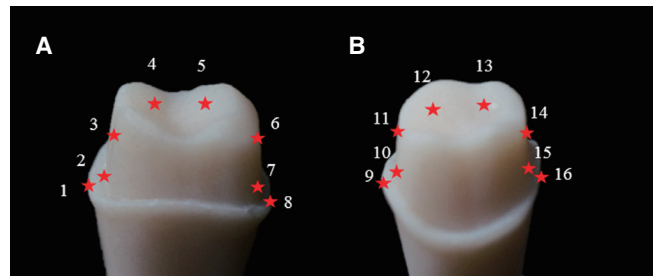


Fig. 4. Sixteen measuring points of the marginal and internal gaps. (A) Bucco-ligual view, (B) Mesio-distal view.

morphological and rounded margins, it is practically necessary to determine the number of measurements, given that it is difficult to describe a certain gap with only one measurement point.³⁰ Therefore, the measurement points in the current study were selected according to the contour difference of the crown and the abutment.³⁰

The marginal gap (points 1, 8, 9, and 16) is the vertical discrepancy between the margin preparation and the crown. The deep chamfer (points 2, 7, 10, and 15) is the vertical discrepancy between the crown and the point where the margin changes to the axial wall. The axial wall (points 3, 6, 11, and 14) is the center of the cusp and between the deep

chamfer, and the occlusal area (points 4, 5, 12, and 13) is the point of the trisection portion of the occlusal area's cusp.

The 16 measuring points included those for the marginal gap (points 1, 8, 9, and 16), rounded chamfer (points 2, 7, 10, and 15), axial wall (points 3, 6, 11, and 14), and occlusal area (points 4, 5, 12, and 13).

The 2-D sections of the 3DSA were utilized as a new verification method. This is a method for measuring the section deviation, which is the deviation between the reference data and the scan data for the entire area in the unit surface. In addition, the deviation from a particular location and the variation in the cross section above the whole area were measured (Geomagic User Guide and Tutorial, 3D Systems Inc., Rock Hill, SC). For optical scanning, powder (Entwickler Nr. 3, Helling GmbH, Germany)³¹ was spread on the required area of the PMMA (Pekkton Ivory, Cendres +Métaux), the stone cast of an abutment tooth, and the internal side of the 15 crowns. These were scanned with an optical scanner (Smart Scan R5, Breuckmann GmbH, Meersburg, Germany)^{32,33} with a feature accuracy of less than 7 μm (Fig. 1) and saved as STL files. The abutment tooth of the master model (reference STL, nominal data) and the internal region of the crown (scan data) were alignment-transformed with a 3-D inspection software (Verify, Geomagic GmbH, Stuttgart, Germany) with the obtained STL file. The three-dimensional evaluation method is based on the basic principle of the merging software, which is to mathematically find the best fit for the abutment teeth and dental prostheses at the closest distance.^{34,35,36} Therefore, accurate merging on one surface can cause errors on other surfaces due to compensation, which does not allow the representation of realistic cement values.^{34,35,36} In this study, alignment transformation was performed to compensate for this. The x, y, and z axis planes of the object to be compared are formed without being shifted to one side, and the planes corresponding to the axis are uniformly merged (Geomagic Verify User Guide). The alignment-transform function of the scan data can be manually transformed to the nominal data by picking pair points or using a manipulator. This method is used to turn the scan data into nominal data when the auto alignment method does not produce the desired results. The transform command also supports the use of a transformation matrix if the user already knows the specific transformation values (Geomagic Verify User Guide). To accurately measure the gap between the external region of the model and the internal region of the crown, a model-conjugated abutment tooth was cut in the buccolingual direction and another tooth was cut in the mesiodistal direction by using the function of multiple sections after the whole digital deviation (Fig. 2B). The measurement area of the marginal and internal gaps (16 points) was then measured by applying the 2-D section (Fig. 5). The measurement procedure was repeated in the same measurement area as that used in the 3DSA performed with the batch process method. The batch process is used to replace only the scan data file corresponding to the entire process overlapping the nominal data and scan data because they perform the whole

process exactly.

The marginal and internal gap values were not normally distributed according to the Shapiro-Wilk test of normality ($P < .01$). The 16 points were categorized into four regions as follows: marginal gap (points 1, 8, 9, and 16), deep chamfer (points 2, 7, 10, and 15), axial wall (points 3, 6, 11, and 14), and occlusal area (points 4, 5, 12, and 13). A nonparametric version of the two-way analysis of variance with rank-transformed values was used to compare the gap in each region. For the marginal gap, deep chamfer, and axial wall, the interaction between the measurement type and fabrication method was not significantly different ($P > .05$), and a main-effects model was used to investigate the differences between the regions. For the occlusal area, the interaction between the measurement type and fabrication method was significantly different ($P < .05$), and a full factorial model was used to investigate the differences between the regions. The Tukey's honest significant difference (HSD) test was used for post-hoc comparisons. A sample size of 5 per group was determined using G*Power,³⁷ assuming an effect size of 0.74, an alpha level of 0.05, and a minimum power level of 0.81. The type I error level was set at 0.05.

All statistical analyses were performed with the Statistical Package for Social Sciences software (SPSS v 21.0, IBM Corporation, Armonk, NY, USA).

RESULTS

Table 1 shows the mean (\pm standard deviation) marginal and internal gaps of the molars for each fabrication and measurement method. Significant differences in the marginal gap ($P < .010$), deep chamfer ($P < .001$), axial wall ($P < .001$), and occlusal area ($P < .001$) were observed between the fabrication methods. A significantly greater difference in the occlusal area was observed between the measurement methods ($P < .030$). No significant differences in the marginal gap ($P > .350$), deep chamfer ($P > .719$), and axial wall were found between the measurement methods ($P > .150$) (Table 2).

The Tukey HSD post-hoc test revealed no significant difference between the LC and ZC, or between the ZC and PC. However, the marginal gap region was significantly larger in the LC than in the PC (Table 2). The LC and ZC did not significantly differ in terms of their deep chamfer regions, but the LC had a significantly larger deep chamfer region than both the ZC and PC. The axial wall region of the ZC was significantly larger than that of the LC, which was significantly greater than that of the PC. The LC and ZC did not significantly differ in terms of their occlusal regions, and the PC had a significantly smaller occlusal region than both the LC and ZC. The Tukey HSD post-hoc test revealed that the SRT and 3DSA were significantly different only in terms of the occlusal region.

The PC exhibited the lowest values in all the regions when both the SRT and 3DSA measurement methods were used. In the marginal gap and occlusal regions, the following order was observed for both the measurement methods,

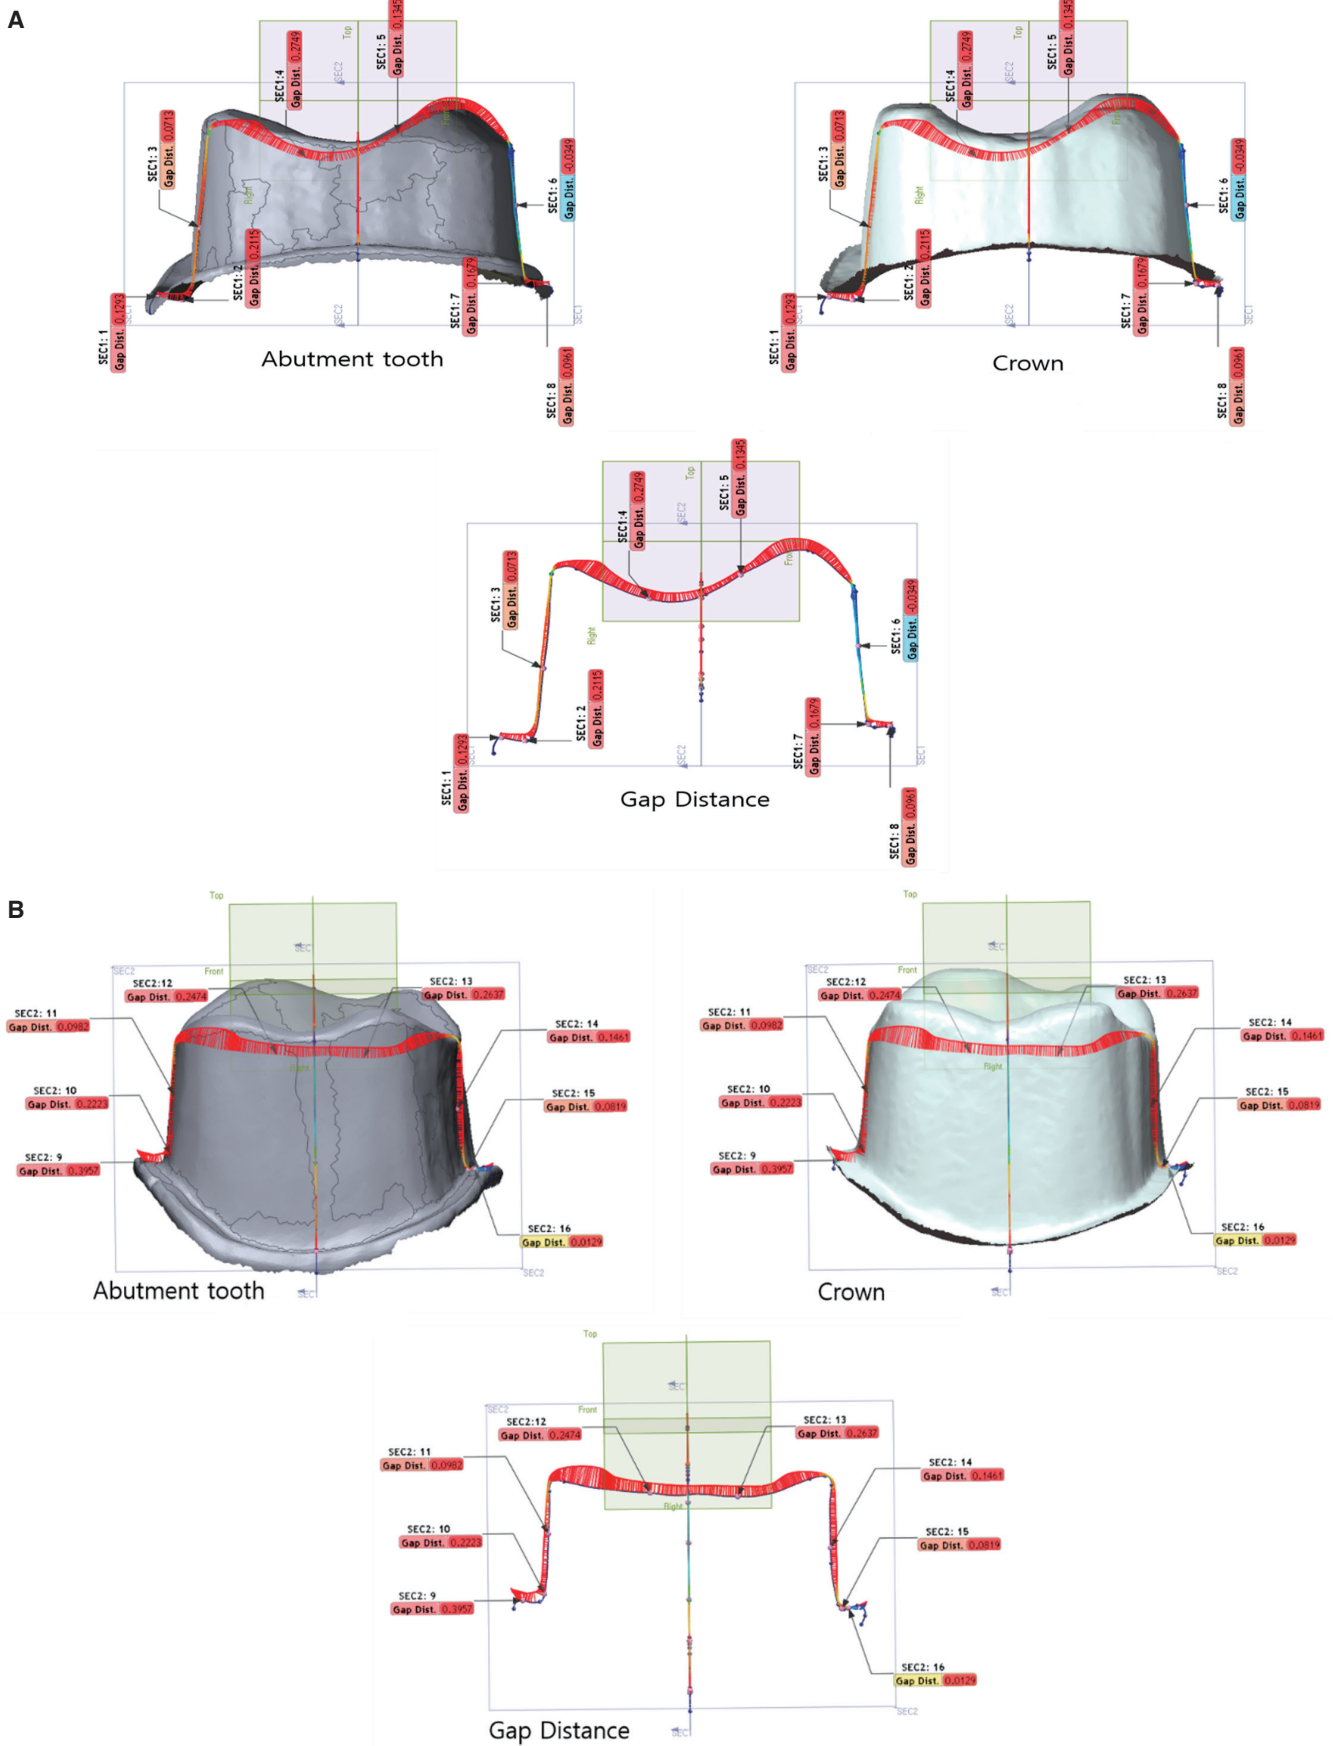


Fig. 5. Section of geometric dimensioning and tolerancing in the three-dimensional superimposition analysis. (A) Bucco-lingual direction, (B) Mesio-distal direction.

Table 1. Gap measurements (in µm) at 16 molar points, according to the fabrication method (n = 5 per group)

Measurement		SRT			3DSA		
Fabrication method		LC	ZC	PC	LC	ZC	PC
Point		Mean ± SD	Mean ± SD	Mean ± SD	Mean ± SD	Mean ± SD	Mean ± SD
Marginal gap	1	114.22 ± 38.33	105.12 ± 31.85	65.48 ± 20.73	101.3 ± 12.16	93.68 ± 20.60	84.23 ± 27.46
	8	116.40 ± 84.90	92.64 ± 18.07	53.50 ± 15.01	128.60 ± 6.82	126.30 ± 9.28	55.06 ± 42.12
	9	81.70 ± 25.88	58.84 ± 23.65	80.96 ± 22.37	142.72 ± 61.56	61.92 ± 63.15	65.40 ± 29.71
	16	73.64 ± 34.61	51.64 ± 22.25	67.36 ± 27.11	23.58 ± 10.83	105.58 ± 73.97	76.84 ± 21.04
Deep Chamfer	2	168.90 ± 59.34	148.26 ± 33.73	142.78 ± 38.59	171.04 ± 5.98	179.88 ± 36.08	113.02 ± 62.64
	7	180.06 ± 76.36	169.48 ± 43.69	123.74 ± 53.23	212.22 ± 1.81	189.52 ± 4.31	96.26 ± 55.02
	10	185.20 ± 25.52	204.76 ± 49.96	142.36 ± 24.28	201.10 ± 98.43	132.16 ± 42.74	122.42 ± 79.74
	15	198.74 ± 45.50	124.88 ± 43.62	142.30 ± 46.40	71.78 ± 7.55	180.60 ± 27.55	139.14 ± 55.31
Axial wall	3	62.76 ± 22.96	62.66 ± 18.93	58.66 ± 10.94	33.2 ± 28.24	91.2 ± 11.76	24.16 ± 30.48
	6	60.40 ± 7.79	87.06 ± 19.00	56.10 ± 9.17	69.52 ± 10.18	88.78 ± 10.69	60.19 ± 26.08
	11	112.36 ± 32.77	130.80 ± 22.77	59.52 ± 11.08	115.62 ± 20.07	159.68 ± 38.04	156.86 ± 63.39
	14	123.66 ± 27.65	109.62 ± 27.83	67.06 ± 15.44	120.80 ± 57.50	169.20 ± 45.40	48.26 ± 69.91
Occlusal area	4	228.42 ± 76.32	186.28 ± 21.45	167.44 ± 30.96	149.66 ± 29.50	114.12 ± 6.55	149.22 ± 72.45
	5	168.74 ± 44.24	168.74 ± 44.24	144.98 ± 28.52	172.14 ± 43.71	273.76 ± 2.67	106.00 ± 57.14
	12	202.40 ± 65.12	182.86 ± 20.60	184.36 ± 46.78	273.40 ± 32.38	195.08 ± 8.87	130.36 ± 57.16
	13	219.36 ± 35.14	158.94 ± 23.58	170.14 ± 48.16	260.48 ± 6.11	240.62 ± 2.85	170.26 ± 79.30

LC, lithium disilicate crown; PC, Pekkton crown; SRT, silicone replicate technique; 3DSA, three-dimensional superimposition analysis; ZC, zirconia crown; SD, standard deviation.

Table 2. Marginal and internal gap measurements (mean ± SD) at 16 molar points

		SRT	3DSA	P value
Marginal gap	LC	96.49 ± 51.01 ^{a*}	99.05 ± 55.63 ^a	<i>P</i> (Fabrication method) < .010
	ZC	77.06 ± 32.14 ^{a,b}	96.87 ± 51.68 ^{a,b}	
	PC	66.83 ± 22.31 ^b	63.76 ± 29.63 ^b	
	<i>P</i> value	<i>P</i> (Measurement) > .350		
Deep chamfer	LC	183.23 ± 51.60 ^{a*}	164.04 ± 72.70 ^a	<i>P</i> (Fabrication method) < .001
	ZC	161.85 ± 49.75 ^a	170.54 ± 36.80 ^a	
	PC	137.80 ± 39.46 ^b	117.71 ± 60.82 ^b	
	<i>P</i> value	<i>P</i> (Measurement) > .719		
Axial wall	LC	89.80 ± 36.96 ^{a*}	84.79 ± 48.20 ^a	<i>P</i> (Fabrication method) < .001
	ZC	97.54 ± 33.20 ^b	127.22 ± 47.57 ^b	
	PC	60.34 ± 11.68 ^c	72.37 ± 69.97 ^c	
	<i>P</i> value	<i>P</i> (Measurement) > .150		
Occlusal area	LC	204.73 ± 57.77 ^{A,a*}	239.33 ± 57.13 ^{B,a}	<i>P</i> (Fabrication method) < .001
	ZC	178.59 ± 23.19 ^{A,a}	205.66 ± 31.49 ^{B,a}	
	PC	173.52 ± 44.77 ^{A,a}	138.96 ± 66.30 ^{B,a}	
	<i>P</i> value	<i>P</i> (Measurement) < .030		

*Different letters indicate a statistically significant difference at a type I error rate of 0.05, with uppercases for measurement and lowercases for fabrication methods.

LC, lithium disilicate crown; PC, Pekkton crown; SRT, silicone replicate technique; 3DSA, three-dimensional superimposition analysis; ZC, zirconia crown; SD, standard deviation.

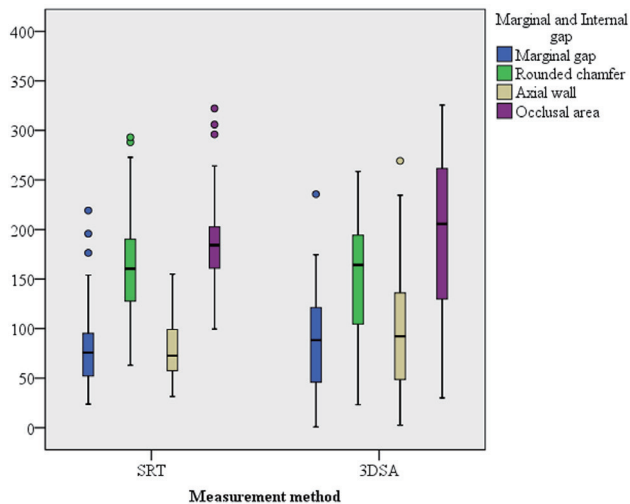


Fig. 6. Mean marginal and internal gaps according to the measurement method. SRT, silicone replicate technique; 3DSA, three-dimensional superimposition analysis.

(high to low) LC, ZC, and PC. In the deep chamfer region, the order was the same with the SRT measuring method; however, with the 3DSA measurement method, the following order was recorded, (high to low) ZC, LC, and PC. The same order was observed in the occlusal region when both the measurement methods were used (Table 2). The 3DSA measurement method showed a larger mean value distribution than the SRT measurement method (Fig. 6).

DISCUSSION

The purpose of this study was to assess the marginal and internal gaps by using three different fabrication methods in order to evaluate the potential clinical applications of PEKKs. We observed a significant difference in the marginal and internal gaps between the different fabrication methods across all the regions. Based on the results of the comparative evaluation of margin fitness for the two measurement methods, the null hypothesis was rejected because the measurements in the occlusal region showed significant differences between the methods. The significant difference in the occlusal area between scan and silicone is due to the limited scanning of the crown area owing to the technical characteristics (some scanners cannot scan deep and narrow structures) of the scanner.³⁸

This study demonstrates that in terms of the marginal fitness, the PC is a more suitable option than the other two fabrication methods. With the LC and ZC, contraction during sintering appears to have a negative effect during the manufacturing of dental prostheses.⁷ PEKK crowns should show better fitness because of the absence of a sintering process and, therefore, of contraction. Furthermore, both the LC and ZC exhibited positive and negative errors in the

inner face generated during the process of combining the digital impressions of the crown. These findings support those of previously published studies on this topic.²⁹⁻⁴¹ The quantitative evaluation of the marginal adaptation is not yet standardized and can be misleading.⁴² According to Guess *et al.*,⁴³ 100 μm is the clinically acceptable marginal gap for ceramics, while McLean and von Fraunhofer reported a gap of less than 120 μm .⁴⁴ Another previous study reported that 100 - 200 μm is the clinically acceptable range for long-term preserved dental prostheses.⁴⁵

The present study showed that in terms of the occlusal region, the LC measured with the SRT, and the LC and ZC measured with the 3DSA exceeded the clinically applicable range of marginal adaptation (Table 1 and Table 2). This was because the corner site of the occlusal surface of the molar region was not an exact reproduction (indicated by the positive and negative errors) due to the bur diameter limitation at the undercut site.^{1,46} However, the measurement value of the occlusal region in the present study was clinically acceptable according to previous reports.^{28,46,47} Anadioti *et al.*²¹ reported a marginal gap for the LC by the SRT of $74.00 \pm 26.00 \mu\text{m}$ and for the LC by 3DSA of $84.00 \pm 24.00 \mu\text{m}$. Hamza *et al.*⁴⁸ reported a vertical marginal gap of $40.20 \pm 6.70 \mu\text{m}$ for lithium disilicate material and $86.10 \pm 28.80 \mu\text{m}$ for zirconia. Meanwhile, Bayramoğlu *et al.*²⁸ confirmed a vertical marginal gap of $109.30 \pm 46.40 \mu\text{m}$ for zirconia. In the present study, the marginal gap region was in the clinically applicable range because with the SRT, the marginal gaps were 96.49 ± 51.01 , 77.06 ± 32.14 , and $66.83 \pm 22.31 \mu\text{m}$ for the LC, ZC, and PC, respectively. With the 3DSA, the marginal gaps were 99.05 ± 55.63 , 96.87 ± 51.68 , and $63.76 \pm 29.63 \mu\text{m}$, respectively. The deep chamfer and axial wall regions were also in the clinically applicable range. Therefore, the LC, ZC, and PC may be considered clinically applicable (Table 1 and Table 2).

Multiple verification methods are available for fitness measurements, including 1) the measurement of the margin between an abutment tooth and a dental prosthesis under a microscope,⁴⁹ 2) the measurement of a cut cross section using an electronic microscope after embedding an abutment tooth and a dental prosthesis conjugated with resin or epoxy,⁵⁰ 3) the SRT that replicates the distance between a dental prosthesis and an abutment tooth or a model with light-body silicone and sustains the form with heavy-body silicone before measuring the cut cross section of interest,^{7,22-24,44} 4) and micro computed tomography to measure the fitness through observations of the internal section of the dental prosthesis.⁵¹ Among these methods, the SRT has been widely utilized owing to its proven credibility and validity.²⁴ The present research utilized a new verification method, the 2-D section of the 3DSA, which involves the measurement of the gap by overlapping a scanned abutment tooth external surface and a scanned dental prosthesis internal surface. To verify this new method, we compared it with the SRT. The SRT produced more stable values with lower minimum and maximum values, and standard deviation range than the 3DSA. The SRT method requires mak-

ing a silicone replica for each measurement, so when the marginal gap between the bucco-lingual section and the mesio-distal section has to be measured, two silicone replicas have to be made. This means that two different silicone replicas are measured. In contrast, with the 3DSA method, the same internal gap can be measured (Fig. 6). However, considering the statistically significant difference only in the occlusal region, the SRT is clinically applicable for the remaining regions (Table 1).

The following limitations of this study need to be discussed. First, the scans of the interior surface of the prostheses had errors, indicating errors in the course of the prosthesis treatment and software application. Studies on intraoral scanning by Jeong *et al.*⁵² in a complete-arch model showed excellent precision as compared to a Blue light scan, which showed scanning errors. And to be increased before and after the sintering had an impact on the precision shrinkage error. Some errors may have occurred in the diameter sizes, milling axis of the design, milling bur using the software, and additional processing steps and affected the precision.⁵³ In addition, the small gap values of the PC should not be overly emphasized. Second, unlike with the SRT, with the 3DSA, repeated measurements had to be performed at the same site if a few outliers were observed on the histogram, as indicated by the stable ranges (Fig. 6). However, compared with the 3-D superimposition 2-D verification methods, the SRT is still insufficient for length measurements. As seen in Figure 6, the measurement of the internal gap has a larger range in the 3DSA group for almost all the areas (both the 50% interval and 25% quartiles are larger). Nevertheless, this study is significant because the methods used involved cutting, and verification requests were made if the same site was considered.

CONCLUSION

The three fabrication methods exhibited marginal gaps within the clinically acceptable range. Although the SRT and 3DSA measurements of the occlusal region significantly differed, no significant differences were observed for the other regions. Thus, both the measurement methods are applicable as verification methods of marginal and internal adaptation.

ORCID

Jin-Young Park <https://orcid.org/0000-0002-8762-6908>
 So-Yeon Bae <https://orcid.org/0000-0002-1836-8714>
 Jae-Jun Lee <https://orcid.org/0000-0001-6348-4784>
 Ji-Hwan Kim <https://orcid.org/0000-0003-3889-2289>
 Hae-Young Kim <https://orcid.org/0000-0003-2043-2575>
 Woong-Chul Kim <https://orcid.org/0000-0002-6730-4960>

REFERENCES

1. Abduo J, Lyons K, Bennamoun M. Trends in computer-aided manufacturing in prosthodontics: a review of the available streams. *Int J Dent* 2014;2014:783948.
2. Bosch G, Ender A, Mehl A. A 3-dimensional accuracy analysis of chairside CAD/CAM milling processes. *J Prosthet Dent* 2014;112:1425-31.
3. Fabbri G, Zarone F, Dellificorelli G, Cannistraro G, De Lorenzi M, Mosca A, Sorrentino R. Clinical evaluation of 860 anterior and posterior lithium disilicate restorations: retrospective study with a mean follow-up of 3 years and a maximum observational period of 6 years. *Int J Periodontics Restorative Dent* 2014;34:165-77.
4. Piconi C, Maccauro G. Zirconia as a ceramic biomaterial. *Biomaterials* 1999;20:1-25.
5. Ueda K, Güth JF, Erdelt K, Stimmelmayer M, Kappert H, Beuer F. Light transmittance by a multi-coloured zirconia material. *Dent Mater J* 2015;34:310-4.
6. Thieme K, Rüssel C. Nucleation and growth kinetics and phase analysis in zirconia-containing lithium disilicate glass. *J Mater Sci* 2015;50:1488-99.
7. Almeida e Silva JS, Erdelt K, Edelhoff D, Araújo É, Stimmelmayer M, Vieira LC, Güth JF. Marginal and internal fit of four-unit zirconia fixed dental prostheses based on digital and conventional impression techniques. *Clin Oral Investig* 2014;18:515-23.
8. Komine F, Blatz MB, Matsumura H. Current status of zirconia-based fixed restorations. *J Oral Sci* 2010;52:531-9.
9. Kang SH, Chang J, Son HH. Flexural strength and microstructure of two lithium disilicate glass ceramics for CAD/CAM restoration in the dental clinic. *Restor Dent Endod* 2013;38:134-40.
10. Oh GJ, Yun KD, Lee KM, Lim HP, Park SW. Sintering behavior and mechanical properties of zirconia compacts fabricated by uniaxial press forming. *J Adv Prosthodont* 2010;2:81-7.
11. Fuhrmann G, Steiner M, Freitag-Wolf S, Kern M. Resin bonding to three types of polyaryletherketones (PAEKs)-durability and influence of surface conditioning. *Dent Mater* 2014;30:357-63.
12. Schwitalla A, Müller WD. PEEK dental implants: a review of the literature. *J Oral Implantol* 2013;39:743-9.
13. Kurtz SM, Devine JN. PEEK biomaterials in trauma, orthopedic, and spinal implants. *Biomaterials* 2007;28:4845-69.
14. Tetelman ED, Babbush CA. A new transitional abutment for immediate aesthetics and function. *Implant Dent* 2008;17:51-8.
15. Mark HF. Encyclopedia of polymer science and technology, concise. John Wiley & Sons, 2013, p. 5-1376.
16. Stawarczyk B, Beuer F, Wimmer T, Jahn D, Sener B, Roos M, Schmidlin PR. Polyetheretherketone-a suitable material for fixed dental prostheses? *J Biomed Mater Res B Appl Biomater* 2013;101:1209-16.
17. Rudolph H, Luthardt RG, Walter MH. Computer-aided analysis of the influence of digitizing and surfacing on the accuracy in dental CAD/CAM technology. *Comput Biol Med* 2007;37:579-87.
18. Luthardt R, Weber A, Rudolph H, Schöne C, Quaas S, Walter M. Design and production of dental prosthetic restorations: basic research on dental CAD/CAM technology. *Int J Comput Dent* 2002;5:165-76.

19. Beuer F, Schweiger J, Edelhoff D. Digital dentistry: an overview of recent developments for CAD/CAM generated restorations. *Br Dent J* 2008;204:505-11.
20. Garcia-Barbosa JA, Arroyo-Osorio JM, Cordoba-Nieto E. The manufacture of a maxillofacial prosthesis from an axial tomography using simulation technologies with a virtual machine tool and four-axis machining. *Dyna* 2016;83:100-5.
21. Anadioti E, Aquilino SA, Gratton DG, Holloway JA, Denry I, Thomas GW, Qian F. 3D and 2D marginal fit of pressed and CAD/CAM lithium disilicate crowns made from digital and conventional impressions. *J Prosthodont* 2014;23:610-7.
22. Raju SR. Comparison of marginal fit of zirconium oxide copings generated using four different CAD-CAM systems: an in vitro study. *J Res Adv Dent* 2013;3:163-71.
23. Tamac E, Toksavul S, Toman M. Clinical marginal and internal adaptation of CAD/CAM milling, laser sintering, and cast metal ceramic crowns. *J Prosthet Dent* 2014;112:909-13.
24. Laurent M, Scheer P, Dejou J, Laborde G. Clinical evaluation of the marginal fit of cast crowns-validation of the silicone replica method. *J Oral Rehabil* 2008;35:116-22.
25. Park JY, Kim HY, Kim JH, Kim JH, Kim WC. Comparison of prosthetic models produced by traditional and additive manufacturing methods. *J Adv Prosthodont* 2015;7:294-302.
26. Meng Z, Yao XS, Yao H, Liang Y, Liu T, Li Y, Wang G, Lan S. Measurement of the refractive index of human teeth by optical coherence tomography. *J Biomed Opt* 2009;14:034010.
27. American National Standards Institute/American Dental Association. ANSI/ADA specification No. 19. Dental elastomeric impression materials. ISO 4823:2000. Chicago: American Dental Association, 2004. Available at: <http://www.iso.ch/iso/en/prods-services/ISOstore/store.html>.
28. Bayramoğlu E, Özkan YK, Yildiz C. Comparison of marginal and internal fit of press-on-metal and conventional ceramic systems for three- and four-unit implant-supported partial fixed dental prostheses: An in vitro study. *J Prosthet Dent* 2015;114:52-8.
29. Laurent M, Scheer P, Dejou J, Laborde G. Clinical evaluation of the marginal fit of cast crowns-validation of the silicone replica method. *J Oral Rehabil* 2008;35:116-22.
30. Park JY, Jeong ID, Lee JJ, Bae SY, Kim JH, Kim WC. In vitro assessment of the marginal and internal fits of interim implant restorations fabricated with different methods. *J Prosthet Dent* 2016;116:536-542.
31. Meyer BJ, Mörmann WH, Lutz F. Optimization of the powder application in the Cerec method with environment-friendly propellant systems. *Schweiz Monatsschr Zahnmed* 1990;100:1462-8.
32. Kim HH, Lee JW, Cha KS, Chung DH, Lee SM. Three-dimensional assessment of upper lip positional changes according to simulated maxillary anterior tooth movements by white light scanning. *Korean J Orthod* 2014;44:281-93.
33. Kuo RF, Chen SJ, Wong TY, Lu BC, Huang ZH. Digital morphology comparisons between models of conventional intraoral casting and digital rapid prototyping. 5th International Conference on Biomedical Engineering in Vietnam 2015;46: 478-80.
34. Bae SY, Park JY, Jeong ID, Kim HY, Kim JH, Kim WC. Three-dimensional analysis of marginal and internal fit of copings fabricated with polyetherketoneketone (PEKK) and zirconia. *J Prosthodont Res* 2017;61:106-12.
35. Persson AS, Andersson M, Odén A, Sandborgh-Englund G. Computer aided analysis of digitized dental stone replicas by dental CAD/CAM technology. *Dent Mater* 2008;24:1123-30.
36. Schaefer O, Kuepper H, Thompson GA, Cachovan G, Hefti AF, Guentsch A. Effect of CNC-milling on the marginal and internal fit of dental ceramics: a pilot study. *Dent Mater* 2013; 29:851-8.
37. Faul F, Erdfelder E, Lang AG, Buchner A. G*Power 3: a flexible statistical power analysis program for the social, behavioral, and biomedical sciences. *Behav Res Methods* 2007;39: 175-91.
38. Jeon JH, Choi BY, Kim CM, Kim JH, Kim HY, Kim WC. Three-dimensional evaluation of the repeatability of scanned conventional impressions of prepared teeth generated with white- and blue-light scanners. *J Prosthet Dent* 2015;114:549-53.
39. Anadioti E, Aquilino SA, Gratton DG, Holloway JA, Denry IL, Thomas GW, Qian F. Internal fit of pressed and computer-aided design/computer-aided manufacturing ceramic crowns made from digital and conventional impressions. *J Prosthet Dent* 2015;113:304-9.
40. Flügge TV, Schlager S, Nelson K, Nahles S, Metzger MC. Precision of intraoral digital dental impressions with iTero and extraoral digitization with the iTero and a model scanner. *Am J Orthod Dentofacial Orthop* 2013;144:471-8.
41. Nedelcu RG, Persson AS. Scanning accuracy and precision in 4 intraoral scanners: an in vitro comparison based on 3-dimensional analysis. *J Prosthet Dent* 2014;112:1461-71.
42. Katsoulis J, Mericske-Stern R, Rotkina L, Zbären C, Enkling N, Blatz MB. Precision of fit of implant-supported screw-retained 10-unit computer-aided-designed and computer-aided-manufactured frameworks made from zirconium dioxide and titanium: an in vitro study. *Clin Oral Implants Res* 2014;25: 165-74.
43. Guess PC, Vagkopoulou T, Zhang Y, Wolkewitz M, Strub JR. Marginal and internal fit of heat pressed versus CAD/CAM fabricated all-ceramic onlays after exposure to thermo-mechanical fatigue. *J Dent* 2014;42:199-209.
44. McLean JW, von Fraunhofer JA. The estimation of cement film thickness by an in vivo technique. *Br Dent J* 1971;131: 107-11.
45. Bindl A, Mörmann WH. Marginal and internal fit of all-ceramic CAD/CAM crown-copings on chamfer preparations. *J Oral Rehabil* 2005;32:441-7.
46. Örtorp A, Jönsson D, Mouhsen A, Vult von Steyern P. The fit of cobalt-chromium three-unit fixed dental prostheses fabricated with four different techniques: a comparative in vitro study. *Dent Mater* 2011;27:356-63.
47. Kahramanoğlu E, Kulak-Ozkan Y. Marginal and internal adaptation of different superstructure and abutment materials using two different implant systems for five-unit implant-supported fixed partial dentures: an in vitro study. *Int J Oral Maxillofac Implants* 2013;28:1207-16.
48. Hamza TA, Ezzat HA, El-Hossary MM, Katamish HA,

- Shokry TE, Rosenstiel SF. Accuracy of ceramic restorations made with two CAD/CAM systems. *J Prosthet Dent* 2013; 109:83-7.
49. Song TJ, Kwon TK, Yang JH, Han JS, Lee JB, Kim SH, Yeo IS. Marginal fit of anterior 3-unit fixed partial zirconia restorations using different CAD/CAM systems. *J Adv Prosthodont* 2013;5:219-25.
50. Lins L, Bemfica V, Queiroz C, Canabarro A. In vitro evaluation of the internal and marginal misfit of CAD/CAM zirconia copings. *J Prosthet Dent* 2015;113:205-11.
51. Neves FD, Prado CJ, Prudente MS, Carneiro TA, Zancopé K, Davi LR, Mendonça G, Cooper LF, Soares CJ. Micro-computed tomography evaluation of marginal fit of lithium disilicate crowns fabricated by using chairside CAD/CAM systems or the heat-pressing technique. *J Prosthet Dent* 2014; 112:1134-40.
52. Jeong ID, Lee JJ, Jeon JH, Kim JH, Kim HY, Kim WC. Accuracy of complete-arch model using an intraoral video scanner: An in vitro study. *J Prosthet Dent* 2016;115:755-9.
53. Ji MK, Park JH, Park SW, Yun KD, Oh GJ, Lim HP. Evaluation of marginal fit of 2 CAD-CAM anatomic contour zirconia crown systems and lithium disilicate glass-ceramic crown. *J Adv Prosthodont* 2015;7:271-7.