

Accurate Bulk Quantitation of Droplet Digital Polymerase Chain Reaction

Chen Sun, Leqian Liu, Harish N. Vasudevan, Kai-Chun Chang, and Adam R. Abate*

Cite This: *Anal. Chem.* 2021, 93, 9974–9979

Read Online

ACCESS |




Metrics & More



Article Recommendations



Supporting Information

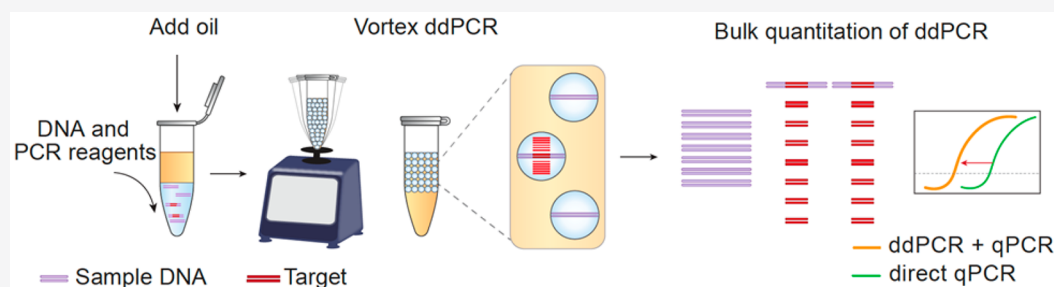

ABSTRACT: Droplet digital PCR provides superior accuracy for nucleic acid quantitation. The requirement of microfluidics to generate and analyze the emulsions, however, is a barrier to its adoption, particularly in low resource settings or clinical laboratories. Here, we report a novel method to prepare ddPCR droplets by vortexing and readout of the results by bulk analysis of recovered amplicons. We demonstrate the approach by accurately quantitating SARS-CoV-2 sequences using entirely bulk processing and no microfluidics. Our approach for quantitating reactions should extend to all digital assays that generate amplicons, including digital PCR and LAMP conducted in droplets, microchambers, or nanoliter wells. More broadly, our approach combines important attributes of ddPCR, including enhanced accuracy and robustness to inhibition, with the high-volume sample processing ability of quantitative PCR.

The quantitation of nucleic acids is important for basic science and clinical applications. Quantitative polymerase chain reaction PCR (qPCR) measures the target concentration by monitoring the exponential rise of amplicons and is the gold standard due to its specificity and superb sensitivity.¹ By contrast, digital PCR (dPCR) subdivides the sample such that partitions contain one or no target molecule; after end-point amplification, positives are enumerated, yielding the target concentration.^{2–4} Digital PCR affords numerous advantages over qPCR, including absolute quantitation and enhanced accuracy for small concentration changes, making it especially valuable for clinical applications.^{5–7} It has secondary benefits, including increased resistance to reaction inhibition^{8,9} and the ability to differentiate intact from fragmented molecules,^{10,11} which are valuable in the identification of viable pathogens in minimally processed samples.^{12,13}

Droplet digital PCR (ddPCR) uses microfluidics to partition samples in water droplets suspended in oil. While the approach is superbly accurate, the requirement of microfluidics is a barrier to its adoption, making it costly compared to qPCR and difficult to integrate into clinical laboratories using standardized well plate formats. Particle-templated emulsification (PTE) partitions samples without microfluidics; the resultant emulsions are similar in monodispersity to microfluidically generated ones and, thus, can be used to conduct most droplet assays, including ddPCR.¹⁴ While removal of microfluidic

droplet generation is a great simplification, subsequent quantification still requires a custom droplet reader, negating much of the advantage.^{15–17} To realize the benefits of ddPCR in settings in which microfluidic instrumentation is impractical, a new approach for enumerating positive droplets that uses only common laboratory equipment and methods is needed.

In this paper, we demonstrate accurate bulk quantitation of droplet digital PCR with common lab equipment. To partition the samples, we use bulk homogenization with a vortexer. To quantitate the samples, we compare different methods for bulk enumeration of positive droplets, including fluorescence, gel electrophoresis, and qPCR. Of these, we find qPCR detection of droplet products yields the highest sensitivity and accuracy over the widest dynamic range. Thus, our approach combines important attributes of ddPCR, including enhanced accuracy and robustness to inhibition, with the accessibility and scalability of bulk processing in well plates. We demonstrate the method by using it to quantify SARS-CoV-2 nucleic acids.

Received: February 26, 2021

Accepted: June 11, 2021

Published: July 12, 2021



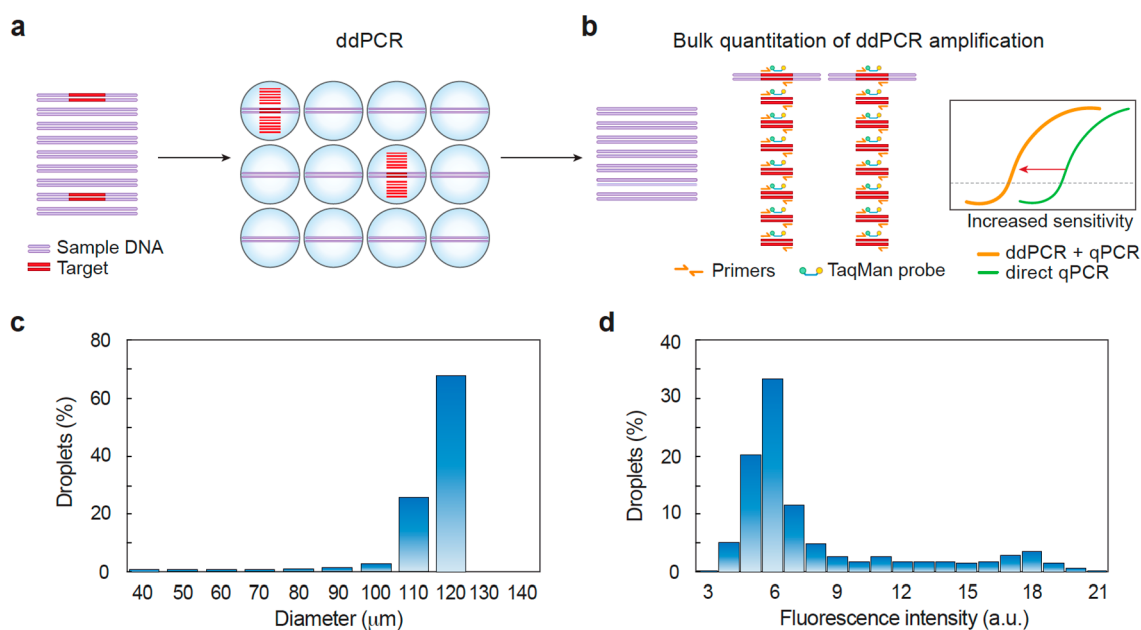


Figure 1. Schematic of workflow for bulk quantitation of ddPCR. (a) A mixed DNA sample is emulsified and processed for ddPCR. The target molecules are amplified in individual droplets. (b) The number of target molecules in the starting sample is proportional to the amount of amplification products, which are quantified by bulk measurement. qPCR quantification of the ddPCR products shows enhanced sensitivity compared to direct qPCR by elevating the qPCR signal. (c) Size distribution of microfluidic emulsions ($n = 950$) shows microfluidics generate monodispersed emulsions. (d) Fluorescence intensity distribution of microfluidic emulsions ($n = 540$) indicates that the assay has a nonzero background.

While we focus on droplet dPCR, the principles of our bulk quantitation should apply to any dPCR approach in which amplicons can be recovered from the partitions and analyzed, including nanoliter well and microchamber technologies.^{3,18–20}

MATERIALS AND METHODS

Bulk Readouts of ddPCR. After ddPCR, droplets were transferred to a flat-bottom well plate and the bulk fluorescence was measured by a microplate reader (Tecan, Infinite 200 PRO). For BioA and Qubit measurement, 1 μL of Proteinase K (800 units/mL, NEB, no. P8107S) was diluted in 20 μL of H_2O and added to the thermocycled emulsions. The emulsions were then broken using 10 μL of 10% (v/v) solution of perfluoro-octanol (Sigma-Aldrich, no. 370533), followed by gentle vortexing for 5 s and centrifugation for 1 min (Benchmark Scientific, MyFuge Mini centrifuge). After droplet breaking, the tubes were incubated for 10 min at 55 $^\circ\text{C}$ to digest the remaining enzymes in the solution. Another incubation of 95 $^\circ\text{C}$ for 10 min was used to deactivate the Proteinase K. A volume of 1 μL of the resulting solution was added directly to the Bioanalyzer (Agilent 2100) or Qubit (Invitrogen, Qubit 2.0 Fluorometer) to quantify the ddPCR products. The concentration of the peak of the correct molecular length was read out from the Bioanalyzer. The total DNA concentration in the sample was measured by Qubit.

For the qPCR readout, 1 μL of the PK treated solution was taken and diluted 100 times in DNA-free water. We used a TaqMan PCR with primers and probe targeting the ddPCR amplicon. The 20 μL qPCR reaction was assembled from 10 μL of Platinum Multiplex PCR Master Mix (Life Technologies, no. 4464269), 1.5 μL of N2 primer set (2019-nCoV RUO Kit, Integrated DNA Technologies, no. 10006713), 1 μL of diluted ddPCR products, and 7.5 μL of H_2O . The qPCR was performed in a QuantStudio 5 real-time PCR system using the

following parameters: 95 $^\circ\text{C}$ for 2 min; 40 cycles of 95 $^\circ\text{C}$ for 15 s, 55 $^\circ\text{C}$ for 1 min, and 72 $^\circ\text{C}$ for 30 s. C_t values for each sample were recorded as a measurement of the concentration of the target.

Droplet Formation by Vortexing. The vortex ddPCR reaction mix was prepared the same as for microfluidic ddPCR. A volume of 30 μL of Droplet Generation Oil for Probes was added to the 0.2 mL PCR tube containing 20 μL of the ddPCR reaction mix. The tube was then placed on a vortex (Scientific Industries, digital vortex-genie 2) and agitated at 3000 rpm for 10 min. After vortexing emulsification, the samples were thermal cycled for ddPCR and readout by qPCR as described above. For positive drop visualization, one ddPCR using TaqMan primer and probe (N2 primer set) was performed. Droplets were imaged using a EVOS microscope (Thermo Fisher). The emulsion breaking and qPCR quantitation of ddPCR are performed the same way as above.

RESULTS AND DISCUSSION

An important advantage of ddPCR over qPCR is its ability to accurately quantify small differences in target concentration, especially near the detection limit of the assay.^{15,21} This benefit arises from the linear nature of ddPCR. Because qPCR is exponential, stochasticity in reaction initiation amplifies over cycles to limit the precision with which small differences in target concentration can be measured. By contrast, when cycled to the end point, irrespective of when each droplet amplification initiates, the number of positive droplets in ddPCR is directly proportional to the number of input target molecules (Figure 1a). This allows accurate measurement of the target concentration,

$$C = D_t/V \quad (1)$$

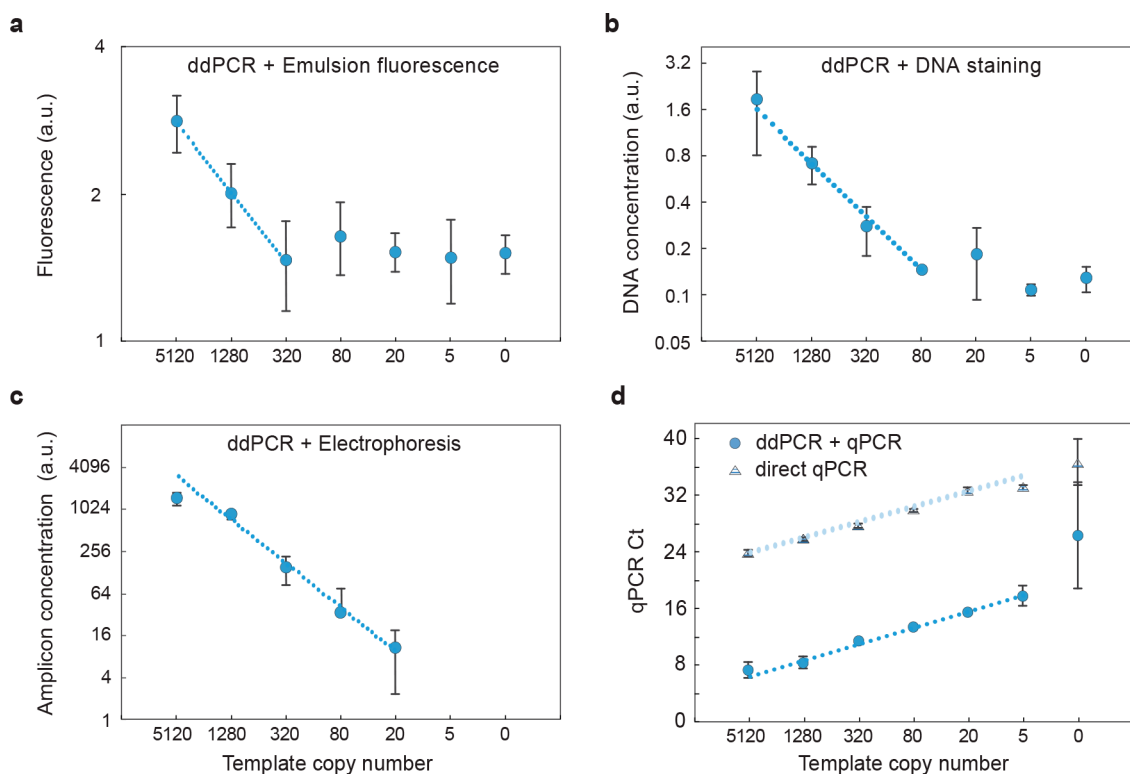


Figure 2. Bulk quantitation of microfluidic ddPCR products: (a) total fluorescence of ddPCR emulsions measured with a plate reader (Tecan), (b) detection of stained total DNA recovered from ddPCR emulsions (Qubit), (c) quantitation of amplicon peak with gel electrophoresis (Bioanalyzer) of ddPCR emulsions, and (d) qPCR quantitation of ddPCR amplicons. ddPCR+qPCR shifts the qPCR C_t to lower cycles, allowing enhanced sensitivity compared to qPCR alone. $n = 3$, error bars represent standard deviation.

where C is the target concentration, D_+ the number of positive droplets, and V the total volume of the sample and is the basis of ddPCR's ability to obtain an "absolute" count of target molecules, while qPCR returns only relative values unless a standard curve is provided.⁹ Thus, enumerating positive droplets is an essential step in ddPCR and is typically accomplished using a droplet reader comprising a microfluidic optical instrument.^{16,17} In addition to being costly, these instruments are difficult to integrate into high-volume testing because each sample must be manually processed; consequently, they are reserved primarily to settings that can bear the high labor and equipment costs.³ A superior strategy would be to infer a positive droplet number from a bulk measurement compatible with plate-processing of samples; this would significantly lower the barrier to adoption and enable high-throughput processing in plates.

In principle, the total fluorescence of an emulsion provides a straightforward way to infer the number of positive droplets because it is the sum of the contributions of the positive F_+ and negative F_- droplet fluorescence,

$$F = F_+ + F_- \quad (2)$$

$$F_+ = \sum f_i v_i \quad \text{and} \quad F_- = \sum f_j v_j \quad (3)$$

with f_i the fluorescence density and v_i the volume of the i th positive droplet; and f_j the fluorescence density and v_j the volume of the j th negative droplet. In the limit $F_+ \gg F_-$ and assuming each positive droplet contributes an average quantum of fluorescence \bar{f} (Figure 1c), the number of positive droplets

$$D_+ \approx F/\bar{f} \quad (4)$$

Thus, for a suitable background fluorescence, it is possible to infer D_+ from bulk measurement of the fluorescence emerging from an emulsion.²² Nevertheless, bulk fluorescence is a poor observable due to the optical properties of ddPCR emulsions. Unless the carrier oil is index matched to the droplets, emulsions are opaque;^{23,24} the amount of signal detected from a droplet deep within the emulsion may thus differ from one near the surface. In addition, common methods for measuring fluorescence in wells read from the bottom which limits reproducibility, since collection efficiency will depend on where the emulsion is in the tube and how long it has settled before being read. Most importantly, ddPCR assays have nonzero background (f_j is not negligible compared to f_i) (Figure 1d) such that the condition $F_+ \gg F_-$ is usually only met when the number of positive drops is large; this limits sensitivity for the most important low concentrations.

In addition to fluorescence, ddPCRs produce amplicons (Figure 1b). In principle, if similar conditions are met of low background and uniform generation from droplets, bulk measurement of amplicons should allow inference of positives in analogy to eq 4,

$$D_+ \approx A/\bar{a} \quad (5)$$

where A is the total number of amplicons generated by a ddPCR and \bar{a} the average number generated per positive droplet. Like total fluorescence, this approximation is justified when the number of amplicons generated by the positive droplets is much greater than by the negatives ($A_+ \gg A_-$). In this respect, amplicon detection is superior to fluorescence because well-designed PCRs generate few off-target products.

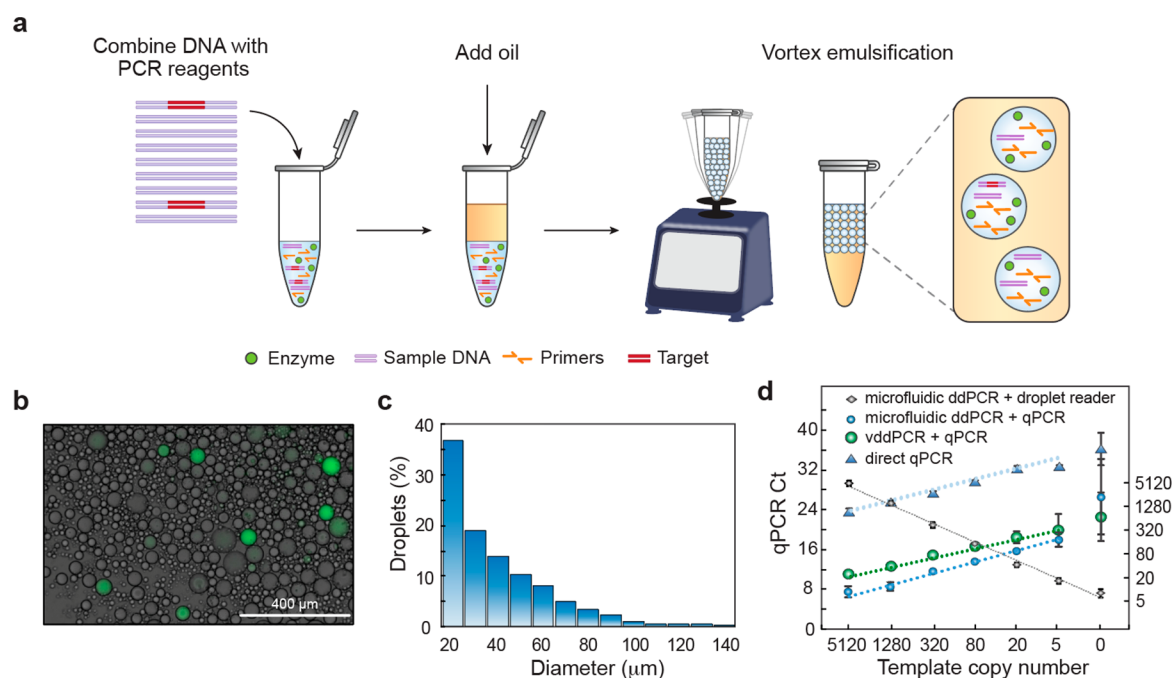


Figure 3. Vortex emulsification qPCR readout enables accurate vddPCR. (a) The DNA sample is added to a tube, oil with stabilizing surfactant is introduced, and the mixture emulsified by vortexing. (b) Vortexed emulsions are thermally cycled. An aliquot is amplified with TaqMan probes to enable visualization. (c) Size distribution of the vortex emulsified droplets obtained by imaging ($n = 1323$). (d) qPCR readout of vddPCR allows accurate quantitation of targets over a range of concentrations. Microfluidic ddPCR, due to the uniformity of the droplets, shows slightly better accuracy and consistency for targets below 20 molecules compared to vddPCR. The droplet reader quantitates microfluidic ddPCR but requires a specialized instrument.

In addition, opacity of the emulsion is not a factor, and amplicons can be measured using a variety of common and sensitive techniques, including staining, on-chip electrophoresis, and qPCR.^{1,25,26}

To investigate whether amplicon quantitation provides a suitable means for estimating D_+ in bulk, we compare the efficacy of these methods for a dilution series of SARS-CoV-2 nucleic acids (Figure 2). We generate all ddPCR assays with commercially available microfluidics,²⁷ and each sample is divided into 20 000 droplets. As expected due to the high background, bulk fluorescence poorly quantifies ddPCR results, yielding a detection sensitivity of ~ 320 molecules (Figure 2a). Recovering and staining DNA from the droplets and quantitating with a fluorescence reader yields a sensitivity of ~ 80 molecules; this technique, however, is nonspecific and detects all recovered DNA irrespective of sequence, yielding a suboptimal background (Figure 2b). To reduce background, we target the amplicons for detection using on-chip gel electrophoresis; this allows quantitation of the peak representing the correct molecular length (Figure S1). The result is an improved detection sensitivity of ~ 20 molecules (Figure 2c), which is nearly as good as direct qPCR analysis of the sample, also having a sensitivity of ~ 20 molecules (Figure 2d, upper points). The measurement becomes less accurate at high concentrations due to multiple targets being encapsulated in the droplets. Importantly, since electrophoresis measures the lengths of all amplicons in the sample, it is readily multiplexed by designing amplicons of different length.²⁶ Moreover, when performed in an emulsion, multiplexed reactions tend to be robust because products do not compete for amplification.²⁸

Below this detection limit, gel electrophoresis is ineffective because the recovered molecules are too few to be detected. To increase detection sensitivity further, we thus need a more

sensitive amplicon quantitation approach. qPCR is a sensitive technique for quantifying nucleic acids and has the benefits of being specific and multiplexable since primers can be targeted to different sequences. As such, with qPCR of ddPCR products, we achieve a detection of just ~ 5 molecules (Figure 2d). Below this limit, detection becomes unreliable because there are so few molecules and there is large variability due to statistical loading of targets in the sample.²⁹ In concordance with this, we observe increased standard deviation when the sample has ~ 5 targets. We observe amplification in no template controls in both direct qPCR and ddPCR+qPCR, likely due to airborne contamination or nonspecific amplification. When targets are abundant, qPCR affords excellent quantitation (Figure 2d). However, direct qPCR has higher C_t values because it detects targets directly, while ddPCR+qPCR detects the amplicons generated by the droplets; the result is that much more DNA is present at the beginning of the qPCR analysis, yielding smaller C_t values. This demonstrates that bulk quantitation of ddPCR-generated amplicons, like direct droplet enumeration, is ultimately limited by statistical loading of targets in the sample and not by the assay sensitivity or accuracy.

While ddPCR+qPCR affords the best sensitivity of all methods we test and even surpasses qPCR, the requirement of microfluidics to generate the emulsions is a major limitation. Indeed, emulsions can be generated by simpler methods, including bead beating, sonication, and pipetting.^{14,30,31} Vortexing also produces emulsions, with the benefits of being simple, fast, and amenable to parallel processing. However, these bulk methods generate polydisperse emulsions in which droplet size varies substantially compared to microfluidics. While accurate ddPCR has been demonstrated in polydisperse emulsions when droplets are imaged

and counted,³² it is unclear whether this holds for bulk detection because, when cycled to the end point, the number of amplicons generated in a droplet scales with its volume. Thus, the total number of amplicons in the recovered pool will depend on the volumes of the positive droplets, which will vary,

$$A = \sum_i a_i v_i \quad (6)$$

with a_i the amplicon concentration and v_i the volume produced by the i th positive droplet. In the limit of large A_+ , however, the sum can be approximated in terms of the average \bar{a} , simplifying the expression to

$$A \approx D_+ \bar{a} \quad (7)$$

such that eq 5 still holds. Below this limit, statistical variation in the droplet volume dominates the measurement. Where this approximation holds will thus depend on the size distribution of the droplets, such that more polydispersed emulsions will lose their quantitiveness at higher A_+ . To investigate this concept, we perform another experiment in which we quantify polydispersed vortex ddPCR (vddPCR) emulsions generated by vortexing (Figure 3a). As expected, the emulsions are polydispersed, though positive droplets are clearly visible (Figure 3b); in addition, the size distribution is much broader than for the microfluidic emulsion (Figure 3c). When we measure the recovered amplicons, we find excellent quantitation, with minimal error down to 20 molecules. Below this, statistical variation in droplet size increases error (Figure 3d, right) though the measurement remains quantitative down to ~ 5 molecules and similar to microfluidic monodispersed emulsions (Figure 2d). Furthermore, vortex-generated emulsions have smaller average droplet sizes than the microfluidic ones and, thus, the sample is subdivided into more partitions, increasing the dynamic range at higher concentrations.

CONCLUSIONS

Our approach is a major advance because it allows fast and scalable digital PCR without microfluidics, generating the droplets by vortexing and reading out the results by common bulk techniques, including electrophoresis and qPCR. While bulk emulsified samples afford higher accuracy than qPCR, statistical variation in droplet size results in increased measurement error for rare targets compared to monodispersed emulsions. In instances in which this error is unacceptable, PTE can generate monodispersed emulsions by vortexing.¹⁴ This approach affords other valuable features, including the ability to tune droplet size to optimize the number of amplicons generated for bulk quantitation. For example, larger droplets generate more amplicons per original target molecule, thereby increasing sensitivity of the bulk quantitation and overall limit of detection. Alternatively, dividing the sample into more droplets reduces multiple encapsulations, affording better accuracy for high input samples. Using droplets of different sizes to analyze the same sample increases the dynamic range.³² By implementing multiplexing, several targets can be detected simultaneously²⁸ and to estimate the intactness of molecules based on how their subsequences codistribute,¹⁰ which is important for clinical diagnostics in which differentiation of fragmented and intact pathogenic genomes is necessary for reducing false positive test results. However, a limitation is that vortexing can fragment long DNA molecules, so encapsulation conditions must be optimized to enable such long-target detections. In addition,

multiplexing by measuring ddPCR amplicons of different length should allow simultaneous detection and quantitation of insertion, deletion, and splice mutants in research or clinical samples. Our approach thus combines key benefits of ddPCR with the simplicity and scalability of plate processing and, thus, can be readily implemented to increase the accuracy and robustness of nucleic acid testing.

ASSOCIATED CONTENT

Supporting Information

The Supporting Information is available free of charge at <https://pubs.acs.org/doi/10.1021/acs.analchem.1c00877>.

Additional experimental sections on ddPCR using commercial droplet generator and Figure S1, images showing quantitation of the ddPCR amplicons using on-chip electrophoresis (PDF)

AUTHOR INFORMATION

Corresponding Author

Adam R. Abate – Department of Bioengineering and Therapeutic Sciences, University of California San Francisco, San Francisco, California 94158, United States; California Institute for Quantitative Biosciences, University of California San Francisco, San Francisco, California 94158, United States; Chan Zuckerberg Biohub, San Francisco, California 94158, United States; orcid.org/0000-0001-9614-4831; Email: adam@abatelab.org

Authors

Chen Sun – Department of Bioengineering and Therapeutic Sciences, University of California San Francisco, San Francisco, California 94158, United States; orcid.org/0000-0003-1216-5091

Leqian Liu – Department of Bioengineering and Therapeutic Sciences, University of California San Francisco, San Francisco, California 94158, United States

Harish N. Vasudevan – Department of Bioengineering and Therapeutic Sciences, University of California San Francisco, San Francisco, California 94158, United States; Department of Radiation Oncology, University of California San Francisco, San Francisco, California 94158, United States

Kai-Chun Chang – Department of Bioengineering and Therapeutic Sciences, University of California San Francisco, San Francisco, California 94158, United States; orcid.org/0000-0001-7200-3532

Complete contact information is available at: <https://pubs.acs.org/doi/10.1021/acs.analchem.1c00877>

Notes

The authors declare no competing financial interest.

ACKNOWLEDGMENTS

We thank Joshua Batson at the Chan Zuckerberg Biohub for helpful discussion. This work was supported by the Chan Zuckerberg Biohub and the National Institutes of Health (NIH) (Grant Nos. R01-EB019453-01 and R01-HG008978-01).

REFERENCES

- (1) Heid, C. A.; Stevens, J.; Livak, K. J.; Williams, P. M. *Genome Res.* 1996, 6 (10), 986–994.

- (2) Vogelstein, B.; Kinzler, K. W. *Proc. Natl. Acad. Sci. U. S. A.* **1999**, *96* (16), 9236–9241.
- (3) Quan, P. L.; Sauzade, M.; Brouzes, E. *Sensors* **2018**, *18* (4), 1271.
- (4) Heyries, K. A.; Tropini, C.; VanInsberghe, M.; Doolin, C.; Petriv, O. I.; Singhal, A.; Leung, K.; Hughesman, C. B.; Hansen, C. L. *Nat. Methods* **2011**, *8* (8), 649–U64.
- (5) Pohl, G.; Shih, L. M. *Expert Rev. Mol. Diagn.* **2004**, *4* (1), 41–47.
- (6) Alteri, C.; Cento, V.; Antonello, M.; Colagrossi, L.; Merli, M.; Ughi, N.; Renica, S.; Matarazzo, E.; Di Ruscio, F.; Tartaglione, L.; Colombo, J.; Grimaldi, C.; Carta, S.; Nava, A.; Costabile, V.; Baiguera, C.; Campisi, D.; Fanti, D.; Vismara, C.; Fumagalli, R.; Scaglione, F.; Epis, O. M.; Puoti, M.; Perno, C. F. *PLoS One* **2020**, *15* (9), e0236311.
- (7) Hayden, R. T.; Gu, Z.; Ingersoll, J.; Abdul-Ali, D.; Shi, L.; Pounds, S.; Caliendo, A. M. *J. Clin. Microbiol.* **2013**, *51* (2), 540–546.
- (8) Dingle, T. C.; Sedlak, R. H.; Cook, L.; Jerome, K. R. *Clin. Chem.* **2013**, *59* (11), 1670–1672.
- (9) Hindson, C. M.; Chevillet, J. R.; Briggs, H. A.; Gallichotte, E. N.; Ruf, I. K.; Hindson, B. J.; Vessella, R. L.; Tewari, M. *Nat. Methods* **2013**, *10* (10), 1003.
- (10) Lance, S. T.; Sukovich, D. J.; Stedman, K. M.; Abate, A. R. *Virology* **2016**, *13*, 201.
- (11) Han, J.; Lee, J. Y.; Bae, Y. K. *Biochim. Biophys. Acta, Gen. Subj.* **2019**, *1863* (8), 1235–1242.
- (12) Deiana, M.; Mori, A.; Piubelli, C.; Scarso, S.; Favarato, M.; Pomari, E. *Sci. Rep.* **2020**, *10*, 18764.
- (13) Pavsic, J.; Zel, J.; Milavec, M. *Anal. Bioanal. Chem.* **2016**, *408* (1), 67–75.
- (14) Hatori, M. N.; Kim, S. C.; Abate, A. R. *Anal. Chem.* **2018**, *90* (16), 9813–9820.
- (15) Baker, M. *Nat. Methods* **2012**, *9* (6), 541–544.
- (16) Hatch, A. C.; Fisher, J. S.; Tovar, A. R.; Hsieh, A. T.; Lin, R.; Pentoney, S. L.; Yang, D. L.; Lee, A. P. *Lab Chip* **2011**, *11* (22), 3838–3845.
- (17) Guo, M. T.; Rotem, A.; Heyman, J. A.; Weitz, D. A. *Lab Chip* **2012**, *12* (12), 2146–2155.
- (18) Kalinina, O.; Lebedeva, I.; Brown, J.; Silver, J. *Nucleic Acids Res.* **1997**, *25* (10), 1999–2004.
- (19) Ottesen, E. A.; Hong, J. W.; Quake, S. R.; Leadbetter, J. R. *Science* **2006**, *314* (5804), 1464–1467.
- (20) Shen, F.; Du, W. B.; Kreutz, J. E.; Fok, A.; Ismagilov, R. F. *Lab Chip* **2010**, *10* (20), 2666–2672.
- (21) Suo, T.; Liu, X.; Feng, J.; Guo, M.; Hu, W.; Guo, D.; Ullah, H.; Yang, Y.; Zhang, Q.; Wang, X.; Sajid, M.; Huang, Z.; Deng, L.; Chen, T.; Liu, F.; Xu, K.; Liu, Y.; Zhang, Q.; Liu, Y.; Xiong, Y.; Chen, G.; Lan, K.; Chen, Y. *Emerging Microbes Infect.* **2020**, *9* (1), 1259–1268.
- (22) Morinishi, L. S.; Blainey, P. J. *Visualized Exp.* **2015**, 103.
- (23) Chantrapornchai, W.; Clydesdale, F. M.; McClements, D. J. *Food Res. Int.* **2001**, *34* (9), 827–835.
- (24) Liao, P. Y.; Jiang, M. C.; Chen, Z. T.; Zhang, F. L.; Sun, Y.; Nie, J.; Du, M. J.; Wang, J. B.; Fei, P.; Huang, Y. Y. *Proc. Natl. Acad. Sci. U. S. A.* **2020**, *117* (41), 25628–25633.
- (25) Nakayama, Y.; Yamaguchi, H.; Einaga, N.; Esumi, M. *PLoS One* **2016**, *11* (3), e0150528.
- (26) Le Roux, D.; Root, B. E.; Reedy, C. R.; Hickey, J. A.; Scott, O. N.; Bienvenue, J. M.; Landers, J. P.; Chassagne, L.; de Mazancourt, P. *Anal. Chem.* **2014**, *86* (16), 8192–8199.
- (27) Bio-Rad. *Droplet Digital PCR Applications Guide*, <http://www.bio-rad.com/en-us/category/digital-pcr>, 2014.
- (28) Dobnik, D.; Stebih, D.; Blejec, A.; Morisset, D.; Zel, J. *Sci. Rep.* **2016**, *6*, 35451.
- (29) Basu, A. S. *Slas Technol.* **2017**, *22* (4), 369–386.
- (30) Gaikwad, S. G.; Pandit, A. B. *Ultrason. Sonochem.* **2008**, *15* (4), 554–563.
- (31) Yeung, A.; Dabros, T.; Masliyah, J.; Czarnecki, J. *Colloids Surf., A* **2000**, *174* (1–2), 169–181.
- (32) Byrnes, S. A.; Chang, T. C.; Huynh, T.; Astashkina, A.; Weigl, B. H.; Nichols, K. P. *Anal. Chem.* **2018**, *90* (15), 9374–9380.