









REVIEW ARTICLE

Design and clinical application of injectable hydrogels for musculoskeletal therapy

Øystein Øvrebø^{1,2,3}  | Giuseppe Perale^{4,5,6}  | Jonathan P. Wojciechowski^{7,8,9}  |
Cécile Echalié^{7,8,9,10}  | Jonathan R. T. Jeffers¹¹  | Molly M. Stevens^{7,8,9}  |
Håvard J. Haugen^{2,3}  | Filippo Rossi¹ 

¹Department of Chemistry, Materials and Chemical Engineering "Giulio Natta", Politecnico di Milano, Milano, Italy

²Department of Biomaterials, Institute of Clinical Dentistry, University of Oslo, Oslo, Norway

³Material Biomimetic AS, Oslo Science Park, Oslo, Norway

⁴Industrie Biomediche Insubri SA, Mezzovico-Vira, Switzerland

⁵Faculty of Biomedical Sciences, University of Southern Switzerland, Lugano, Switzerland

⁶Ludwig Boltzmann Institute for Experimental and Clinical Traumatology, Vienna, Austria

⁷Department of Materials, Imperial College London, London, UK

⁸Department of Bioengineering, Imperial College London, London, UK

⁹Institute of Biomedical Engineering, Imperial College London, London, UK

¹⁰Hybrid Technology Hub, Centre of Excellence, Institute of Basic Medical Science, University of Oslo, Oslo, Norway

¹¹Department of Mechanical Engineering, Imperial College London, London, UK

Correspondence

Håvard J. Haugen, Department of Biomaterials, Institute of Clinical Dentistry, University of Oslo, Geitmyrsveien 71, 0455 Oslo, Norway.
Email: h.j.haugen@odont.uio.no

Funding information

Aker Scholarship; H2020 Marie Skłodowska-Curie Actions, Grant/Award Number: 801133; Norges Forskningsråd, Grant/Award Number: 327512; UK Research and Innovation, Grant/Award Number: MR/R015651/1

Abstract

Musculoskeletal defects are an enormous healthcare burden and source of pain and disability for individuals. With an aging population, the proportion of individuals living with these medical indications will increase. Simultaneously, there is pressure on healthcare providers to source efficient solutions, which are cheaper and less invasive than conventional technology. This has led to an increased research focus on hydrogels as highly biocompatible biomaterials that can be delivered through minimally invasive procedures. This review will discuss how hydrogels can be designed for clinical translation, particularly in the context of the new European Medical Device Regulation (MDR). We will then do a deep dive into the clinically used hydrogel solutions that have been commercially approved or have undergone clinical trials in Europe or the United States. We will discuss the therapeutic mechanism and limitations of these products. Due to the vast application areas of hydrogels, this work focuses only on treatments of cartilage, bone, and the nucleus pulposus. Lastly, the main steps toward clinical translation of hydrogels as medical devices are outlined. We suggest a framework for how academics can assist small and medium MedTech enterprises conducting the initial clinical investigation and post-market clinical follow-up required in the MDR. It is evident that the successful translation of hydrogels is governed by acquiring high-quality pre-clinical and clinical data confirming the device mechanism of action and safety.

KEYWORDS

bone regeneration, cartilage regeneration, clinical translation, hydrogels, medical devices, regenerative medicine, viscosupplementation

1 | HYDROGELS AS MEDICAL DEVICES

Hydrogels represent a group of biomaterials consisting of water-swollen polymer or colloidal networks.¹ Hydrogels are viscoelastic materials that have attracted attention in regenerative medicine due to their ability to structurally mimic the extracellular matrix (ECM),² thereby creating a conducive environment for cell proliferation and tissue regeneration. The viscoelastic properties of hydrogels allow them to function as stem cell carriers or scaffolds for controlled drug release. Within the review by Correa and colleagues,³ these applications of hydrogels are discussed in the context of clinical translation. From a regulatory perspective, hydrogels can be considered medical devices if their therapeutic effect comes from their intrinsic structure, because their physical, chemical, or mechanical effects are the primary mechanism of action for their therapeutic function. To be classified as medical devices hydrogels cannot have any medicinal component, effect, or mechanism of action. For the case of medical devices, harmonized in the European market, the relevant regulation is EU 2017/745, which entered in force on May 26, 2021. Melvin and Torre⁴ have discussed the rationale behind the new regulation. Recently, Catoira et al.⁵ have discussed how the regulation affects the translation of hydrogels. Hence, this review will consider how hydrogels can be designed to satisfy these regulations. However, expanding cells or integrating cell-stimulating therapeutics into the medical device results in these hydrogel systems being regulated as medicinal products (drugs/biologics). Indeed, they are considered as drugs when their principal mode of action is pharmacological, metabolic, or immunological.⁶ The consequence of the medicinal regulation is that a more thorough investigation of the biocompatibility and therapeutic effect is required before such solutions can be approved for clinical application. This increases the translational barriers and the time before patients can benefit from the treatment. Therefore, it is attractive to translate hydrogel solutions as medical devices such that the therapy can reach the clinic earlier and is more affordable. A detailed discussion of the classification can be found in Section 4.

Particularly in applications for musculoskeletal disorders, there is an unmet need for minimally invasive therapies, where the use of injectable hydrogels has tremendous potential. The demand is driven by an aging population that gives two unique opportunities: (1) an increasing number of patients outlive the longevity of permanent medical devices; thus, hydrogel therapies can be used to delay permanent implantation, (2) minimally invasive therapies give a treatment opportunity for the growing population group that would otherwise not survive the trauma induced by conventional surgeries.⁷ Examples of these type of devices are represented by hydrogels for joint lubrication,^{8,9} injectable scaffolds for guided bone¹⁰ or cartilage regeneration,¹¹ or nucleus pulposus (NP) replacements.¹² These are widely different applications for diverse tissues with different loading modes and levels. Consequently, a one-fit-all hydrogel is an unlikely strategy, and thought should be put into the clinical requirements of the material when designing the hydrogel.

2 | HYDROGEL DESIGN

Hydrogels are an extensively investigated class of biomaterials, and an increasing number of products have reached the clinic. In the following section, we will go through the design steps of the hydrogels and discuss what considerations need to be taken to improve the likelihood of clinical translation and to comply with the European Medical Device Regulations (MDRs). The design process is summarized in Figure 1.

2.1 | Material selection

The first step in the design process is to select a suitable polymer to form the hydrogel. There is a larger group of naturally derived polymers such as collagen,¹³ hyaluronic acid (HA),¹⁴ chitosan,¹⁵ cellulose,¹⁶ and alginate.¹⁷ Although not exclusively, plant-based polymers tend to be composed of saccharides, such as cellulose, and animal-based polymers tend to compose of protein, for example, collagen.¹⁸ These have been attractive as their natural origin makes them favorably biocompatible and biodegradable but can introduce issues such as immunogenicity and limited mechanical properties.¹⁹ From a translational perspective, these are limited by high cost and batch-to-batch variability.^{5,19,20} Alternatively, synthetic polymers such as poly(ethylene glycol) (PEG),²¹ poly(vinyl alcohol),²² poly(acrylic acid),²³ and poly(acrylamide)²⁴ can be used. Synthetic polymers are industrially more used as they are more favorable from both cost and regulatory perspective, the two being also connected. Synthetic polymers can be produced in more robustly repeatable manners and more efficiently with respect to naturally derived ones, making them readily scalable.²⁵ Synthesis is typically a more straightforward production process and ensures controlled environmental factors thus limiting the risk of contamination. Synthetic polymers are favorable versus naturally derived raw materials as they allow for improved traceability and higher degree of availability which finally reduces the cost.^{25,26} However, their clinical adoption has been limited, and those that exist usually provide a mechanical mechanism of action, for example, PEG-hydrogel as a spacer between prostate and rectum to protect the rectum during radiotherapy.²⁷ For the regenerative market, the translation is insignificant, which has been attributed to their low biocompatibility.²⁸ The low biocompatibility is likely related to lack of cell-specific bioactivity, including cell adhesive and migratory cues, and cell-mediated material degradation.²⁹ This highlights how biocompatibility is vital for the success of any hydrogel, and the biological response should be central to the choice of the polymer for the hydrogel. Implanted materials can either integrate physiologically, leading to minimal or no scarring, or the material can induce chronic inflammation and a foreign body response.³⁰ After injection, the material must provide appropriate biochemical and biophysical signals to recruit host cells that will eventually produce new native tissue.³¹ Immune cells also play a key role in the signaling cascade leading to tissue regeneration, and appropriate engineering of the local immune response can boost the tissue regeneration.³² For instance,

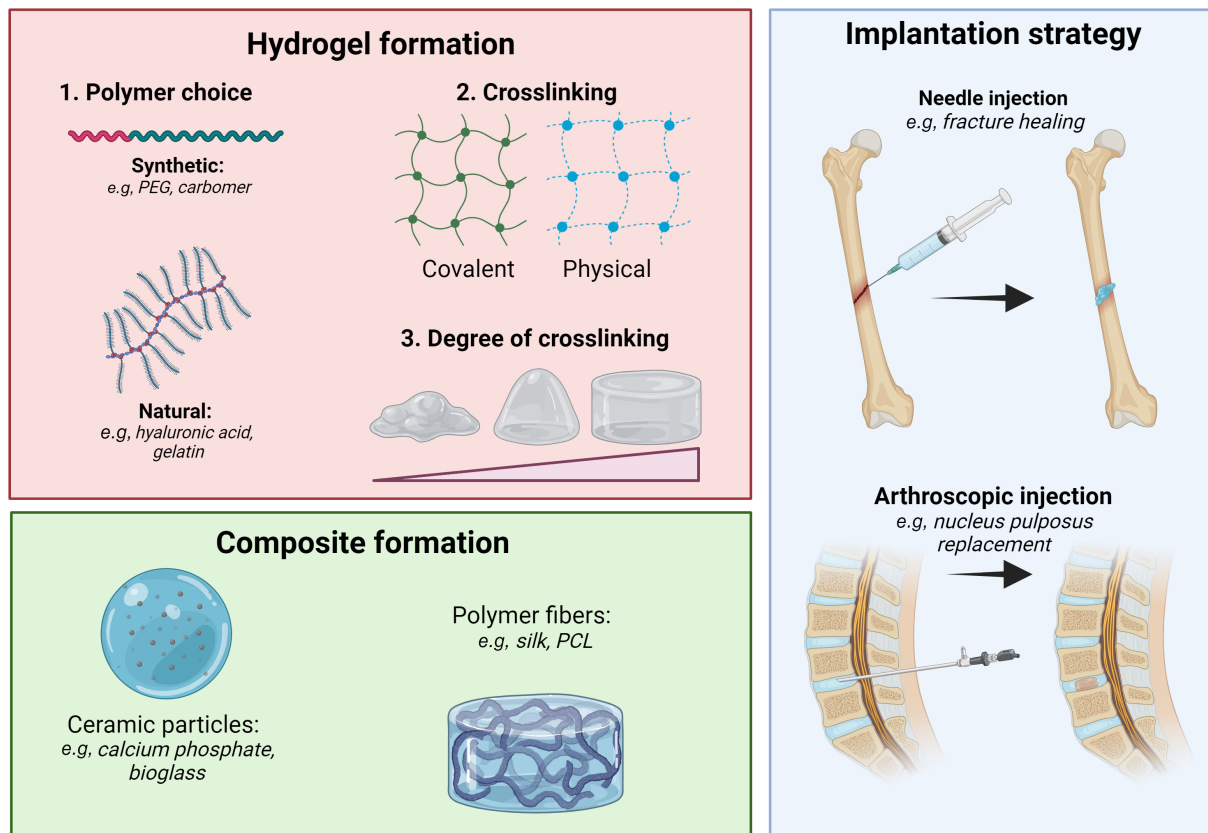


FIGURE 1 Schematic of the design process of hydrogels as medical devices for musculoskeletal application. The process consists of three design blocks, first, the hydrogel is developed, then any particles or other composite inclusions are added before the delivery strategy is chosen

monocytes and macrophages releasing cytokines including BMP-2, BP-4, and TGF- β 1 support osteoblast differentiation and proliferation.³³ The current gold standard for understanding biocompatibility remains clinical trials, but essential information can also be derived from well-designed pre-clinical trials. When selecting the polymer, we have two conflicting interests; from a biological perspective, natural biopolymers are favorable due to higher biocompatibility, meanwhile synthetic polymers have more controllable properties, including swelling, degradation, phase transitions, and mechanical properties.³⁴ Additionally, synthetic polymers are more favorable from a regulatory and financial perspective. To balance these interests co-gel solutions such as PEG-HA³⁵ and gelatin methacrylate-PEG diacrylate³⁶ are promising strategies at combining features from both groups of polymers. Moreover, synthetic polymers can be functionalized with proteins and peptides to improve cell attachment and proliferation. For instance, the inclusion of RGD-peptides in PEG gels has demonstrated these capabilities on multiple cell types.^{37,38}

2.2 | Crosslinking/gelation

The next step is to form the gel-network by crosslinking the polymer chains. There are two options here, and the polymer can be physically

or chemically crosslinked. Physical crosslinking is a reversible process where weak non-covalent interactions (e.g., van der Waals, hydrogen bonding, electrostatic interactions) keep the network stable. The advantage here is that the gel can be formed without using a crosslinking agent and the gel is easier to mold into the defect geometry.³⁹ Alternatively, chemical crosslinking (covalent bonds) can be used. The covalent bonds tend to convey to the gel's improved mechanical properties and higher stability.⁴⁰ The gel stability is a vital matrix design as long degradation times and the inability to be remodeled by the cells will hamper tissue growth. In contrast, a fast degradation time will leave an unfilled void after the gel degradation.⁴¹ The degree of crosslinking, meaning the number of bonds that interconnect the polymers to each other, is an important parameter for the material properties. With a higher degree of crosslinking, we can expect a higher viscosity, stiffness, and longer degradation time.^{42,43} It has early been established that with increased degree of crosslinking, the gel's ability to swell decreases.⁴⁴ The equilibrium degree of swelling affects a series of properties such as solute diffusion coefficient, mechanical properties, and the mobility of therapeutic agents.⁴⁵ From a translational perspective, chemical crosslinking means introducing new chemicals and at least one more chemical reaction. It must be proven that the biomaterial remains biocompatible and that there is not an increase of leachables such as unreacted crosslinker. Dialysis tends to be an efficient method for removing such

impurities, but the removal and biocompatibility must be proven. This is further discussed in Section 5.

2.3 | Composite design

Like with other biomaterial types, composite materials can be formed using hydrogels. This is a favorable strategy as the final material will have inherent properties from base materials in addition to the properties derived from the interaction between material components. In terms of hydrogels, this could be the introduction of fibers, for instance, to improve mechanical properties or guide tissue growth, or particles, for example, a ceramic phase which can boost bone regeneration. Li and co-workers⁴⁶ combined a hydrogel of thiolated HA and polyethylene glycol diacrylate (PEGDA) gel covalently crosslinked to fragmented, electrospun polycaprolactone fibers. The fibers gave improved mechanical properties compared to the HA-PEG gel alone, thereby they could mimic the mechanical properties of native fat tissue. Moreover, their *in vivo* trials with subcutaneous injection of the material in a rat and a rabbit model suggest improved macrophage polarization toward a pro-regenerative phenotype and enhanced angiogenesis.

The inclusion of an inorganic phase in the polymeric hydrogel material has been a popular strategy for bone regeneration. Chahal and colleagues⁴⁷ developed a PEG hydrogel with amorphous calcium phosphate particles. They demonstrated that the particles both gave a higher stiffness, and slowly released calcium and zinc ions into the solution, creating conducive properties for bone regeneration. Although they observed a qualitative increase in gel mineralization, they could not demonstrate statistical significance. Furthermore, the human mesenchymal stem cells (MSCs) they used were unable to attach to the gel before they functionalized the PEG with RGD tripeptide motifs. This highlights the importance of choosing a polymer with high bioactivity to succeed clinically and demonstrates one of the shortfalls of most fully synthetic systems. Semi-synthetic systems, however, are promising as they allow for tunable properties such as gelation mechanism and adhesion to tissues. Researchers from the Langer lab⁴⁸ developed a cellulose hydrogel with PEG-block-poly (lactic acid) nanoparticles as non-covalent crosslinking nodes that gave the gel shear-thinning and self-healing properties. *In vivo* in mice (subcutaneously in the back) they demonstrated biocompatibility with a mild neutrophil-induced inflammation at day 3 and clearance by macrophages from day 7. A consistent release pattern was observed when particles were loaded with model dual-hydrophobic/hydrophilic drugs. Wang and colleagues⁴⁹ formed a mechanically strong, transparent, and self-healing hydrogel by coating clay nanosheets with sodium polyacrylate and physically crosslinking it with dendritic G2 binder.

Any inclusion will make it, from a regulatory perspective, a completely new biomaterial. Therefore, it will require the standard omni-comprehensive testing due for any novel formulation. This includes the application of ISO 10993 family of standards that encompass biocompatibility testing up to clinical studies, and for biodegradable biomaterials the documentation requirements that degradation products do not accumulate in any body organs.⁵⁰

2.4 | Implantation method

Although the implantation method of the hydrogel is not directly a design variable affecting the gel properties, the hydrogel should be designed with implantation feasibility in mind. There are primarily two strategies of implantation in current use. The traditional is surgical incision implantation, where a surgeon cuts a flap through the patient's dermis and physically places the implant at the desired location. The advantage of this intervention is that the gel can be pre-shaped prior to the surgery and have higher mechanical stiffness. The disadvantage is that the incision surgery gives a longer hospitalization time, longer recovery time, increased postoperative pain,⁵¹ and higher risk of bacterial infections.⁵² Therefore, injectable solutions are attractive minimally invasive strategies that give less trauma,⁵³ less blood loss, shorter surgeries, and rapid recovery.⁵⁴ This brings its own technical challenges, as the gel must have low enough viscosity to be injectable through a needle or arthroscopic instruments. To have adequate viscosity during injection, it might be favorable to use a low degree of crosslinking,⁴³ a physically crosslinked gel exhibiting shear-thinning properties,^{48,55} or utilize *in situ* crosslinking of the hydrogel using methods such as click-chemistry,⁵⁶ ultrasound,⁵⁷ and photo-initiated crosslinking.^{11,12} For *in situ* crosslinking, it is imperative to ensure that there are no adverse chemical reactions between the material and the surrounding biological tissue. For instance, thiol groups are naturally occurring in the body, so if a thiol-based Michael addition strategy is used for gelation, there is a risk of undesired cross-reactivity, oxidation, or metabolism.⁴⁰ This has inspired the focus on bioorthogonal chemistry, a class of high-yielding reactions based on selective transformation not commonly found in biology.⁵⁸

An innovative solution for injection of a hydrogel therapy is the Flowbone[®] solution developed by researchers at EPFL in Switzerland. They have developed a biphasic gel solution for bone regeneration where the first phase consists of covalently crosslinked HA with hydroxyapatite particles incorporated, that is carried in a second aqueous phase comprising more hydroxyapatite particles.⁵⁹ The biphasic system allows a low viscosity and thereby injectability. This solution also allows for the loading drugs such as bisphosphonates,⁶⁰ which is now under investigation in pre-clinical trials.

Other solutions chose a tactic where the crosslinking occurs *in situ*, such as Regentis Biomaterial's GelrinC[®], which is discussed below. The *in situ* strategy allows for a low viscosity during injection, while the high viscosity and mechanical properties are obtained after injection.

3 | APPLICATIONS

A series of hydrogel-based products have been approved for clinical use in the EU and the United States, particularly for viscosupplementation (VS) in joints for osteoarthritis (OA). Furthermore, regenerative gels are now emerging that in addition to providing temporary pain relief and functional improvement, attempt to regrow or support the regrowth of the tissue for a longer-lasting therapeutic

TABLE 1 Clinically available injectable hydrogel products for treatments of musculoskeletal indications

Indication and treatment mode	Product (manufacturer)	Composition	Delivery method	Therapeutic claim	CE/FDA approvals
Osteoarthritis					
VS	Gel-One ^{®61,62} (Zimmer Biomet)	Cinnamic acid functionalized HA crosslinked with UV light	Single 3 mL injection	Pain relief up to 26 weeks	FDA
	Orthovisc ^{®63} (Anika Therapeutics)	SHA (1.0–2.9 MDa) in saline water	Three separate injections of 30 mg in 2 mL solution	Pain relief up to 6 months	FDA
	Monovisc ^{®64} (Anika Therapeutics)	High MW HA, lightly crosslinked with biscarbodiimide	One 4 mL injection	6 months pain relief	FDA
	Hymovis ^{®65} (Fidia Farmaceutici)	HA 500–730 kDa, functionalized with 2–3% hexadecylamine	Two times 3 mL at a week interval	Lubrication and pain relief up to 12 months	FDA
	Arthroamid ^{®66,67} (Contura International)	2.5% polyacrylamide in sterile water—non-degradable	Single session injection of 6 × 1 mL through 21G cannula (syringes replaced using luer-lock system)	Long-lasting pain relief (52 weeks proven) ^a	CE & Clinical Trials (US)
Regeneration	BST-CarGel ^{®68,69} (Smith & Nephew)	Chitosan dissolved in saline water and autologous blood	Mini-arthrotomy or arthroscopy in combination with bone marrow stimulations such as microfracture	Superior hyaline cartilage regeneration compared to microfracture alone	CE
	RegenoGel ^{®70} (ProCore)	HA (1.6 MDa) conjugated to purified platelet-rich plasma-derived fibrinogen	Synovial fluid is first removed through a 21G needle, before 4 mL of gel is injected. Two administrations 3 months apart	Pain relief and cartilage regeneration	Clinical trials (EU and US)
Bone defects ^b	GelrinC ^{®71-73} (Regentis Biomat.)	PEGDA with denatured fibrinogen	Injected after microfracture, crosslinked using UVA light	Degrades over 6–12 months while being replaced by regenerated cartilage	Clinical trials (EU and US)
	DDD				
	Emdogain ^{®74,75} (Straumann)	Porcine EMD in propylene glycol alginate gel [30 mg/m]	Flap incision or flapless injection in dental application	Regenerates periodontal tissue (cementum, periodontal ligament, bone)	CE & FDA
	Perioglas ^{®76} (NovaBone)	Calcium phosphosilicate particles + a PEG and glycerine gel-like binder	Either as a moldable putty or through syringe injection	Dental bone regeneration	CE & FDA
	Actifuse ^{®77,78} (Baxter)	Phase-pure silicon-substituted calcium phosphate in poloxamer 407	Injectable through syringe	Bone void filler in spinal and orthopedic application	CE & FDA
	Dynagraft III ^{®79} (Integra)	DBM in poloxamer carrier	Injectable through syringe or delivered as a putty	Bone void filler	FDA
	AlphaGRAFT [®] (Alphatech)	DBM in poloxamer carrier	Extruded through syringe	Bone void filler	FDA
	AlloFuse ^{®79} (AlloSource)	29% allographic DBM in polyethylene oxide polypropylene oxide block copolymer	Mixed with autologous bone for spinal fusion or injected in trauma cases	Void filler, graft extender	FDA
	Optium ^{®79} (LifeNet Health)	Allographic DBM in glycerol	Allographic DBM in glycerol	Bone graft extender and void filler	FDA

(Continues)

TABLE 1 (Continued)

Indication and treatment mode	Product (manufacturer)	Composition	Delivery method	Therapeutic claim	CE/FDA approvals
	Grafton DBM [®] gel ^{80,81} (Medtronic)	Allographic DBM in glycerol	Mixed with autologous bone for spinal fusion or injected in trauma cases	Bone graft extender and void filler	FDA
	Tactoset [®] 82 (Anika Therapeutics)	HA carrier with calcium phosphate	The HA and CaP are mixed then injected. Hardens within 15–20 min	Bone void filler for orthopedic application	FDA
	Kinex [®] Bioactive Gel ⁸³ (Globus Medical)	Bioglass, collagen and HA	Injectable solution	Bone void filler	FDA
DDD					
Nucleus pulposus replacement	GelStix [®] 84 (Replication Med.)	Polyacrylonitrile	Injected through a 22G needle and swells in situ	Pain relief from 1 month after surgery for at least 12 months	CE
	HYADD4-G ^{85,86} (Fidia Farmaceutici)	HA 500–730 kDa, functionalized with 2%–3% hexadecylamine	1.5 mL [8 mg/mL] intradiscal injections guided by X-ray	Statistically significant pain relief up to 24 weeks	Clinical Trials
	BioDisc [®] 87,88 (CryoLife)	Albumin + glutaraldehyde hydrogel	Crosslink in situ within 2 min	Reduction in pain after 6 months	Unknown ^c
	NuCore [®] 89,90 (Spine Wave)	Block polymers of silk and elastin crosslinked in situ with diisocyanate	Injected with a sealed vented needle to recover disc height (0.3–1.9 mL)	Reduction in back and leg pain, regained disc height	Unknown ^c

Note: The list of products for viscosupplementation (VS) is non-exhaustive due to many products on the market. Instead, representative products for different materials and crosslinking mechanisms are presented. The other types of products are exhaustive to the authors' best knowledge.

Abbreviations: CaP, calcium phosphate; DBM, demineralized bone matrix; DDD, degenerative disc disease; EMD, enamel matrix derivatives; FDA, Food and Drug Administration; HA, hyaluronic acid; PBS, phosphate-buffered saline; SHA, sodium hyaluronate; VS, viscosupplementation.

^aClinical trial has a 5-year follow-up period.

^bBone defects = trauma, oncology, craniofacial.

^cSeems to be discontinued.

effect. In this section, we describe some of the leading clinical products for VS. In addition, we will discuss the products that have undergone clinical trials or been commercialized in the EU or the United States to regenerate bone, cartilage, or NP tissue. The products we will discuss are summarized in Table 1. We present their application indications, therapeutic effect, delivery method, and composition. Apart from VS, the list is exhaustive to the authors' best knowledge but might suffer from lack of data availability as many manufacturers choose to keep data on file rather than publishing their results. With the introduction of the European EUDAMED database, this is expected to change within the EU market. Bone putties (DBM/inorganic particles in hydrogel carrier) have been excluded for bone regeneration products unless they are marketed as injectable gels.

Many manufacturers have chosen to not publish their findings but keep their data privately on file. This applies to the products AphaGRAFT[®], Kinex[®], AlloFuse[®], and Tactoset[®], meaning we have limited information on these products which can limit our discussion of these solutions.

3.1 | Cartilage treatment

An exciting area where injectable hydrogels have become an established treatment is cartilage degeneration in joints. This is primarily indicated by OA, a disease-causing degeneration of the cartilage and the subchondral bone in the joints and affects roughly a third of people above 65 years,⁹¹ thereby having a high socioeconomic cost. In addition to degenerated cartilage and subchondral bone, synovitis and systemic inflammation are part of the pathogenesis.⁹² Patients with mild to moderate OA usually are treated with intra-

articular injection of corticosteroids, as it provides an anti-inflammatory effect.⁹³ However, corticosteroids are just capable of treating the symptoms, that is, reducing pain, but not able to stop the progress of OA.⁹⁴ Therefore, VS has become a popular treatment alternative as it provides a longer therapeutic effect.⁹⁵

For late-stage OA, arthroplasty is the preferred treatment, where the joint is partially or totally replaced with a prosthesis that is typically made of cobalt chrome or titanium alloys.⁹⁶ An alternative treatment is microfractures to release chondroprogenitor cells to the diseased location, but this tends to form fibrocartilage instead of desired hyaline cartilage.⁹⁷ The fibrocartilage has inferior mechanical properties than the native hyaline cartilage,⁹⁸ providing a temporary solution. Injectable hydrogels have become an attractive strategy for treatment in OA, both for delaying arthroplasty and attempting to regenerate the damaged cartilage toward more native-like cartilage than what can be achieved from microfracture. The two primary therapies, VS and regeneration, are illustrated in Figure 2.

3.1.1 | Viscosupplementation

There are multiple solutions based on HA injection into the knee for pain relief through VS (Table 1). There are two generations of VS products. The first generation consisted of HA solutions dissolved in an aqueous solution. The second generation consisted of crosslinked HA. To maintain injectability for the crosslinked gels, some of these are granulated HA gels chunks (typically less than 80 μm) that are mixed in an aqueous solution. This is for instance the case for Anika's Monovisc[®], as can be deduced from its patent.⁹⁹ The clinical efficacy of VS therapies is debated. In a more extensive meta-analysis including 89 trials with 12,677 patients involved, they could not observe

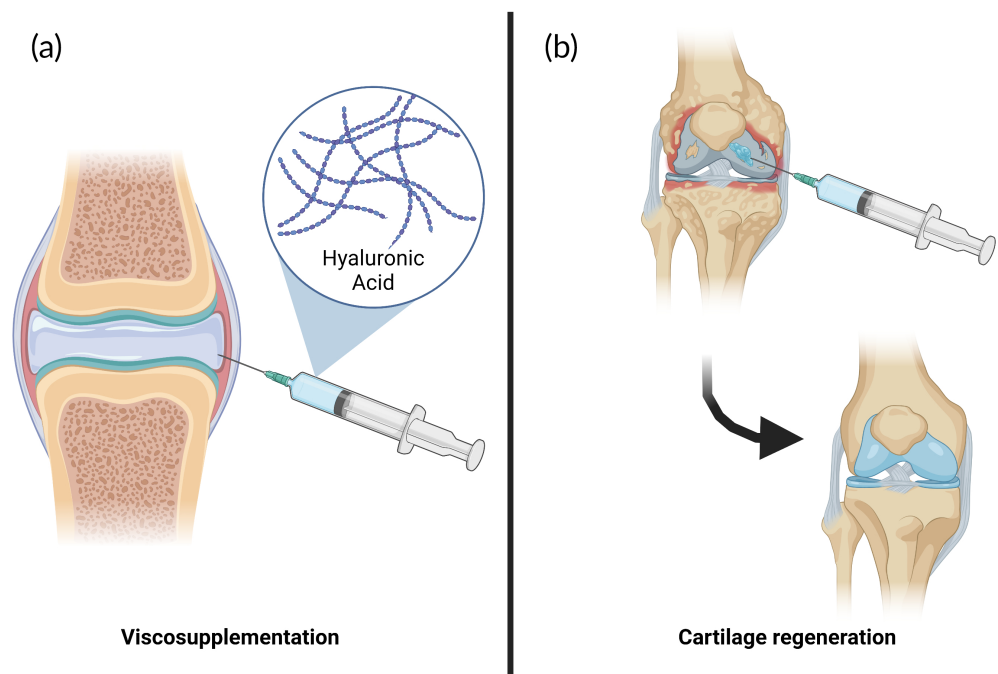


FIGURE 2 Treatment of cartilage defects caused by osteoarthritis. (a) Viscosupplementation using hyaluronic acid to obtain improved joint movement and pain relief. (b) Cartilage regeneration using injectable hydrogels

any clinically relevant benefit.¹⁰⁰ There were, however, indications that high molecular (>6000 kDa) or covalently crosslinked HA could provide a beneficial therapeutic effect.¹⁰⁰ In contrast, in another meta-analysis considering only FDA-approved VS in randomized, saline-controlled trials (29 studies; 4866 patients; active: 2673, control: 2193) they concluded that these products are safe and effective through 26 weeks in patients with symptomatic OA.¹⁰¹ Simultaneously, a consensus of eight European experts on OA discussed the clinical effect of HA in VS: they unanimously agreed that VS is an efficient strategy for managing mild to moderate knee OA, is a cost-efficient treatment in knee OA, but is not an alternative to surgery in advanced hip OA.¹⁰²

Although most of the solutions are based on HA, it is essential to consider the chemical composition and design of the gel. As mentioned before, high molecular weights and covalent crosslinking seem to be preferable. A higher molecular weight HA is believed to have improved residence time and adhesion to the cartilage providing more lasting lubrication under loading,¹⁰³ while a crosslinked HA gel would degrade slower than a non-crosslinked HA solution,¹⁰⁴ giving a longer therapeutic effect. For instance, for a lightly crosslinked VS such as Monovisc[®], one injection provides 6 months of therapeutic effect,⁶⁴ compared to three injections for a conventional non-crosslinked VS such as Orthovisc[®]. This gives significant indirect cost savings in the form of fewer hospitalization visits and reduced pain to the patient. More importantly, it can reduce the occurrence of more serious adverse events such as pseudoseptic reactions (inflammation and swelling of joint without infection, occurs in 1%–3% of patients) that typically occurs after second or third injection.¹⁰⁵

Recent clinical trials demonstrated that injection of HA has anti-inflammatory and antioxidative properties, which can decrease the progression of OA.¹⁰⁶ This effect seems to be mediated through receptor signaling via binding with cluster determinant 44, toll-like receptors 2 and 4, intercellular adhesion molecule I, and layilin, providing a multifactorial mechanism.¹⁰⁷ Additionally, there are indications that high molecular weight HA promotes an anti-inflammatory response, meanwhile, low molecular weight HA favors an inflammatory response.¹⁰⁷ Altogether, intra-articular injections of HA-based VS have demonstrated an effect, and there is still room to tune the hydrogel composition to obtain solutions providing better lubrication with enhanced therapeutic benefit.

A recent commercialization is VS made from polyacrylamide such as Contura's Arthrosemid[®]. Arthrosemid[®] is a gel consisting of covalently crosslinked polyacrylamide, which is non-degradable.⁶⁶ It was used initially for veterinary application in horses with OA,¹⁰⁸ but recently the therapeutic effect has been demonstrated to be functional up to 52 weeks in humans.⁶⁷ As the material is non-degradable, the therapeutic effect is expected to be significantly longer. An *in vivo* subcutaneous rat model comparing the acrylamide gel to a HA gel as soft tissue fillers suggested significantly different *in vivo* behavior. The acrylamide underwent cell infiltration by macrophages and fibroblasts and tissue integration, meanwhile, cell infiltration did not occur in the HA gel which was encapsulated by a thin fibrous layer.¹⁰⁹

The relevance of the model is limited as the study was conducted in a small animal with a subcutaneous application instead of intra-articular. However, the results may suggest that the clinical mechanisms of HA and acrylamide gels are different.

3.1.2 | Cartilage regeneration

Although VS, such as Monovisc[®] and Orthovisc[®], can typically provide pain relief for up to 6 months, they do not regenerate functional cartilage. This has led to an enormous focus on cartilage regeneration, and there is a series of products in clinical trials. They use different tactics for regeneration; conventionally, a microfracture procedure where bone marrow-derived MSCs are released into the defect site has been used for cartilage regeneration, but with considerable variability and inconsistency.¹¹⁰ Both the BST-CarGel[®] solution and the GelinC[®] build on this procedure by providing the released MSCs with a scaffold for guided cartilage regeneration. Their mechanism differs slightly. The BST-CarGel[®] consists of chitosan dissolved in aqueous glycerol phosphate (buffer at physiological pH), that when mixed with blood forms a clot with increased mechanical properties and longer stability.⁶⁸ The capability of chitosan as a hemostatic agent is derived from its poly(cationic) nature that allows it to bind with the negatively charged thrombocytes and erythrocytes in the blood.¹¹¹ A 5-year follow-up study for treatment of OA in the knee demonstrated significantly better cartilage regeneration with BST-CarGel[®] compared to microfracture alone,⁶⁹ and their animal trials suggest that the gel also regenerates cartilage with increased hyaline characteristics.¹¹² GelinC[®] on the other hand, is based on PEGDA mixed with denatured human fibrinogen and can be injected in liquid form but solidifies into a gel upon 90 s of UVA irradiation.⁷² It can be used for both chondral and osteochondral lesions and showed statistical improvement compared to the absence of treatment after 24-months follow-up.⁷¹ Their MRI data suggested a zonal variation in the cartilage, which they interpret as the cartilage might be hyaline-like rather than fibrous.

Although some indications, neither of the solutions has proven to produce native-like hyaline cartilage in humans. Part of the reason they cannot prove it is that one cannot take histology samples from living patients. Instead, they must use methods such as magnetic resonance imaging (MRI). Unfortunately, clinical MRIs tend to have a moderate resolution, limiting some of the quality of the data used in the analysis.

Although GelinC[®] and BST-CarGel[®] have shown short-term improvement, the success is governed by the long-term results, economic viability, and clear improvement from microfracture alone. Frappier and colleagues¹¹³ demonstrated this by evaluating the economic value of BST-CarGel[®] solution versus microfracture alone using Germany as a reference market. Their results suggest that a positive investment return is reached after 4 years and more than €6400 of cost saved over a 20-year period. Some essential limitations to this study are a lack of long-term clinical data for BST-CarGel[®] versus microfracture, and it only considers cost and not the quality of life of

the patient. Nevertheless, the data suggest that it is clinically feasible to use these different solutions along with microfracture. This should motivate other research to develop new solutions with improved efficacy and at lower costs. A key challenge the field should address is successfully regenerating native-like hyaline cartilage and developing non-invasive methods that can aid in its characterization *in vivo*. Most likely some type of agents, such as microfibers or a biomolecule, is required to guide the direction of the tissue regrowth. Furthermore, regrowth should preferably follow the zonal tissue architecture that can be observed in the native articulate cartilage.^{114,115} Ideally, the cartilage should recruit chondrocytes or MSCs without the need for autologous chondrocyte transplantation or microfracture, but there are currently no such solutions to the authors' best knowledge. At the time of this review, microfracture procedures are estimated to cost €4329 and autologous chondrocyte implantation €14,238.¹¹⁶ On top of this comes the cost of the hydrogel used. Hydrogel scaffolds that can induce regeneration using only locally recruited chondrocytes can provide considerable cost savings through reduced surgery times and trauma to the patients.

Another trend that starts to arise is VS-like products with additional regenerative capabilities. An example of this is ProCore's RegenoGel[®] solution that was commercially approved in Israel in 2016 and recently completed their FDA phase 4 clinical trials. RegenoGel[®] is based on HA that is mixed with purified platelet-rich plasma-derived fibrinogen that conjugates to form an injectable gel.⁷⁰ In their clinical trials, they have been able to demonstrate that the gel is efficient at treating the symptoms of OA, that is, pain and knee stiffness, for at least 6 months after treatment start,⁷⁰ but more detailed studies are required to investigate the long-term effect and the ability to regenerate cartilage. Nevertheless, their *in vivo* cartilage-bone explant mouse model suggests that the material recruits endogenous cells and differentiates them toward a chondrocyte lineage, yielding significant deposition of GAG-proteins and collagen type 2.¹¹⁷ Although promising for cartilage regeneration, they have yet to demonstrate cartilage regeneration in humans.

3.2 | Bone regeneration

Healthy bone is vital for structural stability in the musculoskeletal system, and defects result in pain, disability, and reduced mobility in individuals. Additionally, the treatment of bone defects is a tremendous burden to healthcare providers, estimating an annual cost of \$5 billion in the United States alone.¹¹⁸ Even though bone defects are rarely directly mortal, the trauma-induced can be hard to recover from. If we consider the case of hip fractures, for elder women (>65 years) there is a 10% likelihood of mortality within 3 months of a hip fracture.¹¹⁹ Similarly, a larger meta-analysis demonstrated that the risk of mortality is increased by a 6- and 8-fold the first 3 months after hip fracture for older women and men (>50 years), respectively.¹²⁰ Nor are there any good treatment alternatives in these cases. In fact, another meta-analysis demonstrated that the mortality rate 1 year after hip fracture surgery is 24.5%,¹²¹ suggesting two scenarios: (1) the current medical

devices do not have an appropriate therapeutic effect for the elderly population, or (2) the current surgical procedure's invasiveness leads to a challenging recovery for elderly patients.

Bone defects can be widely different, and the products used depend on defect size and loading level.¹²² Therefore, this section has been split into three subsections: (1) dental and maxillofacial, (2) trauma and oncology, and (3) spinal fusion. We treat spinal fusion as a separate application as it is the largest application area of bone grafts measured according to market value¹²³ and compared with the dental and traumatic and oncologic applications, this is a form of heterotopic ossification. Hydrogels for bone regeneration has been illustrated for two indications in Figure 3.

3.2.1 | Dental and maxillofacial

Straumann's Emdogain[®] dominates the dental market and has more than 20 years of clinical documentation.¹²⁴ Emdogain[®] is based on a porcine enamel matrix derivative, a cocktail of proteins consisting of amelogenin (90%) and a few other nanamelogenin such as ameloblastin, enamelin, and tuftelin, carried in an aqueous gel solution composed of propylene glycol alginate.³⁹ Several of these proteins are identified as intrinsically disordered polypeptides with a one-to-many signaling effects *in vivo* and allow for the formation of multiple tissues in the injection location.¹²⁵ Emdogain[®] has been proven to regenerate multiple periodontal tissues, including the osseo-like tissues, acellular cementum,¹²⁶ and alveolar bone,¹²⁷ in addition to connective tissues such as periodontal ligament.¹²⁸ The details of the therapeutic effect of Emdogain[®] have been discussed in detail in our former review.³⁹ A limitation worth noting with Emdogain[®] is that since it is physically crosslinked, the degradation occurs quicker than it would with a covalently crosslinked hydrogel. The consequence of this is that the mechanical properties degrade quickly, and it can no longer keep the soft tissue flap up, causing a collapse of the gel and limiting the space available for bone regeneration.¹²⁹

Another product that is well established in the dental domain is NovaBone's Perioglas[®] putty. Initially, it was commercialized as a moldable putty, but a syringe and a cartridge injection system have since been developed. The gel-like putty consists of calcium sodium phosphosilicate, more specifically Bioglass[®] 45S5 particles of 32–710 μm diameter, delivered through a gel-like binder of PEG.⁷⁶ The binder is water-soluble and is resorbed within 48–72 h after implantation,⁷⁶ hence it is the Bioglass[®] that has the main therapeutic effect. According to Jones,¹³⁰ the Bioglass[®] draws its bioactivity from two mechanisms: (1) the accumulation of glass dissolution products provides nucleation sites for a hydroxycarbonate apatite layer that bonds to the surrounding bone. This layer also allows the protein to attach and cells to attach, proliferate and produce ECM; (2) the release of dissolution products also plays an active role in driving osteogenesis through guiding osteoprogenitor cells down an osteoblastic differentiation path, and the osteoblasts are transitioned from a resting stage (G0) to a growth stage (G1). There are, however, concerns regarding inflammatory foreign body reaction

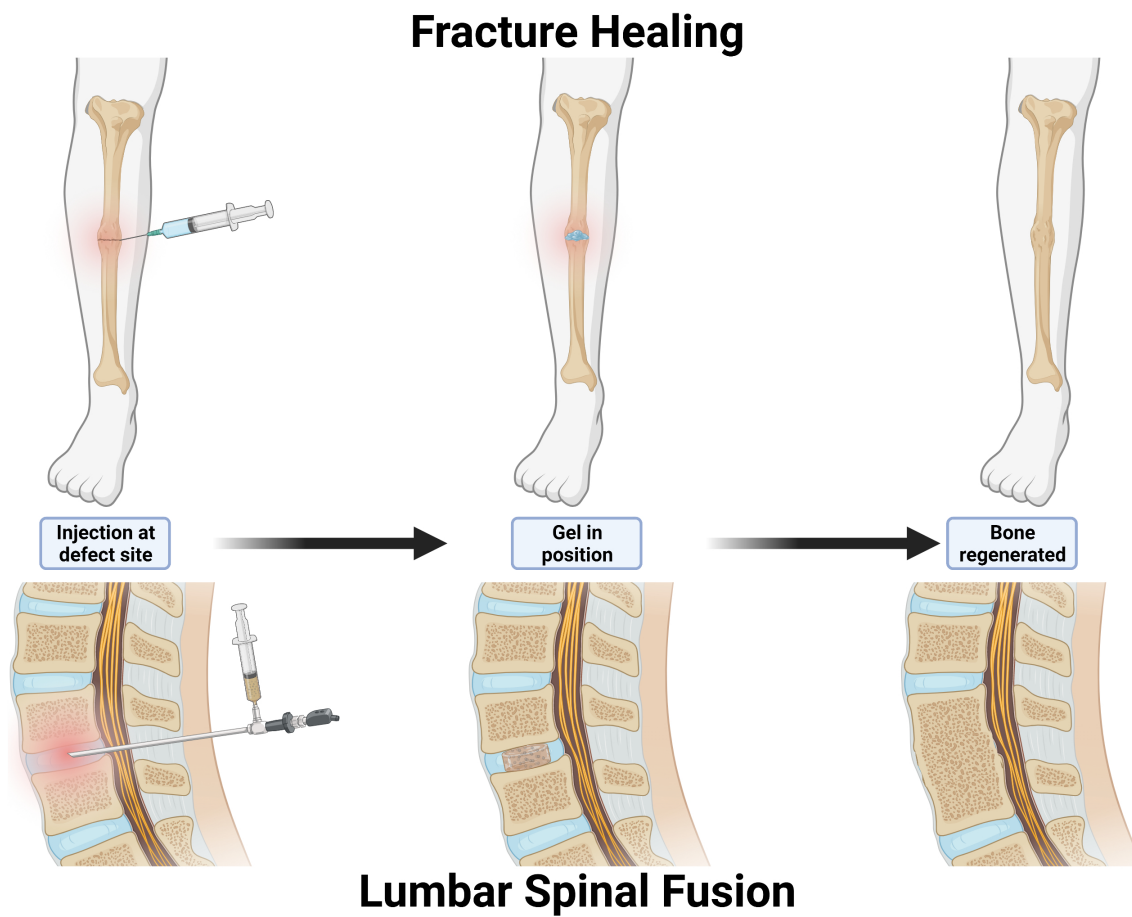


FIGURE 3 Illustration of hydrogel application for bone regeneration. Top panel: fracture healing in traumatology using a needle-injected hydrogel. Bottom panel: spinal fusion using arthroscopic injection of a ceramic particle loaded hydrogel

around the bioglass particles that might limit the clinical success of the putty.¹³¹

3.2.2 | Orthopedics: Trauma and oncology

An approved product for orthopedics is the Baxter Actifuse[®] Flow. It consists of silicon substituted calcium phosphate particles of size 90–500 μm carried in an aqueous polymer carrier consisting of poloxamer 407 (P407).^{77,78} The P407 is a triblock polymer with a hydrophobic polypropylene glycol core and hydrophilic PEG side arms, that goes through a thermoreversible gelation mechanism, meaning that the solution gels above a given temperature.¹³² The temperature for which the sol–gel transition occurs decreases with the P407 concentration, and it has been demonstrated that for a concentration of 16.5% (wt.% in purified water) the solution gels at a temperature of 27.1°C.¹³³ It can be speculated that the Actifuse[®] Flow carrier has a P407 concentration of 16.5 wt.% or lower, meaning that it will be liquid at room temperature while at physiological temperatures it would form a gel. The solution has successfully treated benign bone defects in the pediatric population.¹³⁴ A series of similar solutions has been made combining demineralized bone matrix (DBM) particles in similar

reverse-phase medium-based hydrogels. This includes both Dynagraft[®] III and AlphaGRAFT[®] that combines DBM particles with poloxamer gel, meanwhile, AlloFuse[®] combines DBM particles in a carrier of polyethylene oxide polypropylene oxide block copolymer. Optium[®] and Grafton[®] DBM uses glycol as a carrier. Unfortunately, with the exception of Medtronic with their Grafton[®] product, these manufacturers have chosen to keep their data on file so the products cannot be discussed directly. In general terms, DBM is an attractive biomaterial as the acid-extraction process allows the retention of growth factors such as bone morphogenic proteins (BMPs), yielding osteoinductive properties, but it is a challenge for manufacturers to sterilize DBMs without inactivating these growth factors.¹³⁵ Due to the risk of immunoreactions and transmission of infections, the use of DBM and other allograft products is regulatorily unfavorable in Europe, and with the new MDR, it is expected to be limited further.¹³⁶

A more recent solution is Anika's Tactoset[®] solution where calcium phosphate particles and HA are mixed into a hardening, injectable gel solution.⁸² Currently, it has only been published as a technical note with limited information on the composition and therapeutic effect. A similar solution is Globus Medical's Kinex[®] composed of bioglass and collagen in a HA gel.⁸³ However, the manufacturer has

chosen to keep their data on file; hence no research is published on this solution.

3.2.3 | Orthopedics: Spinal fusion

Spinal fusion is a common surgery requiring bone-growing implants, with approximately 200,000 lumbar spinal fusions conducted in 2015 in the United States alone.¹³⁷ Spinal fusion is performed to compensate for degenerative disc disease (DDD) where the height of intervertebral disc (IVD) has reduced leading to the compression of the spinal cord, which translates to back pain. Degenerative disc, the first step toward DDD, affects more than 90% of people above 50 years.¹³⁸ When the degeneration progresses, spinal fusion is an attractive surgery for pain mitigation and preventing damage to the spinal cord. The surgery typically consists of a cage being inserted to mechanically regain the spacing between the vertebrae, then bone grafts are used to stimulate bone growth to fuse together the adjacent vertebrae. Conventionally an open surgery is used, but there is now a trend to use minimally invasive procedures (MIP) such as key-hole surgery.¹³⁹ MIP can be incompatible with conventional bone grafts due to large size or high viscosity; hence this trend favors injectable solutions such as hydrogels. Moreover, MIP spinal fusion requires less bone to be removed for access to the IVD, which means less

autologous bone available as graft material, increasing the demand for alternative grafting materials. Between 9% and 39% of lumbar spinal fusions fail,¹⁴⁰ indicating a need for more potent bone regrowth solutions. Spinal fusion requires heterotopic ossification, meaning bone tissue growth in soft-tissue locations where bone is usually not present. This makes it a challenging task, and a graft only exhibiting osteoconductive properties is suboptimal. Ideally, for treatment of large defects and for heterotopic ossification the graft should be osteoinductive, a phenomenon induced when the material creates a local homeostatic imbalance by binding to calcium and/or phosphate ions, causing depletion of these ions.^{141,142} Hence, an osteoinductive material is likely to quickly induce a stable fusion than a graft that is just osteoconductive. This has motivated many to introduce BMP in their graft products, for example, Medtronic uses rhBMP-2 in their Infuse® (US)/Induct® (EU) bone graft. However, according to the European regulation, the BMP makes it considered a medicinal product. Furthermore, the use of rhBMP-2 in this product has been linked to several adverse events where the high doses of the growth factor, mainly when used for “off-label” cervical spinal surgeries, causes an inflammatory effect yielding high complication rates.¹⁴³ A similar BMP-7 based product named OP-1® from Stryker has failed to obtain FDA approval for similar spinal applications. However, effective hydrogel therapies are emerging that do not depend on BMP-based growth factors to obtain their therapeutic effect. The before mentioned

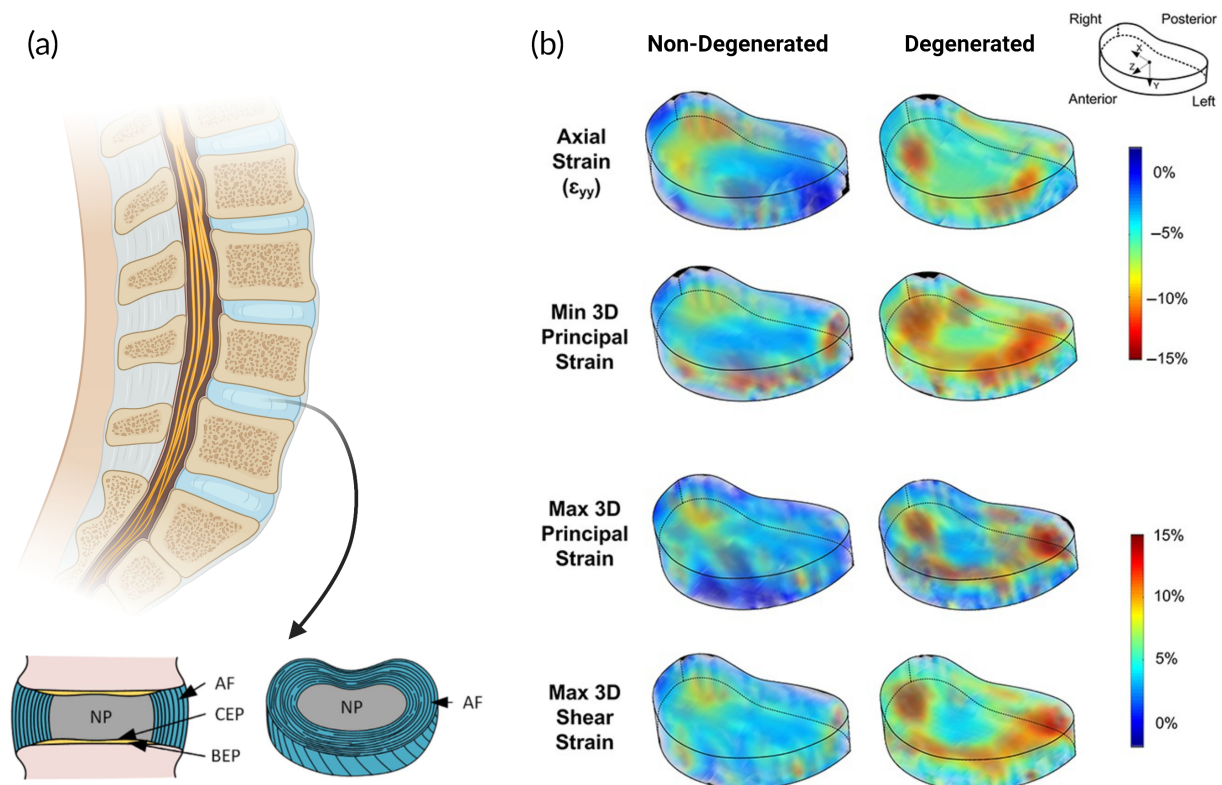


FIGURE 4 (a) Illustration of the intervertebral disc. (b) Strain and stress levels in non-degenerated and degenerated intervertebral discs demonstrating how the degenerated disc is prone to higher stress levels, particularly around the AF region. Reproduced and adapted from 137, 138. Reprinted with permission from copyright CC BY 4.0. AF, annulus fibrosus; BEP, bony endplate; CEP, cartilaginous endplate; NP, nucleus pulposus

Baxter Actifuse[®] Flow has successfully been used for spinal fusion procedure.¹⁴⁴ When used in a comparative clinical study to the Medtronic Infuse[®] graft, they were able to demonstrate similar fusion rates (Actifuse[®] 9/9, Infuse[®] 8/9 cases) and both products yielded similar alleviation of pain and improved quality of life.¹⁴⁵ Also, DBM solutions have been approved clinically for spinal application. The Grafton[®] DBM was tested in a clinical trial with a total of 120 patients undergoing posterolateral spinal fusion, of which 81 (70%) completed the 24-month radiographic study.⁸⁰ Grafton[®] was used on one side of the spine and autograft on the other, and in 42 (52%) of the Grafton[®] cases, successful fusion was obtained versus 44 (54%) for the autograft side. The authors concluded that the Grafton[®] DBM gel can be used to extend autograft material during spinal fusion.

3.3 | Nucleus pulposus

Spinal fusion tends to be conducted due to DDD, where the IVD has degraded and lost its height or fractured. The IVD is found between all the vertebrae of the spine. It has three main components; the hydrogel-like NP in the core, surrounded by the annulus fibrosus (AF), and cartilaginous end plates (CEP) at the top and bottom (Figure 4a).¹⁴⁶

The NP consists of approximately 50% (dry weight) proteoglycan proteins that play a vital role in binding water in the NP and shock absorbance.¹⁴⁷ During disc degradation, the concentration of proteoglycans decreases, causing a drop in stiffness.¹⁴⁶ This increases the risk of AF bulging, increases the compressive strain on the AF (Figure 4b), and increases the chances of peripheral failure of the end plates.¹⁴⁸ Therefore, a potential treatment of DDD would be to repair the NP.

A solution that has been approved for the European market is GelStix[®]. GelStix[®] uses a dehydrated polyacrylonitrile that is injected into the NP through a 22-G needle in the form of a filament, where it gets hydrated from the surrounding body liquids and expands 10-fold.⁸⁴ In a 12-month follow-up with 29 patients, 86.2% rated the procedure as very good or good, and pain relief was observed already after 1 month.⁸⁴ However, there have been reported complications associated with this procedure. Durdag and colleagues reoperated a woman with a GelStix[®] implanted as she was admitted with severe radicular pain.¹⁴⁹ The pain was linked to a fragment of implant that had penetrated through an annular tear and caused compression to the spinal root. The authors speculate that the implant may have been initially wrongly placed in the AF, highlighting the importance of the correct placement of the implant.

HA with a similar composition to the solutions used for VS has been used for treatment of the NP. In a 24-week follow-up period, Mazza and co-workers observed relief from chronic lower back pain due to DDD compared to the baseline.⁸⁵ They had two patients drop out due to adverse events, but this is not believed to be related to the treatment. However, the clinical efficacy is proven only over a short time period. Considering the surgical risk related to bypassing vital organs during injection, this therapy can come short when evaluating

it using a cost-benefit analysis. Hence a longer-lasting therapy should be investigated.

Two other solutions have been tried clinically, but seem to have been discontinued. The NuCore[®] gel for NP replacement consists of elastin and silk co-polymers that are crosslinked in situ.⁸⁹ A 2-year follow-up pilot clinical study with 14 patients demonstrated a significant reduction in back and leg pain, regained disc height, and no side effects.⁸⁹ There have not been any clinical publications on this product since 2009, and it seems to have been discontinued by the supplier. CryoLife started clinical trials on their product BioDisc but have not published the outcome of the trial. In a conference abstract containing interim results, they reported at the 6-month follow-up a decrease in mean Oswestry Disability index from 49.2 to 11 and a decrease in numerical pain score from 5.86 to 1.62,⁸⁸ which could seem promising. However, they also reported that 2 of the 10 patients enrolled experienced recurrent herniation requiring surgery. After this abstract from 2008, there has been no publication, and the product seems to have been discontinued.

Since neither CryoLife nor Spine Wave has disclosed why their products were discontinued, it is not feasible to conclude why they failed to perform in the clinic.

4 | REGULATORY CLASSIFICATION AND CONSEQUENCES

From a regulatory perspective, the first step of translating a medical device is to assign it to the appropriate risk classification group, namely risk class. In Europe with the new MDR, this is reasonably straightforward with injectable hydrogels. Because they are implanted, hence in contact with human tissue over a prolonged period and have a biological effect, it becomes a class III device (highest risk level). This means a premarket clinical investigation is mandatory. This can be mitigated if equivalence to a predicate device can be demonstrated. Nevertheless, appropriate equivalence is practically infeasible unless the manufacturer of the new device either (a) also manufactures the predicate device or (b) has a contractual agreement with the manufacturer of the predicate to access all technical information. In the United States, the risk classification differs from Europe as it depends on product device groups. VS products or dental biologics (e.g., Emdogain[®]) are class III (highest risk), meanwhile more conventional bone graft materials without human growth factors such as Anika's Tactoset[®] or the DBM solutions are class II. For class II and some class III product groups the 510(k)-pathway can be used if it demonstrates substantial equivalence with existing approved devices, demonstrating that the device is safe and efficient, which is significantly cheaper than introducing a new device. In the case of class III, the 510(k) allows the manufacturer to partially bypass the premarket approval application, meaning they do not need to run a clinical investigation, but this is not applicable for the VS products or dental biological materials discussed here. When the 510(k) is not applicable for the class III devices, the product needs to be evaluated on a case-by-case basis by the authorities (US-FDA).

TABLE 2 List of hydrogel solutions for musculoskeletal therapies regulated as medicinal products

Indication and treatment mode	Product (producer)	Composition	Delivery method	Therapeutic claim	FDA approvals
Osteoarthritis					
Cartilage regeneration	NovoCart Inject ^{150,151} (Tetec AG)	Maleimide functionalized human albumin and HA crosslinked with bishio-PEG, and autologous chondrocytes	Arthroscopic injectable autologous chondrocyte transplant	Needle injection through two-chamber solution allowing in situ polymerization	FDA phase III trials
DDD					
Nucleus pulposus replacement	NovoCart Disc ^{152,153} (Tetec AG)	As above	As above	As above	FDA phase II trials

Abbreviations: DDD, degenerative disc disease; FDA, Food and Drug Administration; HA, hyaluronic acid; PEG, polyethylene glycol.

In the review, we have focused on discussing hydrogels as medical devices. However, they can also be classified as medicinal products if their main mechanism of action is through pharmacological, metabolic, or immunological means⁶; this would lead them to the so-called “drug approval process.” A couple of hydrogels that are used for the above-described musculoskeletal treatments are classified by the European Medical Agency and the FDA as medicinal products (biologics/drugs) instead of medical devices as they have the characteristics of combinatory products, Advanced Therapy Medicinal Products (ATMP). A summary of these can be found in Table 2.

Over the last couple of decades, there has been a drastic change in the design rationale of orthopedic biomaterials. From passive structures designed for minimal interaction with the surrounding tissue, for example, titanium-based hip implants, the current generation of biomaterials is designed to actively interact with the surrounding tissue, such as scaffolds for tissue regeneration that stimulates tissue growth. This means that the product's mechanism of action starts approaching that of medicinal products, which will change the applicable regulation framework.¹⁵⁴ Hence engineers need to carefully consider regulatory classification when designing hydrogels. If a hydrogel solution is classified as a medicinal product, it increases the documentation and overall market entry requirement and requires larger and more costly clinical trials. Compared to medical devices, the therapy will take significantly longer time for clinical translation, the R&D investment costs will increase drastically, and the product will eventually be sold at a higher price to the healthcare providers. Moreover, there will be longer product cycles, which means less innovation. In the United States, it takes on average 12 years from pre-clinical trials to market approval for drugs while it only takes 3–7 years for medical devices, and the development costs will increase from the range of tens of millions of dollars for medical devices up to the excess of \$1 billion for pure drugs.^{155,156}

Products where a medical device (i.e., the gel) carries a therapeutic agent such as growth factor or expanded cells no longer gets its primary mode of action through physical means, and the classification changes to medicinal products. For example, Tetec AG (Germany) has developed two such products for cartilage treatment (NovoCart Inject[®]) and IVD regeneration (NovoCart Disc[®]). The NovoCart[®] gel

functions as an autologous chondrocyte carrier and is used in a 2-step surgical procedure, hence is regulated after the complex ATMP framework. In the first step, the chondrocytes are harvested and expanded in GMP facilities. In the second step, the cells are added to a liquid consisting of human albumin and HA. During the injection procedure, the cell/polymer mixture is mixed with a bishio-PEG crosslinker which causes the crosslinking of the gel in situ through a Michael-type addition reaction between the thiol groups of the PEG and the maleimide groups of the functionalized human albumin.¹⁵⁷ In a short-term follow-up (12 months) for cartilage regeneration, they could observe a reduction in pain, an increase in activity and quality of life among the patients.¹⁵⁰ In a smaller 24-months study, they demonstrated clinically favorable outcome in terms of reduced pain and a MOCART 2.0 score of 70 ± 13.6 , suggesting cartilage regrowth with morphological integrity.¹⁵¹ The MOCART 2.0 scoring system uses MRI to quantify the quality of cartilage repair tissue by giving it a score between 0 (worst) to 100 (best).¹⁵⁸ The Novocart[®] inject solution has also been tried clinically for NP regeneration. So far, the phase I part of the joint I/II trials have not raised any concerns about the safety of the product.¹⁵²

5 | FROM LAB TO CLINIC AND EMERGENCE OF POST-MARKET SURVEILLANCE

Translating hydrogels as medical devices is a time-consuming process, and care should be taken to have a clear plan from design to pre-clinical and clinical investigation. The steps from hydrogel development to clinical approval and post-market surveillance have been illustrated in Figure 5. First, the hydrogel needs to be developed; the details of this process have been described above. A thorough material characterization is mandatory for scientific and clinical perspectives and is also useful when explaining the mechanism of action to the notifying body or the US-FDA. Thereafter, it is mandatory to demonstrate biocompatibility according to the applicable ISO 10993 standards, where the manufacturer must justify which are applicable and which are not. A natural sequence for hydrogels for musculoskeletal

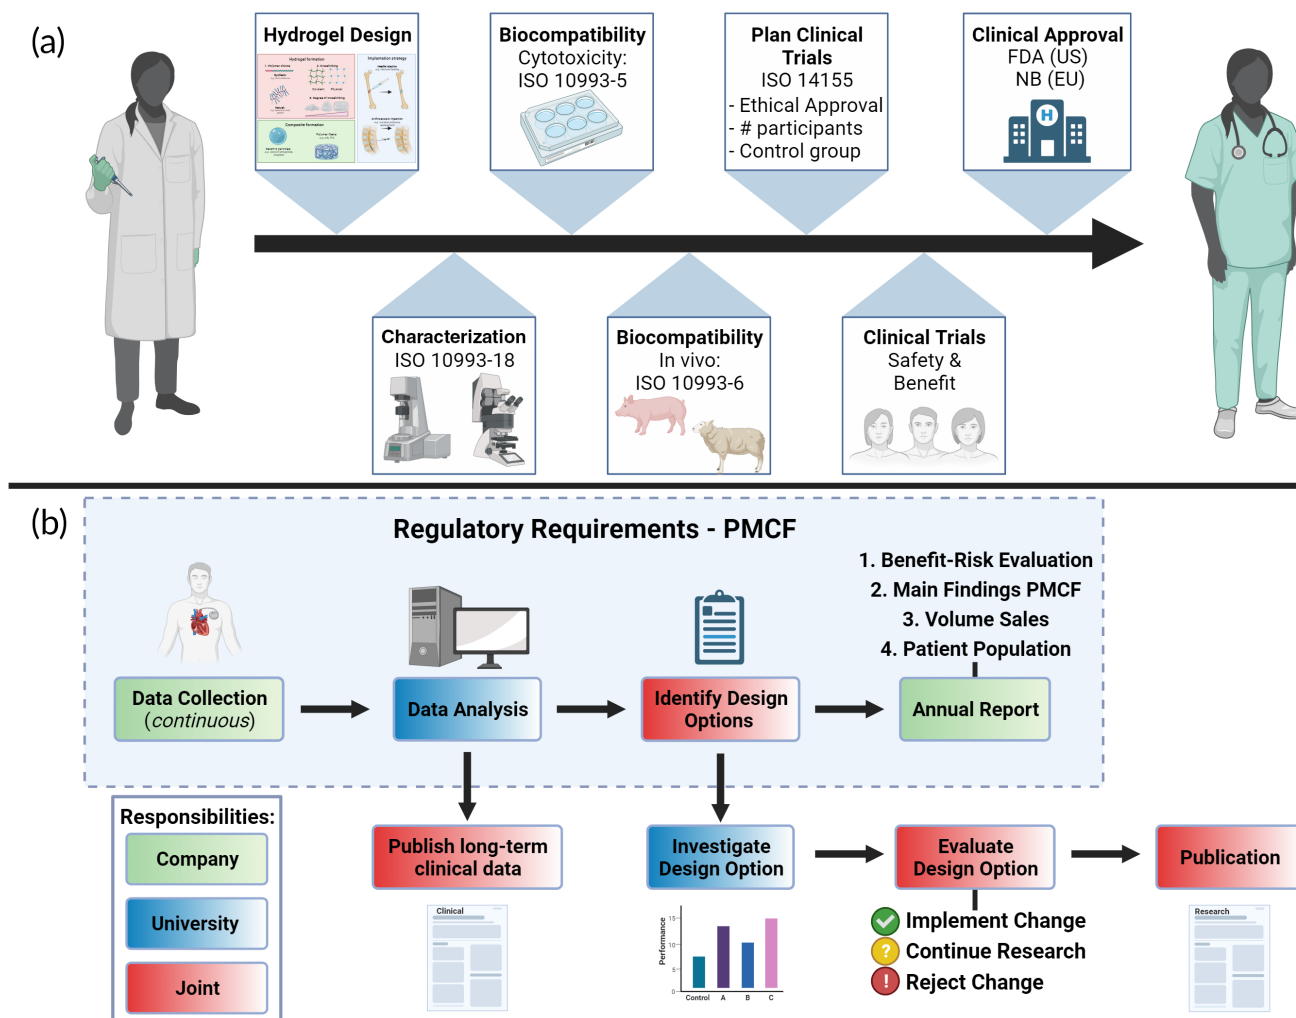


FIGURE 5 (a) Schematic illustrating the main stages involved in the clinical translation of injectable hydrogels. (b) Suggested framework for industrial-academic collaboration on post-market clinical follow-up (PMCF) in accordance with the requirement of the EU MDR 2017/745 regulations for Class III (high-risk) medical devices such as hydrogels. The responsibility division is not resolute, with the expectation of the data collection and the annual report, and should be delegated on a case-to-case basis. FDA, US Food and Drug Administration; ISO, International Organization for Standardization; NB, notifying body

application (implantable with long-term tissue contact) is first characterizing the material's chemical properties according to ISO 10993-18:2020, then in vitro cytotoxicity according to ISO 10993-5:2009, and finally pre-clinical trials according to the ISO 10993-6:2016 where both the local and systematic response should be evaluated in a reliable animal model. If these are followed diligently and the animal model is well designed, it should cover most of the documentation requirements of the regulatory body, and most of the other ISO 10993 standards can be considered non-applicable. However, a justification for this must be given in the device's risk management file.

Before the pre-clinical trials, it is important to have a clear idea of the clinical claims that shall be demonstrated in the animal model stage. Indeed, in pre-clinical trials, selecting an animal and implantation site that represents the clinical pathophysiology and loading is essential. This has been discussed in detail for injectable bone

substitutes by Bongio and colleagues.¹⁵⁹ If the pre-clinical trials are successful, it is necessary to go through clinical trials. Since hydrogels tend to be short-term (>60 min contact with tissue) or long-term implants (>30 days contact with tissue) with a biological effect, they will be classified as high-risk (class III) medical devices according to the EU MDR¹⁶⁰ and require thorough documentation on safety and efficacy. The new EU MDR requires a more comprehensive clinical evaluation than the former regulation, focusing on both direct clinical investigation and literature/market analysis. The specific requirements have been discussed from a notifying body's perspective by Holborow.¹⁶¹ It is worth noting that the new regulations require the clinical investigation to have a representative patient group to the EU population, the participation number must be demonstrated statistically to be large enough to be appropriate for demonstrating safety and performance, and the length and follow-up intervals must give a good picture of the lifetime of the

device.¹⁶² This means that it is technically enough to conduct one clinical trial to get CE approval, but it must be large enough to be exhaustively representative. It is also a requirement that the clinical trials must strictly follow Good Clinical Practice (GCP) guidelines and ISO 14155:2020; hence they must be approved by an ethical committee set up according to national law in the EU member state where the clinical trials are conducted.¹⁶²

The clinical trials for medical devices differ from medicinal products, where there are distinct phases in the clinical trials. The typical set of clinical trials for drugs consists of phase I where safety is demonstrated on a small number of healthy participants, phase II where efficacy is demonstrated on a moderate number of participants, and phase III where efficacy is demonstrated on a larger number of participants. The phase III trial, which ideally is double-blind and randomized, can involve up to thousands of participants lasting months or years.¹⁶³ This might not be feasible or ethical for medical devices. For example, although saline solution as a control for VS is standard procedure, a sham control for an orthopedic bone graft could do significant damage to the patient and thereby be unethical. For these risk cases, using the current treatment alternative as a positive control could be a good alternative, such as autografts as a control for bone graft substitutes. This allows the manufacturers to benchmark their technology, and it is easier to demonstrate its clinical claims and the value provided to patients and healthcare providers. Since clinical trials directly affect the patient's health, patient safety and ethical standards should be central in clinical trials to reassure a high-quality standard. The Declaration of Helsinki is an excellent guideline for meeting the ethical standards, together with GCP and ISO 14155:2020.

Notably, the new EU MDR requires a post-market surveillance register for medical devices (EUDAMED). This is inspired by the successful implementation of orthopedic device registries and the quality of the data these have provided.⁴ With this registry, the regulation requires continuous data gathering and analysis. More specifically the MDR article 83 states¹⁶²: “*The post-market surveillance system shall be suited to actively and systematically gathering, recording and analysing relevant data on the quality, performance and safety of a device throughout its entire lifetime, and to drawing the necessary conclusions and to determining, implementing and monitoring any preventive and corrective actions.*” The medical device industry is characterized by a lot of small, niche suppliers. In Europe, out of 33,000 medical technology companies, 95% are small or medium enterprises (<250 employees), and a majority are small or micro-sized companies (<50 employees).¹⁶⁴ The limited manpower makes it challenging for these companies to designate and dedicate personnel for the post-market clinical follow-up. This provides a golden opportunity for academic researchers to collaborate with these companies to analyze the clinical data, and academics can use their understanding of fundamental biological and clinical mechanisms to explain the collected observations, for example, evaluating porcine versus bovine gelatin in the bone graft SmartBone.¹⁶⁵ If the data are published, it will indeed help the wider research community. Meanwhile, the companies will benefit from this as they can leverage experienced personnel to analyze and explain complex data.

6 | CONCLUDING REMARK AND FUTURE DIRECTION

There is a tremendous discrepancy between the intensity of academic research on hydrogels and the number of products that have been clinically translated for the treatment of musculoskeletal defects. When developing hydrogels, it is crucial to consider the clinical potential of the material, and here pre-clinical and clinical trials are key in predicting whether a material candidate will make it past the evaluation of the regulatory body and succeed clinically. On top of that, practical factors such as the cost of the product, scalability, and ease of use in the clinic should be considered at an early point, together with quality assurance and regulatory affairs matters. As demonstrated in this review, the clinically available materials tend to have extensive clinical documentation, but the understanding and documentation of the hydrogel composition tend to be limited. Concurrently, materials that are intensely investigated in academia and have been thoroughly characterized physiochemically and in vitro are not the ones that have made it to the clinic. When searching “GelMA” on PubMed, it yields 701 articles from the last 11 years. Of these, none are clinical trials. The fact that GelMA has not made it to the clinic is likely a consequence that regulatory bodies are primarily concerned about the material's clinical history. Hence, materials that have made it to the clinic before increased documentation requirements are favorable to use in new implants. Meanwhile, new biomaterials are now expensive and scientifically challenging to translate. It can also indicate that academic research environments need to invest more resources to mature the technology through in vitro, pre-clinical and clinical trials. Particularly, a comprehensive characterization of physiochemical properties, in vitro testing, and use of advanced characterization in animal trials will be helpful for industry, both because it helps them understand the potential of the biomaterial and because it can assist in explaining a device's mechanism of action. A complete understanding of a device's mechanism of action is essential for approval under the new MDR. To increase the likelihood of industrial adoption academics should also demonstrate that any new therapeutic agents can withstand appropriate manufacturing, for instance how an osteoinductive peptide can withstand manufacturing processes with DCM and other solvents,^{166,167} and sterilization processes (e.g., autoclaving, gamma/beta-irradiation [typically 25 kGy], ethylene oxide) without compromising its efficacy. Additionally, verify that the clinical effect and sterility can be maintained with storage over an extended time period in accordance with ISO 11737-2:2020.

In vitro testing is very important for understanding isolated mechanisms. However, in our experience¹⁶⁷⁻¹⁶⁹ there are major differences in response to biomaterials during in vitro tests, where single cell types are used, and in vivo, where there is an assortment of cell types interacting.^{33,170} Although there is progress in technology such as organ-on-chip^{171,172} or co-cultures,¹⁷³ they are yet not capable of mimicking the complexity of tissue response to biomaterials. Simultaneously, animal trials should be kept to a minimum for ethical and economic reasons. To obtain adequate documentation and keep animal trials to a minimum, care should be taken in acquiring high quality

in vivo data. The ISO 10993-6 (*Test for local effect after implantation*) requires only local microscopic assessment using histology. Using only this method gives an incomplete picture as conventional histology does not give spatial information or confirm certain biomarkers.¹⁷⁴ Hence, utilizing additional methods such as cone beam computed tomography,¹⁶⁷ microCT (μ CT),¹⁶⁷ immunohistochemistry,^{167,175–177} small-angle X-ray scattering,^{167,178} X-Ray diffraction analysis,^{167,178} and more newly developed techniques such as fluorescent labeling of abundant reactive entities,¹⁶⁷ optical photothermal infrared microscopy,¹⁶⁷ and nanoscale atomic force microscopy-infrared¹⁶⁷ can give a comprehensive understanding of the material's mechanism of action. Furthermore, there has been an increased focus on the use of intravital microscopy such as fluorescence lifetime imaging microscopy and Raman spectroscopy as their subcellular resolution (approx. 500 nm) allows for studying in detail in vivo host response to implants and for monitoring of implant biology over time in small animal models.³⁰ If academics bring their material candidates all the way through animal trials and conduct thorough in vivo characterization, it will assist industrial R&D engineers in making an educated choice of biomaterials in their medical device design. Realizing funding limits related to translational research will require the industry to support the financing of these research activities in active collaborations.

ACKNOWLEDGMENTS

ØØ and HJH were funded by the Research Council Norway through grant no. 327512. ØØ acknowledges additional funding from the Aker Scholarship. JPW and MMS were funded by the grant from the UK Regenerative Medicine Platform “Acellular/Smart Materials–3D Architecture” (MR/R015651/1). CE received funding from the European Union's Horizon 2020 research and innovation program under the Marie Skłodowska-Curie grant agreement no. 801133. All figures were created with BioRender.com.

CONFLICT OF INTEREST

M.M.S. is co-inventor on patent application 1911235.8 submitted by Imperial College London, related to ultrasound-triggered liposome payload release.

AUTHOR CONTRIBUTIONS

Øystein Øvrebø: Conceptualization (equal); funding acquisition (equal); visualization (lead); writing – original draft (lead). **Giuseppe Perale:** Conceptualization (equal); supervision (supporting); writing – original draft (supporting). **Jonathan P. Wojciechowski:** Visualization (supporting); writing – review and editing (equal). **Cécile Echalièr:** Visualization (supporting); writing – review and editing (equal). **Jonathan R. T. Jeffers:** Supervision (supporting); writing – review and editing (equal). **Molly M. Stevens:** Funding acquisition (equal); supervision (supporting); writing – review and editing (equal). **Håvard J. Haugen:** Conceptualization (equal); funding acquisition (equal); project administration (equal); supervision (equal); writing – original draft (equal). **Filippo Rossi:** Conceptualization (equal); project administration (equal); supervision (equal); writing – original draft (equal).

PEER REVIEW

The peer review history for this article is available at <https://publons.com/publon/10.1002/btm2.10295>.

DATA AVAILABILITY STATEMENT

The PubMed search results on "GelMA" are available upon request from the corresponding author. Otherwise, no data have been used without a reference.

ORCID

Øystein Øvrebø  <https://orcid.org/0000-0001-9170-0202>

Giuseppe Perale  <https://orcid.org/0000-0002-6791-3141>

Jonathan P. Wojciechowski  <https://orcid.org/0000-0002-6272-515X>

Cécile Echalièr  <https://orcid.org/0000-0002-9733-5477>

Jonathan R. T. Jeffers  <https://orcid.org/0000-0001-8496-6889>

Molly M. Stevens  <https://orcid.org/0000-0002-7335-266X>

Håvard J. Haugen  <https://orcid.org/0000-0002-6690-7233>

Filippo Rossi  <https://orcid.org/0000-0003-2665-120X>

REFERENCES

- Zhang YS, Khademhosseini A. Advances in engineering hydrogels. *Science*. 2017;356:6337. doi:10.1126/science.aaf3627
- Tibbitt MW, Anseth KS. Hydrogels as extracellular matrix mimics for 3D cell culture. *Biotechnol Bioeng*. 2009;103(4):655–663. doi:10.1002/bit.22361
- Correa S, Grosskopf AK, Lopez Hernandez H, et al. Translational applications of hydrogels. *Chem Rev*. 2021;121(18):11385–11457. doi:10.1021/acs.chemrev.0c01177
- Melvin T, Torre M. New medical device regulations: the regulator's view. *EFORT Open Rev*. 2019;4(6):351–356. doi:10.1302/2058-5241.4.180061
- Catoira MC, Gonzalez-Payo J, Fusaro L, Ramella M, Boccafocchi F. Natural hydrogels R&D process: technical and regulatory aspects for industrial implementation. *J Mater Sci Mater Med*. 2020;31(8):64. doi:10.1007/s10856-020-06401-w
- European Commission. MEDICAL DEVICES: Guidance document – Borderline products, drug-delivery products and medical devices incorporating, as an integral part, an ancillary medicinal substance or an ancillary human blood – MEDDEV 2. 1/3 rev 3 derivative. 2015.
- Spector M. Biomedical materials to meet the challenges of the aging epidemic. *Biomed Mater*. 2018;13(3):030201. doi:10.1088/1748-605X/aab171
- Milner PE, Parkes M, Puetzer JL, et al. A low friction, biphasic and boundary lubricating hydrogel for cartilage replacement. *Acta Biomater*. 2018;65:102–111. doi:10.1016/j.actbio.2017.11.002
- Zhang X, Wang J, Jin H, Wang S, Song W. Bioinspired supramolecular lubricating hydrogel induced by shear force. *J Am Chem Soc*. 2018;140(9):3186–3189. doi:10.1021/jacs.7b12886
- Douglas TEL, Schietse J, Zima A, et al. Novel self-gelling injectable hydrogel/alpha-tricalcium phosphate composites for bone regeneration: physiochemical and microcomputer tomographical characterization. *J Biomed Mater Res A*. 2018;106(3):822–828. doi:10.1002/jbm.a.36277
- Qi C, Liu J, Jin Y, et al. Photo-crosslinkable, injectable sericin hydrogel as 3D biomimetic extracellular matrix for minimally invasive repairing cartilage. *Biomaterials*. 2018;163:89–104. doi:10.1016/j.biomaterials.2018.02.016
- Schmocker A, Khoushabi A, Frauchiger DA, et al. A photo-polymerized composite hydrogel and surgical implanting tool for a

- nucleus pulposus replacement. *Biomaterials*. 2016;88:110-119. doi:[10.1016/j.biomaterials.2016.02.015](https://doi.org/10.1016/j.biomaterials.2016.02.015)
13. Bernhardt A, Weiser E, Wolf S, Vater C, Gelinsky M. Primary human osteocyte networks in pure and modified collagen gels. *Tissue Eng Part A*. 2019;25(19-20):1347-1355. doi:[10.1089/ten.TEA.2018.0338](https://doi.org/10.1089/ten.TEA.2018.0338)
 14. Martinez-Sanz E, Ossipov DA, Hilborn J, Larsson S, Jonsson KB, Varghese OP. Bone reservoir: injectable hyaluronic acid hydrogel for minimal invasive bone augmentation. *J Control Release*. 2011;152(2):232-240. doi:[10.1016/j.jconrel.2011.02.003](https://doi.org/10.1016/j.jconrel.2011.02.003)
 15. Demirtas TT, Irmak G, Gumusderelioglu M. A bioprintable form of chitosan hydrogel for bone tissue engineering. *Biofabrication*. 2017;9(3):035003. doi:[10.1088/1758-5090/aa7b1d](https://doi.org/10.1088/1758-5090/aa7b1d)
 16. Håkansson KMO, Henriksson IC, de la Peña Vázquez C, et al. Solidification of 3D printed nanofibril hydrogels into functional 3D cellulose structures. *Adv Mater Technol*. 2016;1(7):1600096. doi:[10.1002/admt.201600096](https://doi.org/10.1002/admt.201600096)
 17. Nuutila K, Grolman J, Yang L, et al. Immediate treatment of burn wounds with high concentrations of topical antibiotics in an alginate hydrogel using a platform wound device. *Adv Wound Care (New Rochelle)*. 2020;9(2):48-60. doi:[10.1089/wound.2019.1018](https://doi.org/10.1089/wound.2019.1018)
 18. Shelke NB, James R, Laurencin CT, Kumbar SG. Polysaccharide biomaterials for drug delivery and regenerative engineering. *Polym Adv Technol*. 2014;25(5):448-460.
 19. Nele V, Wojciechowski JP, Armstrong JPK, Stevens MM. Tailoring gelation mechanisms for advanced hydrogel applications. *Adv Funct Mater*. 2020;30(42):2002759. doi:[10.1002/adfm.202002759](https://doi.org/10.1002/adfm.202002759)
 20. Tang G, Zhou B, Li F, et al. Advances of naturally derived and synthetic hydrogels for intervertebral disk regeneration. *Front Bioeng Biotechnol*. 2020;8:745. doi:[10.3389/fbioe.2020.00745](https://doi.org/10.3389/fbioe.2020.00745)
 21. Reid B, Gibson M, Singh A, et al. PEG hydrogel degradation and the role of the surrounding tissue environment. *J Tissue Eng Regen Med*. 2015;9(3):315-318. doi:[10.1002/term.1688](https://doi.org/10.1002/term.1688)
 22. Zhang H, Xia H, Zhao Y. Poly(vinyl alcohol) hydrogel can autonomously self-heal. *ACS Macro Lett*. 2012;1(11):1233-1236. doi:[10.1021/mz300451r](https://doi.org/10.1021/mz300451r)
 23. Rossi F, Santoro M, Casalini T, Veglianesi P, Masi M, Perale G. Characterization and degradation behavior of agar-carbomer based hydrogels for drug delivery applications: solute effect. *Int J Mol Sci*. 2011;12(6):3394-3408. doi:[10.3390/ijms12063394](https://doi.org/10.3390/ijms12063394)
 24. Breiting V, Aasted A, Jørgensen A, Opitz P, Rosetzky A. A study on patients treated with polyacrylamide hydrogel injection for facial corrections. *Aesthetic Plast Surg*. 2004;28(1):45-53. doi:[10.1007/s00266-003-3019-9](https://doi.org/10.1007/s00266-003-3019-9)
 25. Som C, Schmutz M, Borges O, Jesus S, Borchard G, Nguyen V. *Guidelines for Implementing a Safe-by-Design Approach for Medicinal Polymeric Nanocarriers*. Empa; 2019.
 26. Perale G, Hilborn J. *Bioresorbable Polymers for Biomedical Applications: From Fundamentals to Translational Medicine*. Woodhead Publishing; 2016.
 27. Whalley D, Hruby G, Alfieri F, Kneebone A, Eade T. SpaceOAR hydrogel in dose-escalated prostate cancer radiotherapy: rectal dosimetry and late toxicity. *Clin Oncol*. 2016;28(10):e148-e154.
 28. Mandal A, Clegg JR, Anselmo AC, Mitragotri S. Hydrogels in the clinic. *Bioeng Transl Med*. 2020;5(2):e10158. doi:[10.1002/btm2.10158](https://doi.org/10.1002/btm2.10158)
 29. Zhu J, Marchant RE. Design properties of hydrogel tissue-engineering scaffolds. *Expert Rev Med Devices*. 2011;8(5):607-626. doi:[10.1586/erd.11.27](https://doi.org/10.1586/erd.11.27)
 30. Dondossola E, Friedl P. Host responses to implants revealed by intravital microscopy. *Nat Rev Mater*. 2022;7:6-22. doi:[10.1038/s41578-021-00369-x](https://doi.org/10.1038/s41578-021-00369-x)
 31. Rahmati M, Silva EA, Reseland JE, Heyward CA, Haugen HJ. Biological responses to physicochemical properties of biomaterial surface. *Chem Soc Rev*. 2020;49(15):5178-5224. doi:[10.1039/d0cs00103a](https://doi.org/10.1039/d0cs00103a)
 32. Mao AS, Mooney DJ. Regenerative medicine: current therapies and future directions. *Proc Natl Acad Sci U S A*. 2015;112(47):14452-14459. doi:[10.1073/pnas.1508520112](https://doi.org/10.1073/pnas.1508520112)
 33. Loi F, Cordova LA, Pajarinen J, Lin TH, Yao Z, Goodman SB. Inflammation, fracture and bone repair. *Bone*. 2016;86:119-130. doi:[10.1016/j.bone.2016.02.020](https://doi.org/10.1016/j.bone.2016.02.020)
 34. Patenaude M, Hoare T. Injectable, mixed natural-synthetic polymer hydrogels with modular properties. *Biomacromolecules*. 2012;13(2):369-378. doi:[10.1021/bm2013982](https://doi.org/10.1021/bm2013982)
 35. Ouasti S, Donno R, Cellesi F, Sherratt MJ, Terenghi G, Tirelli N. Network connectivity, mechanical properties and cell adhesion for hyaluronic acid/PEG hydrogels. *Biomaterials*. 2011;32(27):6456-6470. doi:[10.1016/j.biomaterials.2011.05.044](https://doi.org/10.1016/j.biomaterials.2011.05.044)
 36. Wang Y, Ma M, Wang J, et al. Development of a photo-crosslinking, biodegradable GelMA/PEGDA hydrogel for guided bone regeneration materials. *Materials (Basel)*. 2018;11(8):1345-1345. doi:[10.3390/ma11081345](https://doi.org/10.3390/ma11081345)
 37. Burdick JA, Anseth KS. Photoencapsulation of osteoblasts in injectable RGD-modified PEG hydrogels for bone tissue engineering. *Biomaterials*. 2002;23(22):4315-4323. doi:[10.1016/s0142-9612\(02\)00176-x](https://doi.org/10.1016/s0142-9612(02)00176-x)
 38. Salinas CN, Anseth KS. The influence of the RGD peptide motif and its contextual presentation in PEG gels on human mesenchymal stem cell viability. *J Tissue Eng Regen Med*. 2008;2(5):296-304. doi:[10.1002/term.95](https://doi.org/10.1002/term.95)
 39. Haugen HJ, Basu P, Sukul M, Mano JF, Reseland JE. Injectable biomaterials for dental tissue regeneration. *Int J Mol Sci*. 2020;21(10):3442. doi:[10.3390/ijms21103442](https://doi.org/10.3390/ijms21103442)
 40. Echaliar C, Valot L, Martinez J, Mehdi A, Subra G. Chemical crosslinking methods for cell encapsulation in hydrogels. *Mater Today Commun*. 2019;20:100536. doi:[10.1016/j.mtcomm.2019.05.012](https://doi.org/10.1016/j.mtcomm.2019.05.012)
 41. Rice MA, Anseth KS. Encapsulating chondrocytes in copolymer gels: bimodal degradation kinetics influence cell phenotype and extracellular matrix development. *J Biomed Mater Res A*. 2004;70(4):560-568. doi:[10.1002/jbm.a.30106](https://doi.org/10.1002/jbm.a.30106)
 42. Holloway JL, Ma H, Rai R, Burdick JA. Modulating hydrogel crosslink density and degradation to control bone morphogenetic protein delivery and in vivo bone formation. *J Control Release*. 2014;191:63-70. doi:[10.1016/j.jconrel.2014.05.053](https://doi.org/10.1016/j.jconrel.2014.05.053)
 43. Tezel A, Fredrickson GH. The science of hyaluronic acid dermal fillers. *J Cosmet Laser Ther*. 2008;10(1):35-42. doi:[10.1080/14764170701774901](https://doi.org/10.1080/14764170701774901)
 44. Inomata H, Wada N, Yagi Y, Goto S, Saito S. Swelling behaviours of N-alkylacrylamide gels in water: effects of copolymerization and crosslinking density. *Polymer*. 1995;36(4):875-877.
 45. Peppas NA, Hoffman AS. *Hydrogels*. *Biomaterials Science*. Elsevier; 2020:153-166.
 46. Li X, Cho B, Martin R, et al. Nanofiber-hydrogel composite-mediated angiogenesis for soft tissue reconstruction. *Sci Transl Med*. 2019;11(490):eaau6210. doi:[10.1126/scitranslmed.aau6210](https://doi.org/10.1126/scitranslmed.aau6210)
 47. Chahal AS, Schweikle M, Lian AM, Reseland JE, Haugen HJ, Tiainen H. Osteogenic potential of poly(ethylene glycol)-amorphous calcium phosphate composites on human mesenchymal stem cells. *J Tissue Eng*. 2020;11:2041731420926840. doi:[10.1177/2041731420926840](https://doi.org/10.1177/2041731420926840)
 48. Appel EA, Tibbitt MW, Webber MJ, Mattix BA, Veisoh O, Langer R. Self-assembled hydrogels utilizing polymer-nanoparticle interactions. *Nat Commun*. 2015;6(1):6295. doi:[10.1038/ncomms7295](https://doi.org/10.1038/ncomms7295)
 49. Wang Q, Mynar JL, Yoshida M, et al. High-water-content mouldable hydrogels by mixing clay and a dendritic molecular binder. *Nature*. 2010;463(7279):339-343. doi:[10.1038/nature08693](https://doi.org/10.1038/nature08693)
 50. Borchard G, Som C, Zinn M, et al. Polymeric nano-biomaterials for medical applications: advancements in developing and implementation considering safety-by-design concepts. *Front Bioeng Biotechnol*. 2020;8:599950.

51. Darzi SA, Munz Y. The impact of minimally invasive surgical techniques. *Annu Rev Med.* 2004;55:223-237. doi:[10.1146/annurev.med.55.091902.105248](https://doi.org/10.1146/annurev.med.55.091902.105248)
52. O'Toole JE, Eichholz KM, Fessler RG. Surgical site infection rates after minimally invasive spinal surgery. *J Neurosurg Spine.* 2009; 11(4):471-476. doi:[10.3171/2009.5.SPINE08633](https://doi.org/10.3171/2009.5.SPINE08633)
53. Spector M, Lim TC. Injectable biomaterials: a perspective on the next wave of injectable therapeutics. *Biomed Mater.* 2016;11(1):014110. doi:[10.1088/1748-6041/11/1/014110](https://doi.org/10.1088/1748-6041/11/1/014110)
54. Zhao L, Weir MD, Xu HH. An injectable calcium phosphate-alginate hydrogel-umbilical cord mesenchymal stem cell paste for bone tissue engineering. *Biomaterials.* 2010;31(25):6502-6510. doi:[10.1016/j.biomaterials.2010.05.017](https://doi.org/10.1016/j.biomaterials.2010.05.017)
55. Ren P, Li J, Zhao L, et al. Dipeptide self-assembled hydrogels with shear-thinning and instantaneous self-healing properties determined by peptide sequences. *ACS Appl Mater Interfaces.* 2020;12(19): 21433-21440. doi:[10.1021/acsami.0c03038](https://doi.org/10.1021/acsami.0c03038)
56. Han S-S, Yoon HY, Yhee JY, et al. In situ cross-linkable hyaluronic acid hydrogels using copper free click chemistry for cartilage tissue engineering. *Polym Chem.* 2018;9(1):20-27.
57. Nele V, Schutt CE, Wojciechowski JP, et al. Ultrasound-triggered enzymatic gelation. *Adv Mater.* 2020;32(7):e1905914. doi:[10.1002/adma.201905914](https://doi.org/10.1002/adma.201905914)
58. Scinto SL, Bilodeau DA, Hincapie R, et al. Bioorthogonal chemistry. *Nat Rev Methods Primers.* 2021;1(1):1-23. doi:[10.1038/s43586-021-00028-z](https://doi.org/10.1038/s43586-021-00028-z)
59. Kettenberger U, Pioletti D; Google Patents, assignee. Composition for bone regeneration. Patent application US20180264175A1. 2018.
60. Kettenberger U, Luginbuehl V, Procter P, Pioletti DP. In vitro and in vivo investigation of bisphosphonate-loaded hydroxyapatite particles for peri-implant bone augmentation. *J Tissue Eng Regen Med.* 2017;11(7):1974-1985. doi:[10.1002/term.2094](https://doi.org/10.1002/term.2094)
61. Strand V, Baraf HSB, Lavin PT, Lim S, Hosokawa H. A multicenter, randomized controlled trial comparing a single intra-articular injection of Gel-200, a new cross-linked formulation of hyaluronic acid, to phosphate buffered saline for treatment of osteoarthritis of the knee. *Osteoarthr Cartil.* 2012;20(5):350-356. doi:[10.1016/j.joca.2012.01.013](https://doi.org/10.1016/j.joca.2012.01.013)
62. Miyamoto K, Sasaki M, Minamisawa Y, Kurahashi Y, Kano H, Ishikawa S. Evaluation of in vivo biocompatibility and biodegradation of photocrosslinked hyaluronate hydrogels (HADgels). *J Biomed Mater Res A.* 2004;70(4):550-559.
63. Brandt KD, Block JA, Michalski JP, Moreland LW, Caldwell JR, Lavin PT. Efficacy and safety of intraarticular sodium hyaluronate in knee osteoarthritis. ORTHOVISC Study Group. *Clin Orthop Relat Res.* 2001;385(385):130-143. doi:[10.1097/00003086-200104000-00021](https://doi.org/10.1097/00003086-200104000-00021)
64. Petterson SC, Plancher KD. Single intra-articular injection of lightly cross-linked hyaluronic acid reduces knee pain in symptomatic knee osteoarthritis: a multicenter, double-blind, randomized, placebo-controlled trial. *Knee Surg Sports Traumatol Arthrosc.* 2019;27(6): 1992-2002. doi:[10.1007/s00167-018-5114-0](https://doi.org/10.1007/s00167-018-5114-0)
65. Priano F. Early efficacy of intra-articular HYADD(R) 4 (Hymovis(R)) injections for symptomatic knee osteoarthritis. *Joints.* 2017;5(2):79-84. doi:[10.1055/s-0037-1603677](https://doi.org/10.1055/s-0037-1603677)
66. Bliddal H, Overgaard A, Hartkopp A, Beier J, Conaghan PG, Henriksen M. Polyacrylamide hydrogel injection for knee osteoarthritis: a 6 months prospective study. *J Orthop Res Ther.* 2021;6(2): S278.
67. Bliddal H, Overgaard A, Hartkopp A, Beier J, Conaghan PG, Henriksen M. Polyacrylamide hydrogel injection for knee osteoarthritis: results of a 52 week prospective study. *Osteoarthr Cartil.* 2021;29:S278-S278.
68. Shive MS, Hoemann CD, Restrepo A, et al. BST-CarGel: in situ chondroinduction for cartilage repair. *Oper Tech Orthop.* 2006;16(4): 271-278.
69. Shive MS, Stanish WD, McCormack R, et al. BST-CarGel (R) treatment maintains cartilage repair superiority over microfracture at 5 years in a multicenter randomized controlled trial. *Cartilage.* 2015;6(2):62-72. doi:[10.1177/1947603514562064](https://doi.org/10.1177/1947603514562064)
70. Kandel L, Agar G, Elkayam O, et al. A novel approach for knee osteoarthritis using high molecular weight hyaluronic acid conjugated to plasma fibrinogen - interim findings of a double-blind clinical study. *Heliyon.* 2020;6(7):e04475. doi:[10.1016/j.heliyon.2020.e04475](https://doi.org/10.1016/j.heliyon.2020.e04475)
71. Schreiner MM, Raudner M, Szomolanyi P, et al. Chondral and osteochondral femoral cartilage lesions treated with GelinC: significant improvement of radiological outcome over time and zonal variation of the repair tissue based on T2 mapping at 24 months. *Cartilage.* 2020;13:1947603520926702.
72. Trattnig S, Ohel K, Mlynarik V, Juras V, Zbyn S, Korner A. Morphological and compositional monitoring of a new cell-free cartilage repair hydrogel technology - GelinC by MR using semi-quantitative MOCART scoring and quantitative T2 index and new zonal T2 index calculation. *Osteoarthr Cartil.* 2015;23(12):2224-2232. doi:[10.1016/j.joca.2015.07.007](https://doi.org/10.1016/j.joca.2015.07.007)
73. Goldshmid R, Cohen S, Shachaf Y, et al. Steric interference of adhesion supports in-vitro chondrogenesis of mesenchymal stem cells on hydrogels for cartilage repair. *Sci Rep.* 2015;5(1):12607. doi:[10.1038/srep12607](https://doi.org/10.1038/srep12607)
74. Heijl L, Heden G, Svardstrom G, Ostgren A. Enamel matrix derivative (EMDOGAIN) in the treatment of intrabony periodontal defects. *J Clin Periodontol.* 1997;24(9 Pt 2):705-714. doi:[10.1111/j.1600-051x.1997.tb00253.x](https://doi.org/10.1111/j.1600-051x.1997.tb00253.x)
75. McGuire MK, Scheyer ET, Schupbach P. A prospective, case-controlled study evaluating the use of enamel matrix derivative on human buccal recession defects: a human histologic examination. *J Periodontol.* 2016;87(6):645-653. doi:[10.1902/jop.2016.150459](https://doi.org/10.1902/jop.2016.150459)
76. Wang Z, Lu B, Chen L, Chang J. Evaluation of an osteostimulative putty in the sheep spine. *J Mater Sci Mater Med.* 2011;22(1):185-191. doi:[10.1007/s10856-010-4175-5](https://doi.org/10.1007/s10856-010-4175-5)
77. Coathup MJ, Cai Q, Campion C, Buckland T, Blunn GW. The effect of particle size on the osteointegration of injectable silicate-substituted calcium phosphate bone substitute materials. *J Biomed Mater Res B Appl Biomater.* 2013;101(6):902-910. doi:[10.1002/jbm.b.32895](https://doi.org/10.1002/jbm.b.32895)
78. Coughlan M, Davies M, Mostert AK, et al. A prospective, randomized, multicenter study comparing silicated calcium phosphate versus BMP-2 synthetic bone graft in posterolateral instrumented lumbar fusion for degenerative spinal disorders. *Spine (Phila Pa 1976).* 2018;43(15):E860-E868. doi:[10.1097/BRS.0000000000002678](https://doi.org/10.1097/BRS.0000000000002678)
79. Zhang H, Yang L, Yang XG, et al. Demineralized bone matrix carriers and their clinical applications: an overview. *Orthop Surg.* 2019;11(5): 725-737. doi:[10.1111/os.12509](https://doi.org/10.1111/os.12509)
80. Cammisia FP Jr, Lowery G, Garfin SR, et al. Two-year fusion rate equivalency between Grafton DBM gel and autograft in posterolateral spine fusion: a prospective controlled trial employing a side-by-side comparison in the same patient. *Spine (Phila Pa 1976).* 2004; 29(6):660-666. doi:[10.1097/01.brs.0000116588.17129.b9](https://doi.org/10.1097/01.brs.0000116588.17129.b9)
81. Martin GJ Jr, Boden SD, Titus L, Scarborough NL. New formulations of demineralized bone matrix as a more effective graft alternative in experimental posterolateral lumbar spine arthrodesis. *Spine (Phila Pa 1976).* 1999;24(7):637-645. doi:[10.1097/00007632-199904010-00005](https://doi.org/10.1097/00007632-199904010-00005)
82. Stark M, DeBernardis D, McDowell C, Ford E, McMillan S. Percutaneous skeletal fixation of painful subchondral bone marrow edema utilizing an injectable, synthetic, biocompatible hyaluronic acid-based bone graft substitute. *Arthrosc Tech.* 2020;9(11):e1645-e1650. doi:[10.1016/j.eats.2020.07.005](https://doi.org/10.1016/j.eats.2020.07.005)
83. Jones JR, Brauer DS, Hupa L, Greenspan DC. Bioglass and bioactive glasses and their impact on healthcare. *Int J Appl Glass Sci.* 2016; 7(4):423-434.

84. Ceylan A, Asik I, Ozgencil GE, Erken B. Clinical results of intradiscal hydrogel administration (GelStix) in lumbar degenerative disc disease. *Turk J Med Sci*. 2019;49(6):1634-1639. doi:10.3906/sag-1901-1
85. Mazza E, Marcia S, Mondaini F, et al. Efficacy and safety of a novel hydrogel (HYADD4-G) in degenerative disc disease patients: a multicentric open label study. *Eur Rev Med Pharmacol Sci*. 2020;24(5):2692-2703. doi:10.26355/eurrev_202003_20539
86. Mainil-Varlet P, Schiavinato A, Ganster MM. Efficacy evaluation of a new hyaluronan derivative HYADD(R) 4-G to maintain cartilage integrity in a rabbit model of osteoarthritis. *Cartilage*. 2013;4(1):28-41. doi:10.1177/1947603512455193
87. Lewis G. Nucleus pulposus replacement and regeneration/repair technologies: present status and future prospects. *J Biomed Mater Res B Appl Biomater*. 2012;100(6):1702-1720. doi:10.1002/jbmb.32712
88. Wardlaw D, Craig NJ, Smith FW, Singal V. Early clinical results of an in situ polymerizing protein hydrogel nuclear repair system. *The British Editorial Society of Bone & Joint Surgery*; 2008:529.
89. Berlemann U, Schwarzenbach O. An injectable nucleus replacement as an adjunct to microdiscectomy: 2 year follow-up in a pilot clinical study. *Eur Spine J*. 2009;18(11):1706-1712. doi:10.1007/s00586-009-1136-0
90. Boyd LM, Carter AJ. Injectable biomaterials and vertebral endplate treatment for repair and regeneration of the intervertebral disc. *Eur Spine J*. 2006;15(Suppl 3):S414-S421. doi:10.1007/s00586-006-0172-2
91. Ringdahl E, Pandit S. Treatment of knee osteoarthritis. *Am Fam Physician*. 2011;83(11):1287-1292.
92. Glyn-Jones S, Palmer AJ, Agricola R, et al. Osteoarthritis. *Lancet*. 2015;386(9991):376-387. doi:10.1016/S0140-6736(14)60802-3
93. Law TY, Nguyen C, Frank RM, Rosas S, McCormick F. Current concepts on the use of corticosteroid injections for knee osteoarthritis. *Phys Sportsmed*. 2015;43(3):269-273. doi:10.1080/00913847.2015.1017440
94. Zeng C, Lane NE, Hunter DJ, et al. Intra-articular corticosteroids and the risk of knee osteoarthritis progression: results from the osteoarthritis initiative. *Osteoarthr Cartil*. 2019;27(6):855-862. doi:10.1016/j.joca.2019.01.007
95. Bannuru RR, Natov NS, Obadan IE, Price LL, Schmid CH, McAlindon TE. Therapeutic trajectory of hyaluronic acid versus corticosteroids in the treatment of knee osteoarthritis: a systematic review and meta-analysis. *Arthritis Rheum*. 2009;61(12):1704-1711. doi:10.1002/art.24925
96. Bennell KL, Hunter DJ, Hinman RS. Management of osteoarthritis of the knee. *BMJ*. 2012;345:e4934. doi:10.1136/bmj.e4934
97. Kreuz PC, Steinwachs MR, Erggelet C, et al. Results after microfracture of full-thickness chondral defects in different compartments in the knee. *Osteoarthr Cartil*. 2006;14(11):1119-1125. doi:10.1016/j.joca.2006.05.003
98. Armiento AR, Alini M, Stoddart MJ. Articular fibrocartilage – why does hyaline cartilage fail to repair? *Adv Drug Deliv Rev*. 2019;146:289-305. doi:10.1016/j.addr.2018.12.015
99. Gooding TB, Kennedy SJ, Sherwood CH; Anika Therapeutics Inc, assignee. Treatment of arthritis and other musculoskeletal disorders with crosslinked hyaluronic acid. US patent US8323617B2. 2012.
100. Rutjes AW, Juni P, da Costa BR, Trelle S, Nuesch E, Reichenbach S. Viscosupplementation for osteoarthritis of the knee: a systematic review and meta-analysis. *Ann Intern Med*. 2012;157(3):180-191. doi:10.7326/0003-4819-157-3-201208070-00473
101. Strand V, McIntyre LF, Beach WR, Miller LE, Block JE. Safety and efficacy of US-approved viscosupplements for knee osteoarthritis: a systematic review and meta-analysis of randomized, saline-controlled trials. *J Pain Res*. 2015;8:217-228. doi:10.2147/JPR.S83076
102. Henrotin Y, Raman R, Richette P, et al. Consensus statement on viscosupplementation with hyaluronic acid for the management of osteoarthritis. *Semin Arthritis Rheum*. 2015;45:140-149. doi:10.1016/j.semarthrit.2015.04.011
103. Liu Z, Lin W, Fan Y, Kampf N, Wang Y, Klein J. Effects of hyaluronan molecular weight on the lubrication of cartilage-emulating boundary layers. *Biomacromolecules*. 2020;21(10):4345-4354. doi:10.1021/acs.biomac.0c01151
104. Khunmanee S, Jeong Y, Park H. Crosslinking method of hyaluronic-based hydrogel for biomedical applications. *J Tissue Eng*. 2017;8:2041731417726464. doi:10.1177/2041731417726464
105. Hunter DJ. Viscosupplementation for osteoarthritis of the knee. *N Engl J Med*. 2015;372(11):1040-1047. doi:10.1056/NEJMc1215534
106. Wang CC, Wang CT, Chou WC, Kao CL, Tsai KL. Hyaluronic acid injection reduces inflammatory and apoptotic markers through modulation of AKT by repressing the oxidative status of neutrophils from osteoarthritic synovial fluid. *Int J Biol Macromol*. 2020;165(Pt B):2765-2772. doi:10.1016/j.ijbiomac.2020.10.154
107. Altman R, Bedi A, Manjoo A, Niazi F, Shaw P, Mease P. Anti-inflammatory effects of intra-articular hyaluronic acid: a systematic review. *Cartilage*. 2019;10(1):43-52. doi:10.1177/1947603517749919
108. Trnibar A, Schougaard H, Camitz L, et al. An international multicentre prospective study on the efficacy of an intraarticular polyacrylamide hydrogel in horses with osteoarthritis: a 24 months follow-up. *Acta Vet Scand*. 2015;57(1):20. doi:10.1186/s13028-015-0110-6
109. Fernandez-Cossio S, Castano-Oreja MT. Biocompatibility of two novel dermal fillers: histological evaluation of implants of a hyaluronic acid filler and a polyacrylamide filler. *Plast Reconstr Surg*. 2006;117(6):1789-1796. doi:10.1097/01.prs.0000214656.07273.b0
110. Erggelet C, Vavken P. Microfracture for the treatment of cartilage defects in the knee joint – a golden standard? *J Clin Orthop Trauma*. 2016;7(3):145-152. doi:10.1016/j.jcot.2016.06.015
111. Radwan-Pragłowska J, Piatkowski M, Deinek V, et al. Chitosan-based bioactive hemostatic agents with antibacterial properties-synthesis and characterization. *Molecules*. 2019;24(14):2629-2629. doi:10.3390/molecules24142629
112. Hoemann CD, Sun J, McKee MD, et al. Chitosan-glycerol phosphate/blood implants elicit hyaline cartilage repair integrated with porous subchondral bone in microdrilled rabbit defects. *Osteoarthr Cartil*. 2007;15(1):78-89. doi:10.1016/j.joca.2006.06.015
113. Frappier J, Stanish W, Brittberg M, et al. Economic evaluation of BST-CarGel as an adjunct to microfracture vs microfracture alone in knee cartilage surgery. *J Med Econ*. 2014;17(4):266-278. doi:10.3111/13696998.2014.897626
114. Albro MB, Bergholt MS, St-Pierre JP, et al. Raman spectroscopic imaging for quantification of depth-dependent and local heterogeneities in native and engineered cartilage. *NPJ Regen Med*. 2018;3(1):3. doi:10.1038/s41536-018-0042-7
115. Bergholt MS, St-Pierre JP, Offeddu GS, et al. Raman spectroscopy reveals new insights into the zonal organization of native and tissue-engineered articular cartilage. *ACS Cent Sci*. 2016;2(12):885-895. doi:10.1021/acscentsci.6b00222
116. Aae TF, Randsborg P-H, Lurås H, Årøen A, Lian ØB. Microfracture is more cost-effective than autologous chondrocyte implantation: a review of level 1 and level 2 studies with 5 year follow-up. *Knee Surg Sports Traumatol Arthrosc*. 2018;26(4):1044-1052.
117. Vainieri ML, Lolli A, Kops N, et al. Evaluation of biomimetic hyaluronic-based hydrogels with enhanced endogenous cell recruitment and cartilage matrix formation. *Acta Biomater*. 2020;101:293-303. doi:10.1016/j.actbio.2019.11.015
118. Perez JR, Kouroupis D, Li DJ, Best TM, Kaplan L, Correa D. Tissue engineering and cell-based therapies for fractures and bone defects. *Front Bioeng Biotechnol*. 2018;6:105. doi:10.3389/fbioe.2018.00105

119. Grønsgag AB, Romundstad P, Forsmo S, Langhammer A, Schei B. Excess mortality after hip fracture among elderly women in Norway. The HUNT study. *Osteoporos Int*. 2012;23(6):1807-1811. doi:[10.1007/s00198-011-1811-y](https://doi.org/10.1007/s00198-011-1811-y)
120. Haentjens P, Magaziner J, Colón-Emeric CS, et al. Meta-analysis: excess mortality after hip fracture among older women and men. *Ann Intern Med*. 2010;152(6):380-390.
121. Hu F, Jiang C, Shen J, Tang P, Wang Y. Preoperative predictors for mortality following hip fracture surgery: a systematic review and meta-analysis. *Injury*. 2012;43(6):676-685. doi:[10.1016/j.injury.2011.05.017](https://doi.org/10.1016/j.injury.2011.05.017)
122. Campana V, Milano G, Pagano E, et al. Bone substitutes in orthopaedic surgery: from basic science to clinical practice. *J Mater Sci Mater Med*. 2014;25(10):2445-2461. doi:[10.1007/s10856-014-5240-2](https://doi.org/10.1007/s10856-014-5240-2)
123. Decision Resources G. Medtech 360 – Bone Graft Substitutes, Market Insights, Global 2019. 2019.
124. Miron RJ, Sculean A, Cochran DL, et al. Twenty years of enamel matrix derivative: the past, the present and the future. *J Clin Periodontol*. 2016;43(8):668-683. doi:[10.1111/jcpe.12546](https://doi.org/10.1111/jcpe.12546)
125. Hsu WL, Oldfield CJ, Xue B, et al. Exploring the binding diversity of intrinsically disordered proteins involved in one-to-many binding. *Protein Sci*. 2013;22(3):258-273. doi:[10.1002/pro.2207](https://doi.org/10.1002/pro.2207)
126. Sculean A, Chiantella GC, Windisch P, Donos N. Clinical and histologic evaluation of human intrabony defects treated with an enamel matrix protein derivative (Emdogain). *Int J Periodontics Restorative Dent*. 2000;20(4):374-381.
127. Heden G. A case report study of 72 consecutive Emdogain-treated intrabony. *Restorative Dent*. 2000;20:127-139.
128. Rasperini G, Silvestri M, Schenk RK, Nevins ML. Clinical and histologic evaluation of human gingival recession treated with a sub-epithelial connective tissue graft and enamel matrix derivative (Emdogain): a case report. *Int J Periodontics Restorative Dent*. 2000;20(3):269-275.
129. Sculean A, Windisch P, Keglevich T, Chiantella GC, Gera I, Donos N. Clinical and histologic evaluation of human intrabony defects treated with an enamel matrix protein derivative combined with a bovine-derived xenograft. *Int J Periodontics Restorative Dent*. 2003;23(1):47-55.
130. Jones JR. Review of bioactive glass: from Hench to hybrids. *Acta Biomater*. 2013;9(1):4457-4486. doi:[10.1016/j.actbio.2012.08.023](https://doi.org/10.1016/j.actbio.2012.08.023)
131. van Dijk LA, Barrere-de Groot F, Rosenberg A, et al. MagnetOs, Vitoss, and Novabone in a multi-endpoint study of posterolateral fusion: a true fusion or not? *Clin Spine Surg*. 2020;33(6):E276-E287. doi:[10.1097/BSD.0000000000000920](https://doi.org/10.1097/BSD.0000000000000920)
132. Dumortier G, Grossiord JL, Agnely F, Chaumeil JC. A review of poloxamer 407 pharmaceutical and pharmacological characteristics. *Pharm Res*. 2006;23(12):2709-2728. doi:[10.1007/s11095-006-9104-4](https://doi.org/10.1007/s11095-006-9104-4)
133. Dumortier G, El Kateb N, Sahli M, Kedjar S, Boulliat A, Chaumeil JC. Development of a thermogelling ophthalmic formulation of cysteine. *Drug Dev Ind Pharm*. 2006;32(1):63-72. doi:[10.1080/03639040500390934](https://doi.org/10.1080/03639040500390934)
134. Kirschner HJ, Obermayr F, Schaefer J, Lieber J. Treatment of benign bone defects in children with silicate-substituted calcium phosphate (SiCaP). *Eur J Pediatr Surg*. 2012;22(2):143-147. doi:[10.1055/s-0032-1308699](https://doi.org/10.1055/s-0032-1308699)
135. Gruskin E, Doll BA, Futrell FW, Schmitz JP, Hollinger JO. Demineralized bone matrix in bone repair: history and use. *Adv Drug Deliv Rev*. 2012;64(12):1063-1077. doi:[10.1016/j.addr.2012.06.008](https://doi.org/10.1016/j.addr.2012.06.008)
136. Haugen HJ, Lyngstadaas SP, Rossi F, Perale G. Bone grafts: which is the ideal biomaterial? *J Clin Periodontol*. 2019;46(Suppl 21):92-102. doi:[10.1111/jcpe.13058](https://doi.org/10.1111/jcpe.13058)
137. Martin BI, Mirza SK, Spina N, Spiker WR, Lawrence B, Brodke DS. Trends in lumbar fusion procedure rates and associated hospital costs for degenerative spinal diseases in the United States, 2004 to 2015. *Spine (Phila Pa 1976)*. 2019;44(5):369-376. doi:[10.1097/BRS.0000000000002822](https://doi.org/10.1097/BRS.0000000000002822)
138. Teraguchi M, Yoshimura N, Hashizume H, et al. Prevalence and distribution of intervertebral disc degeneration over the entire spine in a population-based cohort: the Wakayama Spine Study. *Osteoarthr Cartil*. 2014;22(1):104-110. doi:[10.1016/j.joca.2013.10.019](https://doi.org/10.1016/j.joca.2013.10.019)
139. Mobbs RJ, Sivabalan P, Li J. Minimally invasive surgery compared to open spinal fusion for the treatment of degenerative lumbar spine pathologies. *J Clin Neurosci*. 2012;19(6):829-835. doi:[10.1016/j.jocn.2011.10.004](https://doi.org/10.1016/j.jocn.2011.10.004)
140. Rajaei SS, Kanim LE, Bae HW. National trends in revision spinal fusion in the USA: patient characteristics and complications. *Bone Joint J*. 2014;96-B(6):807-816. doi:[10.1302/0301-620X.96B6.31149](https://doi.org/10.1302/0301-620X.96B6.31149)
141. Bohner M, Miron RJ. A proposed mechanism for material-induced heterotopic ossification. *Mater Today*. 2019;22:132-141.
142. Maazouz Y, Chizzola G, Dobelin N, Bohner M. Cell-free, quantitative mineralization measurements as a proxy to identify osteoinductive bone graft substitutes. *Biomaterials*. 2021;275:120912. doi:[10.1016/j.biomaterials.2021.120912](https://doi.org/10.1016/j.biomaterials.2021.120912)
143. Epstein NE. Pros, cons, and costs of INFUSE in spinal surgery. *Surg Neurol Int*. 2011;2:10. doi:[10.4103/2152-7806.76147](https://doi.org/10.4103/2152-7806.76147)
144. Putz C, Wiedenhöfer B, Gerner HJ, Hüttinger K, Fürstenberg CH. Spinal fusion of an unstable atlantoaxial fracture in a completely tetraplegic patient using silicate-substituted calcium phosphate. *Eur J Trauma Emerg Surg*. 2010;36(2):169-175.
145. Licina P, Coughlan M, Johnston E, Percy M. Comparison of silicate-substituted calcium phosphate (Actifuse) with recombinant human bone morphogenetic Protein-2 (Infuse) in posterolateral instrumented lumbar fusion. *Global Spine J*. 2015;5(6):471-478. doi:[10.1055/s-0035-1566230](https://doi.org/10.1055/s-0035-1566230)
146. Newell N, Little JP, Christou A, Adams MA, Adam CJ, Masouros SD. Biomechanics of the human intervertebral disc: a review of testing techniques and results. *J Mech Behav Biomed Mater*. 2017;69:420-434. doi:[10.1016/j.jmbbm.2017.01.037](https://doi.org/10.1016/j.jmbbm.2017.01.037)
147. Chen YC, Su WY, Yang SH, Gefen A, Lin FH. In situ forming hydrogels composed of oxidized high molecular weight hyaluronic acid and gelatin for nucleus pulposus regeneration. *Acta Biomater*. 2013;9(2):5181-5193. doi:[10.1016/j.actbio.2012.09.039](https://doi.org/10.1016/j.actbio.2012.09.039)
148. Tavana S, Masouros SD, Baxan N, Freedman BA, Hansen UN, Newell N. The effect of degeneration on internal strains and the mechanism of failure in human intervertebral discs analyzed using digital volume correlation (DVC) and ultra-high field MRI. *Front Bioeng Biotechnol*. 2021;8:610907.
149. Durdag E, Ayden O, Albayrak S, Atci IB, Armagan E. Fragmentation to epidural space: first documented complication of Gelstix(TM). *Turk Neurosurg*. 2014;24(4):602-605. doi:[10.5137/1019-5149.JTN.9328-13.1](https://doi.org/10.5137/1019-5149.JTN.9328-13.1)
150. Thier S, Baumann F, Weiss C, Fickert S. Feasibility of arthroscopic autologous chondrocyte implantation in the hip using an injectable hydrogel. *Hip Int*. 2018;28(4):442-449. doi:[10.5301/hipint.5000580](https://doi.org/10.5301/hipint.5000580)
151. Blanke F, Oehler N, Haenle M, Lenz R, Vogt S, Tischer T. All-arthroscopic hydrogel-based autologous chondrocyte transplantation in the knee joint: good clinical and magnetic resonance imaging outcome after 24 months. *Art Ther*. 2021;37(6):1892-1899.e1. doi:[10.1016/j.arthro.2021.01.038](https://doi.org/10.1016/j.arthro.2021.01.038)
152. Tschugg A, Diepers M, Simone S, et al. A prospective randomized multicenter phase I/II clinical trial to evaluate safety and efficacy of NOVOCART disk plus autologous disk chondrocyte transplantation in the treatment of nucleotomized and degenerative lumbar disks to avoid secondary disease: safety results of phase I—a short report. *Neurosurg Rev*. 2017;40(1):155-162. doi:[10.1007/s10143-016-0781-0](https://doi.org/10.1007/s10143-016-0781-0)
153. Tschugg A, Michnacs F, Strowitzki M, Meisel HJ, Thome C. A prospective multicenter phase I/II clinical trial to evaluate safety and efficacy of NOVOCART disc plus autologous disc chondrocyte transplantation in the treatment of nucleotomized and degenerative lumbar disc to avoid secondary disease: study protocol for a

- randomized controlled trial. *Trials*. 2016;17(1):108. doi:[10.1186/s13063-016-1239-y](https://doi.org/10.1186/s13063-016-1239-y)
154. Sattler K, Singh A, Wolf MT, Wang X, Pardoll DM, Elisseff JH. Design, clinical translation and immunological response of biomaterials in regenerative medicine. *Nat Rev Mater*. 2016;1(7):1-17.
155. Van Norman GA. Drugs, devices, and the FDA: part 1: an overview of approval processes for drugs. *JACC Basic Transl Sci*. 2016;1(3):170-179. doi:[10.1016/j.jacbts.2016.03.002](https://doi.org/10.1016/j.jacbts.2016.03.002)
156. Van Norman GA. Drugs, devices, and the FDA: part 2: an overview of approval processes: FDA approval of medical devices. *JACC Basic Transl Sci*. 2016;1(4):277-287. doi:[10.1016/j.jacbts.2016.03.009](https://doi.org/10.1016/j.jacbts.2016.03.009)
157. Benz K, Stippich C, Osswald C, et al. Rheological and biological properties of a hydrogel support for cells intended for intervertebral disc repair. *BMC Musculoskelet Disord*. 2012;13(1):54. doi:[10.1186/1471-2474-13-54](https://doi.org/10.1186/1471-2474-13-54)
158. Schreiner MM, Raudner M, Marlovits S, et al. The MOCART (magnetic resonance observation of cartilage repair tissue) 2.0 knee score and atlas. *Cartilage*. 2019;13:571S-587S. doi:[10.1177/1947603519865308](https://doi.org/10.1177/1947603519865308)
159. Bongio M, van den Beucken JJ, Leeuwenburgh SC, Jansen JA. Pre-clinical evaluation of injectable bone substitute materials. *J Tissue Eng Regen Med*. 2015;9(3):191-209. doi:[10.1002/term.1637](https://doi.org/10.1002/term.1637)
160. Council of the European Union. MDR 2017/745 – Annex VIII. 2017.
161. Holborow R. A notified body's perspective on the clinical evaluation requirements under regulations (EU) 2017/745 on medical devices. *J Med Device Regul*. 2021;18(1):33-47.
162. Council of the European Union. Medical Device Regulation 2017/745. 2017.
163. Faris O, Shuren J. An FDA viewpoint on unique considerations for medical-device clinical trials. *N Engl J Med*. 2017;376(14):1350-1357. doi:[10.1056/NEJMra1512592](https://doi.org/10.1056/NEJMra1512592)
164. Medtech Europe. The European Medical Technology Industry in Figures 2021. 2021.
165. Zhu H, Jostein Haugen H, Perale G, et al. Tailoring resorption rates and osteogenic response in xeno-hybrid bone grafts: the effect of added gelatins. *Engineering*. 2021. (In Press). doi:[10.1016/j.eng.2021.01.010](https://doi.org/10.1016/j.eng.2021.01.010)
166. Perale G, Monjo M, Ramis JM, et al. Biomimetic biomolecules in next generation xeno-hybrid bone graft material show enhanced in vitro bone cells response. *J Clin Med*. 2019;8:2159. doi:[10.3390/jcm8122159](https://doi.org/10.3390/jcm8122159)
167. Rahmati M, Stötzl S, El Khassawna T, et al. Intrinsically disordered peptides enhance regenerative capacities of bone composite xenografts. *Mater Today*. 2021. (In Press). doi:[10.1016/j.mattod.2021.12.001](https://doi.org/10.1016/j.mattod.2021.12.001)
168. Zhu H, Blahnova VH, Perale G, et al. Xeno-hybrid bone graft releasing biomimetic proteins promotes osteogenic differentiation of hMSCs. *Front Cell Dev Biol*. 2020;8:619111. doi:[10.3389/fcell.2020.619111](https://doi.org/10.3389/fcell.2020.619111)
169. Zhu H, Gomez M, Xiao J, et al. Xenohybrid bone graft containing intrinsically disordered proteins shows enhanced in vitro bone formation. *ACS Appl Bio Mater*. 2020;3(4):2263-2274. doi:[10.1021/acsabm.0c00064](https://doi.org/10.1021/acsabm.0c00064)
170. Pajarinen J, Lin T, Gibon E, et al. Mesenchymal stem cell-macrophage crosstalk and bone healing. *Biomaterials*. 2019;196:80-89. doi:[10.1016/j.biomaterials.2017.12.025](https://doi.org/10.1016/j.biomaterials.2017.12.025)
171. Huh D, Matthews BD, Mammoto A, Montoya-Zavala M, Hsin HY, Ingber DE. Reconstituting organ-level lung functions on a chip. *Science*. 2010;328(5986):1662-1668. doi:[10.1126/science.1188302](https://doi.org/10.1126/science.1188302)
172. Zhang YS, Arneri A, Bersini S, et al. Bioprinting 3D microfibrillar scaffolds for engineering endothelialized myocardium and heart-on-a-chip. *Biomaterials*. 2016;110:45-59. doi:[10.1016/j.biomaterials.2016.09.003](https://doi.org/10.1016/j.biomaterials.2016.09.003)
173. Zaatreh S, Haffner D, Strauss M, et al. Thin magnesium layer confirmed as an antibacterial and biocompatible implant coating in a coculture model. *Mol Med Rep*. 2017;15(4):1624-1630. doi:[10.3892/mmr.2017.6218](https://doi.org/10.3892/mmr.2017.6218)
174. Friedemann MC, Mehta NA, Jessen SL, et al. Introduction to currently applied device pathology. *Toxicol Pathol*. 2019;47(3):221-234. doi:[10.1177/0192623319826585](https://doi.org/10.1177/0192623319826585)
175. Ray S, Thormann U, Eichelroth M, et al. Strontium and bisphosphonate coated iron foam scaffolds for osteoporotic fracture defect healing. *Biomaterials*. 2018;157:1-16. doi:[10.1016/j.biomaterials.2017.11.049](https://doi.org/10.1016/j.biomaterials.2017.11.049)
176. Daghma DES, Malhan D, Simon P, et al. Computational segmentation of collagen fibers in bone matrix indicates bone quality in ovariectomized rat spine. *J Bone Miner Metab*. 2018;36(3):297-306. doi:[10.1007/s00774-017-0844-5](https://doi.org/10.1007/s00774-017-0844-5)
177. Schlundt C, El Khassawna T, Serra A, et al. Macrophages in bone fracture healing: their essential role in endochondral ossification. *Bone*. 2018;106:78-89. doi:[10.1016/j.bone.2015.10.019](https://doi.org/10.1016/j.bone.2015.10.019)
178. Zeller-Plumhoff B, Malich C, Kruger D, et al. Analysis of the bone ultrastructure around biodegradable Mg-xGd implants using small angle X-ray scattering and X-ray diffraction. *Acta Biomater*. 2020;101:637-645. doi:[10.1016/j.actbio.2019.11.030](https://doi.org/10.1016/j.actbio.2019.11.030)

How to cite this article: Øvrebø Ø, Perale G, Wojciechowski JP, et al. Design and clinical application of injectable hydrogels for musculoskeletal therapy. *Bioeng Transl Med*. 2022;7(2):e10295. doi:[10.1002/btm2.10295](https://doi.org/10.1002/btm2.10295)