
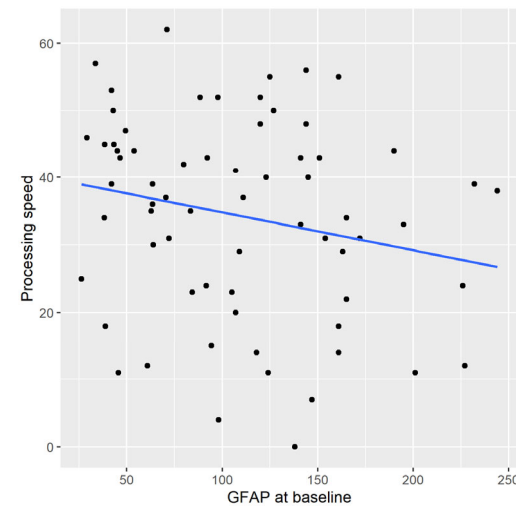
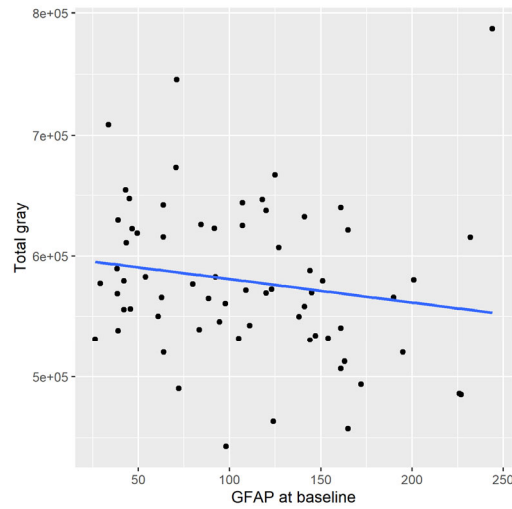
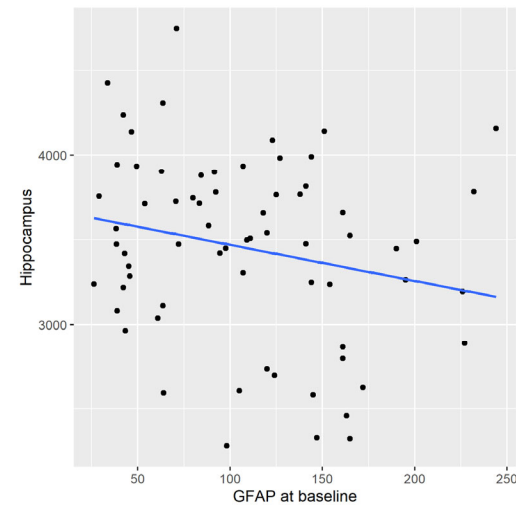


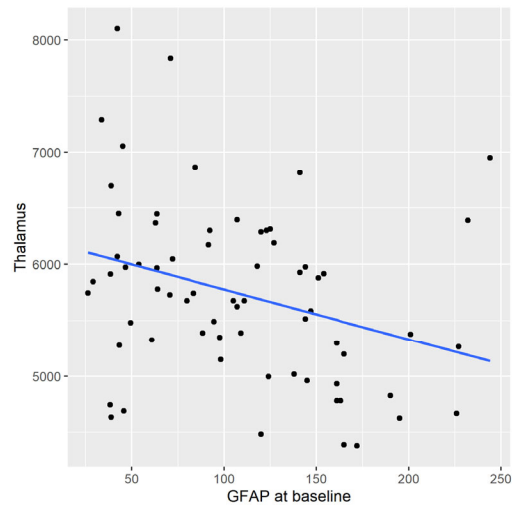

GFAP (measured in pg/mL) and MRI volume measurements (in mm³), along with processing speed (computed from number of correct responses on Symbol Digit Coding test minus errors).