

Plate fixation in periprosthetic femur fractures Vancouver type B1: preliminary report of macroscopic evaluation of the cement mantle and short literature review

Luigi Bibiano¹, Grigor Stamboltsyan², Georgios Touloupakis¹, Stefano Ghirardelli¹, Elena Biancardi¹, Longo Giuseppe Edoardo Giovanni¹, Guido Antonini¹, Cornelio Crippa¹

¹ Department of Orthopedics and Traumatology, San Carlo Borromeo Hospital, Milan, Italy; ² Mater Dei Hospital, Msida, Malta

Summary. The goal of our preliminary report is to investigate hip stem stability and intra-operative cement mantle integrity after screw insertion in plate fixation of periprosthetic Vancouver B1 femur fractures. From a cohort of 50 patients with a periprosthetic femur fracture treated in our department from February 2012 until February 2017, we included in our study patients with a periprosthetic Vancouver B1 femoral fracture in cemented hip arthroplasty and hemiarthroplasty, operated with ORIF using a 4.5/5.0 LCP Proximal Femoral Hook Plate[®] (Synthes, Switzerland) with at least one screw perforating the cement mantle. Anteroposterior and lateral femur views and pelvis X-rays were performed preoperatively. The stability of the hip implant and the cemented mantle integrity was evaluated intra-operatively in a macroscopic way and with a post-operative X-ray in anteroposterior and lateral views. Only 7 patients satisfied the inclusion criteria; no lesion/break of the cement mantle occurred intra-operatively at any step during drilling or screw insertion, also confirmed with C-arm assessment. No cases of stem mobilization were found and cement mantle integrity was maintained in every case. Insertion of screws around a cemented stem for plate fixation in periprosthetic femur fractures Vancouver type B1 could be considered a safe procedure. However, further and more extended studies are necessary for proving additional knowledge at the evaluation of the cement mantle in osteosynthesis procedures. (www.actabiomedica.it)

Key words: cement mantle; periprosthetic Vancouver B1 femur fractures; hip stem stability

Introduction

The incidence of periprosthetic fractures after hip arthroplasty is continuously rising because of an increasing number of hip joint replacements and an enhanced survivorship of the elderly population. Previously reported studies showed an increased risk of periprosthetic femoral fractures in uncemented stems compared to cemented implants (1, 2). Currently, cemented stems are still considered to be one of the most reliable materials available for the treatment of osteo-

porotic hip fractures. Periprosthetic femoral fractures represent a serious complication for elderly patients (1, 2). Plate fixation in Vancouver type B1 periprosthetic femur fractures with cemented stem is a very common approach for the elderly (3-7). The use of screws perforating the cement mantle is a common treatment option when a plate fixation is performed. The goal of this preliminary report is to investigate hip stem stability and intra-operative cement mantle integrity after screw insertion in plate fixation of periprosthetic Vancouver B1 femur fractures.

Material and methods

We retrospectively evaluated the treatment results in a cohort of 50 patients with a periprosthetic femur fracture treated at San Carlo Borromeo Hospital from February 2012 until February 2017.

The informed consent of all the patients was obtained about the use of clinical data for scientific publication.

The periprosthetic femoral fractures in this study were classified according to the Vancouver classification. Inclusion criteria of the study were: (1) Periprosthetic Vancouver B1 femoral fractures (a fracture around or just below to a stable stem) in cemented hip implants, including both total hip arthroplasty and hemiarthroplasty, operated with (2) ORIF using a 4.5/5.0 LCP Proximal Femoral Hook Plate® (Synthes, Switzerland) (3) with screws (one at least) perforating the cement mantle.

The exclusion criteria were (1) periprosthetic fractures on uncemented hip implants and (2) Vancouver B femoral fractures with no screws perforating the cement mantle.

The X-rays of the patients were obtained from the Picture Archiving and Communication System (PACS) of our Institute. Anteroposterior and lateral femur views and pelvis X-rays were performed for each patient preoperatively.

The stability of the hip implant and the cemented mantle integrity was evaluated intra-operatively by performing a mobilization test of the involved femoral stem by using a farabeuf or a lambotte clamp. In the post-operative X-ray in anteroposterior and lateral views, subjective loosening signs of the femoral stem was investigated.

All patients were in supine position on a radio-lucent table. Mainly extended lateral approach to the femur was performed with minimal invasive plate osteosynthesis (MIPO) technique used in some cases. A 4.3 mm or a 3.2 mm drill was used to perforate the femoral bone and the cement mantle. Cephalosporin (2 gr) was administered 30 minutes prior to skin incision for infection prophylaxis. For thromboembolic prophylaxis we administered low molecular weight heparin subcutaneously (according to the patient's weight) until the full weight bearing was reached.

Results

The final cohort of our study consisted of 7 patients who actually satisfied the inclusion criteria, specifically 6 women and 1 man, with a mean age of 85.6 years (range 58-97) at the time of surgery. 4 mono-cortical screws and 10 bi-cortical screws were implanted in the cement mantle. All bi-cortical screws were positioned distal to the stem, 3 mono-cortical screws were placed around the stem and the 1 remaining was put proximal to the stem. Time from admission to surgery was on average 5.8 days (range 2-7 days).

Intraoperative fluoroscopy with C-arm and direct macroscopic evaluation was used to assess the stability of the hip implant and the cement mantle integrity. Follow-up anteroposterior and lateral X-rays were done postoperatively.

No lesion/break of the cement mantle occurred intra-operatively at any step during drilling or screw insertion, also confirmed with C-arm assessment. No cases of stem mobilization were found and cement mantle integrity was maintained in every case (Figg. 1a, 1b, 1c, 1d).

Discussion

First reports on periprosthetic femoral fractures (PFF) predate the modern Total Hip Replacement (THR) designs. First publication was a 70 patient follow-up in 1954 (8). Complications related to use of metal in bones was published in 1957, where the importance of mechanical stresses and strains as contributors to metal loosening or failure was noted (9). The first successful cemented THR system created by Charnley in 1962 was the golden standard for many years coming (10-12). The incidence of periprosthetic fractures around the femur continues to rise due to increasing numbers of primary and revision THRs performed each year (13). Relative and established risk factors for periprosthetic fractures include age, sex, gender, index diagnosis, presence of osteolysis, presence of aseptic loosening, specific type of implant used and revision THR (14-16).

Current surgical treatment options of PFF are widely based on the Vancouver classification system

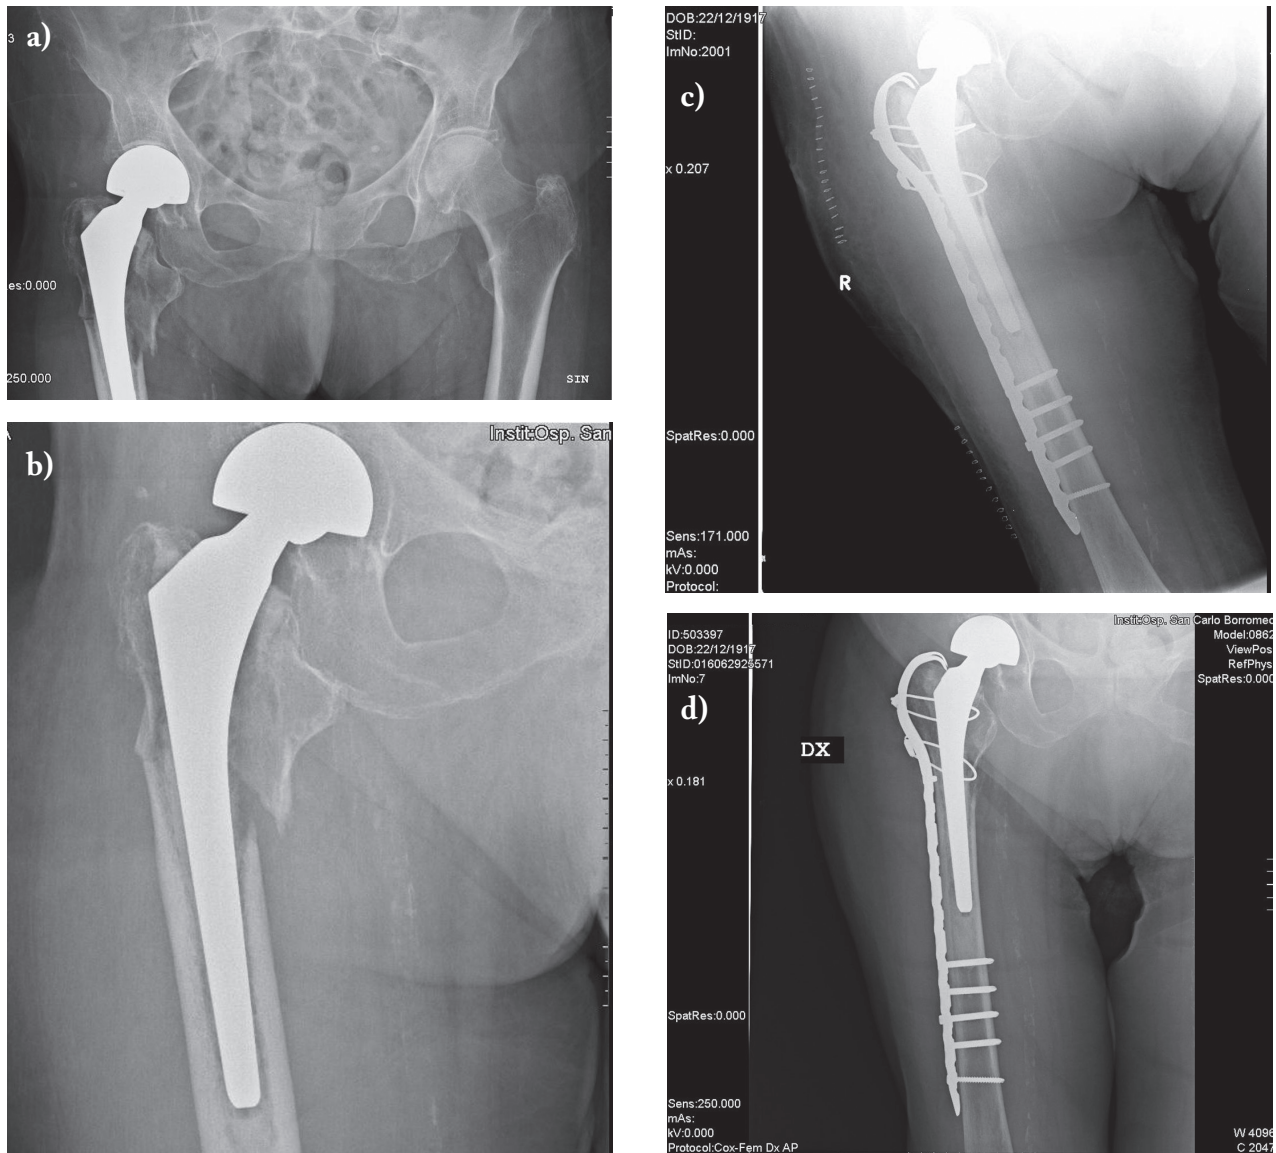


Figure 1. a, b) Preoperative images of a 98 years old female patient with a periprosthetic fracture with suspect of subsidence and stem loosening. Only after intra-operative evaluation of the stem's stability the fracture was classified as Vancouver B1. c) After the insertion of one bicortical and one unicortical screw around the cement mantle, intra-operative macroscopic evaluation didn't reveal stem's instability. d) X-rays at 8 months follow-up show a stable cemented stem with a hook plate and screws

(17). Vancouver type B fractures divide to subgroups depending on the stability of the femoral stem and bone stock. Unfortunately it is not always possible to assess the stability of the stem prior to surgery. In 2009, a study was published revealing 20% unstable femoral stems on initially diagnosed Vancouver Type B1 frac-

tures (18). Many publications recommend the use of plate osteosynthesis for Vancouver Type B1 fractures as opposed to revision of stem for unstable Type B2 and B3 types (19-22). Different types of plates were tested over the past 2 decades with combination of cables, cerclages, locking screws, hook plates etc., with

no widely accepted guidelines of our knowledge. Debates are focused on the different types of fixation to proximal femur as the stable stem can be compromised from the use of screws.

Biomechanical studies also were conducted to assess the stability of different types of plate osteosynthesis. Lever et al. utilized 12 pairs of human cadaveric femurs for 3 different plate fixation systems and concluded that screw plate fixation systems provided more mechanical stability compared to cable plate systems (23). Kampshoff et al. assessed the cement mantle integrity after screw insertion and concluded that bicortical screws passing through the cement cause cracks and further can destabilize the stem (24). The authors noted that the use of a unicortical screw is a much safer option with lower pullout resistance.

Giesinger et al. conducted another biomechanical study on 17 synthetic femurs and found no cracks in cement mantle after bicortical screw insertion (25). Difference is that they used same diameter drill bit and screw inserted right after the screw size was measured. The biomechanical studies conclude that longer clinical trials are needed in vivo to investigate long-term stem stability. New plate designs with variable-angle locked plates with bicortical proximal screws showed significantly greater load-to-failure ratios when compared to unicortical or cable fixation types (26). The screw holes in this system are placed outside the midline of the plate allowing angling of the screws and bicortical purchase. Weak points of this study were the use of synthetic bones and cementless stems.

Lewis et al. conclude in a recent biomechanical study that proximal femoral stability of cemented periprosthetic fracture is improved with tangentially directed bicortical locking screws as compared to unicortical screw or cable fixation (27). Further prospective studies with big samples and long term follow-up will help in choosing the correct algorithm of treatment and establish guidelines for clinical practitioners.

In our experience, osteosynthesis around cemented prostheses is very challenging to manage, as it is difficult to achieve a placement of bicortical screws around a cemented stem. The difficulty of screw placement has lead to the development of new plate designs allowing angular positioning of the screws and the use

of cerclages and cables has been controversial. Screw placement around a cemented stem sometimes gives excellent grip but it may compromise the cement mantle and may lead to cement fragmentation and failure with subsequent mobilization of the femoral stem.

Summarising, the use of unicortical screws alone or together with cables provide additional resistance to lateral bending or torsion when a plate is used, compared to cables alone. It is easier to place unicortical screws around the cement mantle rather than adjusting them around a cemented stem and this concept should be further investigated. If rigid proximal fixation is required, an effort should be made to obtain bicortical fixation. Newly designed implants are necessary to obtain bicortical locking screws directed tangentially to the hip stem. A major concern is the loosening of the construct, caused by screw penetration and cracking of cement mantle.

Moreover, clinical experience of intraoperative procedures should be reported in the studies, as only a few are available, basically reporting the results of drilling and screwing the femoral cement mantle around prosthesis. Many Authors performed the evaluation of the cement mantle in periprosthetic femur fractures. We underline that our preliminary report is the first one that evaluates in vivo the integrity of the cement mantle in plate fixation of periprosthetic femur fractures. It's very important, as these fractures are becoming more common due to increase of average life expectancy.

In our study we had no cases of macroscopic cracks in the cement mantle or stem mobilization, even when bicortical screws were used. Unfortunately, only 7 patients met our inclusion criteria; another remark is that we probably need at least a 1 year follow up after plate fixation, to check what happens after weight bearing.

In the future we expect the development of higher speed drills, which may also help in this process.

Conclusions

The use of screws around a cemented stem for plate fixation in periprosthetic femur fractures Vancouver type B could be considered a safe procedure. However, further and more extended studies are necessary

for proving additional knowledge at the evaluation of the cement mantle in osteosynthesis procedures.

Conflict of interest: None to declare

References

1. Moerman S, Mathijssen NMC, Niesten DD, Riedijk R, Rijnberg WJ, Koëter S, Kremers van de Hei K, Tuinebreijer WE, Molenaar TL, Nelissen RGHH, Vochteloo AJH. More complications in uncemented compared to cemented hemiarthroplasty for displaced femoral neck fractures: a randomized controlled trial of 201 patients, with one year follow-up. *BMC Musculoskelet Disord* 2017 Apr 21; 18(1): 169.
2. Lindberg-Larsen M, Jørgensen CC, Solgaard S, Kjersgaard AG, Kehlet H; Lundbeck. Foundation Centre for Fast-Track Hip and Knee Replacement Collaborative Group. Increased risk of intraoperative and early postoperative periprosthetic femoral fracture with uncemented stems. *Acta Orthop* 2017 Mar 14; 1-5
3. Moloney GB, Toro JB, Helfet DL, Wellman DS. Proximal Periprosthetic Femur Fractures: Strategies for Internal Fixation. *Am J Orthop (Belle Mead NJ)* 2016 May-Jun; 45(4): 213-8.
4. Yassen AT, Haddad FS. The management of type B1 periprosthetic femoral fractures: when to fix and when to revise. *Int Orthop* 2015 Sep; 39(9): 1873-9.
5. Fulkerson E, Koval K, Preston CF, Iesaka K, Kummer FJ, Egol KA. Fixation of periprosthetic femoral shaft fractures associated with cemented femoral stems: a biomechanical comparison of locked plating and conventional cable plates. *J Orthop Trauma* 2006 Feb; 20(2): 89-93.
6. Lochab J, Carrothers A, Wong E, McLachlin S, Aldebeyan W, Jenkinson R, Whyne C, Nousiainen MT. Do Transcortical Screws in a Locking Plate Construct Improve the Stiffness in the Fixation of Vancouver B1 Periprosthetic Femur Fractures? A Biomechanical Analysis of 2 Different Plating Constructs. *J Orthop Trauma* 2017 Jan; 31(1): 15-20.
7. Moloney GB, Westrick ER, Siska PA, Tarkin IS. Treatment of periprosthetic femur fractures around a well-fixed hip arthroplasty implant: span the whole bone. *Arch Orthop Trauma Surg* 2014 Jan; 134(1): 9-14.
8. Horwitz IB, Lenobel MI. Artificial hip prosthesis in acute and nonunion fractures of the femoral neck: follow-up study of seventy cases. *J Am Med Assoc* 1954 Jun 5; 155(6): 564-7.
9. McKee GK, Charnley J, Hicks JH, Zarek JM. Symposium: the use of metal in bone surgery. *Proc R Soc Med* 1957 Oct; 50(10): 837-46.
10. Charnley J. Arthroplasty of the hip. A new operation. *Lancet* 1961 May 27; 1(7187): 1129-32.
11. Charnley J. Total prosthetic replacement of the hip joint using a socket of high-density polyethylene. *Internal Publications*, No 1, Nov 1966, Centre for Hip Surgery. Wrightington Hospital.
12. Charnley J. Total prosthetic replacement of the hip. *Internal Publications*, No 4, Sept 1967, Centre for Hip Surgery. Wrightington Hospital.
13. Cook RE, Jenkins PJ, Walmsley PJ, Patton JT, Robinson CM. Risk factors for periprosthetic fractures of the hip: a survivorship analysis. *Clin Orthop Relat Res* 2008; 466: 1652-6.
14. Singh JA, Jensen MR, Harmsen SW, Lewallen DG. Are gender, comorbidity, and obesity risk factors for postoperative periprosthetic fractures after primary total hip arthroplasty? *J Arthroplasty* 2013; 28: 126-31.
15. Sarvilinna R, Huhtala HS, Sovellius RT, Halonen PJ, Nevalainen JK, Pajamäki KJ. Factors predisposing to periprosthetic fracture after hip arthroplasty: a case (n = 31)-control study. *Acta Orthop Scand* 2004 Feb; 75(1): 16-20.
16. Dhawan RK, Mangham DC, Graham NM. Periprosthetic femoral fracture due to biodegradable cement restrictor. *J Arthroplasty* 2012 Sep; 27(8): 1581.e13-5.
17. Duncan CP, Masri BA. Fractures of the femur after hip replacement. *Instr Course Lect* 1995; 44: 293-304.
18. Corten K, Vanrykel F, Bellemans J, Frederix PR, Simon JP, Broos PL. An algorithm for the surgical treatment of periprosthetic fractures of the femur around a well-fixed femoral component. *J Bone Joint Surg Br* 2009 Nov; 91(11): 1424-30.
19. Kim Y, Tanaka C, Tada H, Kanoe H, Shirai T. Treatment of periprosthetic femoral fractures after femoral revision using a long stem. *BMC Musculoskelet Disord* 2015 May 10; 16: 113. doi: 10.1186/s12891-015-0565-7.
20. Wu ES, Cherian JJ, Kapadia BH, Banerjee S, Jauregui JJ, Mont MA. Outcomes of post-operative periprosthetic femur fracture around total hip arthroplasty: a review. *Expert Rev Med Devices* 2015 Jan; 12(1): 61-72.
21. Bryant GK, Morshed S, Agel J, Henley MB, Barei DP, Taitsman LA, Nork SE. Isolated locked compression plating for Vancouver Type B1 periprosthetic femoral fractures. *Injury* 2009 Nov; 40(11): 1180-6.
22. Froberg L, Troelsen A, Brix M. Periprosthetic Vancouver type B1 and C fractures treated by locking-plate osteosynthesis: fracture union and reoperations in 60 consecutive fractures. *Acta Orthop* 2012 Dec; 83(6): 648-52.
23. Lever JP, Zdero R, Nousiainen MT, Waddell JP, Schemitsch EH. The biomechanical analysis of three plating fixation systems for periprosthetic femoral fracture near the tip of a total hip arthroplasty. *J Orthop Surg Res* 2010 Jul 23; 5: 45.
24. Kampshoff J, Stoffel KK, Yates PJ, Erhardt JB, Kuster MS. The treatment of periprosthetic fractures with locking plates: effect of drill and screw type on cement mantles: a biomechanical analysis. *Arch Orthop Trauma Surg* 2010 May; 130(5): 627-32.
25. Giesinger K, Ebnetter L, Day RE, Stoffel KK, Yates PJ, Kuster MS. Can plate osteosynthesis of periprosthetic femoral fractures cause cement mantle failure around a stable hip stem? A biomechanical analysis. *J Arthroplasty*. 2014 Jun; 29(6): 1308-12.

26. Hoffmann MF, Burgers TA, Mason JJ, Williams BO, Sietsema DL, Jones CB. Biomechanical evaluation of fracture fixation constructs using a variable-angle locked periprosthetic femur plate system. *Injury* 2014 Jul; 45(7): 1035-41.
27. Lewis GS, Caroom CT, Wee H, Jurgensmeier D, Rothermel SD, Bramer MA, Reid JS. Tangential Bicortical Locked Fixation Improves Stability in Vancouver B1 Periprosthetic Femur Fractures: A Biomechanical Study. *J Orthop Trauma* 2015 Oct; 29(10): e364-70.

Received: 12 June 2017

Accepted: 31 July 2017

Correspondence:

Georgios Touloupakis

Via Don Bartolomeo Grazioli 24
20161, Milano

Tel. (+39)3495106291

E-mail: yorgostoulou@gmail.com