



WALKING POSTER PRESENTATION

Open Access

Single breathhold, three-dimensional measurement of left atrial volume and function using sparse CINE CMR imaging with iterative reconstruction

Pierre Monney^{1*}, Orestis Vardoulis², Davide Piccini^{3,4}, Amit Bermano⁵, Amir Vaxman⁶, Craig Gotsman⁵, Janine Schwitter¹⁰, Michael O Zenge⁷, Michaela Schmidt⁷, Mariappan S Nadar⁸, Matthias Stuber^{3,9}, Nikolaos Stergiopoulos², Juerg Schwitter¹

From 18th Annual SCMR Scientific Sessions
Nice, France. 4-7 February 2015

Background

Left atrial (LA) dilatation is associated with a large variety of cardiac diseases and many LA pathologies go along with an adverse prognosis. A time-efficient 3D CMR method to precisely measure the LA volumes and function is therefore highly desirable.

Methods

A highly accelerated prototype cine sequence with sparse sampling and Iterative Reconstruction (sCINE-IR) was used in phantoms and patients to acquire 5 cine slices (2 long axis, LAX and 3 short axis, SAX) through the LA during a single breathhold yielding a spatial/temporal resolution of 1.5mm/30ms (1.5T Aera, Siemens AG, Germany). The LA volumes were reconstructed from these 5 slices using a non-model based method (Bermano A, ACM trans Graph 2011). As a reference in patients, a self-navigated high-resolution whole-heart 3D dataset (3D-HR) was acquired during mid-diastole, from which the LA volume was segmented. Phantom study. Five LA phantoms made of solanum tuberosum L of known volume (water displacement method) and of different shapes were imaged with both 3D-HR and CS in various slice orientations and the calculated volumes were compared. Patients study. Three patients were scanned with both 3D-HR and sCINE-IR. The volumes obtained with 3D-HR and with sCINE-IR during the

corresponding mid-diastolic frame were compared using Bland-Altman method and linear regression.

Results

Phantom study. Volumes measured by sCINE-IR were highly correlated with the true LA volume, with a mean difference of $-4.7 \pm 1.8 \text{ ml}$ (8.7% underestimation, $R^2=0.94$). The calculated volumes were not significantly different when different orientations of the sCINE-IR slices were planned (LAX aligned vs not aligned with the true LA long axis, SAX parallel vs not parallel to the mitral plane, $p=\text{ns}$ for both). The mean difference between 3D-HR and true LA volume was $-1.4 \pm 1.4 \text{ ml}$ (2.3% underestimation, $R^2=0.97$). Patients study. Reference LA volumes were obtained with 3D-HR in 3 patients aged 23-80 years (63ml, 62ml and 395ml). sCINE-IR -calculated volumes of the mid-diastolic frame matched closely the reference volume with a difference of $2.7 \pm 6.5 \text{ ml}$ (2.7% underestimation, $R^2=0.99$). Complete time-volume curves of the LAs were obtained for each patient, allowing to assess LA phasic function (Figure).

Conclusions

With this new method of a highly accelerated sCINE-IR acquisition followed by a 3D non-model based reconstruction, LA volumes could be accurately measured from 5 cine slices acquired during one single breath

¹Center for Cardiac Magnetic Resonance, Cardiology, University Hospital Lausanne (CHUV), Lausanne, Switzerland

Full list of author information is available at the end of the article

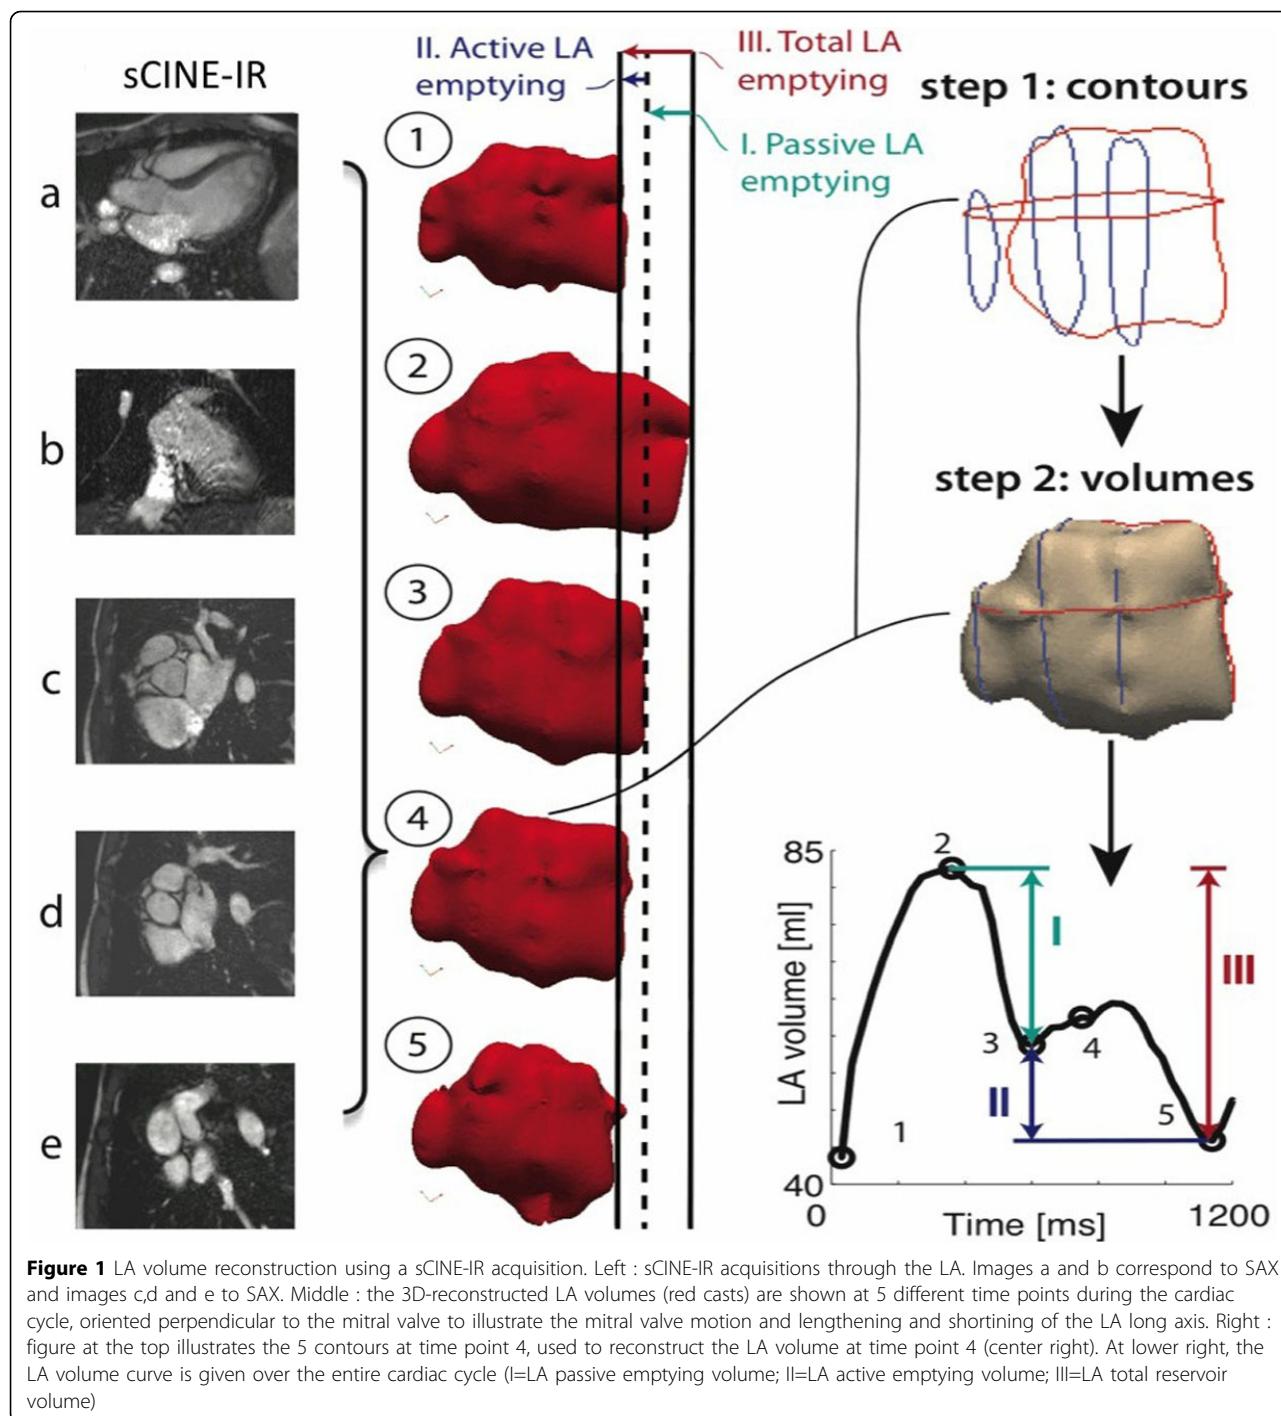


Figure 1 LA volume reconstruction using a sCINE-IR acquisition. Left : sCINE-IR acquisitions through the LA. Images a and b correspond to SAX and images c,d and e to SAX. Middle : the 3D-reconstructed LA volumes (red casts) are shown at 5 different time points during the cardiac cycle, oriented perpendicular to the mitral valve to illustrate the mitral valve motion and lengthening and shortening of the LA long axis. Right : figure at the top illustrates the 5 contours at time point 4, used to reconstruct the LA volume at time point 4 (center right). At lower right, the LA volume curve is given over the entire cardiac cycle (I=LA passive emptying volume; II=LA active emptying volume; III=LA total reservoir volume)

hold. This method opens the possibility to precisely measure LA function over time. The reproducibility of this new technique needs to be assessed on a larger patient cohort.

Funding

None.

Authors' details

¹Center for Cardiac Magnetic Resonance, Cardiology, University Hospital Lausanne (CHUV), Lausanne, Switzerland. ²Laboratory of Hemodynamics and Cardiovascular Technology, Swiss Federal Institute of Technology, Lausanne, Switzerland. ³Center for Biomedical Imaging (CIBM), University of Lausanne, Lausanne, Switzerland. ⁴Advanced Clinical Imaging Technology, Siemens Healthcare, Lausanne, Switzerland. ⁵Center for Graphics and Geometric Computing, Technion, Haifa, Israel. ⁶Geometric Modelling and Industrial Geometry, Vienna University of Technology, Vienna, Austria. ⁷Healthcare sector, Siemens AG, Erlangen, Germany. ⁸Imaging and Computer Vision,

Siemens Corporation, Princeton, NJ, USA. ⁹Radiology, University Hospital Lausanne, Lausanne, Switzerland. ¹⁰University of Fribourg, Fribourg, Switzerland.

Published: 3 February 2015

doi:10.1186/1532-429X-17-S1-Q35

Cite this article as: Monney et al.: Single breathhold, three-dimensional measurement of left atrial volume and function using sparse CINE CMR imaging with iterative reconstruction. *Journal of Cardiovascular Magnetic Resonance* 2015 17(Suppl 1):Q35.

Submit your next manuscript to BioMed Central and take full advantage of:

- Convenient online submission
- Thorough peer review
- No space constraints or color figure charges
- Immediate publication on acceptance
- Inclusion in PubMed, CAS, Scopus and Google Scholar
- Research which is freely available for redistribution

Submit your manuscript at
www.biomedcentral.com/submit

