

Laboratory Investigation

Biomechanical Comparison of Spinal Fusion Methods Using Interspinous Process Compressor and Pedicle Screw Fixation System Based on Finite Element Method

Jisoo Choi, M.S.,¹ Sohee Kim, Ph.D.,^{1,2*} Dong-Ah Shin, M.D., Ph.D.³

Department of Medical System Engineering,¹ School of Mechatronics,² Gwangju Institute of Science and Technology (GIST), Gwangju, Korea
Department of Neurosurgery,³ Yonsei University College of Medicine, Seoul, Korea

Objective : To investigate the biomechanical effects of a newly proposed Interspinous Process Compressor (IPC) and compare with pedicle screw fixation at surgical and adjacent levels of lumbar spine.

Methods : A three dimensional finite element model of intact lumbar spine was constructed and two spinal fusion models using pedicle screw fixation system and a new type of interspinous devices, IPC, were developed. The biomechanical effects such as range of motion (ROM) and facet contact force were analyzed at surgical level (L3/4) and adjacent levels (L2/3, L4/5). In addition, the stress in adjacent intervertebral discs (D2, D4) was investigated.

Results : The entire results show biomechanical parameters such as ROM, facet contact force, and stress in adjacent intervertebral discs were similar between PLIF and IPC models in all motions based on the assumption that the implants were perfectly fused with the spine.

Conclusion : The newly proposed fusion device, IPC, had similar fusion effect at surgical level, and biomechanical effects at adjacent levels were also similar with those of pedicle screw fixation system. However, for clinical applications, real fusion effect between spinous process and hooks, duration of fusion, and influence on spinous process need to be investigated through clinical study.

Key Words : Intervertebral disc degeneration · Pedicle screw · Interspinous device · Finite element analysis · Range of motion.

INTRODUCTION

The lumbar arthrodesis is a prevalent surgical treatment for degenerative disc disease. Lumbar arthrodesis has many advantages such as high fusion rate, preservation of the original disc height, and maintained stability of lumbar spine²⁾. The pedicle screw fixation system implemented by posterior lumbar interbody fusion (PLIF) method has been widely used and regarded as gold standard for lumbar arthrodesis⁹⁾. Although pedicle screw fixation system is a popular surgical treatment for degenerative disc disease, high complication rates have been reported. It is reported that the surgical procedure to implement the pedicle screw fixation system is technically demanding and many complications have been observed¹¹⁾. The most frequently detected complications are screw misplacement and pedicle breakage during surgical operation. Also, postoperative complications

include screw loosening, breakage, and loss of correction. Besides complications related to screw insertion, large blood loss and wound infection have also been identified^{4,8)}. For these reasons, the use of pedicle screw fixation system may need to be limited by considering patient's age and bone condition.

In order to minimize such complications, interspinous spacers such as X-stop and Coflex have been developed without using screw insertion^{13,18,23)}. The Coflex system has been widely investigated through finite element analysis and clinical studies. As a dynamic stabilization system, Coflex preserves the motion range compared to pedicle screw fixation system and is less invasively inserted with convenient surgical process¹⁷⁾. The complications including fracture of spinous process or implant after inserting Coflex were also investigated in previous studies^{3,7)}. Recently, one of interspinous devices, Interspinous Process Compressor (IPC), has been introduced, approved by Korean Food and Drug

• Received : August 21, 2015 • Revised : November 24, 2015 • Accepted : December 1, 2015

* Move to : Department of Robotics Engineering, Daegu Gyeongbuk Institute of Science and Technology (DGIST), Daegu, Korea

• Address for reprints : Dong-Ah Shin, M.D., Ph.D.

Department of Neurosurgery, Yonsei University College of Medicine, 50-1 Yonsei-ro, Seodaemun-gu, Seoul 03722, Korea

Tel : +82-2-2228-2150, Fax : +82-2-393-9979, E-mail : CISTERN@yuhs.ac

• This is an Open Access article distributed under the terms of the Creative Commons Attribution Non-Commercial License (<http://creativecommons.org/licenses/by-nc/3.0>) which permits unrestricted non-commercial use, distribution, and reproduction in any medium, provided the original work is properly cited.

Administration (KFDA), and commercially released as TieGER™ (ANT technology, Yongin, South Korea). The IPC has a unique geometry that is different from other interspinous process spacers as shown in Fig. 1. It consists of a bone block that is inserted between spinous processes and hooks that are fixed on each spinous process, in order to completely fuse the lumbar segments. Although this new spinal fusion implant is expected to have advantages such as reduced damages to ligaments, muscles and vertebrae as the implant is laterally inserted less invasively and screws are not used to fix with vertebrae, the biomechanical effects after the fusion of lumbar segments with the IPC have not been investigated.

The purpose of this study is to investigate the biomechanical effects of the proposed IPC system using finite element analysis before clinical studies. The biomechanical effects such as range of motion (ROM), intervertebral disc stress, and facet contact

force of IPC system were investigated and compared with conventional pedicle screw fixation system.

MATERIALS AND METHODS

The computed tomographic scan data of a healthy 24-years-old male was taken and reconstructed to three dimensional geometry using Mimics software (Materialise Inc., Leuven, Belgium). The 3D geometry was imported to Hypermesh software (Altair Engineering Inc., Troy, MI, USA) and converted from surface to solid type. Then, it was meshed with finite elements. The element types, number of nodes and elements of each component are shown in Table 1. The cortical bone was constructed from the surface of cancellous bone with a thickness of 1 mm and cartilage endplate was extracted from the surface of intervertebral disc with a thickness of 0.5 mm. The final finite element (FE) model had five vertebrae (L1-5), four intervertebral discs, cartilage endplates, and ligaments. The total number of nodes and elements were 398260 and 945960, respectively.

The material properties of each component were obtained

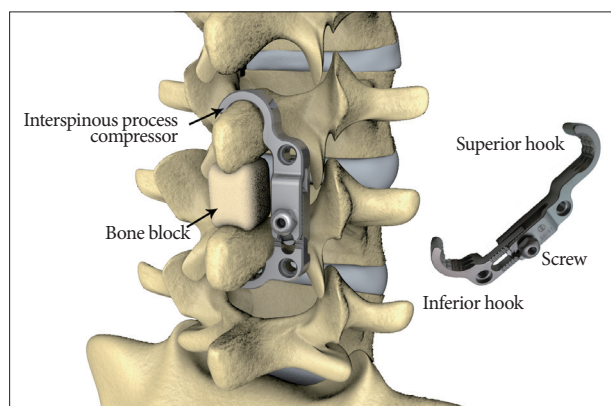


Fig. 1. Geometry of the proposed interspinous process compressor device, which consists of bone block, superior hook, screw, and inferior hook.

Table 1. Element type, number of nodes and elements of each component


Component	Element type	No. of nodes	No. of elements
Cortical bone	Shell	61577	121531
Cancellous bone	Tetrahedral	39928	176598
Posterior bone	Tetrahedral	47297	197019
Nucleus pulposus	Hexahedral	160662	145985
Annulus ground	Hexahedral	128165	107924
Cartilage endplate	Shell	40280	39846
Ligament	Truss	164	100
Entire components		398260	945960

Table 2. Material properties used in the finite element models

Component	Young's modulus (MPa)	Poisson ratio	Reference
Cortical bone	5000	0.3	Rohlmann et al., 2006 ²⁰⁾
Cancellous bone	50	0.2	Rohlmann et al., 2006 ²²⁾
Posterior bone	3500	0.25	Polikeit et al., 2003 ¹⁹⁾
Nucleus pulposus	1	0.499	Shirazi-Adl et al., 1984 ²⁴⁾
Annulus ground	2	0.45	Lavaste et al., 1992 ¹⁶⁾
Cartilage endplate	24	0.4	Goel et al., 1995 ¹⁰⁾
Ligament		0.45	Zhong et al., 2006 ²⁹⁾
ALL	20		
PLL	20		
CL	32.9		
ITL	58.7		
ISL	11.6		
SSL	15		
Pedicle screw, rod (Ti6Al4V)	110000	0.3	Chosa et al. ⁵⁾
PEEK cage	3500	0.3	Vadapalli et al. ²⁶⁾
IPC compressor	110000	0.3	
Bone block	100	0.2	

ALL : anterior longitudinal ligament, PLL : posterior longitudinal ligament, CL : capsular ligament, ITL : inter transverse ligament, ISL : interspinous ligament, SSL : supra-supinous ligament, PEEK : polyether ether ketone

Fig. 2. Finite element models of lumbar spine with no implant (A), PEEK cage and pedicle screw implemented by posterior lumbar interbody fusion method (B) and PEEK cage and interspinous process compressor systems (C). PEEK : polyether ether ketone.

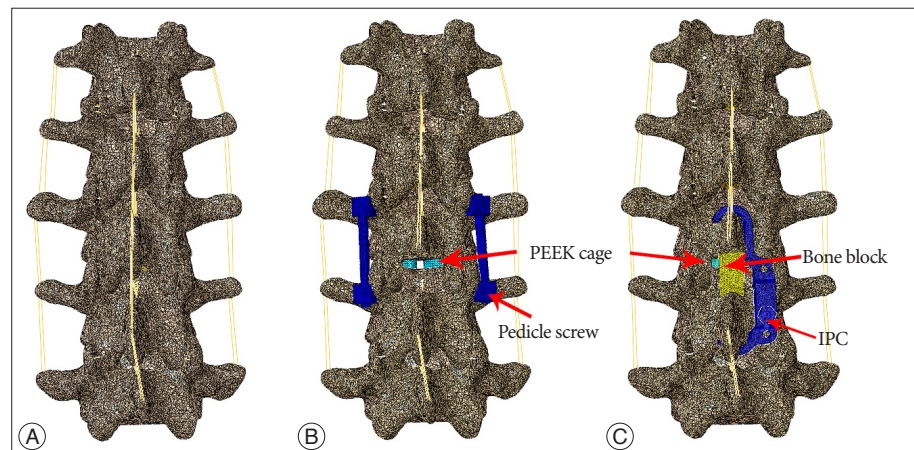

from the literature, as shown in Table 2. Nucleus pulposus has nearly incompressible property. Annulus fibrosus was modeled to be linear elastic. Ligaments were modeled to be linear elastic and they can resist tension only. The FE model was exported to Abaqus software (ABAQUS 6.13; Hibbitt, Karlsson & Sorenson, Inc., Providence, RI, USA) after the material properties were applied to each component of lumbar spine in the model. The frictionless sliding contact condition was applied to the surface of facet joints. The developed 3-dimensional FE model as shown in Fig. 2A was validated by comparing ROM at each intervertebral segment in extension, flexion, lateral bending and axial torsion based on the study by Yamamoto et al.²⁸⁾

In order to compare the biomechanical changes after spine fusion, two types of surgical models, PLIF and IPC models, were developed based on the validated intact spine model. The PLIF model consisted of polyether ether ketone (PEEK) cages, pedicle screws, and rods as shown in Fig. 2B. The length and diameter of the pedicle screw were 45 mm and 6 mm, respectively. The geometry of pedicle screws was approximated as cylinder in order to simplify the simulations. Following the standard surgical method, supraspinous ligament, interspinous ligament, and posterior longitudinal ligament at surgical level were removed, and inferior portion of L3 lamina was also removed. The PEEK cage was inserted between L3 and L4 after intervertebral disc was totally resected. After the cage was inserted, the pedicle screw fixation system was implanted at L3–4 level. The tie interaction was applied to cage and vertebral bodies for the complete fusion. Also, pedicle screws were entirely tied to the vertebral bodies.

Next, the IPC model consisted of PEEK cage, inferior hook, superior hook, and screw that combines superior hook with inferior hook, as shown in Fig. 2C. The size of bone block and length of the hooks were adjusted to fit the developed FE model. The surgical procedure was the same as with the PLIF model. The PEEK cages were inserted at the same place as with the PLIF model. The bone block was inserted between spinous process of L3 and L4. The superior and inferior hooks were placed on spinous processes of L3 and L4. The hooks were connected with screw and tied so that hooks cannot be separated.

The tie interaction was applied to all spinal implants and vertebral bodies for the complete fusion condition.

Two loading conditions were used in this study. The first loading condition was for validation of the intact FE model, following the same protocol used in the study of Yamamoto et al.²⁸⁾. The pure moment of 10 Nm was applied to the superior surface of L1 while the inferior surface of L5 was fixed in all directions. The second loading condition was applied to both intact and surgical models to analyze the biomechanical changes caused by the surgical implants. The follower load of 280 N that represents partial body weight along the curvature of lumbar spine was applied²¹⁾. The truss elements were attached bilaterally along the curvature of lumbar spine as previous studies^{12,15)}. For surgical models, adjusted moments were applied to superior surface of L1 to obtain same lordosis (L1–5) that was calculated with the intact model where the moment of 10 Nm was applied. The moment that causes the same lordosis with intact spine was investigated in each loading condition⁵⁾. The identified moments to apply to both surgical models under extension, flexion, bending, and torsion were 16 Nm, 12.6 Nm, 11 Nm, and 13.5 Nm, respectively. The validation of intact FE model and biomechanical changes caused by the surgical implants were investigated in flexion, extension, lateral bending and axial torsion conditions.

RESULTS

To validate the constructed intact spine model, the ROM of finite element model of intact spine was compared with the results of the study by Yamamoto et al.²⁸⁾ The results were within ± 1 degree of the ROM values reported in Yamamoto et al.'s study in extension, flexion, bending, and torsion, as shown in Fig. 3.

In Fig. 4, the ROM at adjacent levels (L2/3, L4/5) and surgical level (L3/4) was compared among intact and surgical models in extension, flexion, lateral bending, and axial torsion. The ROM of both surgical models remarkably decreased at surgical level (L3/4) compared to the intact model in all motions. The ROM at surgical level was changed by -96% and -94% in extension, -96% and -95% in flexion, -92% and -89% in bending, and

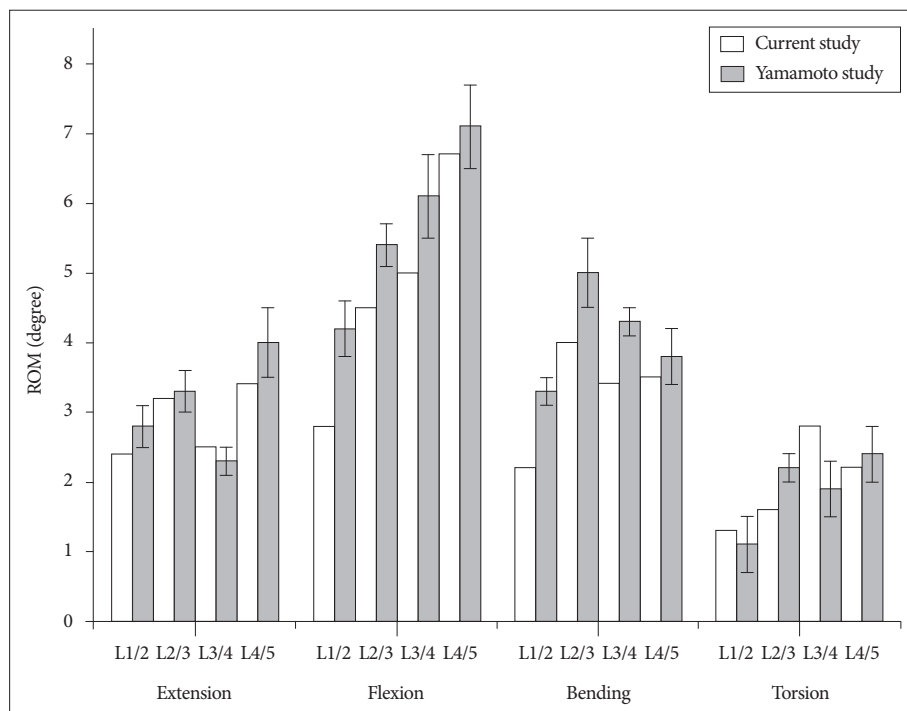


Fig. 3. Comparison of range of motion (ROM) between the present study and Yamamoto et al.'s²⁸⁾ study.

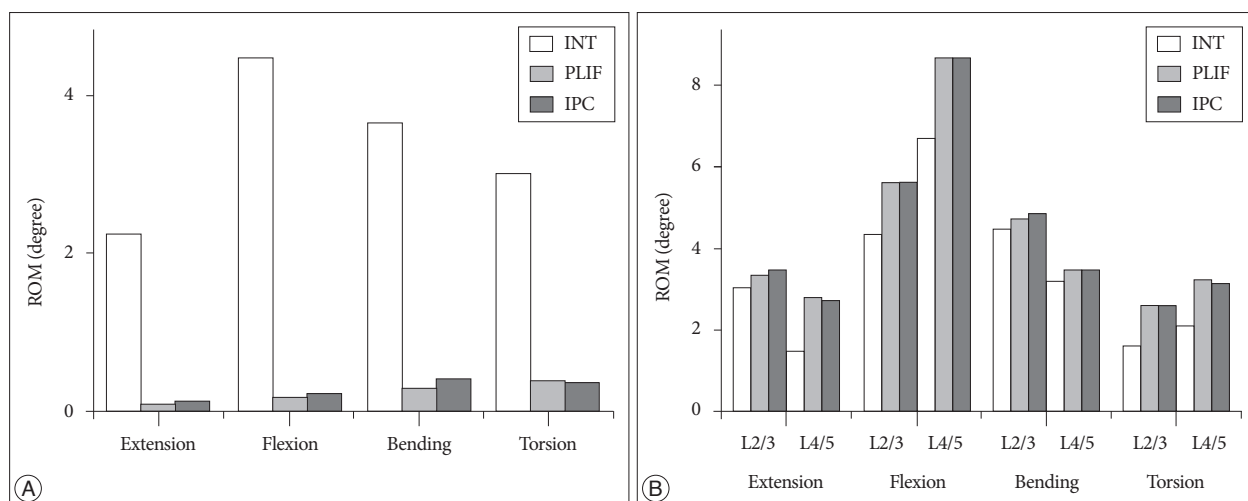


Fig. 4. ROM of the PLIF and IPC models at surgical level (L3/4) (A) and adjacent levels (L2/3, L4/5) (B) in extension, flexion, bending and torsion, compared to the intact model. ROM : range of motion, INT : intact transverse ligament, PLIF : posterior lumbar interbody fusion, IPC : Interspinous Process Compressor.

-87% and -88% in torsion in PLIF and IPC models, respectively, compared to the intact model. The PLIF and IPC models resulted in similar ROM at surgical level, with a difference of less than 0.1 degree. On the other hand, the ROM increased in all motions at adjacent levels (L2/3, L4/5). The ROM at L2-3 level was changed by +10% and +14% in extension, +29% and +30% in flexion, +6% and +8% in bending, and +61% and +61% in torsion in PLIF and IPC models, respectively, compared to the intact model. The ROM at L4-5 level was changed by +90% and +85% in extension, +30% and +30% in flexion, +9% and +9% in bending, and +54% and +50% in torsion in PLIF and IPC models, respectively, compared to the intact model. The ROM

was more increased at L4/5 level than L2/3 level in both surgical models and the surgical models had similar ROM, with a difference within 0.1 degree at adjacent levels.

The stress in intervertebral discs was compared in Fig. 5, among intact and surgical models at adjacent levels (L2/3, L4/5), which are represented as D2 and D4. The stress in D2 was changed by -3% and +3% in extension, +20% and +20% in flexion, -0.4% and +3% in bending, and +12% and +10% in torsion in PLIF and IPC models compared to the intact model, respectively. The stress in D2 increased with the PLIF model in flexion and torsion while it increased in all motions with the IPC model. The stress in D4 was changed by +13% and +11% in

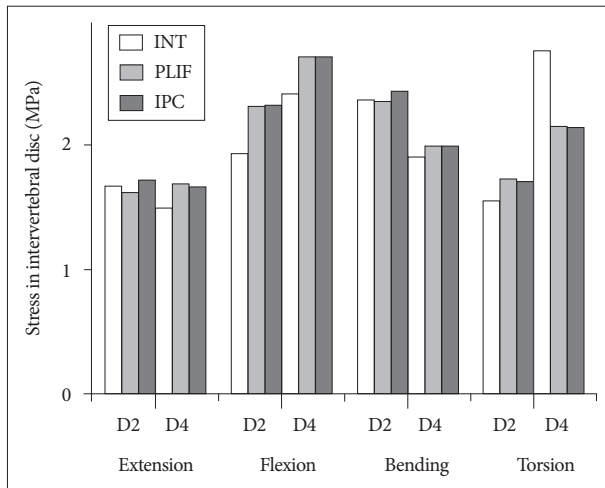


Fig. 5. Von Mises stress in the intervertebral disc of the PLIF and IPC models at adjacent levels (D2, D4) in extension, flexion, bending and torsion, compared to the intact model. INT : intact transverse ligament, PLIF : posterior lumbar interbody fusion, IPC : Interspinous Process Compressor.

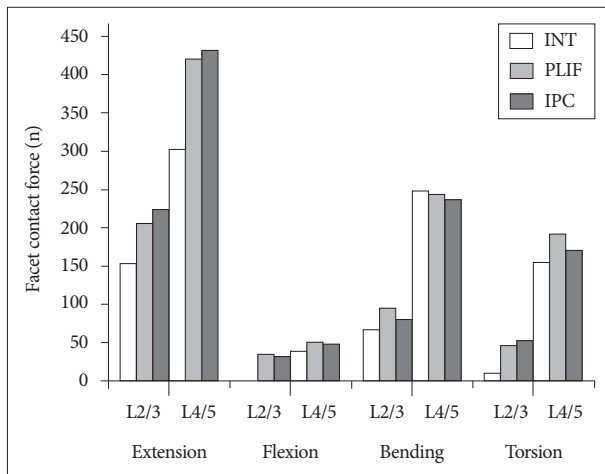


Fig. 6. Facet contact force of PLIF and IPC models at adjacent levels (L2/3, L4/5) in extension, flexion, bending and torsion, compared to the intact model. INT : intact transverse ligament, PLIF : posterior lumbar interbody fusion, IPC : Interspinous Process Compressor.

extension, +12% and +12% in flexion, +4% and +4% in bending, and -22.1% and -22.5% in torsion in PLIF and IPC models, respectively, compared to the intact model. The stress in D4 increased in both surgical models except torsion condition, compared to the intact model. The difference in intervertebral disc stress of IPC and PLIF models was 5.8% in D2 and 1.8% in D4.

The facet contact force at adjacent levels (L2/3, L4/5) was compared in Fig. 6, among intact and surgical models. The facet contact force at surgical level was zero in all motions while it tended to increase at adjacent levels (L2/3, L4/5) in all motions for both PLIF and IPC models. The facet contact force at L2/3 level was changed by +34% and +46% in extension, +42% and +20% in bending, and +364% and +432% in torsion, in PLIF and IPC models, respectively. In flexion, the facet contact force was zero in intact model while it increased in both surgical

models. The facet contact force at L4/5 level was changed by +39% and +43% in extension, +29% and +24% in flexion, -2% and -4% in bending, and +24% and +11% in torsion, in PLIF and IPC models, respectively. The maximum difference in facet contact force of PLIF and IPC models was 15.4% in bending condition.

DISCUSSION

In this study, the biomechanical changes after inserting the IPC were investigated and compared with pedicle screw fixation system using finite element analysis. We used CT images of a healthy, young male to reconstruct three dimensional geometry of lumbar spine. The characteristic of FE model of lumbar spine was represented by applying material properties of each component, based on the previous FE studies as shown in Table 2. A number of previous studies also used CT images of young patient and normal condition of lumbar spine to construct the FE models^{3,14,15,27}. In our FE model, only one level of intervertebral disc (L3/4) was assumed to be degenerative condition, and more importantly, the whole degenerative portion of intervertebral disc was removed following the standard surgical procedure as in previous studies^{12,14,15}. Therefore, the used FE model could be concluded to be appropriate to represent surgical model of degenerative disc disease.

As a spinal fusion device, the IPC model showed comparable biomechanical effects with the conventional PLIF model. At surgical level (L3/4), the intersegmental rotation was remarkably decreased. Accordingly, no facet contact force occurred in both surgical models. The results predicted by FEA in the current study were similar to the previous results^{5,25}. The ROM values were similar between the IPC and PLIF models with a maximum difference of 0.1 degree and no facet contact force occurred in all motions for both surgical models. At adjacent level, on the other hand, the ROM and facet contact force increased according to fusion effect. These adjacent effects had been previously reported and considered as major complications of spinal fusion^{12,14,15}. We obtained similar results using the IPC model. The ROM was maximally changed in extension at L4/5 level in both surgical models. The ROM values were similar between the IPC and PLIF models. The facet contact force of the IPC model was slightly higher than that of the PLIF model in extension, while that of the PLIF model was slightly higher than the IPC model in other motions. In addition, stress in intervertebral discs slightly increased after spinal fusion at L2/3 or L4/5 level as previous study⁵. The stress in adjacent intervertebral discs of the IPC model was slightly higher than that of the PLIF model with the difference of 5.8%.

In summary, the FEA results show that the adjacent effects of using the IPC model were similar to those of using conventional pedicle screw fixation system, based on the assumption that the implants were perfectly fused with the bones. The anterior bone was fused with PEEK cage and posterior bone was also

fixed with screws for PLIF model, and with bone block and interspinous compressor for IPC model. Accordingly, biomechanical effects of using PLIF and IPC methods were not essentially different in all motions.

As limitations of the current study, the spinous process and hooks were modeled to be fused as one body although the hooks were fixed with spinous process using keel in reality. Accordingly, the stress on spinous process was not analyzed, which however should be investigated in future clinical studies as complications such as fracture of spinous process can occur. The actual fusion effect between spinous process and hooks, duration of fusion, and influence on spinous process need to be investigated through clinical study. In addition, interspinous devices such as Coflex and DIAM were analyzed using finite element method in previous studies^{1,3)}. In those studies, the posterior parts were fused with interspinous device and the intervertebral disc was preserved. On the other hand, in our study, the intervertebral disc was entirely removed and PEEK cages were inserted instead. As a result, the biomechanical effects of the IPC system could not be directly compared to other types of interspinous devices reported in previous studies. Such comparative investigations, however, would need to be performed as future works.

CONCLUSION

A new type of spinal fusion device, IPC, was analyzed biomechanically through FEM. Based on the simulated results, it exhibited similar fusion effect at surgical level and similar biomechanical effects at adjacent levels compared to pedicle screw fixation system. The IPC with less invasive local incision and without screw insertion, resulting in reduced damages to ligaments, muscles, and vertebrae of the patient and eliminated complications associated with screws, may extensively be used regardless of patient's age and bone conditions after clinical validations for fusion rates and long term stability.

• Acknowledgements

This work was presented at the 54th Annual Meeting of the Korean Neurosurgical Society on Oct. 17-19, 2014.

This research was supported by grants from the Basic Science Research Program of the National Research Foundation (NRF-2014R1A1A3050285), the Industrial R&D program of MOTIE/KEIT (10052732), and the institute of Medical System Engineering (iMSE) and the Integrative Aging Research Center of Gwangju Institute of Science and Technology (GIST), Korea.

References

1. Anasetti F, Galbusera F, Aziz HN, Bellini CM, Addis A, Villa T, et al. : Spine stability after implantation of an interspinous device : an in vitro and finite element biomechanical study. *J Neurosurg Spine* 13 : 568-575, 2010
2. Bono CM, Lee CK : Critical analysis of trends in fusion for degenerative disc disease over the past 20 years : influence of technique on fusion rate and clinical outcome. *Spine (Phila Pa 1976)* 29 : 455-463; discussion 25, 2004
3. Byun DH, Shin DA, Kim JM, Kim SH, Kim HI : Finite element analysis

- of the biomechanical effect of coflex™ on the lumbar spine. *Korean J Spine* 9 : 131-136, 2012
4. Carreon LY, Puno RM, Dimar JR 2nd, Glassman SD, Johnson JR : Perioperative complications of posterior lumbar decompression and arthrodesis in older adults. *J Bone Joint Surg Am* 85-A : 2089-2092, 2003
5. Chen SH, Zhong ZC, Chen CS, Chen WJ, Hung C : Biomechanical comparison between lumbar disc arthroplasty and fusion. *Med Eng Phys* 31 : 244-253, 2009
6. Chosa E, Goto K, Totoribe K, Tajima N : Analysis of the effect of lumbar spine fusion on the superior adjacent intervertebral disk in the presence of disk degeneration, using the three-dimensional finite element method. *J Spinal Disord Tech* 17 : 134-139, 2004
7. Erbulut DU, Zafarparandeh I, Hassan CR, Lazoglu I, Ozer AF : Determination of the biomechanical effect of an interspinous process device on implanted and adjacent lumbar spinal segments using a hybrid testing protocol : a finite-element study. *J Neurosurg Spine* 23 : 200-208, 2015
8. Fischgrund JS, Mackay M, Herkowitz HN, Brower R, Montgomery DM, Kurz LT : 1997 Volvo Award winner in clinical studies. Degenerative lumbar spondylolisthesis with spinal stenosis : a prospective, randomized study comparing decompressive laminectomy and arthrodesis with and without spinal instrumentation. *Spine (Phila Pa 1976)* 22 : 2807-2812, 1997
9. Gaines RW Jr : The use of pedicle-screw internal fixation for the operative treatment of spinal disorders. *J Bone Joint Surg Am* 82-A : 1458-1476, 2000
10. Goel VK, Monroe BT, Gilbertson LG, Brinckmann P : Interlaminar shear stresses and laminae separation in a disc. Finite element analysis of the L3-L4 motion segment subjected to axial compressive loads. *Spine (Phila Pa 1976)* 20 : 689-698, 1995
11. Jutte PC, Castelein RM : Complications of pedicle screws in lumbar and lumbosacral fusions in 105 consecutive primary operations. *Eur Spine J* 11 : 594-598, 2002
12. Kang KT, Kim HJ, Son J, Yeom JS, Chun HJ : Comparing an instrumented posterior fixation system with rigid and semi-flexible rods using finite element analysis. *Int J Precis Eng Manuf* 16 : 163-170, 2015
13. Kim HJ, Bak KH, Chun HJ, Oh SJ, Kang TH, Yang MS : Posterior interspinous fusion device for one-level fusion in degenerative lumbar spine disease : comparison with pedicle screw fixation - preliminary report of at least one year follow up. *J Korean Neurosurg Soc* 52 : 359-364, 2012
14. Kim HJ, Chun HJ, Moon SH, Kang KT, Kim HS, Park JO, et al. : Analysis of biomechanical changes after removal of instrumentation in lumbar arthrodesis by finite element analysis. *Med Biol Eng Comput* 48 : 703-709, 2010
15. Kim TY, Kang KT, Yoon DH, Shin HC, Kim KN, Yi S, et al. : Effects of lumbar arthrodesis on adjacent segments : differences between surgical techniques. *Spine (Phila Pa 1976)* 37 : 1456-1462, 2012
16. Lavaste F, Skalli W, Robin S, Roy-Camille R, Mazel C : Three-dimensional geometrical and mechanical modelling of the lumbar spine. *J Biomech* 25 : 1153-1164, 1992
17. Lo CC, Tsai KJ, Chen SH, Zhong ZC, Hung C : Biomechanical effect after Coflex and Coflex rivet implantation for segmental instability at surgical and adjacent segments : a finite element analysis. *Comput Methods Biomech Biomed Engin* 14 : 969-978, 2011
18. Park SC, Yoon SH, Hong YP, Kim KJ, Chung SK, Kim HJ : Minimum 2-year follow-up result of degenerative spinal stenosis treated with interspinous u (coflex). *J Korean Neurosurg Soc* 46 : 292-299, 2009
19. Polikeit A, Nolte LP, Ferguson SJ : The effect of cement augmentation on the load transfer in an osteoporotic functional spinal unit : finite-element analysis. *Spine (Phila Pa 1976)* 28 : 991-996, 2003
20. Rohlmann A, Bauer L, Zander T, Bergmann G, Wilke HJ : Determination of trunk muscle forces for flexion and extension by using a validated finite element model of the lumbar spine and measured in vivo data. *J Bio-*

- mech** 39 : 981-989, 2006
21. Rohlmann A, Neller S, Claes L, Bergmann G, Wilke HJ : Influence of a follower load on intradiscal pressure and intersegmental rotation of the lumbar spine. **Spine (Phila Pa 1976)** 26 : E557-E561, 2001
 22. Rohlmann A, Zander T, Bergmann G : Spinal loads after osteoporotic vertebral fractures treated by vertebroplasty or kyphoplasty. **Eur Spine J** 15 : 1255-1264, 2006
 23. Serhan H, Mhatre D, Defossez H, Bono CM : Motion-preserving technologies for degenerative lumbar spine : the past, present, and future horizons. **SAS J** 5 : 75-89, 2011
 24. Shirazi-Adl SA, Shrivastava SC, Ahmed AM : Stress analysis of the lumbar disc-body unit in compression. A three-dimensional nonlinear finite element study. **Spine (Phila Pa 1976)** 9 : 120-134, 1984
 25. Thomsen K, Christensen FB, Eiskjaer SP, Hansen ES, Fruensgaard S, Bünger CE : 1997 Volvo Award winner in clinical studies. The effect of pedicle screw instrumentation on functional outcome and fusion rates in posterolateral lumbar spinal fusion : a prospective, randomized clinical study. **Spine (Phila Pa 1976)** 22 : 2813-2822, 1997
 26. Vadapalli S, Sairyo K, Goel VK, Robon M, Biyani A, Khandha A, et al. : Biomechanical rationale for using polyetheretherketone (PEEK) spacers for lumbar interbody fusion-a finite element study. **Spine (Phila Pa 1976)** 31 : E992-E998, 2006
 27. Xiao Z, Wang L, Gong H, Zhu D : Biomechanical evaluation of three surgical scenarios of posterior lumbar interbody fusion by finite element analysis. **Biomed Eng Online** 11 : 31, 2012
 28. Yamamoto I, Panjabi MM, Crisco T, Oxland T : Three-dimensional movements of the whole lumbar spine and lumbosacral joint. **Spine (Phila Pa 1976)** 14 : 1256-1260, 1989
 29. Zhong ZC, Wei SH, Wang JP, Feng CK, Chen CS, Yu CH : Finite element analysis of the lumbar spine with a new cage using a topology optimization method. **Med Eng Phys** 28 : 90-98, 2006