



POSTER PRESENTATION

Open Access

# Stiffness-matched segmented metallic guidewire for interventional cardiovascular MRI


Burcu Basar<sup>1,2\*</sup>, Adrienne E Campbell-Washburn<sup>1</sup>, Toby Rogers<sup>1</sup>, Merdim Sonmez<sup>1</sup>, Anthony Z Faranesh<sup>1</sup>, Kanishka Ratnayaka<sup>1</sup>, Robert J Lederman<sup>1</sup>, Ozgur Kocaturk<sup>1,2</sup>

From 18th Annual SCMR Scientific Sessions  
Nice, France. 4-7 February 2015

## Background


Conductive guidewires and intravascular catheters are at risk of RF-induced heating under MRI [1]. Heating is found predominantly at the tip of conductive wires [2], and is modulated by wire diameter, length and insulation

thickness [3]. Non-conductive materials, such as polymer, impart unsatisfactory mechanical properties on guidewires in terms of flexibility, stiffness, and torquability, for navigating tortuous cardiovascular structures and for safely delivering catheter devices.

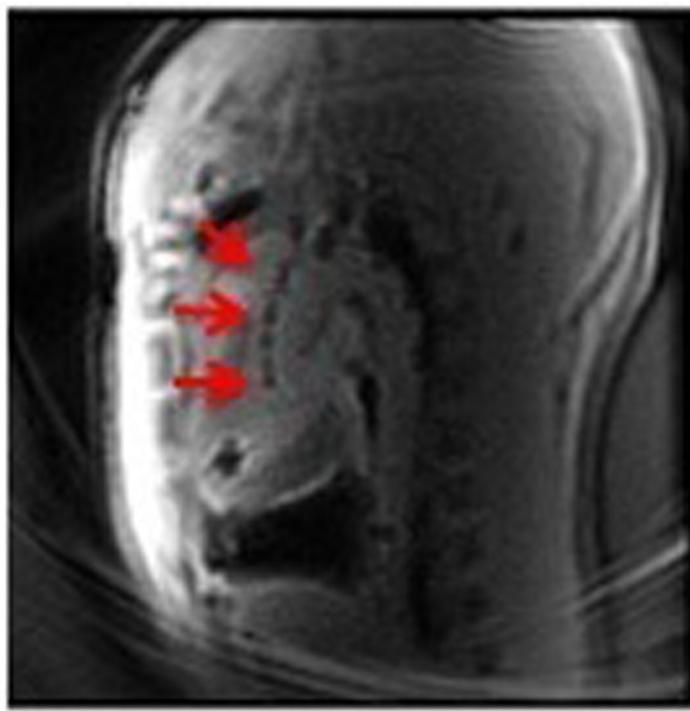

**Figure 1 In vivo left heart catheterization in swine using MRI safe guidewire design.** Iron-oxide markers on device tip shown with red arrows. TE/TR=1.9/4.2 ms, slice thickness=6mm, matrix=192x192, flip angle=15.

<sup>1</sup>Division of Intramural Research, National Heart, Lung and Blood Institute, National Institutes of Health, Bethesda, MD, USA  
Full list of author information is available at the end of the article

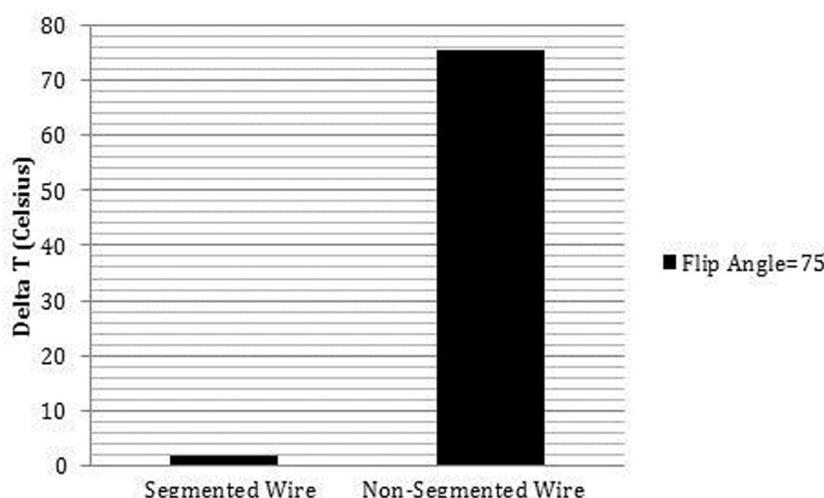

**Figure 2** Deviation from baseline temperature readings acquired over 30 seconds prior to scanning during *in-vitro* heating experiments.

We developed a novel MRI guidewire design that avoids RF heating yet preserves the mechanical features of conventional X-ray guidewires. Short non-resonant segments of nitinol are connected using stiffness-matched insulated notched couplers, preventing standing wave formation yet appearing mechanically indistinguishable from nitinol guidewires.

## Methods

The core of a passive 120cm guidewire was constructed from nitinol rod segments shorter than a quarter-wavelength *in vivo* at 1.5T (10cm). The segments were joined by electrically insulated nitinol tubes. A surrounding outer braided polymer enhanced torque response, insulation and safety. The distal tip was insulated using non-braided polymer and low durometer thermoplastic polymer for flexibility and trackability. Iron-oxide markers created MRI susceptibility artifacts for enhanced visualization *in vivo* in a swine (Fig 1).

RF heating was measured in an ASTM F2182 gel phantom. Tip and shaft temperature was measured using a fiber optic probe (*OpSense*) at 1.5T (*Aera*, Siemens) [4]. Heating was measured at high flip angle (75°) bSSFP (TR/TE, 2.88/1.44 ms; thickness, 6 mm; FOV, 350×350 mm; matrix, 192×144) and compared to a custom non-segmented nitinol core wire with identical jacketing serving as a control.

## Results

The segmented MRI guidewire exhibited a maximum temperature increase of 1.6°C at the tip, compared with 74°C for the non-segmented comparator, during a 60s scan at a flip angle of 75° (Fig 2). Systematic temperature measurements along the shaft detected negligible

heating, confirming successful electrical insulation by the inter-segment connectors. Trackability in a tortuous vascular phantom resembled commercial comparators (*Glidewire*, Terumo).

## Conclusions

We demonstrate a simple and intrinsically safe new design for passive metallic MRI guidewires. The guidewire exhibits negligible heating at high flip angles in conformance with ISO standards (<2°C) [5], yet mechanically resembles a high-performance conventional metallic guidewire. This may represent a significant advance once applied in clinical MRI catheterization.

## Funding

Supported by NHLBI Z01-HL006041. BB, OK, and RJL are co-inventors on patent applications assigned to NIH.

## Authors' details

<sup>1</sup>Division of Intramural Research, National Heart, Lung and Blood Institute, National Institutes of Health, Bethesda, MD, USA. <sup>2</sup>Institute of Biomedical Engineering, Bogazici University, Istanbul, Turkey.

Published: 3 February 2015

## References

1. Yeung: *Magn Reson Imaging* 2002, **47**:187-193.
2. Nitz: *J Magn Reson Imaging* 2001, **13**:105-114.
3. Weiss: *Magnet Reson Med* 2005, **54**:182-189.
4. Sonmez: *J Cardiov Mag Reson* 2012, **14**:38.
5. ISO/TS 10974 2012.

doi:10.1186/1532-429X-17-S1-P414

Cite this article as: Basar et al.: Stiffness-matched segmented metallic guidewire for interventional cardiovascular MRI. *Journal of Cardiovascular Magnetic Resonance* 2015 **17**(Suppl 1):P414.