



Evaluation of marginal discrepancy of pressable ceramic veneer fabricated using CAD/CAM system: Additive and subtractive manufacturing

Seen-Young Kang, Ha-Na Lee, Ji-Hwan Kim, Woong-Chul Kim*

Department of Dental Laboratory Science and Engineering, College of Health Science, Korea University, Seoul, Republic of Korea

PURPOSE. The purpose of this study was to evaluate the marginal discrepancy of heat-pressed ceramic veneers manufactured using a CAD/CAM system. **MATERIALS AND METHODS.** The ceramic veneers for the abutment of a maxillary left central incisor were designed using a CAD/CAM software program. Ten veneers using a micro-stereolithography apparatus (AM group), ten veneers using a five-axis milling machine (SM group), and ten veneers using a traditional free-hand wax technique (TW group) were prepared according to the respective manufacturing method. The ceramic veneers were also fabricated using a heat-press technique, and a silicone replica was used to measure their marginal discrepancy. The marginal discrepancies were measured using a digital microscope ($\times 160$ magnification). The data were analyzed using a nonparametric Kruskal-Wallis H test. Finally, post-hoc comparisons were conducted using Bonferroni-corrected Mann-Whitney U tests ($\alpha=.05$).

RESULTS. The mean \pm SD of the total marginal discrepancy was 99.68 ± 28.01 μm for the AM group, 76.60 ± 28.76 μm for the SM group, and 83.08 ± 39.74 μm for the TW group. There were significant differences in the total marginal discrepancies of the ceramic veneers ($P<.05$). **CONCLUSION.** The SM group showed a better fit than the AM and TW groups. However, all values were within the clinical tolerance. Therefore, CAD/CAM manufacturing methods can replace the traditional free-hand wax technique. [*J Adv Prosthodont 2018;10:347-53*]

KEYWORDS: Additive manufacturing; Subtractive manufacturing; Computer-aided design and computer-aided machining (CAD/CAM); Ceramic veneer; Heat pressing

INTRODUCTION

The ceramic veneer restoration around an anterior area has recently attracted attention owing to the increased demand for better esthetics and reduced psychological burden of tooth removal. Ceramic veneers have been an area of focus

in the restoration of dental esthetics.¹⁻³

Among the different types of materials used for such esthetics, lithium disilicate glass matrix ceramics have been widely used owing to their superior appearance, mechanical characteristics, adhesive cementation, and adequate marginal adaptation.⁴ Lithium disilicate ceramic restorations are manufactured by initially shaping a pattern, and then applying heat pressing to a ceramic ingot.⁵ Therefore, the state of the pattern is thought to be one of the important factors affecting the quality of ceramic veneers after heat pressing.

Patterns applied for lithium disilicate ceramic veneers have thus far been manufactured using a traditional free-hand wax-up method, in which the wax is carved by the dental technician. Such wax has a high coefficient of thermal expansion, and shrinks by 0.4% when carving a wax pattern and by 0.2% during the burnout.^{5,6} In addition, the skills of those manufacturing the wax patterns influence their fit, particularly the fit of the final ceramic veneer, which can be problematic.

Corresponding author:
Woong-Chul Kim
Department of Dental Laboratory Science and Engineering, College of Health Science, Korea University, 145, Anam-ro, Seongbuk-gu, Seoul 02841, Republic of Korea
Tel. +82232905665; e-mail, kuc2842@korea.ac.kr
Received December 14, 2017 / Last Revision July 25, 2018 / Accepted September 29, 2018

© 2018 The Korean Academy of Prosthodontics
This is an Open Access article distributed under the terms of the Creative Commons Attribution Non-Commercial License (<http://creativecommons.org/licenses/by-nc/3.0>) which permits unrestricted non-commercial use, distribution, and reproduction in any medium, provided the original work is properly cited.

This study was supported by Korea University Grant (K1716861).

A computer-aided design and computer-aided machining (CAD/CAM) system has been introduced and widely used for manufacturing patterns for lithium disilicate ceramic restoration.⁶ Additive and subtractive manufacturing methods are used in the creation of patterns using a CAD/CAM system.⁷

Additive manufacturing, patterns are often manufactured using a micro-stereolithography apparatus (Micro-SLA system). The photo-curable resin used for this system is generally a mixture of an oligomer, a monomer, and a photo-initiator, and has lower polymerization shrinkage and superior reproduction.⁸ In the actual pattern manufacturing, a prototype pattern is achieved by accumulating resins with thicknesses of 0.025 - 0.05 mm for each layer, and continuously laminating at a point unit through UV irradiation on the surface of a photopolymer liquid.

However, with subtractive manufacturing, materials in a wax block form are cut and processed to manufacture the patterns. A five-axis milling machine is often used to manufacture veneer patterns. A five-axis milling machine can be freely processed beneath the cut and has the advantage of high processing precision, allowing the milling bur to approach the processed parts in rectangular directions.

Fit is a very important aspect for a ceramic veneer to function over a long period in an oral cavity. If the fit of a ceramic veneer is poor, certain problems, including fracture of the restoration, an early elimination and even esthetic degradation from peripheral stains, may occur.^{3,9,10}

The marginal discrepancy between the prosthesis and abutment is usually measured for the fit of a ceramic veneer.^{3,11} There have been many studies on the marginal fit of general fixed prostheses. However, only a few studies investigated the marginal fit of ceramic veneers manufactured by CAD/CAM system. Moreover, few studies are about the differences in marginal fit depending on the application of additive or subtractive manufacturing, both of which are used in a CAD/CAM system, and on the use of a traditional free-hand wax-up method.

Therefore, the purpose of this study was to comparatively analyze the differences in the marginal discrepancies of ceramic veneers manufactured using additive and subtractive processing technologies of a CAD/CAM system, as well as a traditional free-hand wax-up method.

The null hypothesis of this study is that there are no differences in the marginal discrepancies of ceramic veneers based on the different pattern manufacturing methods applied.

MATERIALS AND METHODS

A maxillary left incisor (Model PE-PRO 001, Nissin Dental products, Inc., Kyoto, Japan) model was prepared to manufacture the ceramic veneers. To manufacture the study models, an impression was then made using both light-body (Aquasil Ultra XLV Regular Set, Dentsply Detrey GmbH, Konstanz, Germany) and heavy-body (Aquasil Ultra Rigid Regular Set, Dentsply Detrey GmbH, Konstanz, Germany) silicone (Fig. 1).

To manufacture patterns using a traditional free-hand wax-up method, a two-layer die spacer (Nice Fit, Shofu, Inc., Kyoto, Japan) was applied to the surface of type IV study models, where the thickness of the die spacer on the surface was about 20 μm . An adequate outward shape was then carved through a free-hand wax-up technique using modeling wax (Geo Wax, Renfert GmbH, Hilzingen, Germany). A total of ten wax-pattern veneers were acquired, and a single skillful experimenter conducted the carving for consistency.

Meanwhile, to manufacture the patterns using additive and subtractive manufacturing methods, working models were scanned using a lab scanner (Identica Blue, Medit, Seoul, Korea). From the scanned stereolithography, an STL file was used to design the outer shape of the upper-left incisor using the CAD software (Exocad DentalCAD, Exocad GmbH, Darmstadt, Germany). The cement spacing was set to 20 μm .

For the additive manufacturing, 3-D printing was conducted by applying an STL file to a μ -SLA (ProJet 1200, 3D systems, Rock Hill, SC, USA) system.^{4,12} During the printing process, a laminate veneer was produced through UV irradiation of a polymerized plastic cartridge resin (VisiJet FTX Green, 3D systems, Rock Hill, SC, USA). In addition, three patterns were allowed to be arranged on a single platform.¹³ Then, the resin pattern of the laminate veneer was further hardened using a UV lamp for 10 minutes.

For the subtractive manufacturing, an STL file was applied to a dental CAM software program (Hyperdent, Open Mind Technologies AG, Wessling, Germany) to calculate the tool path. The results of the calculated tool path were stored in the numerical control (NC) data. A total of ten wax patterns were acquired through milling on a five-axis milling device (DWX-50, Roland DG Corporation, Shizuoka, Japan) using the stored NC file. In addition, a wax block (Vipi Block wax, Vipi, Pirassununga, Brazil) dedicated to milling applications was used as the milling material.

Vacuum investing of a total 30 of pattern samples manufactured using the three methods was conducted with phosphate-bonded investments (Prime vest HS, BK Giuliani, Ludwigshafen, Germany), and the samples were hardened for 1 hour, as suggested by the manufacturer. The investment ring was cast at 850°C for 1 hour and 20 minutes. A ceramic ingot (IPS e.max Press LT, Ivoclar Vivadent, Schaan, Liechtenstein) was injected into the inlet of the cast investment ring. After being combined with a plunger, heat pressing was applied in a vacuum porcelain furnace (EP 600, Ivoclar Vivadent, Schaan, Liechtenstein) at 850°C for 18 minutes. The investment ring was slowly cooled to room temperature. After removal of the investment, the inner silicon dioxide film and any impurities were eliminated by applying a sand blasting method with 4 bars into the inner part of the shaped ceramic veneer using a glass bead consisting of 50 μm particles.

A silicone replica technique was used to measure the marginal discrepancy. To this end, the master model fitting was conducted by injecting light-body silicone (Aquasil

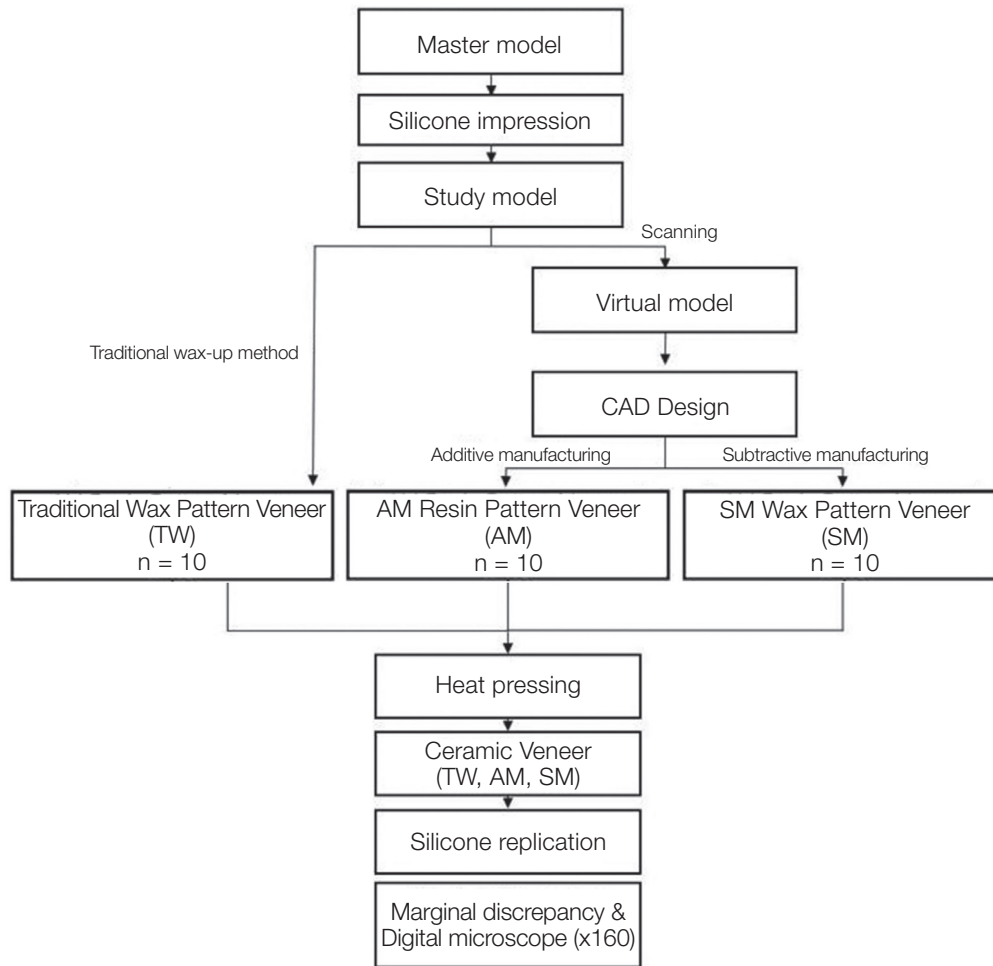


Fig. 1. Study flow.

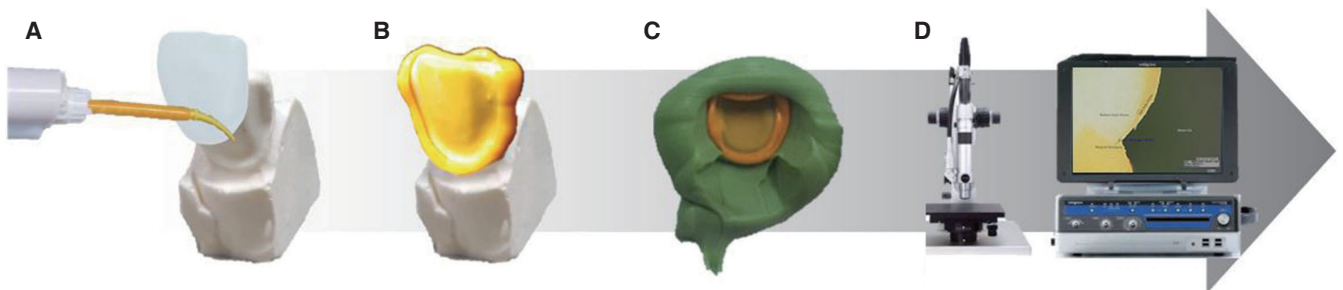


Fig. 2. Silicone replica technique processing for measurement of marginal discrepancy: (A) silicone injection (B) silicone replica inner surface (C) fixed with medium body silicone (D) measurement with digital microscope.

Ultra XLV Regular Set, Dentsply Detrey GmbH, Konstanz, Germany) into the inner surface of the ceramic veneer. Then, a light-body silicone film layer was manufactured by applying a finger pressure of about 20 N. This layer was then fixed using heavy body silicone (Aquasil Ultra Rigid Regular Set, Dentsply Detrey GmbH, Konstanz, Germany).¹²

Twelve areas were measured, which were designated and cross-sectioned by dividing the silicone replica mold into buccal, lingual, distal, and mesial areas. Finally, the marginal discrepancy was measured using a digital microscope (KH-7700, Hirox, Hackensack, NJ, USA) (Fig. 2, Fig. 3, Fig. 4).

A statistical analysis of the measurements was conduct-

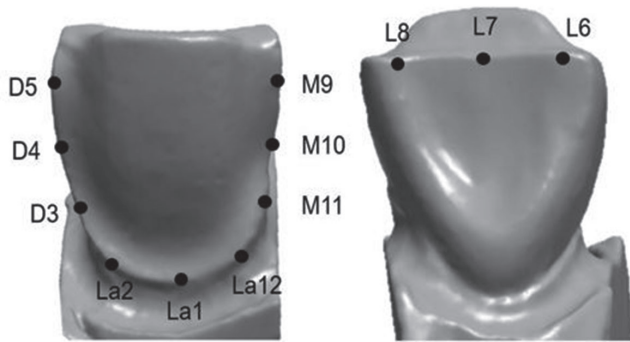


Fig. 3. Measurement areas of marginal discrepancy: labial areas = (La1, La2, La12), distal area = (D3, D4, D5), mesial area = (M9, M10, M11), lingual area = (L6, L7, L8).

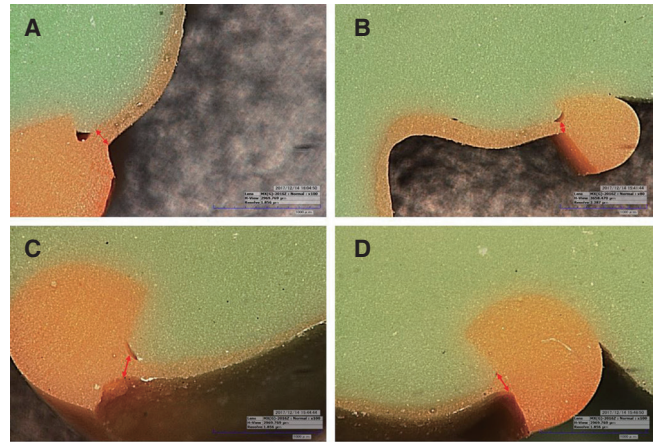


Fig. 4. Cross-sections of silicone replica using digital microscope (original magnification 160×): (A) labial margin (B) lingual margin (C) mesial margin (D) distal margin.

ed using statistical software (IBM Statistics for Windows, v23.0, IBM Corp). To test the regularity of the marginal discrepancy in the measured areas, depending on manufacturing methods, Shapiro-Wilk and Kolmogorov-Smirnov tests were conducted; however, the results did not indicate a normal distribution ($P < .05$). Therefore, a nonparametric Kruskal-Wallis test and a Mann-Whitney U Test were conducted, adjusting the significance using the Bonferroni method, which is an ex-post analysis technique.

RESULTS

The marginal discrepancy results are shown in Table 1 to Table 5. The means, standard deviations, maxima, minima, medians, and confidence intervals are shown in the tables, along with the statistical significance of each measurement.

As shown in Table 1, the TW group had the largest mean value of the labial discrepancy, $90.79 \pm 47.61 \mu\text{m}$, whereas SM group had the lowest value, $65.96 \pm 26.34 \mu\text{m}$, suggesting a significant difference in the labial discrepancies between the two groups ($P < .002$).

As shown in Table 2, the AM group had the largest mean value of distal discrepancy, $86.87 \pm 17.09 \mu\text{m}$, whereas the TW group had lowest value, $63.93 \pm 33.84 \mu\text{m}$, suggesting a significant difference in the distal discrepancies between the two groups ($P < .001$).

As shown in Table 3, the AM group had the largest mean value of mesial discrepancy, $101.79 \pm 25.09 \mu\text{m}$, whereas the SM group had the lowest value, $81.12 \pm 29.43 \mu\text{m}$, suggesting a significant difference in the mesial discrepancies between the two groups ($P < .019$).

As shown in Table 4, the AM group had the largest mean value of lingual discrepancy, $119.32 \pm 29.46 \mu\text{m}$, whereas the SM group had the lowest value, $76.60 \pm 28.76 \mu\text{m}$, suggesting a significant difference in the lingual discrepancies between the two groups ($P < .001$).

Table 5 shows the total mean \pm standard deviation of the marginal discrepancies. The AM group had the largest value at $99.68 \pm 28.01 \mu\text{m}$, followed by the TW group at $83.08 \pm 39.74 \mu\text{m}$, and the SM group at $76.60 \pm 28.76 \mu\text{m}$. The results indicate statistically significant differences among these groups ($P < .001$).

Table 1. Mean, standard deviation (SD), maximum (Max), minimum (Min), median (Med), confidence interval (CI) of descriptive statistics of lingual marginal discrepancies in ceramic veneers (unit: μm)

Group	Labial marginal discrepancy						95% CI		P value
	Mean	SD	Max	Min	Med	Lower	Upper		
AM	90.75 ^a	27.82	168.90	41.20	91.80	80.35	101.14	$P < .002$	
SM	86.87 ^b	17.09	137.00	35.20	58.10	56.12	75.79		
TW	90.79 ^a	47.61	200.00	41.20	74.45	73.01	108.57		

AM: additive manufacturing; SM; subtractive manufacturing; TW: traditional free-hand wax-up
Values in the ^{a,b} column represent statistically significant differences ($P < .05$).

Table 2. Mean, standard deviation (SD), maximum (Max), minimum (Min), median (Med), confidence interval (CI) of descriptive statistics of distal marginal discrepancies in ceramic veneers (unit: μm)

Group	Distal marginal discrepancy							P value
	Mean	SD	Max	Min	Med	95% CI		
						Lower	Upper	
AM	86.87 ^a	26.34	117.40	46.20	86.05	80.49	93.26	<i>P</i> < .001
SM	66.40 ^b	14.87	114.50	48.90	64.10	60.84	71.95	
TW	63.93 ^b	33.84	145.10	27.90	53.30	51.29	76.57	

AM: additive manufacturing; SM: subtractive manufacturing; TW: traditional free-hand wax-up
 Values in the ^{a,b} column represent statistically significant differences (*P* < .05).

Table 3. Mean, standard deviation (SD), maximum (Max), minimum (Min), median (Med), confidence interval (CI) of descriptive statistics of mesial marginal discrepancies in ceramic veneers (unit: μm)

Group	Mesial marginal discrepancy							P value
	Mean	SD	Max	Min	Med	95% CI		
						Lower	Upper	
AM	101.79 ^a	25.05	171.40	60.90	99.35	92.43	111.14	<i>P</i> < .001
SM	81.12 ^b	29.43	150.10	38.70	71.90	70.13	92.10	
TW	88.39 ^b	32.96	167.60	34.30	89.9	76.08	100.70	

AM: additive manufacturing; SM: subtractive manufacturing; TW: traditional free-hand wax-up
 Values in the ^{a,b} column represent statistically significant differences (*P* < .05).

Table 4. Mean, standard deviation (SD), maximum (Max), minimum (Min), median (Med), confidence interval (CI) of descriptive statistics of lingual marginal discrepancies in ceramic veneers (unit: μm)

Group	Lingual marginal discrepancy							P value
	Mean	SD	Max	Min	Med	95% CI		
						Lower	Upper	
AM	119.32 ^a	29.49	219.40	74.40	110.50	108.30	130.33	<i>P</i> < .019
SM	92.92 ^b	33.06	158.20	43.40	88.65	80.57	105.26	
TW	89.20 ^b	38.39	163.60	22.60	78.00	74.86	103.53	

AM: additive manufacturing; SM: subtractive manufacturing; TW: traditional free-hand wax-up
 Values in the ^{a,b} column represent statistically significant differences (*P* < .05).

Table 5. Mean, standard deviation (SD), maximum (Max), minimum (Min), median (Med), confidence interval (CI) of total marginal discrepancies in ceramic veneers (unit: μm)

Group	Total marginal discrepancy							P value
	Mean	SD	Max	Min	Med	95% CI		
						Lower	Upper	
AM	99.68 ^a	28.01	219.40	41.20	98.85	94.62	104.74	<i>P</i> < .001
SM	76.60 ^b	28.76	158.20	35.2	66.55	71.40	81.80	
TW	83.08 ^b	39.74	200.00	22.6	73.65	75.89	90.26	

AM: additive manufacturing; SM: subtractive manufacturing; TW: traditional free hand wax-up
 Values in the ^{a,b} column represent statistically significant differences (*P* < .05).

DISCUSSION

In dental science, the use of digital imaging through a CAD/CAM system has recently increased. A shift from analogue to digital-based methods has also occurred in medical treatments as well as the manufacturing of prostheses. As part of this period of transition, the clinical availability of a digital-based method using a CAD/CAM system rather than an analog-based system in the manufacturing of ceramic veneer patterns was examined in the present study.

In this study, the null hypothesis that the marginal fit is unaffected by the processing method used for generating patterns for ceramic veneers was rejected ($P < .05$).

A total of 20 ceramic veneers manufactured using additive and subtractive techniques were used as the experimental group, and for a comparison with the experimental manufacturing group, ten ceramic veneers of the same form were created as the control group using a traditional free-hand wax-up method. The marginal discrepancy was measured on a total of 360 points (12 points for each sample), thereby increasing the reliability of the 30 samples.

This study used a silicone replica technique to measure the marginal discrepancy. This silicone replica technique, which measures the thickness of the inner surface by filling light-body silicone into a prosthesis, is widely used in measurements of marginal discrepancy because it can prevent damage to the prosthesis and the occurrence of an abutment.^{12,14}

There has been no consensus on the values or criteria of the fit of a prosthesis clinically allowed by the dental community. Although the American Dental Association states in ADA No. 8¹⁵ that the proper fit of a fixed prosthesis ranges from 25 to 40 μm , it is impossible to reach such a goal using current manufacturing technology. Sulaiman suggested 100 μm ¹⁶ and McLean and von Fraunhofer suggested 120 μm for a clinically proper peripheral fit of a fixed prosthesis,¹⁷ whereas Vojdani proposed a range of 200 to 300 μm .¹⁸ Notwithstanding, many researchers have recently reported that a range of less than 120 μm is proper and can be clinically accepted, and thus the present study suggests that a discrepancy of less than 120 μm is clinically allowable.

As shown in Table 5, the mean value of the marginal discrepancy of the SM group was superior to those of the AM and LW groups, with statistical significance ($P < .001$). Notwithstanding, the mean values of the three groups, as well as the marginal discrepancies in the four measured areas, buccal, lingual, distal, and mesial, were within the allowable limit of less than 120 μm (Table 1, Table 2, Table 3, Table 4).

The AM and SM groups were uniformly manufactured using an automated system. However, the difference between the AM and SM groups varied based on the axis applied. For the SM group, a five-axis milling machine was used, which has a complex form because a straight feeding axis for the x-, y-, and z-axis and two rotation feed axes of a and b were added; in addition, it was able to achieve more precise cutting in areas under the cut.¹⁹ The AM group was

manufactured using three-axis 3D printing technology, which is less accurate than a five-axis machine, and was therefore thought to affect the marginal discrepancy.²⁰ In addition, a layering error, which typically appears during the lamination process, can occur. For this reason, the optical diffraction increased as the UV source irradiated a wide area of resin through a mirror.¹² Such a pattern also appeared similarly in preliminary studies. Therefore, the fit of the resin is not only reduced, but the fit of the final completed ceramic veneer can vary owing to shrinkage of the polymerized resin.

Hence, a five-axis milling machine is recommended for manufacturing ceramic veneer patterns. Although many factors are thought to have an effect on the findings, more studies on Micro SLA are required in particular because its marginal discrepancy is higher than that of the milling process or the traditional free-hand wax-up method. For the SM group, it is believed that the existing wax-up technique can be replaced with current digital processing methods.

However, this study also has certain limitations. First, although the measurement of a silicone replica technique is known to have high accuracy and reliability, it may be difficult to exclude the shrinkage and expansion of the silicone. Second, the abutment used in this study is a standard die but may be clinically improper. Third, although a skillful researcher tried to maintain consistency when applying the traditional wax-up method, there is a limit in controlling the experimental error.

In further studies, other forms of abutments should be applied; in particular, a clinical evaluation of the inside of a patient's oral cavity should be additionally conducted.

CONCLUSION

Despite various advantages of dental technologies, the most important aspect is the completion of the manufactured device. The SM veneer showed better values than AM and TW veneers. Although the marginal discrepancy of the ceramic veneers manufactured in this study varied significantly according to the manufacturing methods used, the range, which was less than 120 μm , is suitable for clinical applications.

ORCID

Woong-Chul Kim <https://orcid.org/0000-0002-6730-4960>

REFERENCES

1. Marchionatti AME, Wandscher VF, May MM, Bottino MA, May LG. Color stability of ceramic laminate veneers cemented with light-polymerizing and dual-polymerizing luting agent: A split-mouth randomized clinical trial. *J Prosthet Dent* 2017;118:604-10.
2. Peumans M, De Munck J, Fieuws S, Lambrechts P, Vanherle G, Van Meerbeek B. A prospective ten-year clinical trial of porcelain veneers. *J Adhes Dent* 2004;6:65-76.

3. Aboushelib MN, Elmahy WA, Ghazy MH. Internal adaptation, marginal accuracy and microleakage of a pressable versus a machinable ceramic laminate veneers. *J Dent* 2012;40:670-7.
4. Shamseddine L, Mortada R, Rifai K, Chidiac JJ. Fit of pressed crowns fabricated from two CAD-CAM wax pattern process plans: A comparative in vitro study. *J Prosthet Dent* 2017;118:49-54.
5. Ural C, Burgaz Y, Saraç D. In vitro evaluation of marginal adaptation in five ceramic restoration fabricating techniques. *Quintessence Int* 2010;41:585-90.
6. Homsy FR, Özcan M, Khoury M, Majzoub ZAK. Marginal and internal fit of pressed lithium disilicate inlays fabricated with milling, 3D printing, and conventional technologies. *J Prosthet Dent* 2018;119:783-90.
7. van Noort R. The future of dental devices is digital. *Dent Mater* 2012;28:3-12.
8. Stampfl J, Baudis S, Heller C, Liska R, Neumeister A, Kling R, Ostendorf A, Spitzbart M. Photopolymers with tunable mechanical properties processed by laser-based high-resolution stereolithography. *J Micromech Microeng* 2008;18:125014.
9. Hamza TA, Ezzat HA, El-Hossary MM, Katamish HA, Shokry TE, Rosenstiel SF. Accuracy of ceramic restorations made with two CAD/CAM systems. *J Prosthet Dent* 2013;109:83-7.
10. Neves FD, Prado CJ, Prudente MS, Carneiro TA, Zancopé K, Davi LR, Mendonça G, Cooper LF, Soares CJ. Micro-computed tomography evaluation of marginal fit of lithium disilicate crowns fabricated by using chairside CAD/CAM systems or the heat-pressing technique. *J Prosthet Dent* 2014;112:1134-40.
11. Lin TM, Liu PR, Ramp LC, Essig ME, Givan DA, Pan YH. Fracture resistance and marginal discrepancy of porcelain laminate veneers influenced by preparation design and restorative material in vitro. *J Dent* 2012;40:202-9.
12. Park JY, Bae SY, Lee JJ, Kim JH, Kim HY, Kim WC. Evaluation of the marginal and internal gaps of three different dental prostheses: comparison of the silicone replica technique and three-dimensional superimposition analysis. *J Adv Prosthodont* 2017;9:159-69.
13. Kim DY, Jeon JH, Kim JH, Kim HY, Kim WC. Reproducibility of different arrangement of resin copings by dental microstereolithography: Evaluating the marginal discrepancy of resin copings. *J Prosthet Dent* 2017;117:260-5.
14. Sakornwimon N, Leevailoj C. Clinical marginal fit of zirconia crowns and patients' preferences for impression techniques using intraoral digital scanner versus polyvinyl siloxane material. *J Prosthet Dent* 2017;118:386-91.
15. Association AD. ANSI/ADA Specification No. 8 for zinc phosphate cement. Guide to dental materials and devices. 5th ed Chicago; ADA; 1970-1.
16. Sulaiman F, Chai J, Jameson LM, Wozniak WT. A comparison of the marginal fit of In-Ceram, IPS Empress, and Procera crowns. *Int J Prosthodont* 1997;10:478-84.
17. McLean JW, von Fraunhofer JA. The estimation of cement film thickness by an in vivo technique. *Br Dent J* 1971;131:107-11.
18. Vojdani M, Torabi K, Farjood E, Khaledi A. Comparison the Marginal and Internal Fit of Metal Copings Cast from Wax Patterns Fabricated by CAD/CAM and Conventional Wax up Techniques. *J Dent (Shiraz)* 2013;14:118-29.
19. Abduo J, Lyons K, Bennamoun M. Trends in computer-aided manufacturing in prosthodontics: a review of the available streams. *Int J Dent* 2014;2014:783948.
20. Al-Imam H, Gram M, Benetti AR, Gotfredsen K. Accuracy of stereolithography additive casts used in a digital workflow. *J Prosthet Dent* 2018;119:580-5.