

A New Method for Pseudo-increasing Frame Rates of Echocardiography Images Using Manifold Learning

Parisa Gifani, Hamid Behnam, Zahra Alizadeh Sani¹

Departments of Biomedical Engineering, Iran University of Science and Technology, ¹Cardiac Imaging, Rajaei Cardiovascular Medical and Research Center, Tehran, Iran

ABSTRACT

Increasing frame rate is a challenging issue for better interpretation of medical images and diagnosis based on tracking the small transient motions of myocardium and valves in real time visualization. In this paper, manifold learning algorithm is applied to extract the nonlinear embedded information about echocardiography images from the consecutive images in two dimensional manifold spaces. In this method, we presume that the dimensionality of echocardiography images obtained from a patient is artificially high and the images can be described as functions of only a few underlying parameters such as periodic motion due to heartbeat. By this approach, each image is projected as a point on the reconstructed manifold; hence, the relationship between images in the new domain can be obtained according to periodicity of the heart cycle. To have a better tracking of the echocardiography, images during the fast motions of heart we have rearranged the similar frames of consecutive heart cycles in a sequence. This provides a full view slow motion of heart movement through increasing the frame rate to three times the traditional ultrasound systems.

Key words: Echocardiography images, frame rate, Locally linear embeddings algorithm, manifold learning

INTRODUCTION

Echocardiography is one of the widely used diagnostic tools in the imaging world, because it is noninvasive, safe, and inexpensive; it also allows real-time visualization of the size and shape of the heart, its pumping capacity and the location and extent of any damage in its tissues.

An important issue in echocardiography is to track the rapid variations of myocardium and heart valves in real time. Thus, it is necessary to have a high frame rate imaging system to illustrate the fast moving structures.

A real time ultrasound image is made up of many information lines obtained in a very short period of time. Typical number of lines in the field of view ranges from about 100 to over 200 lines per frame. There exist a proper number of lines to have a good lateral resolution. In an ordinary cardiac imaging, by considering 128 lines per frame, 20 cm depth and 1500 m/s for the speed of sound, the maximum frame rate is around 30 (frames/sec). But for fast moving structures, such as heart valves, a frame rate up to 80 (frames/sec) may be required. For fetal echocardiography and small animal imaging, where typically high heart rates take place, high frame-rate and full-view ultrasound imaging is an emerging topic, but it is a challenging issue

in echocardiography of adult.^[1] Some simple methods for increasing the frame rate are expressed in literatures. Konofagou *et al.*^[2] and D'hooge *et al.*,^[3] increased the frame rate to above 200 Hz by reducing the view angle and decreasing the number of lines in a sector. Applying this method, the time needed to construct the whole image reduced and the frame rate increased. Kanai *et al.*^[4,5] used a sparse sector-scan format. He achieved the peak frame rate of 450 Hz by decreasing the number of ultrasound beams to a value about 16. However, reducing the field of view was not suitable for full-view cardiac imaging. Also, the lateral resolution was decreased proportional to the number of lines.

Wang *et al.*^[6] proposed a high frame rate imaging technique based on ECG gating and retrospective multi-sector composite method. Other developed methods for increasing the frame rate are coded-excitation ultrasound imaging,^[7] parallel beam forming technique^[8] and synthetic aperture (SA) ultrasound imaging.^[9] However, these methods require complicated calculations.

In this paper, a new method based on considering cyclic movement of the heart using manifold learning algorithm for increasing frame rates of echocardiography images is proposed. Manifold learning is a recently introduced

Address for correspondence:

Dr. Hamid Behnam, School of Electrical Engineering, Iran University of Science & Technology (IUST), Hengam Ave., Resalat Squ., Tehran 16844, Iran. E-mail: behnam@iust.ac.ir

approach in nonlinear dimension reduction which can extract the relationship between frames of consecutive images in low-dimensional space.^[10,11] Image manifolds have been shown to be useful representation tools for magnetic resonance imaging (MRI) sequences,^[12-15] facial images,^[16,17] and tracking.^[18-20]

The paper is organized as follows. The 'method' section gives a brief background in manifold learning and followed by a description of LLE^[11] (Locally Linear Embeddings) algorithm which is used. Embedding echocardiography images and increasing the frame rate using manifold learning is explained in sections four and five, respectively. Benefits and limitations of this research are summarized in the 'conclusion' section.

MATERIALS AND METHODS

Dimensionality reduction is important in machine learning for simplifying of analyzing large data sets in classification, compression, and visualization of high dimensional data.

Multidimensional scaling (MDS)^[21] and principal component analysis (PCA)^[22] are the traditional linear techniques for dimensionality reduction. These methods often fail to discover complex nonlinear data structures. Various studies have shown that nonlinear techniques outperform their linear counterparts in highly nonlinear artificial tasks.^[15] Manifold learning is a recent approach for nonlinear dimensionality reduction. A lot of data sets often consist of a large number of samples, each of which involves many features. Manifold learning algorithms attempt to uncover intrinsic parameters in order to find a low-dimensional representation of the data. We can refer to Isomap,^[10] LLE,^[11,23] Laplacian embeddings,^[24] and Local Tangent Space Alignment (LTSA)^[25] as examples of manifold learning algorithms.

In cardio-pulmonary imaging, the dimensionality of a frame in a video sequence – which usually considered as number of pixels in a frame – is normally a large value. But, in fact, frame variations of a particular patient can be small due to the deformation caused by the patient's heartbeat, imaging geometry, noise and time-varying effects of contrast agents. Accordingly, when there are only a few comprising causes of the variation, these images naturally have a low dimensional structure which can be extracted by manifold learning algorithms. As some applications, manifold embedding is applied to segmentation,^[12,13] interpolation,^[14] and noise reduction^[15] of cardiac MRI images.

In echocardiography, images which are taken with the same imaging geometry of the same patient have one principle degree of freedom and that is the phase of the heartbeat. Indeed, changes in the heartbeat phase lead to

variations in the shape of the heart, but not to its position dominantly. Hence, manifold learning can depict each image as a point on the reconstructed manifold and the relationship between images in the new domain can be obtained according to periodicity of the heart cycle.^[26,27] The main trait of LLE algorithm is that similar frames in high-dimensional space retain their neighborhoods in low-dimension space too.^[11,23] Accordingly, we choose this algorithm as a proper one in manifold learning algorithms. In the next section, we briefly introduce the principles of this algorithm.

LLE Algorithm

LLE algorithm transforms N observations of X data set with dimensionality D into a new dataset Y which consists of N samples with dimensionality d (where $d < D$, and often $d \ll D$). This process retains the geometry of the data as much as possible. In other words:

$$x_1, x_2, \dots, x_n \in R^D \xrightarrow{f} y_1, y_2, \dots, y_n \in R^d \quad (1)$$

The embedding is optimized to preserve the local configurations of nearest neighbors. The algorithm is divided into three different steps and summarized in Figure 1.

In the first step, the K nearest neighbors for each data point is described as measured by Euclidean distance. The outcomes of the LLE are normally steady in a range of neighborhood sizes.^[23] In this research by practical computation, the stable range was $8 < k < 12$ and we select $k=10$ nearest neighbors for each data point.

In the second step of the LLE, every data point reconstruct from its nearest neighbors. This can be expressed as the cost function by minimizing the reconstruction error:

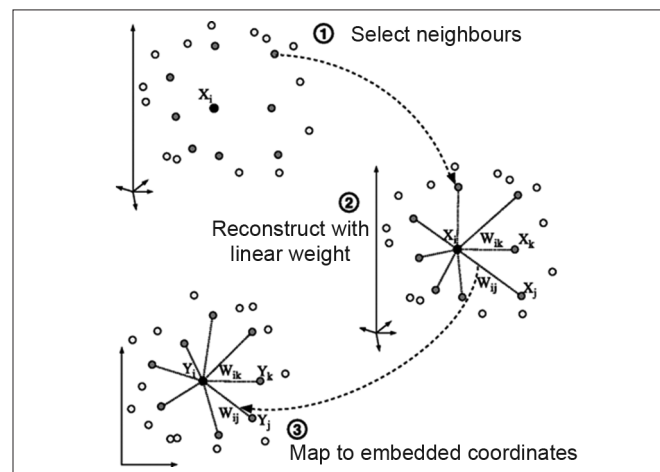


Figure 1: Diagram of the LLE algorithm. The three main steps are: (1) define the neighborhood for each point, (2) solve for the reconstruction weights, and (3) learn embedding which preserves the reconstruction weights. Image obtained^[23]

$$E(w) = \sum_{i=1}^N \left| \vec{x}_i - \sum_{j=1}^k w_{ij} \vec{x}_j \right|^2 \quad (2)$$

Where x_i is the current data point, x_j denotes one of the nearest neighbors, and W_{ij} is the corresponding reconstruction weight between x_i and x_j . To calculating the weights, the $E(w)$ in (2) is minimized by considering two constraints: a sparseness constraint and an invariance constraint. Note that $W_{ij}=0$ if x_j is not in the neighborhood of x_i , hence, any data point x_i is rebuilt exclusively from its neighbors. This fact is equal to the sparseness constraint. The invariance constraint is satisfied by putting sum of rows of the weight matrix equal one ($\sum_j w_{ij}=1$). Accordingly, the LLE obtains the least squares solution to w by assuming these constraints.

In the final step of the algorithm, each low dimension output y_i is projected by high dimension input x_i with quoting global internal coordinates on the manifold. This is conceivable by choosing the d dimensional coordinates of each output y_i to minimize the cost function (3):

$$\phi(y) = \sum_{i=1}^N \left| \vec{y}_i - \sum_{j=1}^k w_{ij} \vec{y}_j \right|^2 \quad (3)$$

Equation (3), like the one in cost function (2) is based on locally linear reconstruction errors. The only dissimilarity here is that w_{ij} are fixed and output y_i are optimized. In this step of the algorithm original inputs, x_i is not included. Hence, the geometric information in w_{ij} describes the embedding completely. Therefore, the goal is calculating y_i with low dimension in the same way that high dimensional inputs x_i are reconstructed by w_{ij} weights. By rewriting (3) as the quadratic form:

$$\begin{aligned} \phi(y) &= \sum_i \left| \vec{y}_i - \sum_j w_{ij} \vec{y}_j \right|^2 \\ &= \sum_{ij} M_{ij} (\vec{y}_i \cdot \vec{y}_j) = y^T M y \end{aligned} \quad (4)$$

The sparse, symmetric, and semipositive definite matrix M has $N \times N$ dimensions and is equal to:

$$M_{ij} = \delta_{ij} - w_{ij} - w_{ji} + \sum_k w_{ki} w_{kj} = (I - W)^T (I - W) \quad (5)$$

where I is the identity matrix. Finally, by solving eigenvalue problem of cost matrix M , the embedding cost function (4) can be minimized. The bottom $d+1$ non-zero eigenvectors of cost matrix prepare an ordered set of d embedding coordinates.^[23]

Data acquisition

The apical two-dimensional gray scale sequences of

three healthy volunteers were acquired using a Vivid 3 ultrasound machine with a 2.0 MHz probe and stored in AVI format with 200×200 resolution, including the ECG display. Four-chamber and two-chamber views were used. For conducting the present study, sequences of three successive cycles were stored with care being taken to ensure that there was no probe or respiratory movement during the data acquisition.

Embedding echocardiography images

LLE algorithm was implemented on three cases of normal echocardiography images. One case had $N=80$ frames of two heart cycles and the others contain three heart cycles with $N=120$ frames. Each frame was a matrix with resolution of 200×200 pixels which reshaped to 1×40000 array, so the dimension of first space was 40000, which was very high. We embed the images in two dimensional space by LLE with $K=10$ nearest neighbors. The plot of normalized eigenvalues shows that almost all the information in the cardiac cycle is captured in two dimensions; thus, the images have been embedded in a two-dimensional space by the LLE algorithm. Figures 2-4 show the image manifolds of these cases.

In these figures, each symbol is a projection of the original consecutive images connected to each other via a line. Three points are highlighted with their corresponding images for better understanding.

Because of the various shapes and dynamical nature of the heart in different subjects, the corresponding manifolds are not similar. But in a particular subject, the manifold cycles are similar. However, in all the cases, the cyclic nature of the cardiac motion leads to a close curve. It should be considered that because of variable heart rate of each case, the number of frames per cardiac cycle is variable too.

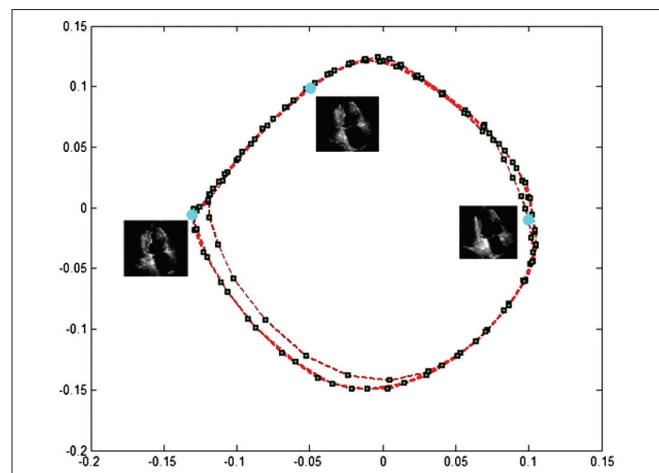


Figure 2: The two dimensional non-linear embedding of three cycles in normal hearts using LLE algorithm (using $k=10$ neighbors), first case

Pseudo increasing echocardiography frame rate

In echocardiography, high temporal resolution is required for the dynamic heart to observe rapid motion of the myocardium and valves for early detection of cardiac diseases. Thus, high frame rate is an essential factor in ultrasound cardiac imaging. Several methods for increasing ultrasound frame rate were mentioned in the 'introduction' section.

A novel method for increasing frame rate and providing slow motion analysis can be extracted from image manifold information. As mentioned before, by manifold embedding with LLE algorithm, the similar frames of echocardiography images remain neighbors to each other in two-dimension space and relationship between the frames is obtained in a close cycloid. In this method, consecutive cycles of the heart are used and their manifolds are drawn in one trajectory.

For pseudo increasing frame rate, we arrange similar frames of multiple heart beat cycles which are extracted from the manifold. Thus, the consecutive frames are sequenced. In the other words, instead of having 3 heart beat cycles each of which has 40 frames, we can have one cycle with 120 frames. Figure 5 shows an image manifold of three cycles of normal four-chamber view with different colors for each cycle. Because imaging procedure is independent of heart beat movement, the probability of registering frames on each other in obtained manifold is very low. In other words, the similar images stand nearby in manifold but not exactly in a same position.

Figure 6 shows four consecutive frames of first cycle and Figure 7 shows ten frames containing specified frames from two other cycles that embedded between these four frames. These Figures demonstrate advantage of proposed method in increasing frame rate and providing slow motion analysis. Slow motion of opening mitral valve in 10 continues frames can be tracked better.

By this approach, we can simply increase frame rate by the advantages of having full view demonstration and without any damage on lateral resolution. Also the computation time with matlab 2009a and 2 GHz CPU configuration was less than five seconds which is a very fast method.

The results obtained with our method were validated by the experienced echo cardiologist (golden standard) on three healthy volunteers. The cardiologist emphasized on accuracy and usefulness of the presented method.

CONCLUSION

Since echocardiography images have natural and non-linear deformations, linear dimension reduction methods cannot recognize the correct relationship between frames. LLE algorithm is one of the most popular

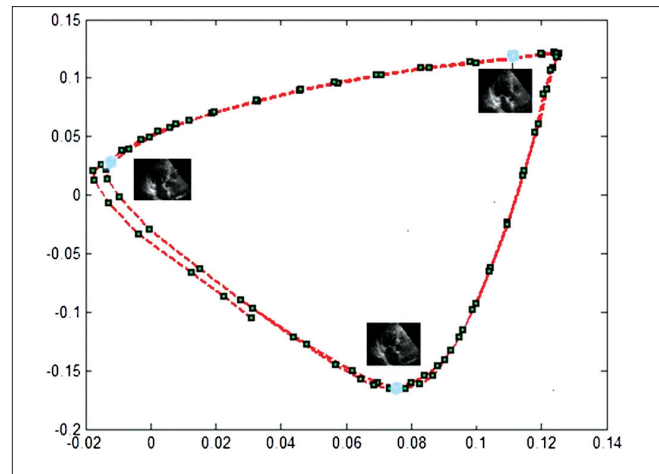


Figure 3: The two dimensional non-linear embedding of two cycles in normal hearts using LLE algorithm (using $k=10$ neighbors), second case

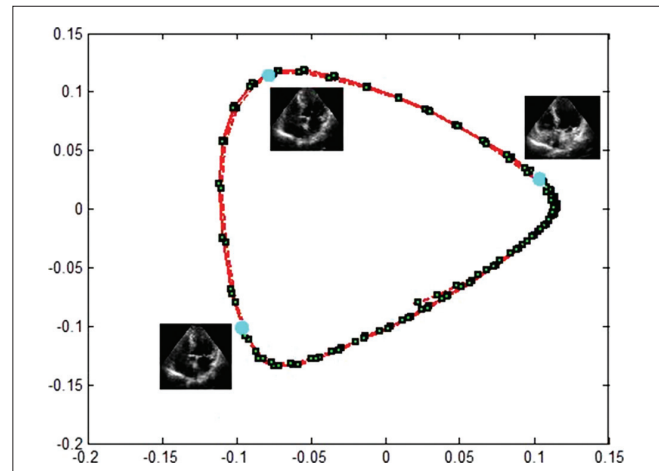


Figure 4: The two dimensional non-linear embedding of three cycles in normal hearts using LLE algorithm (using $k=10$ neighbors), third case

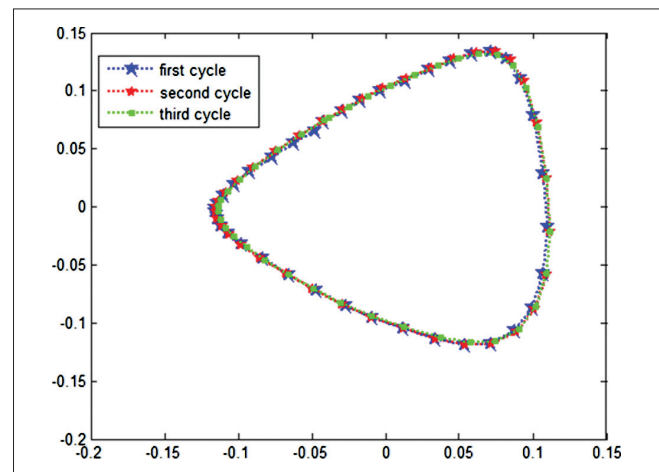


Figure 5: Image manifold of three heart beat cycle. Each cycle has different color

manifold learning and non-linear dimension reduction methods. The main advantage of LLE algorithm is that similar frames in high-dimensional space retain their

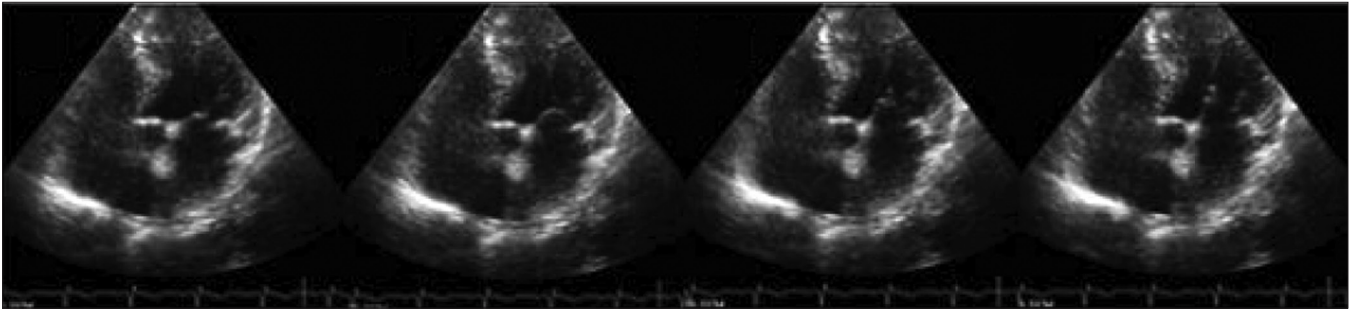


Figure 6: Four continuous frame of one cycle. Opening mitral valve is distinctive in frames

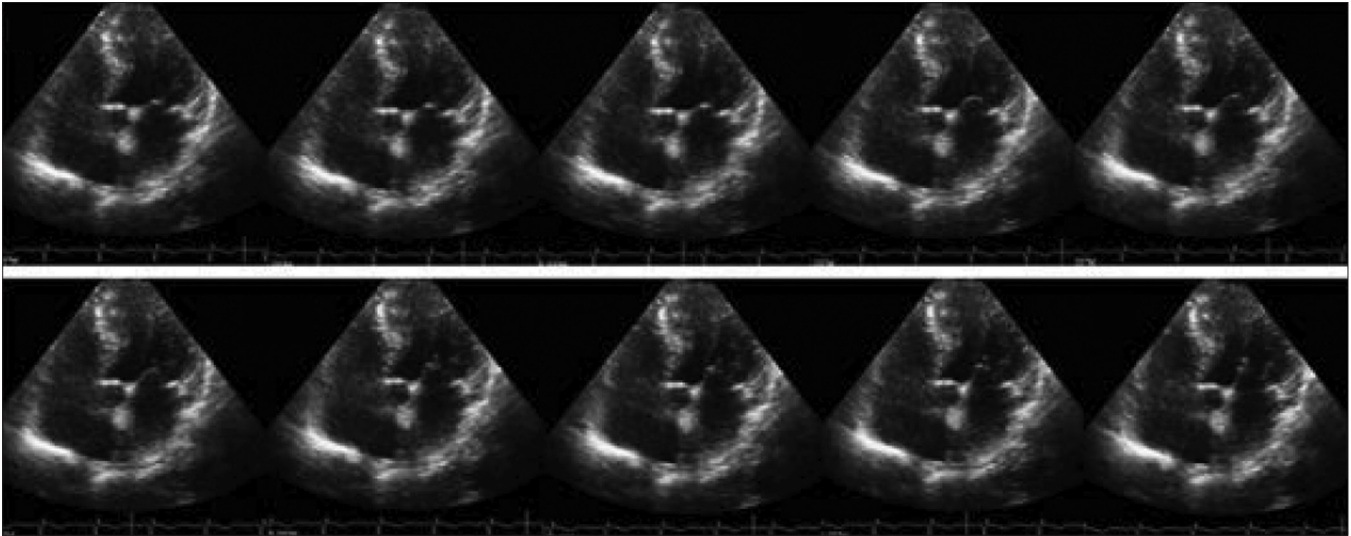


Figure 7: Ten frames of continues sequence extracted from three cycles of image manifold of Figure 5. The numbered frames correspond to frames in Figure 6

neighborhoods in low-dimension space too; this fact was the important reason for selecting the LLE algorithm as a desired method.

Results of using LLE algorithm in analyzing echocardiography images in other applications, such as de-noising^[27] and extracting end-systole and -diastole frames,^[26] emphasize on benefits and power of this algorithm on echocardiography images.

Because the heart movement is independent of imaging procedure and there is no synchronization between ECG and imaging, the probability of exact similarity of frames in different cycles is low. Hence, in dimension reduction, the neighborhood mapped points do not obvolve exactly. After recognizing the relations between frames, we achieved increasing frame rate by arranging consecutive frames of multiple heart beat cycle which are extracted from manifold. By this approach, we can pseudo increase frame rate two or three times more than the original frame rate. The most benefit of this method is illustrating fast movements of myocardium and heart valves in a full view image without decreasing lateral resolution.

An important issue in this method is fixing patient and

probe while doing echocardiography. Because any sudden movement of probe or patient causes drastic differences in frames and the manifold trajectory in consecutive heart cycles would not be the same.

Although the results show that the proposed method is applicable for normal cases, we are going to develop the algorithm on a wide range of normal and abnormal cases in order to find a diagnosis protocol for different heart diseases.

We believe that manifold learning algorithm can make a new horizon in analyzing the medical images and particularly echocardiography images.

REFERENCES

1. Hoit BD. Echocardiographic assessment of the mouse heart. In: Hoit BD, Walsh RA, editors. Cardiovascular Physiology in the Genetically Engineered Mouse. Norwell, MA: Kluwer Academic Publishers; 2001; p.177-90.
2. Konofagou EE, D'Hooge J, Ophir J. Myocardial elastography- A feasibility study *in vivo*. *Ultrasound Med Biol* 2002;28:475-82.
3. D'hooge J, Konofagou E, Jamal F, Heimdal A, Barrios L, Bijnens B, et al. Two dimensional ultrasonic strain rate measurement of the human heart *in vivo*. *IEEE Trans Ultrason Ferroelectr Freq Control* 2002;49:281-6.

4. Kanai H, Koiwa Y, Zhang JP. Real-time measurements of local myocardium motion and arterial wall thickening. *IEEE Trans Ultrason Ferroelectr Freq Control* 1999;46:1229-41.
5. Kanai H, Satoh H, Hirose K, Chubachi N. A new method for measuring small local vibrations in the heart using ultrasound. *IEEE Trans Biomed Eng* 1993;40:1233-42.
6. Wang S, Lee W, Luo J, Konofagou EE. A composite imaging technique for high frame-rate and full-view cardiovascular ultrasound and elasticity imaging. *IEEE Ultrason Symp* 2007. p. 880-3.
7. Shen J, Ebbini ES. Filter-based coded-excitation system for high-speed ultrasonic imaging. *IEEE Trans Med Imaging* 1998;17:923-34.
8. Fabian M, Ballu KN, Hossack JA, Blalock TN, Walker WF. Development of a parallel acquisition system for ultrasound research. *Proc SPIE* 2001;4325:54-62.
9. Jensen JA, Nikolova SI, Gammelmarka KL, Pedersen MH. Synthetic aperture ultrasound imaging. *Ultrasonics* 2006;44:5-15.
10. Tenenbaum JB, Silva V, Langford J. A global geometric framework for nonlinear dimensionality reduction. *Science* 2000;290:2319-23.
11. Roweis ST, Saul LK. Nonlinear dimensionality reduction by locally linear embedding. *Science* 2000;290:2323-6.
12. Zhang Q, Souvenir R, Pless R. Segmentation informed by manifold learning. *Germany: LNCS, Springer; 2005;3757:398-413.*
13. Zhang Q, Pless R. A segmenting cardiopulmonary images using manifold learning with level sets. *Computer Vision for Biomedical Image Applications. Vol. 3765. Berlin/Heidelberg: Springer; 2005. p. 479-88.*
14. Souvenir R, Zhang Q, Pless R. Image manifold interpolation using free-form deformations. *Proc. Int. Conf. on Image Processing. Atlanta, GA: 2006. p. 1437-40.*
15. Souvenir R, Pless R. Image distance functions for manifold learning. *Image Vis Comput* 2007;25:365-73.
16. Raytchev B, Yoda I, Sakaue K. Head pose estimation by nonlinear manifold learning. In: Goldfarb L, ed. *Proc. IEEE Int'l Conf. on Pattern Recognition, Vol.4. Washington, 2004. 462-466.*
17. Zhang J, Li SZ, Wang J. Nearest manifold approach for face recognition. *Proc. IEEE Int'l Conf. on Automatic Face and Gesture Recognition. Korea, Seoul. 2004. p. 223-28*
18. Guo F, Qian G. Monocular 3D tracking of articulated human motion in silhouette and pose manifolds. *Image Video Process* 2008;1:1-18.
19. Lee, C.-S. and Elgammal, A.: Modeling View and Posture Manifolds for Tracking. *Proc. IEEE International Conference on Computer Vision. 2007;1-8.*
20. Lee KC, Kriegman D. Online learning of probabilistic appearance manifolds for video-based recognition and tracking. *Proc IEEE Int Conf Comput Vis Pattern Recognit* 2005;1:852-9.
21. Cox T, Cox M. *Multidimensional scaling. London, UK: Chapman and Hall; 1994.*
22. Hotelling H. Analysis of a complex of statistical variables into principal components. *J Educ Psychol* 1933;24:417-41.
23. Saul L, Roweis S. Think globally, fit locally: Unsupervised learning of low dimensional manifolds. *J Mach Learn Res* 2003;4:119-55.
24. Belkin M, Niyogi P. Laplacian Eigenmaps and spectral techniques for embedding and clustering. *Adv Neural Inf Process Syst* 2002;14: 585-91.
25. Zhang Z, Zha H. Principal manifolds and nonlinear dimensionality reduction via local tangent space alignment. *SIAM J Sci Comput* 2004;26:313-38.
26. Gifani P, Behnam H, Shalbaf A, Sani ZA. Automatic detection of end-diastole and end-systole from echocardiography images using manifold learning. *Physiol Meas* 2010;31:1091-103.
27. Gifani P, Behnam H, Ahmadinejad N, Satarazde R. Noise reduction of echocardiography images using manifold learning. *Proc. 16th Iranian Conf. on Biomed Eng, Tehran, Iran 2008; 568-73.*

How to cite this article: Gifani P, Behnam H, Sani ZA. A new method for pseudo-increasing frame rates of echocardiography images using manifold learning. *J Med Sign Sens* 2011;2:107-12

Source of Support: Nil, **Conflict of Interest:** None declared

BIOGRAPHIES



Parisa Gifani received the B.S. degree in Electrical Engineering from Ferdowsi University of Mashhad, Mashhad, Iran, in 2007 and the M.S. degree in Medical Engineering from Iran University of Science and Technology, Tehran, Iran in 2010. Now

she is a Ph.D. candidate in Medical Engineering from Iran University of Science and Technology, Tehran, Iran. Her research interests are Medical Image processing and Echocardiography.



Hamid Behnam received the B.S. degree in Electrical Engineering from Iran University of Science and Technology, Tehran, Iran, in 1988, the M.S. degree in Medical Engineering from Sharif University of Technology, Tehran, Iran, in 1992, the Ph.

D. degree in Applied Electronics from Tokyo Institute of Technology, Tokyo, Japan in 1998. Since 1998 till 2004, he was a researcher at Iran Research Organization for Science and Technology and from 2004 he has been a faculty member

at Iran University of Science and Technology, in Tehran, Iran. Currently, he is an Assistant Professor of Biomedical Engineering at the IUST. His research interests are Ultrasound in Medicine, Medical Image processing and Medical signal processing.



Zahra Alizadeh Sani earned a medical degree at Mashhad University of Medical Sciences, Mashhad, Iran in 1998. She was Resident of Cardio Vascular Diseases in Mashhad University of Medical Sciences, Mashhad, Iran in Oct. 2002-Sep. 2006 and

completed fellowships in Echocardiography (Sep.2007-Mar.2009), at Iran University of Medical Sciences, and in Basic Cardiac MR (June.2009), St-Marien-Hospital Bonn Germany. Her research interests are Cardiovascular MRI, Physics, Pulse sequence, clinical application, Cardiovascular CT, Angiography, physics, technique, clinical application Echocardiography, physics, clinical application. Since 2009, she works as an assistant professor of Cardiovascular Imaging in Cardiovascular Imaging department, Shaheed Rajaei Cardiovascular and Medical center, Tehran University.