

LETTER TO THE EDITOR

Exhaled breath diagnostics of lung and gastric cancers in China using nanosensors

Dear Editor,

Breath analysis is a promising diagnostic approach for various conditions [1, 2]. It is based on the identification of volatile organic compounds (VOCs) emitted in the breath, which creates a unique volatolomic signature [3]. Owing to their characteristics, VOCs can be measured non-intrusively from the breath or other body sources [3, 4]. Several studies have shown the diagnostic potential for a variety of conditions based on VOC analysis [5-9]. Malignant diseases, where early detection is crucial, are the main focus of VOC analysis, with lung cancer (LC) and gastric cancer (GC) being the most studied. LC and GC together were responsible for approximately 2.5 million deaths globally in 2018 [10]. The aim of VOC analysis of the breath using sensors is to identify a “VOC-print” comprising the total abundances and ratios of the compounds in the breath, giving an overall unique chemical pattern [11]. This technology can help to address specific challenges concerning LC screening and GC mortality [12,13]. To facilitate real-world applications, different ethnic- and culture-based populations should be sampled. Here, we carried out a VOC-based clinical trial for GC and LC detection in China to classify these two major malignancies with different genetic and cultural backgrounds, using our developed sensors [1] with newly-developed sensor-printing and sampling methods.

A total of 545 breath samples (one/two samples per subject) were collected from 426 adult participants between January 2018 and July 2019 at the Jiangyin Hospital Affiliated to the Southeast University Medical College in China. The study population consisted of three groups: LC patients ($n = 158$), GC patients ($n = 115$), and healthy volunteers ($n = 153$), as detailed in Table 1. All participants gave their informed consent for inclusion before participating in the study.

Exhaled alveolar breath was collected in a controlled manner. End-tidal expired air was directly trapped and pre-concentrated in Tenax[®] TA sorption tubes (Buchem BV,

Apeldoorn, The Netherlands). These new tubes were specially constructed for direct sampling at the SunshineHaick Co. (China) (see Supplementary Methods).

The nanomaterial-based sensor system (nanosensor) was originally developed at Technion (Haifa, Israel) [5, 7] and was recently redesigned as a benchtop device for breath VOC analysis-based LC and GC detection in China (Figure S1). The collected samples were exposed to the nanosensor array. The sensors comprised layers of gold nanoparticles (GNPs) with 13 different organic ligands in two formats (manual and printed), resulting in 26 different sensors inserted in each nanosensor system. The printed method is a novel approach using an inkjet printer and a unique micro-barrier ring developed to overcome topological irregularities (Figures S2 and S3).

Fifteen sensors were chosen (Table S1) after checking that their responses were reproducible with no background noise [7, 9]. One or two sample tubes per volunteer were introduced to the sensor array chamber, which was specially assembled with a thermal desorption (TD) system, enabling the sample tube to be exposed directly to the sensor array.

Exposure to the breath samples or the calibration compounds resulted in rapid and reversible changes of the sensors' electrical resistance. Breath components were identified from the time-dependent resistance response of each sensor. Each sensor responded to all (or to a certain subset) of the VOCs found in the exhaled breath samples. Breath patterns were obtained from the collective response of the sensors by applying discriminant factor analysis (DFA). The DFA output variables constitute mutually orthogonal dimensions. We divided the dataset for each binary analysis (i.e., LC vs. control, GC vs. control, and GC vs. LC) into training (70% samples) and testing sets (30% samples). Leave-one-out cross-validation was used to calculate the classification success in terms of the numbers of true positive (TP), true negative (TN), false positive (FP), and false negative (FN) predictions. Given

List of Abbreviations: VOC, volatile organic compounds; LC, lung cancer; GC, gastric cancer; GC-MS, gas chromatography connected to mass spectrometry; GNP, gold-nanoparticles; SiO₂, silicon dioxide; SU-8, photosensitive polymer; TD, thermal desorption; DFA, discriminant factor analysis; TP, true positive; TN, true negative; FP, false positive; FN, false negative; ROC, receiving operating characteristics; AUC, area under the curve.

This is an open access article under the terms of the Creative Commons Attribution-NonCommercial-NoDerivs License, which permits use and distribution in any medium, provided the original work is properly cited, the use is non-commercial and no modifications or adaptations are made.

© 2020 The Authors. *Cancer Communications* published by John Wiley & Sons Australia, Ltd. on behalf of Sun Yat-sen University Cancer Center

TABLE 1 Main demographic and clinical characteristics of the study population

Characteristic	Whole population	Healthy volunteers	Lung cancer patients [†]				Gastric cancer patients [‡]						
			Total	Stage I	Stage II	Stage III	Stage IV	Unknown	Total	Stage I	Stage II	Stage III	Stage IV
Total (cases)	426	153	158	96	12	7	36	7	65	24	8	17	66
Age [years, median (range)]	60 (23-81)	47 (23-74)	67 (36-81)	62 (36-80)	67 (49-81)	65 (37-79)	67 (45-80)	67 (63-77)	67 (30-80)	65 (48-80)	66 (48-72)	69 (54-80)	67 (30-80)
Gender [cases (%)]													
Male	261 (61)	107 (70)	76 (48)	32 (33)	6 (50)	6 (86)	28 (78)	4 (57)	78 (68)	18 (75)	4 (50)	11 (65)	45 (68)
Female	165 (39)	46 (30)	82 (52)	64 (67)	6 (50)	1 (14)	8 (22)	3 (43)	37 (32)	6 (25)	4 (50)	6 (35)	21 (32)
Smoking status [cases (%)]													
Yes	91 (21)	30 (20)	37 (23)	14 (15)	3 (27)	5 (71)	13 (36)	2 (29)	24 (21)	5 (21)	3 (38)	5 (29)	11 (17)
No	335 (79)	123 (80)	121 (77)	82 (85)	9 (75)	2 (29)	23 (64)	5 (71)	91 (79)	19 (79)	5 (63)	12 (71)	55 (83)
Alcohol use [cases (%)]													
Yes	99 (23.2)	37 (24)	40 (25.3)	13 (14)	3 (25)	5 (71)	15 (42)	4 (57)	22 (19)	4 (17)	2 (25)	2 (12)	14 (21)
No	326 (76.5)	116 (76)	117 (74.1)	83 (86)	9 (75)	2 (29)	20 (56)	3 (43)	93 (81)	20 (83)	6 (75)	15 (88)	52 (79)
Unknown	1 (0.2)	0	1 (0.6)	0	0	0	1 (3)	0	0	0	0	0	0
Asthma [cases (%)]													
Yes	3 (1)	3 (2)	0 (0)	0 (0)	0 (0)	0 (0)	0 (0)	0 (0)	0 (0)	0 (0)	0 (0)	0 (0)	0 (0)
No	423 (99)	150 (98)	158 (100)	96 (100)	12 (100)	7 (100)	36 (100)	7 (100)	115 (100)	24 (100)	8 (100)	17 (100)	66 (100)
<i>H. pylori</i> infection* [cases (%)]													
Yes	4 (1)	-	-	-	-	-	-	-	4 (3)	1 (4)	1 (13)	0 (0)	2 (3)
No	59 (14)	-	-	-	-	-	-	-	59 (51)	9 (38)	3 (38)	10 (59)	37 (56)
Unknown	52 (2)	-	-	-	-	-	-	-	52 (45)	14 (58)	4 (50)	7 (41)	27 (41)
Number of breath samples	545	153	222	136	16	7	54	9	170	31	13	24	102

*The data of *H. pylori* infection were only available for patients with gastric cancer.

†The tumor stage was determined according to the eighth edition of the Union for International Cancer Control (UICC) TNM classification of malignant diseases.

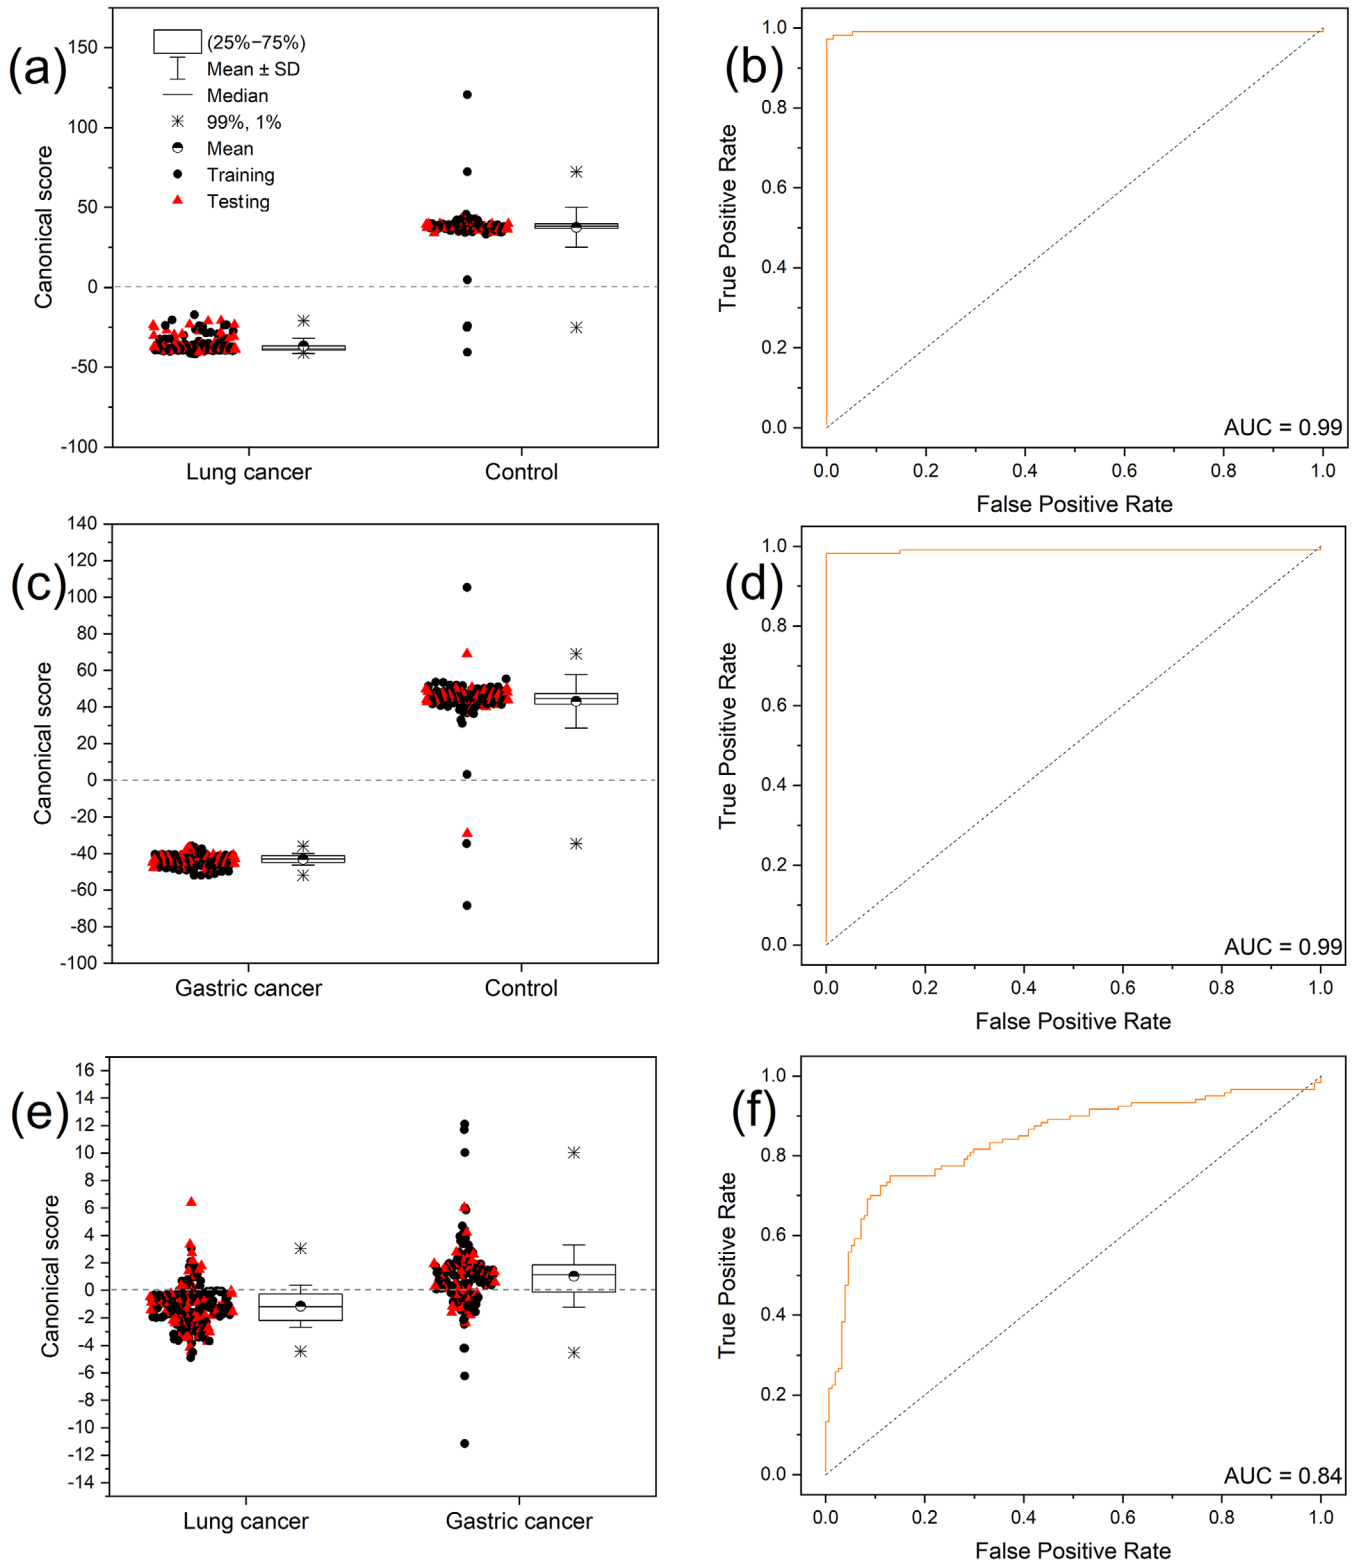


FIGURE 1 Data classification of the clinical trial based on leave-one-out cross validation through discriminant factor analysis of the sensor array results. Box plots on the first canonical score of the training set (blue square) and testing set (red star) for LC versus Control (a), GC versus Control (c), and LC versus GC (e). ROC analysis of the training set including the AUC for LC versus Control (b), GC versus Control (d), and LC versus GC (f). The horizontal dashed line in the box plots represents the cut-off value of the model. Abbreviations: LC, lung cancer; GC, gastric cancer; ROC, receiver operating characteristic analysis; AUC, area under the curve.

TABLE 2 Classification success of discriminant factor analysis models for nanosensor array analysis

Statistics	Training set			Testing set		
	LC vs. C	GC vs. C	LC vs. GC	LC vs. C	GC vs. C	LC vs. GC
Accuracy (%)	99	99	81	100	99	72
Sensitivity (%)	100	100	86	100	100	76
Specificity (%)	97	98	75	100	98	66
PPV (%)	98	98	82	100	98	75
NPV (%)	100	100	81	100	100	67
TP (cases)	156	117	133	66	53	52
TN (cases)	103	107	90	47	43	33
FP (cases)	3	2	30	0	1	17
FN (cases)	0	0	21	0	0	16

PPV – positive predictive value; NPV – negative predictive value; TP – true positive; TN – true negative; FP – false positive; FN – false negative.

k measurements, the model was computed using $k-1$ training vectors. Receiver operating characteristic (ROC) analysis was used to test the performance of the training set data and to calculate the cut-off values (see details in Supplementary Methods supporting information).

Evaluation of the developed nanosensor system involved simulating the sample analysis by four similar nanosensor systems so that the reproducibility of different devices using known mixtures could be assessed. The clinical data were analyzed on the developed nanosensor system (Supplementary Methods and Figure S1).

The reproducibility of a diagnostic system is important. A reliable test requires high precision among different systems using the same sensing technology. Here, we ran 21 repeated breath samples collected over 1 month from the same individual, as well as simulated breath mixtures from LC and GC patients, on four different systems running in parallel. The results showed that similar sensors from different systems gave comparable responses with a relative standard deviation of 0.1% for the response signals within the tested groups (Supplementary Methods and Figures S4, S5).

The new tube approach, i.e., direct sampling, was evaluated. Data on the capacity for breath collection were highly reproducible throughout the exposure on the device (Figure S5). Breath samples differed in humidity. Although the absorbent material Tenax could reduce the water content of the samples, it could not be removed completely. Therefore, to eliminate variation, the humidity was compensated using a linear regression of known humidity levels (Figure S6). The classification model based on a training set of LC versus control showed high accuracy, sensitivity, and specificity, with 0.99 area under the curve (AUC) in the ROC analysis (Table 2, Figure 1a, b). Likewise, all measures were 100% in the testing set. Similarly, GC versus control gave high levels of all performance measures for both the training and testing sets (Table 2, Figure 1c, d). The third classification model of LC versus GC gave high levels of measures, yet slightly

lower, though clinically acceptable (Table 2, Figure 1e, f). A number of outliers were found in the control group. The reason for such a response was unclear. We assumed that those people were unaware of the presence of cancer or they could be momentary electrical noises from specific sensors. Nevertheless, as can be seen, these outliers did not affect the performance of the model.

We further assessed the capacity of the system to distinguish early-stage (I, II) from late-stage (III, IV) cancers. For LC, the accuracy was 59% and 81% for the training and testing sets, respectively. For GC, the accuracy was 48% and 83% for the training and testing sets, respectively. The low accuracies could be attributed to the rather low numbers in each subgroup influencing the classifier. However, it is important to check whether stage I can be distinguished from stages II-IV, as stage I is considered localized and can be surgically removed in most cases. The latter classification for LC and GC gave 71% and 69% accuracy in the validation tests, suggesting that it was feasible to identify cases that remained localized and were suitable for surgical resection.

A number of confounding factors that could affect the analysis outcome were tested. The effects of gender, smoking and alcohol consumption were tested for LC and GC. Chronic conditions such as asthma are also important confounding factors [5, 6], but we could not test this in the present clinical study as only three subjects were recognized as asthmatic. The confounding factor analysis showed that most of the factors examined had a near-random influence on the classifier. For LC versus control, gender, smoking, and alcohol consumption gave AUCs of 0.62, 0.54, and 0.48 in the ROC analysis, respectively (Figure S7). The age factor gave AUC of 0.80, implying its influence on classification. Indeed, there was a rather big difference between the average age of LC patients (63.5 years) and healthy volunteers (47.5 years). However, the classifier for the comparison between LC and control gave a 99% accuracy; thus, even if age differences had some

influence, most of the differences could be attributed to the health condition itself, *i.e.*, sick versus healthy. For GC versus control, gender, smoking, and alcohol consumption gave AUCs of 0.45, 0.49, and 0.58, respectively, in the ROC analysis (Figure S8). Age gave an AUC of 0.88, again implying some influence on classification, but the sick versus healthy factor was much stronger (99% accuracy). Therefore, it is likely that age had a minor influence on the main classification, as for LC described above. No reliable statistical analysis was possible to determine whether the presence of *Helicobacter pylori* was a confounding factor, as only six GC patients were identified as *H. pylori* positive, though we previously showed that this factor had no influence on GC classification in a European population [9]. For LC versus GC, confounding factor analysis for gender, smoking, and alcohol consumption gave AUCs of 0.54, 0.55, and 0.53, respectively, in the ROC analysis. For the age factor, as in the two comparisons above for LC versus control and GC versus control, the AUC was 0.73 (Figure S9).

In conclusion, Patients with LC and GC have significantly different patterns of VOCs in breath opposed to healthy controls. Changes in breath VOCs can be easily measured using a nanosensor-array system. Fast and inexpensive sample collection can be done by direct breath sampling into dedicated Tenax tubes. The importance of confounding data was assessed and should continue to be tested in future studies. The data presented here are another step towards a real-world clinical diagnostic system for fast and affordable cancer detection and management.

DECLARATIONS

ETHICS APPROVAL AND CONSENT TO PARTICIPATE

The study was conducted in accordance with the Declaration of Helsinki, and the protocol was approved by the Ethics Committee of Jiangyin Hospital Affiliated to Southeast University Medical College, China (Project identification code No. 044). Chinese clinical trial registry is ChiCTR1900026033 (<http://www.chictr.org.cn>).

CONSENT FOR PUBLICATION

Not applicable

AVAILABILITY OF DATA AND MATERIALS

All data are available upon request.

COMPETING INTERESTS

The authors declare that they have no competing interests

FUNDING

This study received partial funding from the Horizon 2020 Information Communication Technology (ICT) Program under the breath Volatile Organic compound analysis for

GAstric cancer Screening (VOGAS) project (grant agreement no. 824986). In addition, the project was partially funded by Jiangsu Sunshine Haick Co., which provided the breath sampling kits and systems.

AUTHORS' CONTRIBUTIONS

AG: data management, project design, data analysis, methodology, and manuscript revision; YYB: methodology, data interpretation, figure construction, and writing and revision of original draft; GY, WM, DS, LD, CW, QW, XS, JH, ZX, BH, and SW: clinical work and sample collection; YM and VKW: methodology and sensor preparation; HH: conception, coordination, funding acquisition, supervision of the project, and manuscript revision

ACKNOWLEDGMENTS

The authors acknowledge all the following for their support in discussion and technical advice concerning the study: Yidong Mi, Fei Shen, Xiaochen Wang, Jun Ge, Lin Gao, Feng Lin, Shaoping Liu, Qingfeng Lin, YeiLv, Wenjun Qian, Zhili Liu, Shuai Yan, Yuhong Zhang, ShaSha, Guoyi Shao, Weidong Zhong, Weiwei Tu, Xiangming Cao, Lei Xi, Simin Wang, Jie Zeng, Anqing Zhu, Yehua Mi.

Alaa Gharra^{1†}

Yoav Y. Broza^{1†} 

Guiping Yu^{4†}

Weidong Mao²

Dong Shen²

Lichun Deng²

Chun Wu²

Qiong Wang²

Xia Sun²

Jianming Huang³

Zhuoqi Xuan³

Bing Huang⁴

Song Wu⁴

Yana Milyutin¹

Viki Kloper-Weidenfeld¹

Hossam Haick¹

¹Department of Chemical Engineering and Russell Berrie Nanotechnology Institute, Technion – Israel Institute of Technology, Haifa, Israel

²Department of Oncology, Jiangyin Hospital Affiliated to Southeast University Medical College, Jiangyin, Jiangsu, 214400, P. R. China

³Department of Gastrointestinal Surgery, Jiangyin Hospital Affiliated to Southeast University Medical College, Jiangyin, Jiangsu, 214400, P. R. China

⁴Department of Chest Surgery, Jiangyin Hospital Affiliated to Southeast University Medical College, Jiangyin, Jiangsu, 214400, P. R. China

Correspondence

Hossam Haick, Department of Chemical Engineering and Russell Berrie Nanotechnology Institute, Technion – Israel Institute of Technology, 320003, Haifa, Israel.
Email: hhossam@technion.ac.il

†These authors contributed equally to the work

Trial registration: ChiCTR1900026033, *Chinese clinical trial registry* (<http://www.chictr.org.cn>), retrospectively registered on September 18, 2019.

ORCID

Yoav Y. Broza  <https://orcid.org/0000-0003-0185-2312>

REFERENCES

- Nakhleh MK, Amal H, Jeries R, Broza YY, Aboud M, Gharra A, et al. Diagnosis and Classification of 17 Diseases from 1404 Subjects via Pattern Analysis of Exhaled Molecules. *ACS Nano*. 2017;11:112-125.
- Einoch Amor R, Nakhleh MK, Barash O, Haick H. Breath analysis of cancer in the present and the future. *Eur Respir Rev*. 2019 Jun 30;28(152).
- Broza YY, Mochalski P, Ruzsanyi V, Amann A, Haick H. Hybrid volatolomics and disease detection. *Angew Chem Int Ed Engl*. 2015;54:11036-11048.
- Broza YY, Zuri L, Haick H. Combined volatolomics for monitoring of human body chemistry. *Sci Rep*. 2014 Apr 9;4:4611.
- Broza YY, Khatib S, Gharra A, Krilaviciute A, Amal H, Polaka I, et al. Screening for gastric cancer using exhaled breath samples. *Br J Surg*. 2019 Aug;106(9):1122-1125.
- Broza YY, Braverman I, Haick H. Breath volatolomics for diagnosing chronic rhinosinusitis. *Int J Nanomedicine*. 2018;13:4661-4670.
- Peng G, Tisch U, Adams O, Hakim M, Shehada N, Broza YY, et al. Diagnosing lung cancer in exhaled breath using gold nanoparticles. *Nat Nanotechnol*. 2009 Oct;4(10):669-673.
- Xu ZQ, Broza YY, Ionsecu R, Tisch U, Ding L, Liu H, et al. A nanomaterial-based breath test for distinguishing gastric cancer from benign gastric conditions. *Br J Cancer*. 2013;108:941.
- Amal H, Leja M, Funka K, Skapars R, Sivins A, Ancans G, et al. Detection of precancerous gastric lesions and gastric cancer through exhaled breath. *Gut*. 2016 Mar;65(3):400-407.
- Ferlay J, Colombet M, Soerjomataram I, Mathers C, Parkin DM, Pineros M, et al. Estimating the global cancer incidence and mortality in 2018: GLOBOCAN sources and methods. *Int J Cancer*. 2018 Oct 23.
- Broza YY, Vishinkin R, Barash O, Nakhleh MK, Haick H. Synergy between nanomaterials and volatile organic compounds for non-invasive medical evaluation. *Chem Soc Rev*. 2018 Jul 2;47(13):4781-4859.
- Wang Z, Wang Y, Huang Y, Xue F, Han W, Hu Y, et al. Challenges and research opportunities for lung cancer screening in China. *Cancer Commun (Lond)*. 2018 Jun 7;38(1):34.
- Gao K, Wu J. National trend of gastric cancer mortality in China (2003-2015): a population-based study. *Cancer Commun (Lond)*. 2019 May 2;39(1):24.

SUPPORTING INFORMATION

Additional supporting information may be found online in the Supporting Information section at the end of the article.