


Eye-tracking fluoroscopy system: a new artificial intelligence-based system to communicate activate watching of the monitor during endoscopy

OPEN
ACCESS

Minimizing radiation exposure time is one of the three principles of radiation safety. However, fluoroscopy is often used unnecessarily when endoscopists are not looking at the fluoroscopy monitor. Unnecessary radiation exposure is due to the complexity of fluoroscopic endoscopy procedures, wherein multiple operators independently view different parts of multiple monitors. These procedures usually need an endoscopist for endoscope maneuvers and one or more assistants for other devices; therefore, a radiologic technologist, who manages radiation exposure, cannot always monitor the line of sight of all operators at once. As limited tools are available to reduce endoscopic radiation exposure time [1], we developed a new eye-tracking fluoroscopy system that informs the radiologic technologist when the operators' line of sight is directed toward the monitor. It can track the operators' line of sight and flash a "watching" alert on the detection monitor once a line of sight to the fluoroscopy monitor is detected. This system, jointly developed with NEC Corporation (Tokyo, Japan), was designed to detect remote gaze of operators simultaneously using artificial intelligence (AI)-based face-recognition technology. Radiologic technologists can use this system by attaching an external camera to the fluoroscopy monitor (► Fig. 1) and connecting the camera to the detection monitor and the AI software.

The system could detect the operators' line of sight to the fluoroscopy monitor with high accuracy. This was demonstrated in an experimental study by three personnel wearing radiation safety glasses and personal protective equipment, who raised their hands only when gazing at the fluoroscopy monitor (► Fig. 2). The line of sight detected included both deliberate and unconscious gaze by operators. The system worked in real

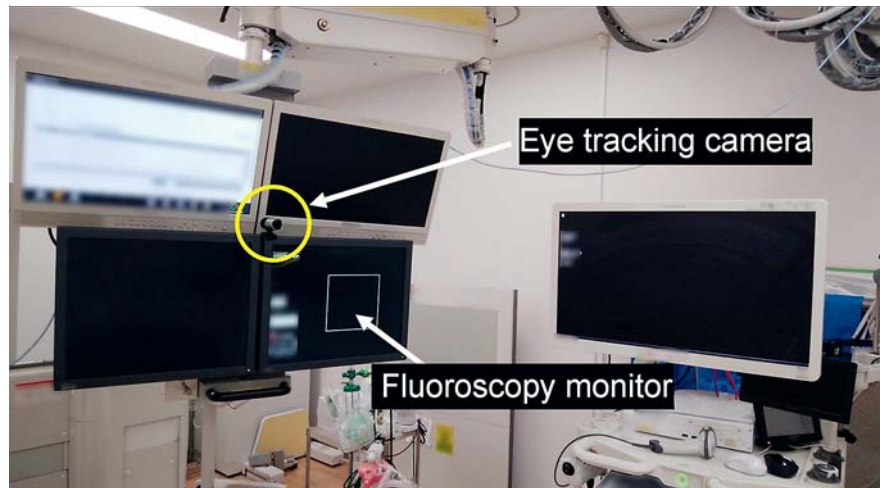

► Fig. 1 The eye-tracking camera located in the center of multiple monitors, with the fluoroscopy monitor at the lower right.



► Fig. 2 Detection of direct lines of sight to the fluoroscopy monitor displayed on the detection monitor.

time during endoscopic procedures (► Fig. 3). Radiation exposure could thus be minimized by detecting line of sight during actual endoscopy (► Video 1). This AI-based eye-tracking system is a promising tool to reduce radiation exposure time of patients and operators during fluoroscopic endoscopy procedures.


Endoscopy_UCTN_Code_TTT_1AR_2AK

Competing interests

The authors would like to declare that the system used in this study was provided by NEC Corporation (Tokyo, Japan).



► **Fig. 3** The eye-tracking fluoroscopy system during actual endoscopy.

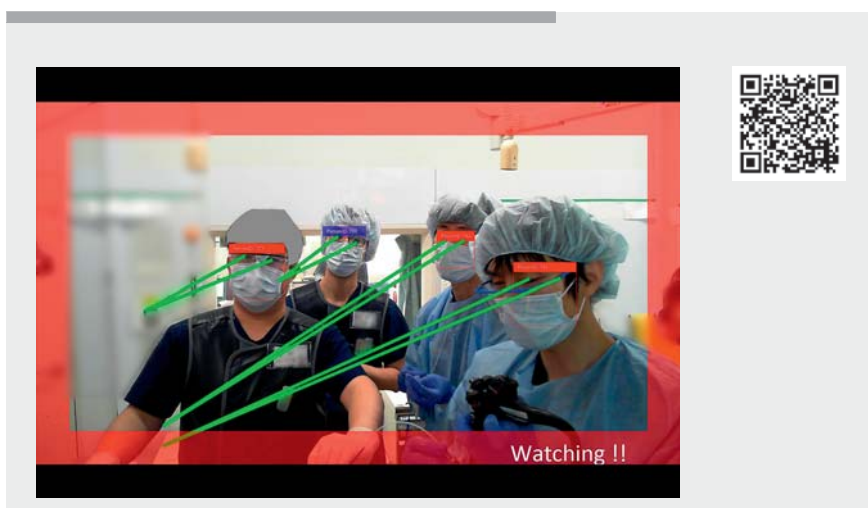

► **Video 1** Eye-tracking fluoroscopy system for reducing radiation exposure time during endoscopy.

Reference

- [1] Kwok K, Hasan N, Duloy A et al. American Society for Gastrointestinal Endoscopy radiation and fluoroscopy safety in GI endoscopy. *Gastrointest Endosc* 2021; 94: 685–697

Bibliography

Endoscopy 2023; 55: E179–E180

DOI 10.1055/a-1960-2610

ISSN 0013-726X

published online 11.11.2022

© 2022. The Author(s).

This is an open access article published by Thieme under the terms of the Creative Commons Attribution-NonDerivative-NonCommercial License, permitting copying and reproduction so long as the original work is given appropriate credit. Contents may not be used for commercial purposes, or adapted, remixed, transformed or built upon. (<https://creativecommons.org/licenses/by-nc-nd/4.0/>)

Georg Thieme Verlag KG, Rüdigerstraße 14, 70469 Stuttgart, Germany



ENDOSCOPY E-VIDEOS

<https://eref.thieme.de/e-videos>



Endoscopy E-Videos is an open access online section, reporting on interesting cases

and new techniques in gastroenterological endoscopy. All papers include a high quality video and all contributions are freely accessible online. Processing charges apply (currently EUR 375), discounts and waivers acc. to HINARI are available.

This section has its own submission website at

<https://mc.manuscriptcentral.com/e-videos>

The authors

Masaki Takinami¹, Junichi Kaneko¹, Megumu Koda¹, Masafumi Nishino¹, Takanori Sakaguchi², Shohachi Suzuki², Takanori Yamada¹

1 Division of Gastroenterology, Iwata City Hospital, Shizuoka, Japan

2 Department of Surgery, Iwata City Hospital, Shizuoka, Japan

Corresponding author

Masaki Takinami, MD

Division of Gastroenterology, Iwata City Hospital, 512-3 Ookubo, Iwata, Shizuoka 438-8550, Japan

masaki.takinami@gmail.com