

RESEARCH

Open Access

# *In vitro* detection of adrenocorticotrophic hormone levels by fluorescence correlation spectroscopy immunoassay for mathematical modeling of glucocorticoid-mediated feedback mechanisms

Martin Gerald Puchinger<sup>1\*</sup>, Clemens Alexander Zarzer<sup>2</sup>, Philipp Kügler<sup>2</sup>, Erwin Gaubitzer<sup>1</sup> and Gottfried Köhler<sup>1</sup>

## Abstract

Performing quantitative, highly sensitive measurements at a single molecule level is often necessary to address specific issues related to complex molecular and biochemical systems. For that purpose, we present a technique exploiting both the flexibility of immunoassays as well as the low operating costs and high throughput rates of the fluorescence correlation spectroscopy (FCS) method. That way we have established a quantitative measurement technique providing accurate and flexibly time resolved data of single molecules. Nanomolar changes in adrenocorticotrophic hormone (ACTH) levels have been detected in a short time-frame that are caused by fast feedback actions in AtT-20 anterior pituitary glands *in vitro*. Especially with respect to clinical diagnostic or mathematical modeling this improved FCS setup may be of high relevance in order to accurately quantify the amounts of peptide hormones—such as ACTH—as well as signaling molecules, transcription factors, etc., being involved in intra- and extracellular reaction networks.

**Keywords:** ACTH, FCS, AtT-20, Cortisol, CRH, Glucocorticoid membrane receptor, ODE model, Parameter identification

## Introduction

Adrenocorticotrophic hormone (ACTH) is a 39-amino acid long straight-chain peptide hormone (4.5 kDa) that is derived from a 266-amino acid precursor pro-opiomelanocortin. It is secreted by the anterior pituitary gland and is considered one of the major stress hormones within the hypothalamic–pituitary–adrenal (HPA)-axis system: The hypothalamus secretes corticotrophin-releasing hormone (CRH), which stimulates the release of ACTH in the corticotrophic anterior pituitary gland [1]. Consequently, ACTH causes the production of cortisol in the adrenal glands. However, beside corticotrophic feedback actions several other feedback controls on the metabolomic or genomic level provide a complex and multifaceted system. One of the most prominent and


well-studied feedback controls is the down-regulation of ACTH production by cortisol. The down-regulation is mediated via two feedback mechanisms working on a genomic and non-genomic levels (see Figure 1). Hence, we observe fast (within seconds to minutes) and slow (after several hours) negative feedback actions in response to the exposure with cortisol [2]. These feedback mechanisms are still subject of research and particularly their interplay is not fully understood. Hence, as ACTH represents the main response in regard to this glucocorticoid feedback, an accurate detection of *in vitro* extracellular ACTH concentration is of high relevance.

The fluorescence correlation spectroscopy (FCS) has proven to be a powerful tool for studying supramolecular associations [3,4], DNA hybridization reactions [5], and detecting single molecule concentrations [6,7]. Due to its high sensitivity, short analysis time and small sample volume requirements FCS have become a valuable tool in molecular biology.

\* Correspondence: martin.puchinger@univie.ac.at

<sup>1</sup>Department of Structural and Computational Biology, Max F. Perutz Laboratories (MFPL), University of Vienna, Campus-Vienna-Biocenter 5, Vienna 1030, Austria

Full list of author information is available at the end of the article

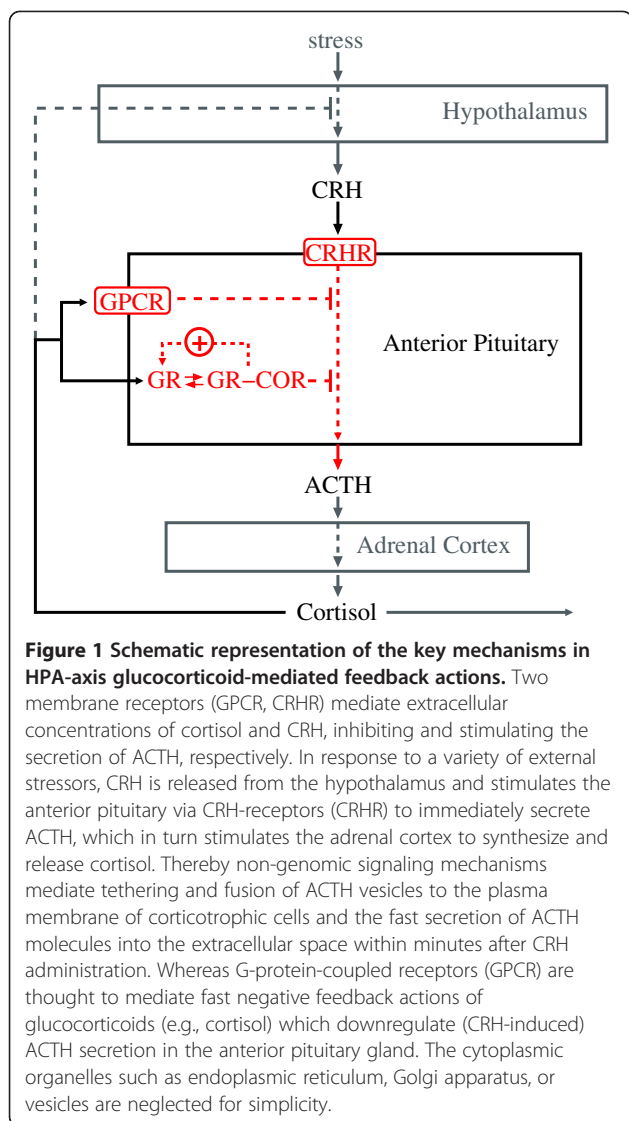

In this article, we present an improved FCS setup to detect nanomolar changes of peptides *in vitro* by combining the fast FCS technique [8] with the highly specific routines of an immunoassay. We exemplify this procedure by means of the *in vitro* measurement of the ACTH peptide secretion from AtT-20 mouse pituitary cells. Particularly, we use a labeled monoclonal antiACTH antibody (specific for the N-terminal epitope on the ACTH peptide) to capture the ACTH molecule, making it visible for the FCS. However, in order to detect low molecular weight peptides such as ACTH, the binding of a second unlabeled monoclonal antiACTH antibody to the C-terminal site of the ACTH peptide is necessary in order to cause a significant change in the diffusion time between the free labeled antibody and the mAb(N)-ACTH-mAb(C) immunocomplex. By measuring this discrepancy in the FCS, the concentration of the target peptide can accurately be determined.

## Materials and methods

### Cell culture

The used AtT-20 cells (ATCC no. CCL-89) were purchased from the American Type Culture Collection (ATCC, Manassas, USA) and passaged at a subcultivation ratio of 1:4 every 5 days. Cells were seeded onto polystyrene 24-well tissue culture plates (Nalge Nunc International, Japan) at a density of  $1.0 \times 10^4$  cells/ml, grown in Dulbecco's Modified Eagle's Medium (Sigma-Aldrich Inc., St. Louis, USA) supplemented with 10% fetal bovine serum, 1.5 g/l sodium bicarbonate, 10 Units/ml penicillin, and 10  $\mu$ g/ml streptomycin, and maintained in an incubator (HERAccl<sup>®</sup>, Thermo Scientific, USA) at 37°C, 6% CO<sub>2</sub> and 95% relative humidity. After 92 and 114 h of cell growing, AtT-20 cells were exposed to doses of 10 nM CRH and up to 100 nM cortisol (both from Sigma-Aldrich Inc.) for 1 min to 1 h. The supernatant was carefully removed from the cell layer and centrifuged ( $800 \times g$ , 37°C, 10 min).

### FCS


FCS measurements were performed on a Confocor spectrofluorimeter (Carl Zeiss-Evotec, Jena, Germany) equipped with an air-cooled 488 nm Argon-laser (LASOS Lasertechnik GmbH, Jena, Germany) and a water immersion objective (C-Apochromat 63  $\times$  /1.2 W Korr). The intensity of the laser was set to 70  $\mu$ W. Intensity fluctuations were recorded by an avalanche photodiode (SPCM-CD 3017) in photon counting mode, autocorrelated with a hardware correlator (ALV 5000, ALV, Langen, Germany), and analyzed with the FCS ACCESS (Carl Zeiss-Evotec) software package using a multicomponent fit model (see Figure 2).

### Focus control and pinhole adjustment

A drop of the organic fluorescent dye Rhodamine 6 G (diluted 1:200) was used to automatically position the chambered coverglass (Nalge Nunc International, Japan) in focus of the confocal optics of the spectrofluorimeter by a scanning procedure as well as to automatically adjust the pinhole to its correct position. The focus in z-direction was set 150  $\mu$ m over the coverglass to record diffusions of fluorescent particles through the focal element in the drop of sample. The pinhole diameter was set to 35  $\mu$ m.

### Calibration of confocal volume

The confocal detection volume was determined by measuring the correlation time of a 10-nM solution of rhodamine 6 G in water with the known diffusion coefficient  $D$  of  $2.8 \times 10^{-6}$  cm<sup>2</sup>/s, employing the relationship  $D = r^2/(4\tau_D)$  and resulting in a confocal volume element of 0.17  $\mu$ m in radian and 0.88  $\mu$ m in axial dimension. In addition, DyLight488-labeled monoclonal antibody dilution series with known concentrations (ranging from 1

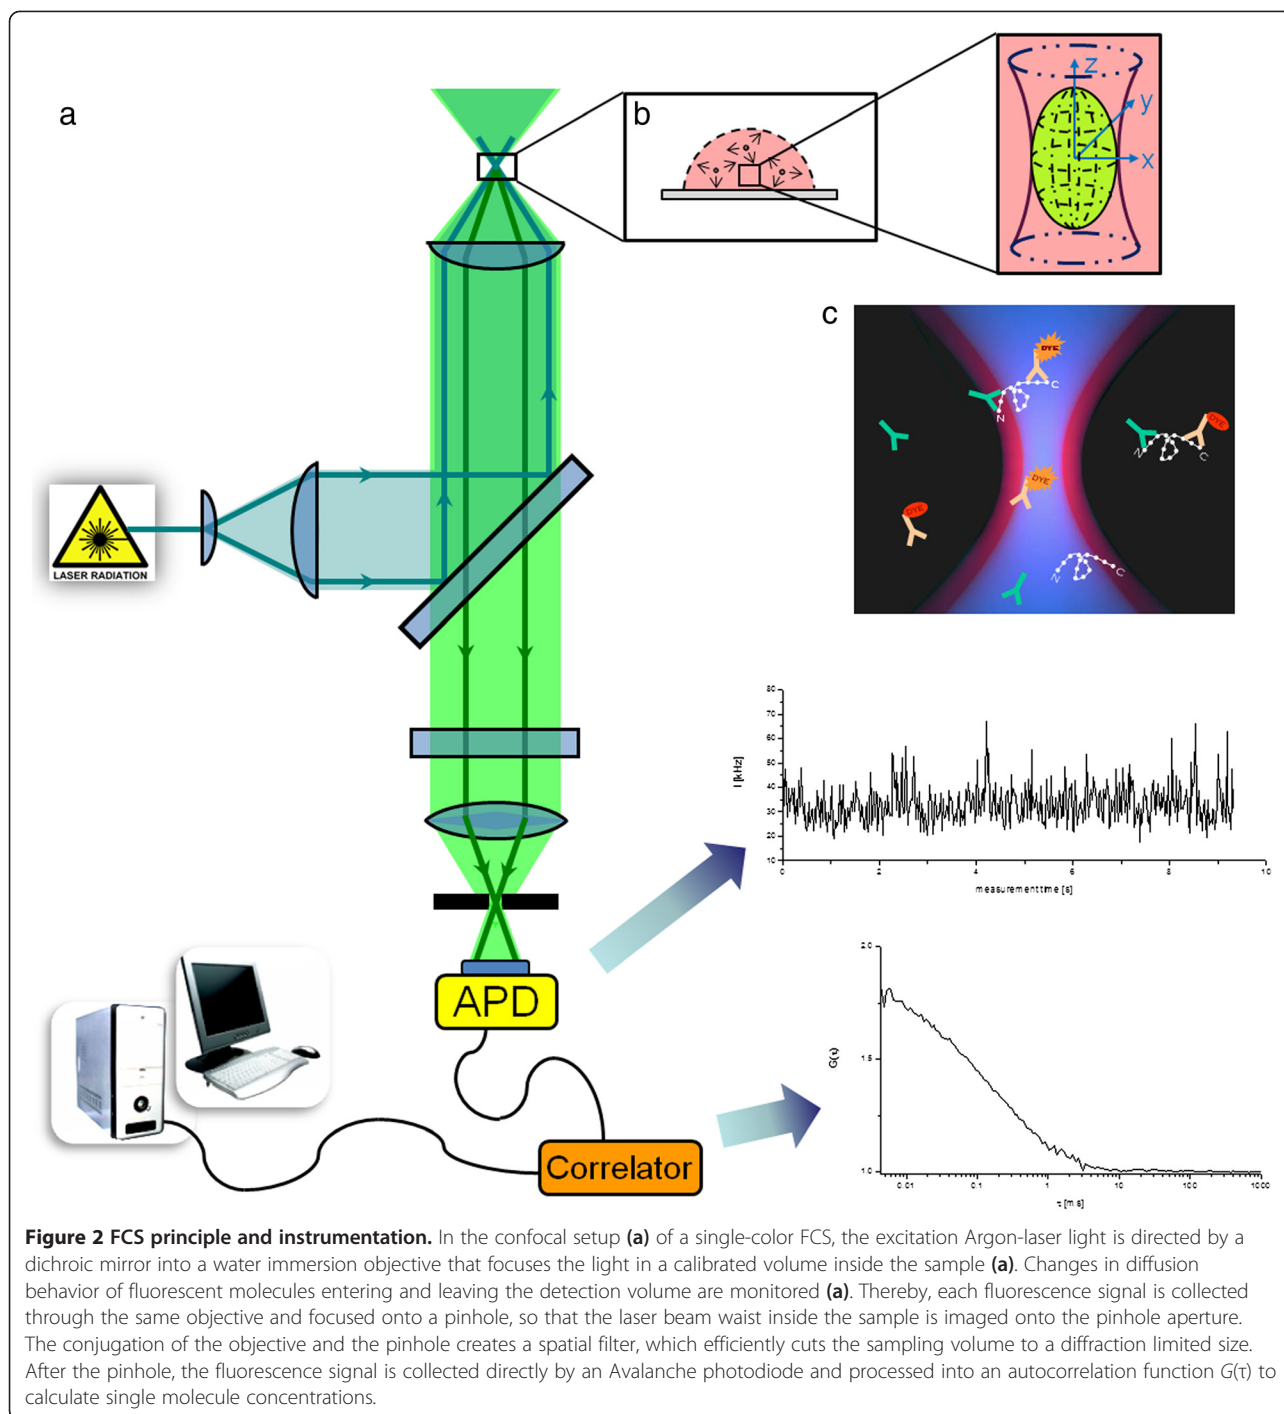

to 80 nM) were measured and showed similar molarities in FCS. Confocal volume calibrations using rhodamine 6 G were carried out on each experimental day or after 3 h measurement time.

#### FCS immunoassay

60 nM antiACTH(N-term)-monoclonal IgG1 antibodies (Phoenix Pharmaceuticals Inc., Belmont, USA) and 60 nM-

labeled antiACTH(C-term)-IgG1 antibodies (Fitzgerald Industries International, Concord, USA; labeled with DyLight488 from Pierce Biotechnology, Rockford, USA) were added in the cell-free supernatant and incubated (30°C, 15 min) to ensure a quick and absolute ACTH-capture of both monoclonal antibodies. Western blotting analysis and ELISA measurements prior to FCS showed no crossreactivity between both antibodies in absence of

ACTH. A drop (25  $\mu$ l) of sample was pipetted on the chambered coverglass, excited with an 488-nm Ar-laser attenuated by an optical density filter (1.0-in. diameter), and the fluctuations in fluorescence intensity of the mAb (N)-ACTH-mAb(C) immunocomplex compared to the free labeled antibody were monitored in series of 50 measurements with identical setup (measurement time: 10 s; correlator scaling: 10 s) for each sample (see Figure 2).

### Calculation

Statistical analysis of the autocorrelation function by a 2-component fitting procedure computationally distinguishes the labeled unbound antibody fraction from the desired ACTH-bound form (immunocomplex). The normalized autocorrelation function  $G(\tau)$  describes the fluctuations of a signal  $F(t)$  from the mean intensity at any time compared to fluctuations at any later time  $F(t + \tau)$ . It is given by

$$G(\tau) = \frac{\langle \delta F(t), \delta F(t + \tau) \rangle}{\langle F(t) \rangle^2},$$

where the angular brackets in the function represent the ensemble average,  $\delta F(t)$  denotes the corresponding variance, and  $\tau$  is known as the delay or correlation time interval over which the fluctuations are compared.

For a single diffusing species (a one-component model) in a Gaussian confocal volume, the autocorrelation function  $G(\tau)$  is defined by [3]

$$G(\tau) = 1 + \frac{1}{N \left(1 + \frac{\tau}{\tau_D}\right) \sqrt{1 + \frac{\tau}{\left(\frac{z}{r}\right)^2 \tau_D}}},$$

where  $N$  is the particle number and  $\tau_D$  the molecular diffusion time of the excited fluorophores moving in a three-dimensional confocal volume through an axial ( $z$ ) to radial ( $r$ ) dimension.

The molecular diffusion time for a one photon excitation is given by the following relationship to the diffusion coefficient  $D$  [ $\text{cm}^2/\text{s}$ ]

$$\tau_D = \frac{r^2}{4D}$$

The obtained autocorrelation functions were evaluated using a two-component model by fixing the diffusion time of the unbound labeled antibody fraction ( $\tau_{D1}$ ) which was achieved from one-component fitting procedure.

The analytical formula for the two-component model, which was successfully applied in a previous work [3], was used in a modified form and is given by

$$G(\tau) = 1 + \frac{1}{N'} [(1 - Y)g_{D1}(\tau) + Yg_{D2}(\tau)]$$

*with*  $N' = N_1 + N_2$

$$g(\tau) = \left(1 + \frac{\tau}{\tau_D}\right)^{-1} \left(1 + \frac{\tau}{\left(\frac{z}{r}\right)^2 \tau_D^2}\right)^{-0.5}$$

This yields values of diffusion times ( $\tau_{D1}$ ,  $\tau_{D2}$ ) and of the related mole fractions  $Y$  and  $(1 - Y)$  for the two components. Autocorrelation analysis was performed for a fixed structural parameter of 5 defining the ratio between the height and the width of the detection volume. This parameter was obtained from calibration with rhodamine 6 G in water. The fit model determines the average number of fluorescent molecules within the detection volume, and the characteristic diffusion times. Evaluations of the autocorrelation function of only labeled antibodies result in diffusion times of  $\tau_1 = 220 \pm 8 \mu\text{s}$  (mean  $\pm t$ -student) through the confocal volume using a one-component fitting procedure. These results are in accordance to the diffusion time of the IgG-antibody ( $D$  of  $3.7 \pm 0.2 \times 10^{-7} \text{ cm}^2/\text{s}$ ) of  $200 \mu\text{s}$  calculated by Stokes–Einstein relation. Formation of the immunocomplex results in a characteristic diffusion behavior of  $\tau_2 = 483 \pm 83 \mu\text{s}$  (mean  $\pm t$ ) through the confocal volume compared to freely labeled anti-ACTH IgG antibody in solution ( $\tau_1$  fixed to  $\tau_1 = 220 \mu\text{s}$ ; see Figure 3).

As the amplitude of an autocorrelation function is inversely proportional to the average number of fluorescent particles within the confocal volume ( $V_{\text{conf}}$  of  $5 \times 10^{-16} \text{ l}$ )


$$G(0) = \frac{1}{N_{D1,2}},$$

the absolute concentration of free labeled IgG antibodies ( $N_{D1}$ ) and of the ACTH immune complexes (equal to number of ACTH molecules;  $N_{D2} = N_{\text{ACTH}}$ ) can be obtained by

$$c_{\text{ACTH}} = \frac{N_{\text{ACTH}}}{6.023 \cdot 10^{23} \text{ mol}^{-1} \cdot 5 \times 10^{-16} \text{ l}}$$

$$= \frac{N_{\text{ACTH}}}{30.115 \times 10^7} \text{ mol/l}$$

$$c_{\text{IgG}} = \frac{N_{\text{IgG}}}{30.115 \times 10^7} \text{ mol/l}$$

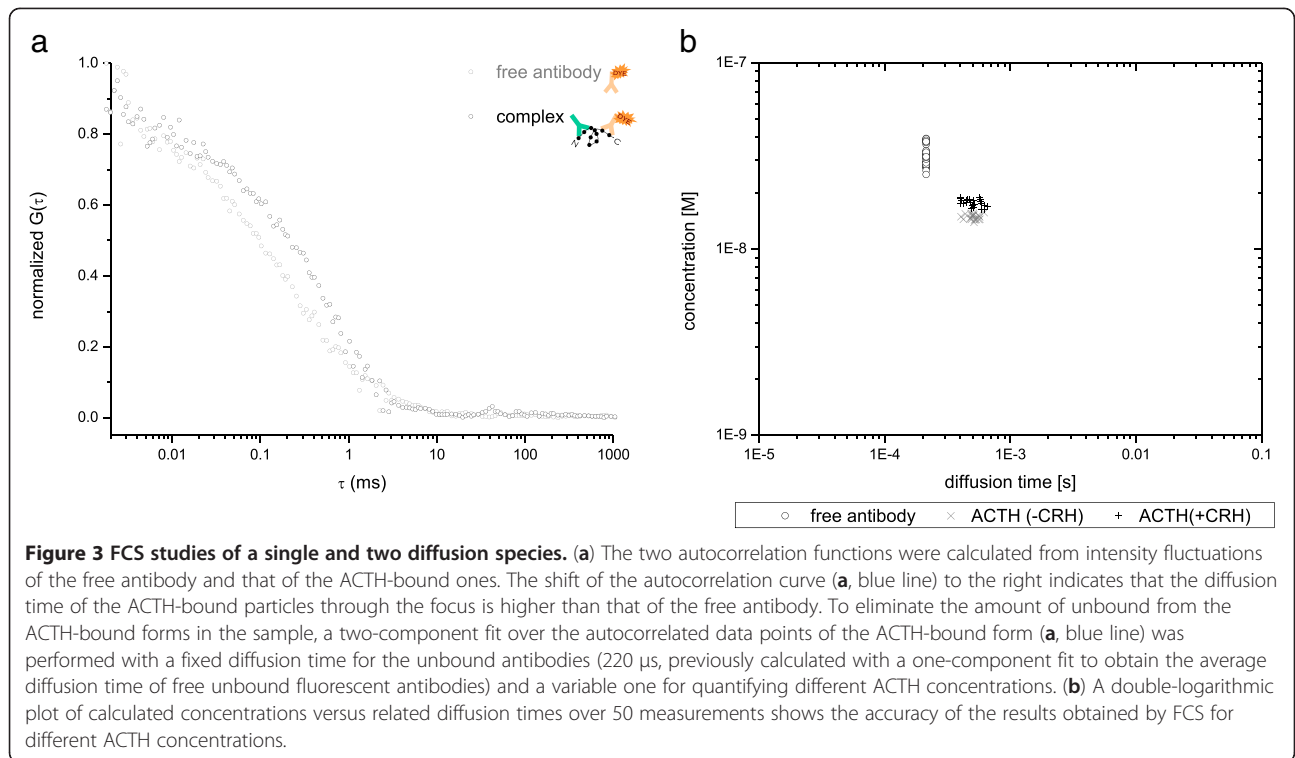


## Results

### Dose response relation of CRH and cortisol to ACTH secretion

The experimental results show a basal ACTH secretion which is not affected by extracellular CRH and cortisol signals (see Figure 4) and thus it seems not to be

modulated by the main feedback controls. Moreover, our data feature a strong ACTH response ( $17.427 \pm 0.422$  nM) to an extracellular dose of 10 nM CRH over 22 h (compared to that of 5 and 36 nM), indicating an increased ACTH secretion in the AtT-20 cells *in vitro*. In addition to an extracellular dose of 10-nM CRH, an

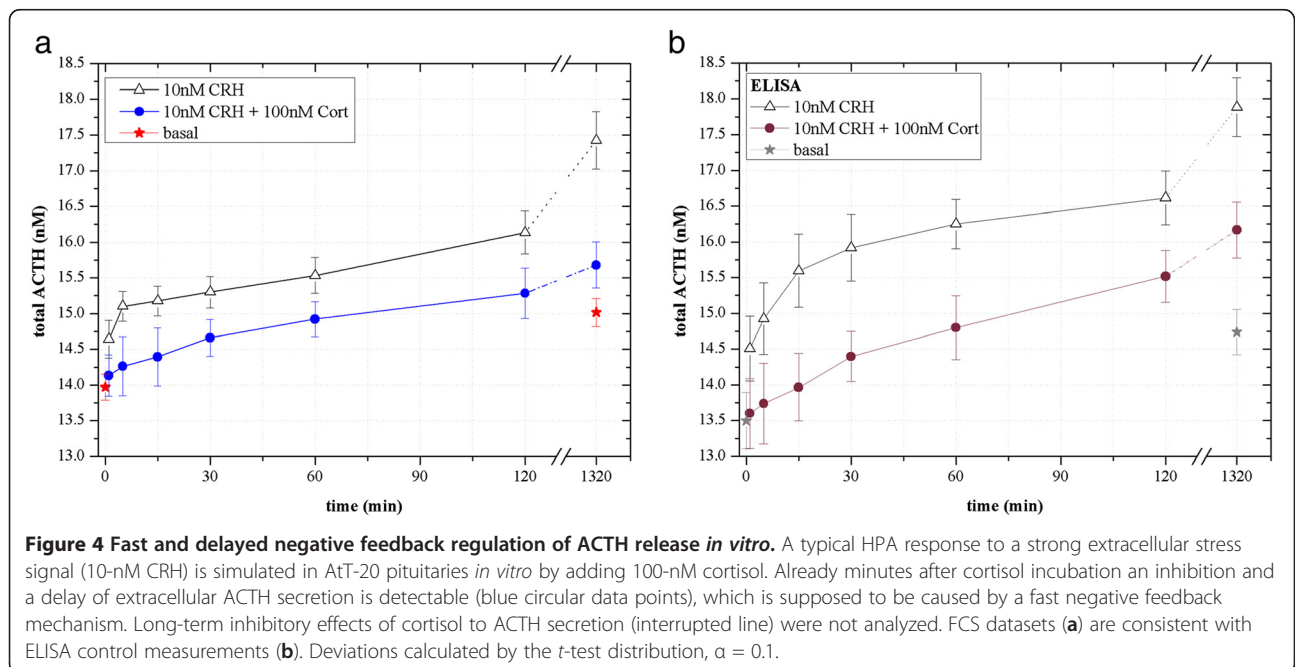

administration of 50 nM cortisol partly inhibited the stimulated ACTH secretion after 22 h compared to that in absence of cortisol. A maximal inhibition of the ACTH release was achieved by adding 100-nM cortisol leading to ACTH levels close to the basal one (Table 1).

### Fast feedback regulation of ACTH release

In order to demonstrate the capabilities of the method we focused on the fast negative feedback control by cortisol. Due to the fast sampling and the low sample volume we were able to detect significant differences in ACTH response within 5–15 min after CRH and/or cortisol incubation (see Figure 4).

### Validation of FCS results

FCS and immunoassays (with chemiluminescent, fluorescent, or HRPO signals) are both known as quite sensitive detection techniques. Thus, a two-site ELISA (MDBioscience, Switzerland) is used to validate the data obtained by FCS. Table 2 and Figure 4 show that the ELISA results are consistent with the detected FCS datasets.

### Mathematical modeling of feedback mechanisms

The improved setup for the FCS method is particularly suitable for experiments which have to be conducted repeatedly and demand a high (quantitative) accuracy of the data. A central motivation to develop such a technique comes from a mathematical modeling task initiated by the research presented in [9]. We are interested in the interplay of the genomic and non-genomic negative feedback of cortisol on the secretion of ACTH and its effect on the dynamics of the HPA-axis. This research goal demands to model both intracellular mechanisms as well as interactions of the different glands. This cannot be achieved in full detail. Consequently, we concentrated on the main feedback mechanisms related to the anterior pituitary gland and the basic controls between the hypothalamus and the adrenal

**Table 1 *In vitro* studies in AtT-20s within 22 h**

CRH (nM)	Cort (nM)	Cell population (cells/ml)	ACTH (nM)
0	0	205164 ± 12889	15.016 ± 0.201
5	0	335938 ± 20522	16.764 ± 0.593
<b>10</b>	<b>0</b>	324219 ± 23935	<b>17.427 ± 0.422</b>
36	0	302084 ± 28168	16.146 ± 0.564
54	0	237500 ± 15630	15.364 ± 0.575
10	50	312500 ± 28125	16.673 ± 0.467
<b>10</b>	<b>100</b>	298438 ± 20625	<b>15.679 ± 0.337</b>

Cell proliferation and ACTH response to various doses of extracellular CRH and cortisol within/over 22 h of incubation (114 h total incubation time). Optimal concentrations for CRH stimulation and cortisol inhibition of ACTH secretion were used for studying feedback regulation of ACTH release (bold values). Deviations calculated by the *t*-test distribution,  $\alpha = 0.1$ .

**Table 2 Validation of FCS results**


Time (min)	ACTH (FCS)		ACTH (ELISA)	
	% change <sup>a</sup>	% dev	% change to FCS	% dev
Basal				
0	0.00	±1.28	-3.39	±2.91
1320	+7.48	± 1.29	-1.86	±2.16
+10 nM CRH				
1	+4.79	±1.82	-0.91	±3.11
5	+8.08	±1.39	-1.16	±3.35
15	+8.62	±1.36	+2.77	±3.29
30	+9.51	±1.43	+4.05	±2.96
60	+11.18	±1.62	+4.61	±2.12
120	+15.50	±1.86	+2.97	±2.27
1320	+24.74	±2.32	+2.63	±2.31
+10 nM CRH + 100 nM cortisol				
1	+1.16	±2.03	-3.77	±3.58
5	+2.08	±2.88	-3.68	±4.12
15	+3.02	±2.85	-2.97	±3.38
30	+4.94	±1.75	-1.80	±2.44
60	+6.80	±1.63	-0.81	±3.01
120	+9.40	±2.31	+1.52	±2.33
1320	+12.23	±2.07	+3.10	±2.41

Validation of FCS results by ELISA measurements. The % difference in ACTH concentrations obtained from ELISA measurements refers to the FCS dataset of the same sample (in the same row in the table).

<sup>a</sup>The temporal % change of ACTH concentration to the basal ACTH-level of 13.9709 nM (mean value) detected by FCS. Deviations calculated by the *t*-test distribution,  $\alpha = 0.1$ .

glands. This approach of bridging several levels of complexity eventually needs validation by experimental data. In that regard the measurement of the ACTH secretion in response to CRH and cortisol serves two goals. First of all the secretion of ACTH is targeted by the main feedback controls we focus on in our model and thus allows us at least a basic assessment of the model. And secondly, we introduce no bias concerning the overall dynamics of the HPA-axis, as we consider only the anterior pituitary cells in our *in vitro* experiment and thus have no interaction with other tissues or glands.

With respect to the modeling technique we followed an approach in [10] which also focused on the anterior pituitary cells. Figure 5 provides a sketch of the considered feedback controls and the used mathematical equations in [10]. In Figure 6, we provide a graphical outline of our model and the corresponding mathematical description as set of the ordinary differential equations. Our extended model follows the approach offered in [10] but in addition considers the fast non-genomic feedback mechanism via the glucocorticoid membrane receptor in the anterior pituitary cells (red-framed pathway). Moreover, the model includes the slow genomic

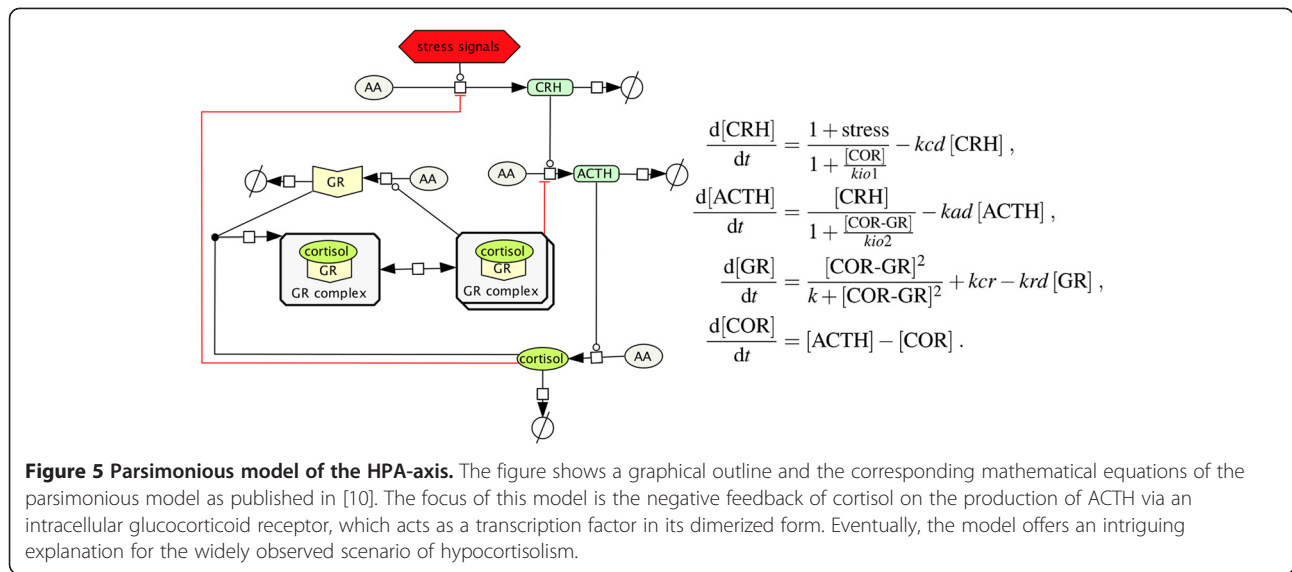


**Figure 5 Parsimonious model of the HPA-axis.** The figure shows a graphical outline and the corresponding mathematical equations of the parsimonious model as published in [10]. The focus of this model is the negative feedback of cortisol on the production of ACTH via an intracellular glucocorticoid receptor, which acts as a transcription factor in its dimerized form. Eventually, the model offers an intriguing explanation for the widely observed scenario of hypocortisolism.


feedback mechanism of cortisol (green-framed pathway) and CRH-mediated genomic and non-genomic effects (blue-framed pathway). To the best of the authors' knowledge the proposed model is the first one of the HPA-axis which incorporates central receptors. Consequently, it differs significantly in size and structure from most models present in literature, which focus on most prominent species cortisol, ACTH, CRH, and vasopressin (cf. [11-14]). Moreover, our model is novel in the

sense that we explicitly model an intracellular compartment and the nucleus. This allows us to take translocation processes into account and thus differ between genomic and non-genomic effects.

In a first attempt we used the model from [10] and tried to reproduce the data obtained by means of our FCS method. Figure 7 shows that if we consider only one of the conducted experiments, i.e., only a dosage of CRH or the scenario of adding CRH as well as cortisol, the model is

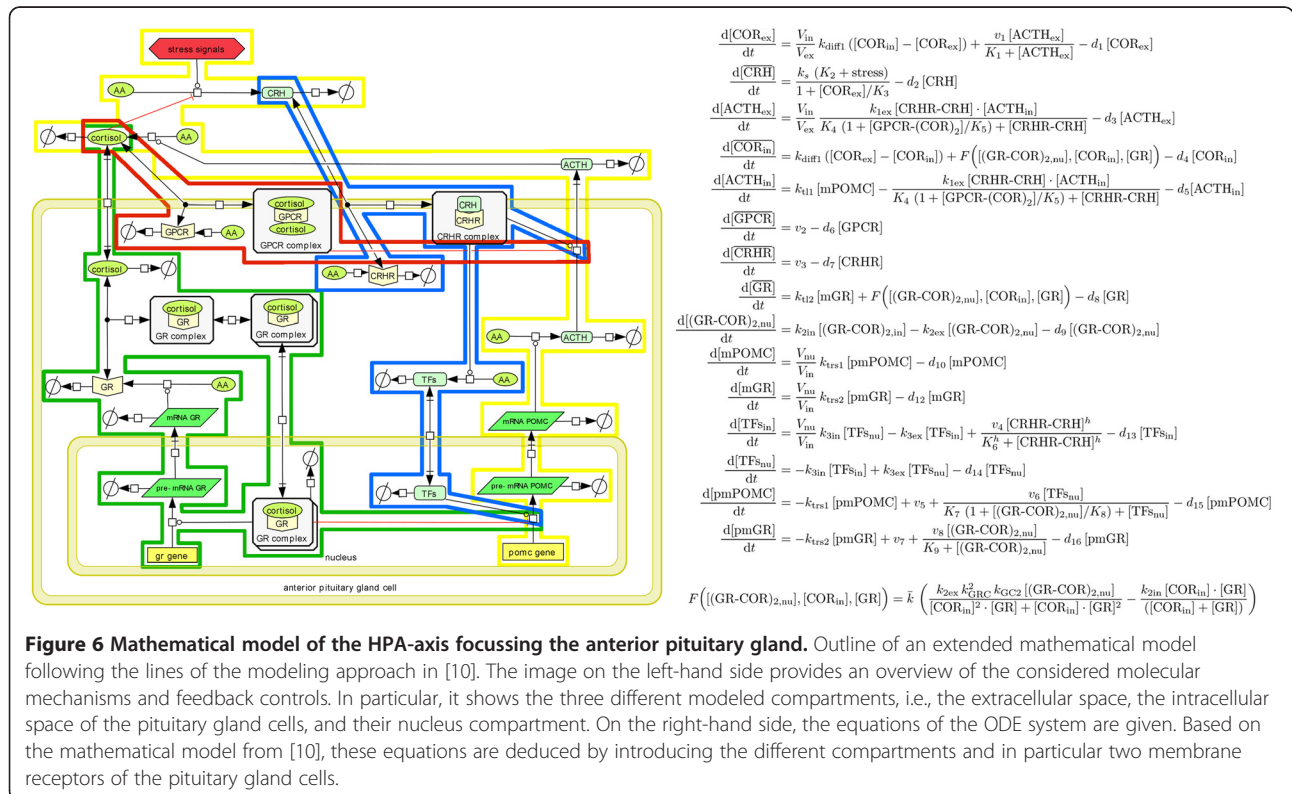


**Figure 6 Mathematical model of the HPA-axis focusing the anterior pituitary gland.** Outline of an extended mathematical model following the lines of the modeling approach in [10]. The image on the left-hand side provides an overview of the considered molecular mechanisms and feedback controls. In particular, it shows the three different modeled compartments, i.e., the extracellular space, the intracellular space of the pituitary gland cells, and their nucleus compartment. On the right-hand side, the equations of the ODE system are given. Based on the mathematical model from [10], these equations are deduced by introducing the different compartments and in particular two membrane receptors of the pituitary gland cells.

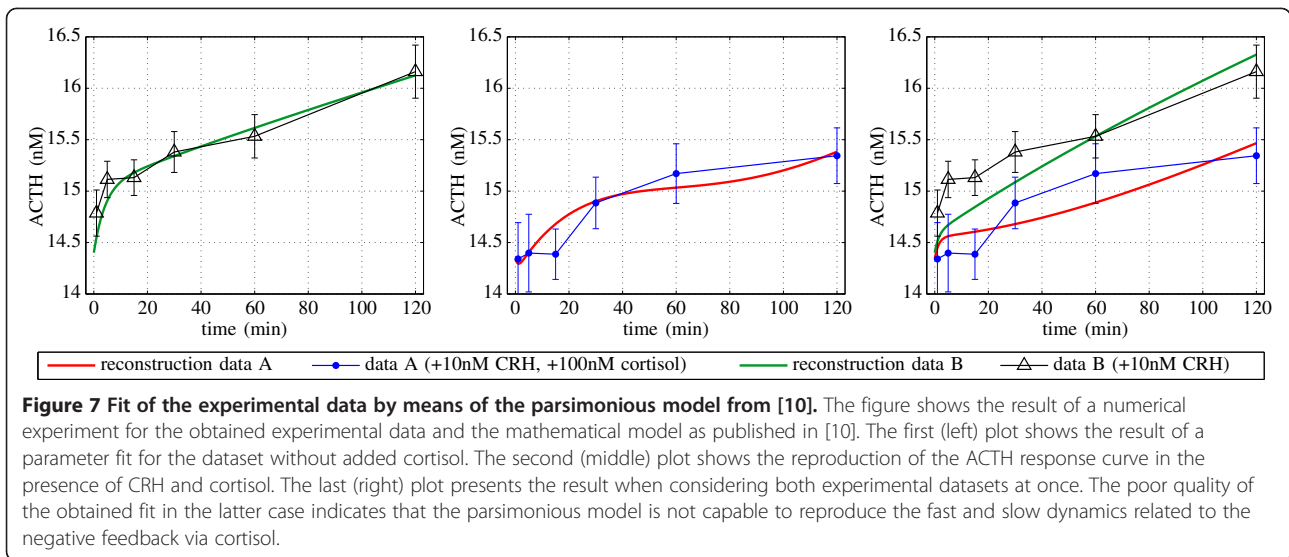

capable to reproduce the basic dynamics. However, we were not able to find any parameter set such that the parsimonious model is able to exhibit both scenarios. The parameter space was searched using the genetic algorithms from the MATLAB global optimization toolbox. In particular, we used different initial populations of about  $10^4$  to  $10^5$  elements. The objective functional was based on Tikhonov-type regularization functional (c.f. [9] for instance).

Figure 8 shows the data fit computed for our extended model. The parameter fit was computed by the Tikhonov regularization, where we used standard global and local optimization algorithms to minimize the objective functional. The extended model allows to correctly reproduce the observed ACTH response behavior. The fact that the model is capable to reproduce the experimental data indicates at least a feasible model and, particularly, supports

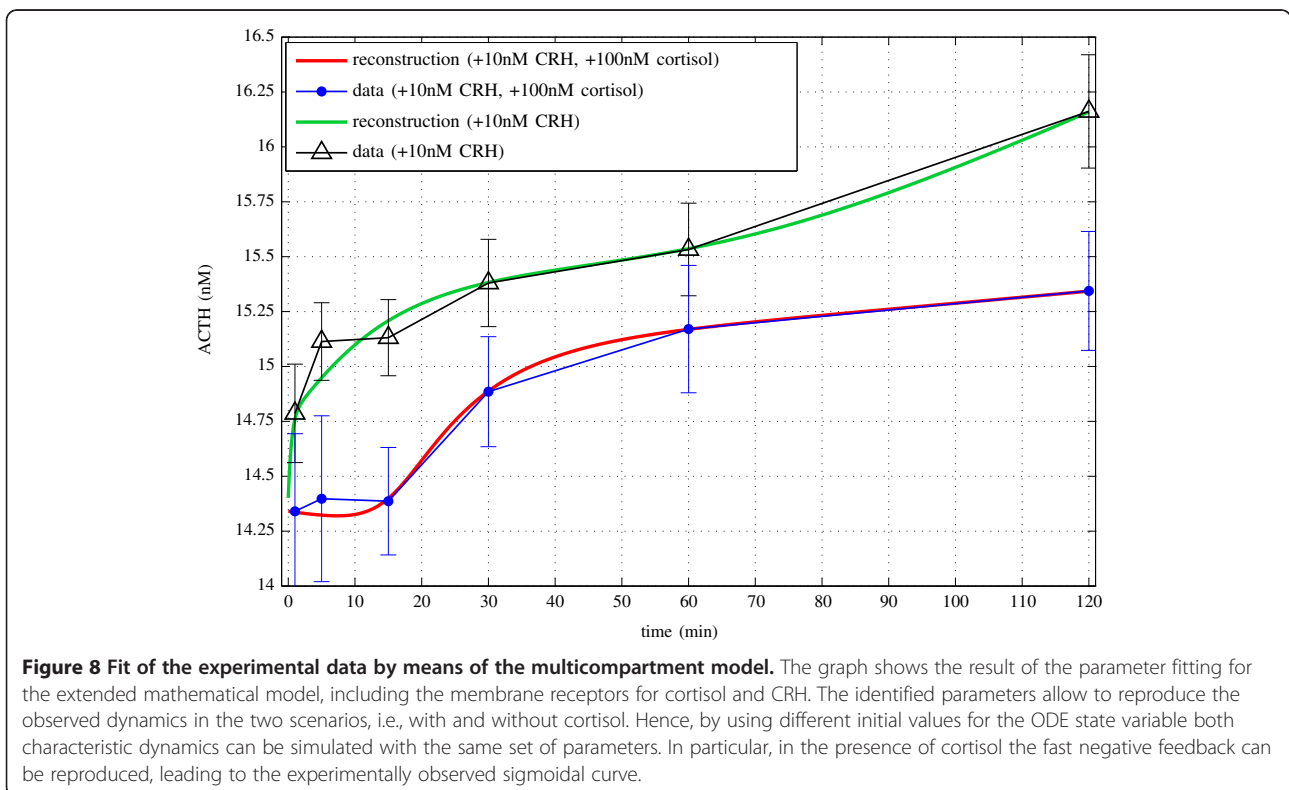



**Table 3 FCS-immunoassay versus ELISA**

Parameter	FCS-assay	ELISA
Sensitivity	$\mu\text{M}$ to sub-nM	nM to sub-nM
Sample volume required	Approximately 20 $\mu\text{l}$	100 $\mu\text{l}$
Measurement time	Approximately 25 min	>2.5 h
Immuno-complex formation	In solution	On the surface
Washing steps required	No	Yes
Calibration curve required	Yes (confocal volume)	Yes
Detection mode	Size-based fluctuations in signal intensities	Changes in signal intensity

the underlying idea of distinguishing between the genomic and non-genomic feedback mechanisms. We emphasize that the present dataset is neither sufficient nor suited to identify the 'true' values of all model parameters. The conducted numerical experiment mainly serves to assess the overall behavior of the extended model, particularly in comparison with the parsimonious model as discussed in [10].

## Conclusion

In 2005, Maier et al. [3] were able to provide evidence of a glucocorticoid receptor in the anterior pituitary cell membrane which may regulate fast response of anterior pituitary cells to cortisol. With our improved FCS setup it was possible to detect lowest changes in extracellular ACTH molarities ( $\pm 0.3$  nM) that arise from signaling of these activated G-protein coupled membrane receptors *in vitro* (see Figure 1). Even 5–15 min after cortisol administration (100 nM) we were able to monitor an inhibition of CRH-induced ACTH secretion by cortisol. Extracellular ACTH levels of  $14.387 \pm 0.428$  nM compared to  $15.131 \pm 0.254$  nM without addition of cortisol were measured. The fast inhibitory effects on CRH-induced ACTH secretion have become evident within at most 5 min after cortisol administration (see Figure 4). However, a detailed temporal restriction of fast and slower feedback actions on extracellular ACTH secretion was not studied with this FCS setup so far, but our results suggested that immediate ACTH secretion which has occurred within minutes after cortisol treatment can only be caused by fast non-genomic feedback actions (see Figure 1) and not by genomic-slow feedback mechanisms which have been shown to occur after several hours [15].

FCS provides a highly flexible, easy-to-use assay format with very small sample volumes (approximately 20  $\mu\text{l}$ ), and increased throughput, as particle numbers can be measured directly after calibrating the confocal volume once, a major disadvantage of ELISAs which need

to be calibrated quite often. In addition, FCS makes it possible to extract complex signals from high background due to the different characteristic time scales over which signal and noise occur.

In conclusion, we have demonstrated that this improved FCS setup can be used for fast and sensitive detection of a specific peptide hormone *in vitro*. By means of the mentioned model system we established this solution-based single molecule detection technique as an alternative to the commonly used approaches, such as ELISAs (with fluorescent, chemiluminescent, or HRPO signal), with respect to rapidity and sensitivity (Table 3). It was possible to even detect nanomolar changes in ACTH secretion with deviations of only 0.2–0.7 nM approximately in response to an extracellular stress signal over a short period of time. The quality of the data obtained by FCS allowed to study fast feedback mechanisms in the HPA-axis regulatory system *in vitro* and allowed to support the development of a mathematical model of that HPA-axis network. As opposed to [10] our model takes both the genomic and non-genomic feedbacks mechanisms into account. As a result it is able to feature both ACTH response curves with a single set of model parameters.

## Abbreviations

ACTH: Adrenocorticotrophic hormone; CRH: Corticotrophin-releasing hormone; CRHR: CRH-receptor; ELISA: Enzyme-linked immunosorbent assay; FCS: Fluorescence correlation spectroscopy; GPCR: G-protein-coupled receptor; GR: Glucocorticoid receptor; HPA: Hypothalamic-pituitary-adrenal; mAb: Monoclonal antibody; POMC: Pro-opiomelanocortin; TF: Transcription factor.

## Competing interests

The authors declare that they have no competing interests.

## Acknowledgments

This study was supported by the Vienna Science and Technology Fund (WWTF) Grant no. MA07-030.

## Author details

<sup>1</sup>Department of Structural and Computational Biology, Max F. Perutz Laboratories (MFPL), University of Vienna, Campus-Vienna-Biocenter 5, Vienna 1030, Austria. <sup>2</sup>Johann Radon Institute for Computational and Applied Mathematics (RICAM), Austrian Academy of Sciences, Altenbergerstr. 69, Linz 4040, Austria.

Received: 21 December 2011 Accepted: 2 October 2012

Published: 26 October 2012

## References

1. JC Buckingham, HC Christian, GE Gillies, JG Philip, AD Taylor, in *The Physiology of Immunity*, ed. by M.D. Kendall, J.A. Marsh (CRC Press, USA, 1996), p. 331
2. B Hinz, R Hirschelmann, Rapid non-genomic feedback effects of glucocorticoids and CRF-induced ACTH secretion in rats. *Pharm. Res.* **17**, 1273–1277 (2000). doi:10.1023/A:1026499604848
3. C Maier, D Rünzler, J Schindelar, G Grabner, W Waldhäusl, G Köhler, A Luger, G-protein-coupled glucocorticoid receptors on the pituitary cell membrane. *J. Cell. Sci.* **118**, 3353–3361 (2005). doi:10.1242/jcs.02462
4. J Wruss, D Rünzler, C Steiger, P Chiba, G Köhler, D Blaas, Attachment of VLDL receptors to an icosahedral virus along the 5-fold symmetry axis: multiple binding modes evidenced by fluorescence correlation

- spectroscopy. *Biochemistry* **46**(21), 6331–6339 (2007). doi:10.1021/bi700262w
5. JC Politz, ES Browne, DE Wolf, T Pederson, Intracellular diffusion and hybridization state of oligonucleotides measured by fluorescence correlation spectroscopy in living cells. *Proc. Natl Acad. Sci. USA* **95**, 6043–6048 (1998). doi:10.1073/pnas.95.11.6043
  6. H Glauner, IR Ruttekolk, K Hansen, B Steemers, YD Chung, F Becker, S Hannus, R Brock, Simultaneous detection of intracellular target and off-target binding of small molecule cancer drugs at nanomolar concentrations. *Br. J. Pharmacol.* **160**, 958–970 (2010). doi:10.1111/j.1476-5381.2010.00732.x
  7. L Tang, C Dong, J Ren, Highly sensitive homogenous immunoassay of cancer biomarker using silver nanoparticles enhanced fluorescence correlation spectroscopy. *Talanta* **81**, 1560–1567 (2010). doi:10.1016/j.talanta.2010.03.002
  8. K Bacia, P Schwill, Fluorescence correlation spectroscopy. *Methods Mol. Biol.* **398**, 73–84 (2007). doi:10.1007/978-1-59745-513-8\_7
  9. HW Engl, C Flamm, P Kügler, J Lu, S Müller, P Schuster, Inverse problems in systems biology. *Inverse Problems* **25**, 123014 (2009). doi:10.1088/0266-5611/25/12/123014
  10. S Gupta, E Aslaksen, BM Gurbaxani, SD Vernon, Inclusion of the glucocorticoid receptor in a hypothalamic-pituitary-adrenal axis model reveals bistability. *Theor. Biol. Med. Model* **4**(8) (2007). doi:10.1186/1742-4682-4-8
  11. V Kyrilov, LA Severyanova, A Vieira, Modeling robust oscillatory behavior of the hypothalamic-pituitary-adrenal axis. *IEEE Trans. Biomed. Eng.* **52**(12), 1977–1983 (2005)
  12. G Li, B Liu, Y Liu, A dynamical model of the pulsatile secretion of the hypothalamo-pituitary-thyroid axis. *Biosystems* **35**(1), 83–92 (1995)
  13. BZ Liu, JH Peng, YC Sun, YW Liu, A comprehensive dynamical model of pulsatile secretion of the hypothalamo-pituitary-gonadal axis in man. *Comput. Biol. Med.* **27**(6), 507–513 (1997)
  14. D Savic, S Jelic, A mathematical model of the hypothalamo-pituitary-adrenocortical system and its stability analysis. *Chaos Solitons Fract.* **26**, 427–436 (2005)
  15. O Wang, JA Majzoub, in *The Pituitary*, ed. by M. Shlomo (Elsevier, Amsterdam, 2011), p. 68

doi:10.1186/1687-4153-2012-17

**Cite this article as:** Puchinger et al.: *In vitro* detection of adrenocorticotrophic hormone levels by fluorescence correlation spectroscopy immunoassay for mathematical modeling of glucocorticoid-mediated feedback mechanisms. *EURASIP Journal on Bioinformatics and Systems Biology* 2012 **2012**:17.

**Submit your manuscript to a SpringerOpen<sup>®</sup> journal and benefit from:**

- Convenient online submission
- Rigorous peer review
- Immediate publication on acceptance
- Open access: articles freely available online
- High visibility within the field
- Retaining the copyright to your article

---

Submit your next manuscript at ► [springeropen.com](http://springeropen.com)

---