

In vitro Demonstration of Melanoma Metastasis in Lymph Nodes of Prepared Specimens Using a Light-emitting Diode-based Multispectral Photoacoustic Ultrasound Imaging System

Tomoyuki Ohta^{1*}, Takako Shirakawa², Shinya Okada³, Naohiro Ishii⁴, Shigeru Kiryu¹

Departments of ¹Radiology, ³Pathology and ⁴Plastic Surgery, International University of Health and Welfare Hospital, Otawara, Tochigi, ²Department of Radiological Science, Tokyo Metropolitan University Graduate School of Health Science, Tokyo, Japan

Abstract

Although an excellent photoacoustic (PA) ultrasound method has been reported for the evaluation of lymph node melanoma metastasis in animal experiments, it remains to be evaluated in clinical trials. Recently, we performed PA ultrasound assessment using light-emitting diodes to detect metastatic melanoma in the lymph nodes of specimens prepared for microscopic examination. The PA effect was not obvious in amelanotic melanoma, but was seen in melanotic melanoma by PA imaging (PAI) and histopathological correlation in cases of primary melanotic melanoma accompanied by metastatic lymph nodes, including the coexistence of amelanotic melanoma and melanotic melanoma. Clinical workup should be performed with not only PAI but also conventional ultrasonography in cases with metastasis related to amelanotic transformation, which would likely be missed by PAI alone.

Keywords: Amelanotic melanoma, melanoma, photoacoustic ultrasound imaging

INTRODUCTION

Although a method for clinical photoacoustic (PA) ultrasound examination to detect lymph node (LN) metastases in melanoma patients has yet to be established, an excellent method for the evaluation of LN metastasis in animal experiments was reported with area under the curve of 0.95 (95% confidence interval [CI], 0.90–1.00),^[1] which will be subjected to clinical trials in the near future. Recently, we performed PA ultrasound assessment using light-emitting diodes (LEDs) to detect metastatic melanoma in the LNs of specimens prepared for microscopic observation. Here, we present the correlation between histopathology and PA imaging (PAI) of the specimens, and also describe potential pitfalls of PAI for the detection of LN metastasis in melanoma patients.

CASE REPORT

A 58-year-old woman visited our plastic surgery clinic due to a skin tumor on the right dorsum of the foot. The skin tumor

appeared as a two-humped pigmented nodular or polypoid lesion. It was resected along with a subcutaneous mass in the right thigh detected on physical examination. Histopathology of the specimen showed melanoma with LN metastasis accompanied by depigmentation. She is currently well without any evidence of recurrence 3 years after resection.

MATERIALS AND METHODS

The specimens were assessed using an AcousticX (Cyberdyne Inc., Tsukuba, Japan) fast switching two-wavelength LED arrays (690 nm/850 nm and 820 nm/940 nm) along with a linear-array 7 MHz ultrasound transducer. In addition, we used a method of displaying the PA signal as an image of the ratio (from 0 to 1) obtained by dividing a smaller PA signal by a larger PA signal from light sources of different wavelengths

Address for correspondence: Dr. Tomoyuki Ohta,

Department of Radiology, International University of Health and Welfare Hospital, Iguchi 537-3, Nasushiobara City, Tochigi 329-2763, Japan.
E-mail: ohta.kent@nifty.com

Received: 19-12-2019 Revised: 22-01-2020 Accepted: 02-03-2020 Available Online: 12-05-2020

Access this article online

Quick Response Code:



Website:
www.jmuonline.org

DOI:
10.4103/JMU.JMU_121_19

This is an open access journal, and articles are distributed under the terms of the Creative Commons Attribution-NonCommercial-ShareAlike 4.0 License, which allows others to remix, tweak, and build upon the work non-commercially, as long as appropriate credit is given and the new creations are licensed under the identical terms.

For reprints contact: WKHLRPMedknow_reprints@wolterskluwer.com

How to cite this article: Ohta T, Shirakawa T, Okada S, Ishii N, Kiryu S. *In vitro* demonstration of melanoma metastasis in lymph nodes of prepared specimens using a light-emitting diode-based multispectral photoacoustic ultrasound imaging system. J Med Ultrasound 2021;29:50-2.

on a Jet Colormap Array (MathWorks Inc., Natick, MA, USA). If the signal magnitude, corrected by the light intensity, did not change markedly with different wavelengths, the ratio was closer to 1 and was displayed as dark red; if the signal magnitude changed with different wavelengths, the ratio decreased and was displayed as dark blue for ratios close to 0. That is, the ratio image means there is a slope in the absorption spectrum chart for most abundant PA absorbers in the skin,^[2] but it does not mean whether the slope is up or down between different wavelengths. Intermediate colors were displayed in the order of orange, yellow, green, and light blue. For detailed tissue comparison, we observed the specimens after staining with hematoxylin and eosin on glass microscope slides with PAI. For evaluation, the glass slides were placed in a small water bath [Figure 1]. The transducer was placed above the water bath and scanned horizontally in parallel to the glass slide at a constant speed to create an overhead view corresponding to a loupe image [Figures 2a and 3a]. In this study, the diagnosis of the presence of melanin was based on histopathological findings as the gold standard. This study was performed in accordance with the Helsinki Declaration of 1975, as revised in 2013, and received approval from the institutional review board (IRB no. 13-B-360). Written informed consent was obtained from the patient.

RESULTS

Loupe images of the primary skin lesions indicated nodular or polypoid melanoma [Figure 2a]. The magnitude of the PA signal at 820 nm was stronger than that at 940 nm, and melanin determined by microscopy was shown in blue on the ratio image [Figure 2b-d]. Although the loupe image of the LN showed three metastatic nests [Figure 3a], only one was pigmented, while the others were amelanotic. The magnitude of the PA signal at 690 nm was slightly stronger than that at 850 nm [Figure 3b and c], and the magnitude of the PA signal at 820 nm was stronger than that at 940 nm [Figure 4a and b]. The location of melanin on microscopic evaluation was indicated in yellow–blue by the light wavelength with 690/850 nm [Figure 3d] and in blue by the light wavelength with 820/940 nm [Figure 4c]. Unexpectedly, PAI at 690 nm [Figure 5a and b] showed the PA effect in the area without melanin where normal lymphocytes were accumulated.

DISCUSSION

In this case, primary melanoma was melanotic, while metastatic nests in the LN included both amelanotic and melanotic melanoma. As expected, the PA effect was not obvious in amelanotic melanoma, but was seen in melanotic melanoma on the ratio images [Figures 3d and 4c]. Although the prevalence is unknown, there have been reports of cases of primary melanotic melanoma with metastasis as amelanotic melanoma.^[3] As melanin production involves cellular differentiation, amelanotic melanoma is considered to be rapidly growing and more primitive, easier to metastasize, and to be related to poor prognosis.^[4] Therefore, screening workup

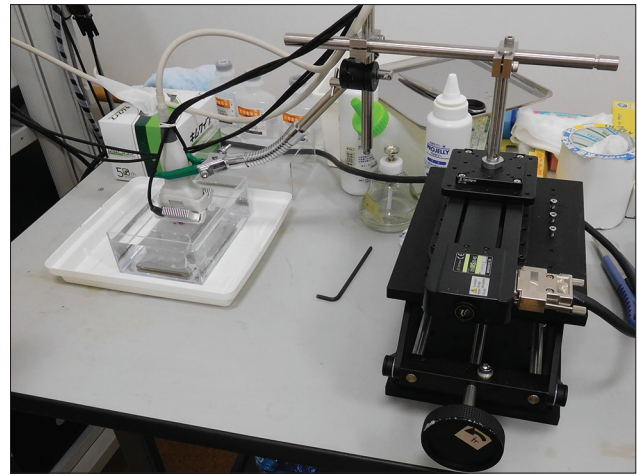


Figure 1: Scene of the experimental scan. The black machine on the right side of the photograph holds a probe with two light-emitting diode light sources with different wavelengths and has a function of scanning at a constant speed. The probe surface is positioned above the specimen on the glass slide held in a small water tank

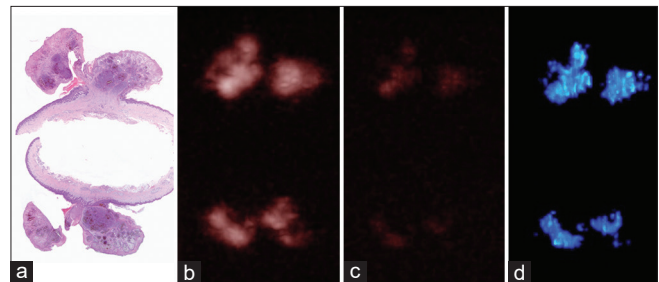


Figure 2: Loupe image of the primary lesion and photoacoustic imaging reconstructed into a plane with different wavelengths (820 nm and 940 nm) and ratio image. (a) The primary lesion seemed to be a nodular or polypoid skin tumor with pigmentation. Histopathological diagnosis was melanoma. (b) The photoacoustic signal was effectively obtained from the site of melanin on photoacoustic imaging at 820 nm. (c) The magnitude of the photoacoustic signal on photoacoustic imaging at 940 nm was weaker than that at 820 nm. (d) The ratio image showed the melanin site in blue, indicating a significant difference in signal intensity obtained at different wavelengths

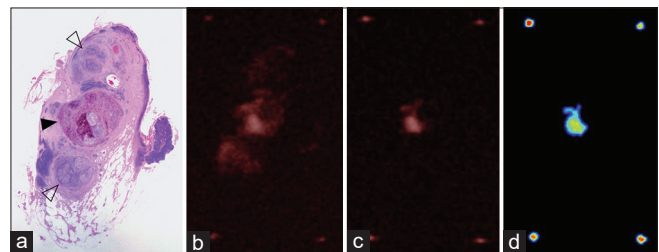


Figure 3: Loupe image of metastatic lesions and photoacoustic imaging reconstructed into a plane with different wavelengths and ratio image. (a) Loupe image showing three metastatic nests in the lymph node. One was melanotic (black arrowhead), the others were amelanotic (open arrowheads). (b) The photoacoustic signal was effectively obtained from the site of melanin at 690 nm. (c) The magnitude of the photoacoustic signal on photoacoustic imaging at 850 nm was weaker. (d) Ratio image showing the melanin site in yellow to blue. The signal intensity difference is smaller at sites in yellow, probably related to the higher density of melanin

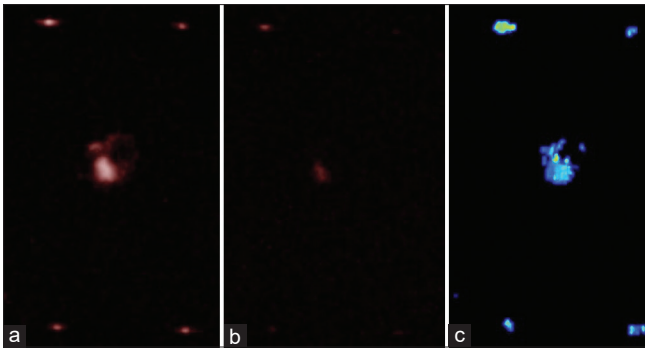


Figure 4: Photoacoustic imaging system reconstructed into a plane with different wavelengths and ratio image. (a) Photoacoustic signal was effectively obtained from the site of melanin at 820 nm. It was difficult to compare the magnitude of the photoacoustic effect acquired at combinations between 690/850 and 820/940 nm because the distance between the probe and the sample may have changed. (b) The magnitude of the photoacoustic signal on photoacoustic imaging at 940 nm was weaker. (c) Ratio image showing the melanin site in blue. There was a significant difference in signal intensity obtained at different wavelengths

for LN metastasis from melanoma, even in cases of primary melanotic melanoma, should be performed by conventional ultrasonographic examination as well as PAI in cases with amelanotic transformation. PA signals were apparently weaker at higher wavelengths with both different light sources at sites positive for melanin on optical microscopy. These findings were consistent with PA signals from melanin. This is because light absorption by melanin is reduced with higher wavelength light sources according to the absorption spectrum chart.^[2]

Although the method described in this study, which used PAI to evaluate specimens that had already been fixed, sliced, and stained on glass slides, has not been widely adopted, we feel that it is significant in terms of precise correlation between imaging and histopathological results. In addition, as described in the results section, the PA effect was also observed in areas where lymphocytes were accumulated, especially at 690 nm [Figure 5a and b]. Based on the histopathological results, it was speculated that the effect was mainly related to hematoxylin bound to the nuclei of lymphocytes. Considering the influence of the PA effect from hematoxylin on PAI, there was no significant influence on the diagnosis of the presence of melanin on ratio images.

CONCLUSION

As PAI is considered to be potentially effective for the screening of LN metastasis in cases with melanotic melanoma, workup should be performed by not only PAI but also conventional ultrasonography in cases with metastasis related to amelanotic transformation, which is considered to be more aggressive and likely to be missed by PAI alone.

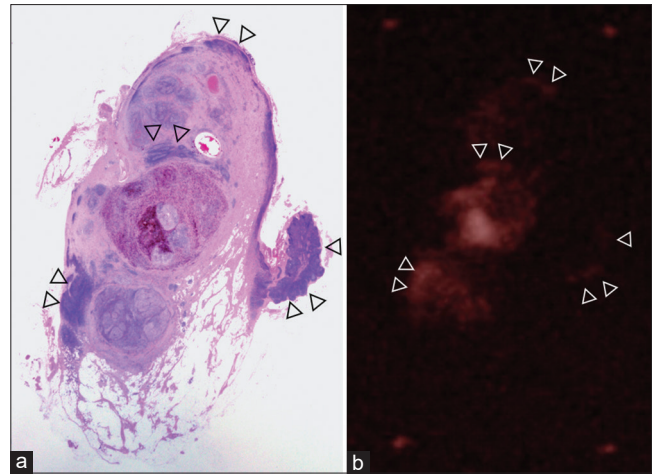


Figure 5: (a and b) Loupe image of metastatic lesions in the lymph node and photoacoustic imaging reconstructed into a plane with a wavelength of 690 nm. The photoacoustic signal was also obtained from the site of lymphocyte accumulation without melanin (open arrowheads). It was speculated that the effect was mainly related to hematoxylin bound to the nuclei of lymphocytes according to the results of histopathological analysis

Acknowledgment

We would like to express our gratitude to Dr. Naoto Sato of Cyberdyne (Tsukuba, Ibaragi Japan) for technical support.

Declaration of patient consent

The authors certify that they have obtained all appropriate patient consent form. In the form the patient has given her consent for her images and other clinical information to be reported in the journal. The patient understands that her name and initials will not be published and due efforts will be made to conceal her identity, but anonymity cannot be guaranteed.

Financial support and sponsorship

Nil.

Conflicts of interest

There are no conflicts of interest.

REFERENCES

1. Sinnamon AJ, Neuwirth MG, Song Y, Schultz SM, Liu S, Xu X, *et al.* Multispectral photoacoustic imaging for the detection of subclinical melanoma. *J Surg Oncol* 2019;119:1070-6.
2. Kratkiewicz K, Manwar R, Rajabi-Estarabadi A, Fakhoury J, Meiliute J, Daveluy S, *et al.* Photoacoustic/ultrasound/optical coherence tomography evaluation of melanoma lesion and healthy skin in a swine model. *Sensors (Basel)* 2019;19: pii: E2815.
3. Ogoshi T, Kido T, Yatera K, Nagata S, Nishida C, Yamasaki K, *et al.* A case of rapidly progressive metastatic pulmonary amelanotic malignant melanoma 16 years after resection of melanoma. *Nihon Kokyuki Gakkai Zasshi* 2011;49:770-4.
4. Shah JP. Amelanotic melanoma. *Prog Clin Cancer* 1975;6:195-7.