


 Cite this: *RSC Adv.*, 2023, **13**, 21550

Trace determination of disinfection by-products in drinking water by cyclic ion chromatography with large-volume direct injection

 Haibao Zhu,^{ab} Zheng Ruan,^a Han Wang,^a Danhua Liu,^a Hongfang Tang^a and Jiahong Wang^{*c}

A novel cyclic ion chromatography (IC) system was developed for the simultaneous determination of trace disinfection by-products (DBPs) in drinking water. Five DBPs (chlorite, bromate, chlorate, dichloroacetic acid, and trichloroacetic acid) were sensitively determined by large-volume direct injection, and the interferences of dominant inorganic anions present in water were eliminated online through the cyclic determination of the target analytes. Under optimized conditions, the obtained limits of detection (LODs) were in the range of 0.18–1.91 $\mu\text{g L}^{-1}$ based on a signal-to-noise ratio (S/N) of 3 and an injection volume of 1.0 mL. The RSDs for peak area and retention time were in the range of 0.13–1.03% and 1.24–4.29%, respectively. Satisfactory recoveries between 92.3% and 106.4% were obtained by adding three concentration gradients of standards to the drinking water samples. The proposed method has advantages such as high sensitivity, facile automation, and no sample pretreatment, and might be a promising approach for routine analysis.

Received 13th April 2023

Accepted 5th July 2023

DOI: 10.1039/d3ra02471g

rsc.li/rsc-advances

1 Introduction

Drinking water disinfection is an indispensable measure to guarantee public health, and can remove viruses, bacteria, and other micro-pollutants as well as provide purified water for human consumption.^{1–3} Disinfection by-products (DBPs) are a series of contaminants produced by the reaction of disinfectants (chlorine, chlorine dioxide, ozone, *etc.*) with natural compounds in water during the disinfection process.⁴ DBPs in drinking water can pose long-term health risks to humans, including potential carcinogenic, mutagenic, and reproductive toxicity, which has attracted considerable public attention.⁵ Chlorite, bromate, and chlorate are three typical hazardous inorganic oxyhalide DBPs, among which bromate has been identified as a potential carcinogen by the World Health Organization (WHO) and the United States Environmental Protection Agency USEPA.^{6,7} Haloacetic acids (HAAs) are also another group of DBPs that are detected in drinking water frequently,⁸ and dichloroacetic acid (DCAA) and trichloroacetic acid (TCAA) are two HAAs with the highest concentrations and carcinogenic risk in drinking water.⁹ Due to their widespread occurrence and

potential health risks, some countries have established limit values for the content of oxyhalide DBPs and HAAs in drinking water. Therefore, it is necessary to conduct routine analysis of these DBPs in drinking water to ensure consumer health.

Multiple analytical methods have been developed for the determination of DBPs in drinking water. For example, the United States Environmental Protection Agency (USEPA) recommends using gas chromatography (GC) to detect HAAs.¹⁰ Before being injected into the GC system, the samples need to undergo pretreatment processes such as acidification, liquid-liquid extraction, and esterification derivatization, which are time-consuming and labor-intensive. Although liquid chromatography coupled with inductively coupled plasma mass spectrometry (ICP-MS) can detect bromate in water, it is limited to determining only one or two compounds, making the simultaneous determination of multiple substances challenging.¹¹ Since chlorite, bromate, and chlorate in drinking water are present in an ionic form, and although DCAA and TCAA exist in a neutral form, their acid-dissociation coefficients ($\text{p}K_{\text{a}}$) are low.¹² Therefore, ion chromatography (IC) coupled with conductivity detection is a more suitable method for determining these substances.

To date, many reports have been published on the use of ion chromatography for determining oxyhalide DBPs and HAAs in drinking water.^{13,14} Compared with gas chromatography and ICP-MS, IC has obvious advantages such as simple sample treatment, rapid determination, and good reproducibility.¹⁵ However, due to the low concentrations of DBPs in water samples, IC with a large-volume injection method is usually

^aSchool of Public Health, Hangzhou Medical College, Hangzhou, Zhejiang 310013, P. R. China

^bKey Laboratory of Microbial Technology for Industrial Pollution Control of Zhejiang Province, College of Environment, Zhejiang University of Technology, Hangzhou, Zhejiang 310014, P. R. China

^cCenter of Safety Evaluation and Research, Hangzhou Medical College, Hangzhou, Zhejiang 310013, P. R. China. E-mail: 202000283@hmc.edu.cn



adopted, which significantly improves the determination sensitivity of DBPs.¹⁶ However, this method also leads to the concentration of dominant inorganic anions (fluoride, chloride, nitrate, sulfate, *etc.*) present in water samples, causing interference with the DBPs determination.¹⁷ This interference is mainly eliminated by optimizing chromatographic conditions and offline pretreatment (*e.g.*, on guard Ag pretreatment column to remove chloride ions and on guard Ba pretreatment column to remove sulfate ions) of water samples before IC injection.¹⁸ At present, there is still no universal ideal online IC technology to completely eliminate the influence of this disturbance on DBPs determination.

In this study, a novel cyclic ion chromatography system with a large-volume direct injection system was established. Automated and selective online elimination of inorganic anions was achieved by using valve-switching technology and cyclic measurement of the target DBPs. The positions of the enrichment column can be automatically changed by repeatedly switching the valve. After the first separation in the analytical column, the affected target DBPs were concentrated on the enrichment column, and a large amount of interfering components were directly discharged into the waste liquid. Then, DBPs which concentrated on the enrichment column were cut onto the analytical column again by column-switching for secondary separation. The elimination of coexisting interfering anions with high concentrations in the sample was realized by cyclic analysis of the DBPs. This method was successfully applied to the simultaneous determination of five DBPs (chlorite, bromate, chlorate, DCAA, and TCAA) in drinking water.

2 Experimental

2.1 Equipment

A Thermo Scientific Dionex ICS 2100 ion chromatograph (Sunnyvale, CA, USA) was employed in this research. It was composed of the following modules: an AS-DV auto-sampler, a dual-piston serial pump, an EG40 eluent generator, a DS6 conductivity detector, and two six-port valves. An ASRS 3000 suppressor (Thermo, Sunnyvale, CA, USA) was used for eluent suppression in the external-water mode. The analytical column was an IonPac AG19 (50 mm × 4 mm i.d., 5 μm) guard column and an IonPac AS19 (250 mm × 4 mm i.d., 5 μm) separation column. Another IonPac AG19 column (50 × 4 mm i.d., 5 μm) was used as the enrichment column. Polyether ether ketone (PEEK) tubes were used to connect all chromatographic modules, and the lengths of the connecting tubes were kept as short as possible to minimize system void volume. The cyclic IC system built with the above modules is shown in Fig. 1.

2.2 Reagents and materials

Standard solutions, including chlorite, bromate, chlorate, DCAA, and TCAA, with a concentration of 1000 mg mL⁻¹, were purchased from Anpu Experimental Technology Co., Ltd (Shanghai, China), respectively. Other anion standards were prepared from corresponding salts (Sinopharm Chemical Reagent Co. Ltd, China). Experimental water was obtained from a Milli-Q water purification

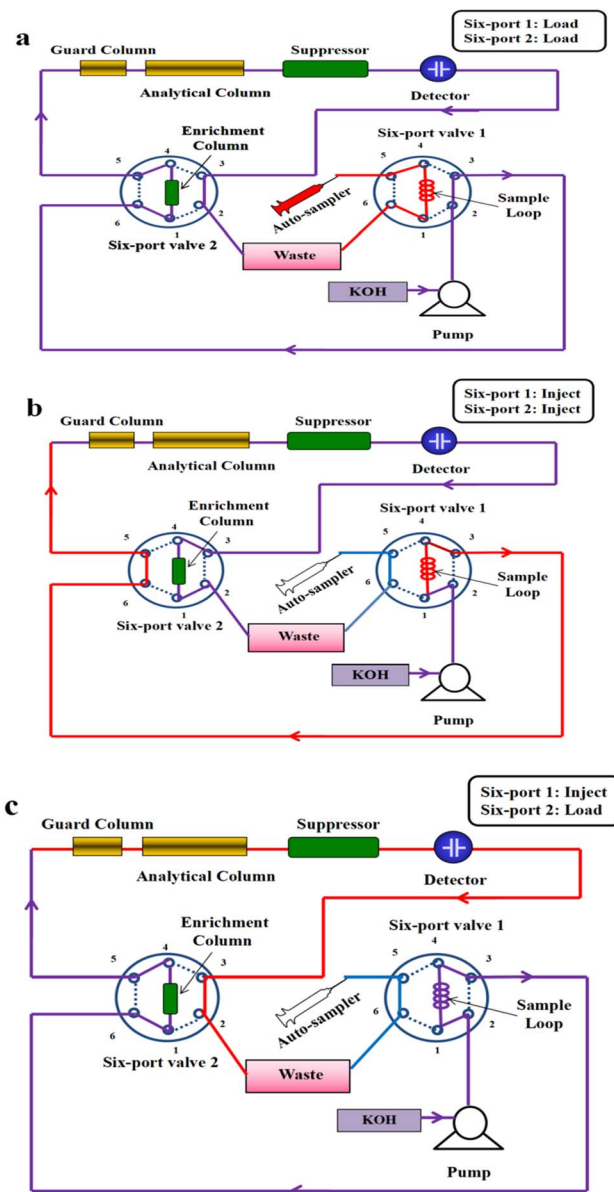


Fig. 1 Chromatographic instrument configurations for the analysis of trace DBPs in drinking water. (a) System balancing and sample injecting; (b) online removal of interfering substances and collection of target components; (c) secondary analysis of target components.

system (Millipore, Bedford, MA, USA). Working standards were prepared by further diluting the above standards to the expected range. The solutions used in the experiment were stored in tightly sealed containers and refrigerated at 4 °C to prevent possible spoilage. Furthermore, stability tests showed that all solutions remained stable for at least three months under the storage conditions of this experiment. Water samples were filtered through a 0.45 μm membrane filter before being injected into the IC system.

2.3 Chromatographic conditions

The eluent generator was set to generate a concentration of 12 mmol per L KOH as an eluent to analyze the target

compounds. The suppressor current was set at 115 mV. Data acquisition, instrument control, and the switching program of the two six-port valves were all controlled by Chromeleon 6.8 software (Dionex, USA). The positions of the enrichment column could be changed by switching the six-port valves. Correspondingly, the mobile phase of the enrichment column was also varied. In different states, the eluent flowing through the enrichment column was either KOH solution or water, which was converted from KOH liquid by the suppressor. The flow rate of the entire process was 1.0 mL min^{-1} , and the sampling loop was set to a large-volume of 1.0 mL. The temperature of the detector cell and analytical column was 35°C and 26°C , respectively.

2.4 Experimental procedure

Four steps were involved in eliminating interferences of conventional anions and determining the concentrations of five DBPs: (i) loading the sample into the sample loop *via* an automatic sampling device, after balancing the chromatographic system; (ii) delivering the sample from the sample loop into the separation column and performing the first separation step; (iii) collecting the disturbed target components by the enrichment column and eliminating the matrix inorganic anions; and (iv) analyzing the disturbed target components for the second time by the analytical column. All these steps were achieved by controlling the cyclic IC system that we constructed in this study.

3 Results and discussion

3.1 Operation procedure of the cyclic IC system

Fig. 1 illustrates the configuration diagram of our cyclic IC system. By switching six-port valve 1 and six-port valve 2, the connection patterns of modules in the IC system can be modified to achieve different objectives. Sample injection was accomplished by switching valve 1 (Fig. 1a and b). The collection and secondary analysis of the disturbed components were mainly achieved by switching valve 2. It was worth noting the suppressor in the IC system can convert the KOH eluent to water. When valve 2 was in the “injection” position (Fig. 1b), the enrichment column was connected behind the detector cell. In this condition, water or waste liquid containing sample ions was the mobile phase which flowing through the enrichment column. As the above liquids had no elution capability, target compounds could be concentrated in the enrichment column. Due to the first separation of the analytical column, the target compounds and the interfering matrix have been separated preliminary. By switching valve 2, the disturbed target compounds were concentrated on the enrichment column, and the interfering components were discharged into the waste directly. Then, with valve 2 in the “load” position, the enrichment column was placed at the front of the guard column (Fig. 1c), and the KOH eluent was the mobile phase which flowing through the enrichment column. The components concentrated on the enrichment column can be eluted onto the analytical column under the action of KOH eluent for the

secondary separation. Owing to most of the matrix have been discharged into the waste, their effects could be eliminated in the process of secondary analysis.

3.2 Selection of chromatographic parameters

Traditional IC methods for the simultaneous determination of oxyhalide DBPs and HAAs have strict requirements on parameters such as the concentration and gradient of KOH eluent, flow rate, and column temperature.¹⁹ In contrast, the chromatographic parameters of the cyclic IC in this study were relatively flexible. However, to expand the cyclic IC system applications, we optimized the IC parameters in terms of improving separation, shortening analysis time, and increasing detection sensitivity. We used a large sample loop (1.0 mL) to improve sensitivity. Meanwhile, an isocratic analysis with 12 mmol per L KOH eluent was selected, taking into account both separation efficiency and analysis time. In addition, the columns of the IC system were kept in a constant temperature environment of 26°C to maintain the stability of the entire process. Based on the above chromatographic parameters, we also focused on optimizing the switching opportunities of the two switching valves (valve 1 and valve 2).

3.3 Interference of the matrix concentration

In this study, the influence of inorganic anion matrices on the determination of DBPs were investigated. Drinking water quality standards in China, the EU, and the US EPA all explicitly stipulate the maximum allowable concentrations of common inorganic anions in drinking water.²⁰ The traditional IC method was used to investigate the effect of the concentration of inorganic anion matrix in water samples on the determination of target DBPs. We found that when the concentrations of fluoride and sulfate are at their maximum allowable levels (fluoride: 1.5 mg L^{-1} , sulfate: 250 mg L^{-1}), neither substance interferes with the determination of the five DBPs. Similarly, trace amounts of nitrite and bromide ions in drinking water do not interfere with the measurement of the target DBPs. Nevertheless, due to the lower resolution between the chromatographic peaks of chloride and DCAA, as well as nitrate and TCAA, when the concentrations of chloride and nitrate increase, they may interfere with the determination of DCAA and TCAA, respectively. As shown in Fig. 2a. When the chloride concentration exceeds 1.5 mg L^{-1} in the determination of drinking water by the traditional IC method, the peak area of DCAA ($100 \mu\text{g L}^{-1}$) decreases significantly. Likewise, the peak area of TCAA ($100 \mu\text{g L}^{-1}$) also experiences a significant decrease when the nitrate concentration exceeds 2.0 mg L^{-1} (Fig. 2b). Therefore, it is necessary to employ the cyclic IC system to eliminate chloride and nitrate interference online.

3.4 Optimization of switching time

Table 1 illustrates the cut windows of the valves and how the system performs clearly. In this study, the cut windows of valve 2 were essential important for the entire experiment, and were strongly associated with the efficiency of matrix elimination and the accurate determination of analytes. Three cut windows of

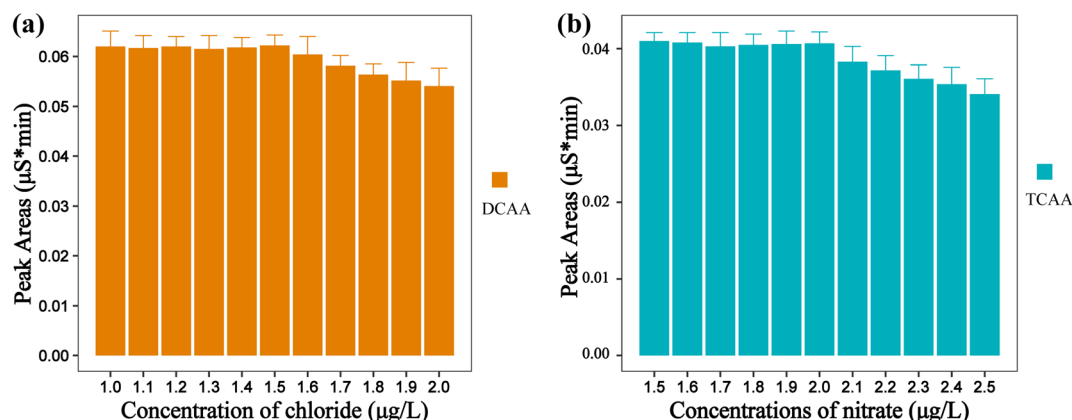


Fig. 2 Effect of inorganic anion matrix content in standard solutions on the peak areas of target substances using the traditional IC method ($n = 6$). (a) DCAA, $100 \mu\text{g L}^{-1}$; (b) TCAA, $100 \mu\text{g L}^{-1}$. Conditions: eluent, 12 mmol per L KOH; flow rate, 1.0 mL min^{-1} ; suppressor current, 115 mV; analytical column, IonPac AG19 + AS19; temperature of the detector cell, $35 \text{ }^\circ\text{C}$; temperature of the analytical column, $26 \text{ }^\circ\text{C}$; sampling volume, 1.0 mL.

valve 2 were optimized in our study by determining actual tap water samples spiked with five DBPs standards. The first opportunity was from 0.0 min to the time (0.5 min) when the sample was completely washed onto the guard column with KOH eluent, ensuring that the sample was entirely eluted onto the analytical column for the first separation after injecting, and not concentrated on the enrichment column. At this point, under the action of the KOH eluent, fluoride, chlorite, and bromate were completely separated in the analytical column, and sequentially eluted out of the chromatographic column and then into the waste after being detected by the detector. Subsequently, the sequentially eluted species were chloride and DCAA, which could not be baseline separated from each other. Therefore, the second cut window was aimed at eliminating the interference of chloride on DCAA. When DCAA eluted from the chromatographic column (9.7 min), the valve 2 was switched,

and the enrichment column was placed behind the detector cell to concentrate DCAA and some chloride ions. We found that if the enrichment column was immediately switched back to the front of the guard column after complete enrichment of DCAA, nitrate ions would interfere with the second analysis of DCAA. To avoid this situation, we set the time of enrichment column cutting back to the front of the guard column at 12.5 min. Nitrite ions were also concentrated on the enrichment column under the conditions of our optimized cut window (9.7–12.5 min) along with all DCAA and a small amount of chloride.

To optimize the second cut window of valve 2 switching, the end time of the switching cut window was set at 12.5 min, while the start time was varied within the range of 9.3 min to 9.9 min. To ensure maximum removal of chloride, it was recommended that the start time of the cut window of valve 2 be delayed as much as possible since the time of the chloride peak is earlier

Table 1 System operation procedure

Time (min)	Valve 1	Valve 2	Position of enrichment column	Events
–0.5–0.0	Load	Load	Before the guard column	System balancing; sample injecting
0.0–0.5	Inject	Inject	After the detector cell	Washing sample onto the analytical column with KOH eluent
0.5–9.7	Inject	Load	Before the guard column	Separating and analyzing of components with retention weaker than DCAA
9.7–12.5	Inject	Inject	After the detector cell	Collecting of DCAA and nitrite online, eliminating the interfering chloride ions
12.5–18.5	Inject	Load	Before the guard column	Separating and analyzing of components with retention weaker than TCAA and stronger than DCAA, analyzing of DCAA by analytical column secondary
18.5–20.1	Inject	Inject	After the detector cell	Collecting of TCAA online, eliminating the interfering nitrate ions
20.1–50	Inject	Load	Before the guard column	Analyzing of TCAA by analytical column secondary, separating and analyzing of components with retention stronger than TCAA
50–60	Load	Load	Before the guard column	Purification chromatographic system; equilibrium chromatographic system

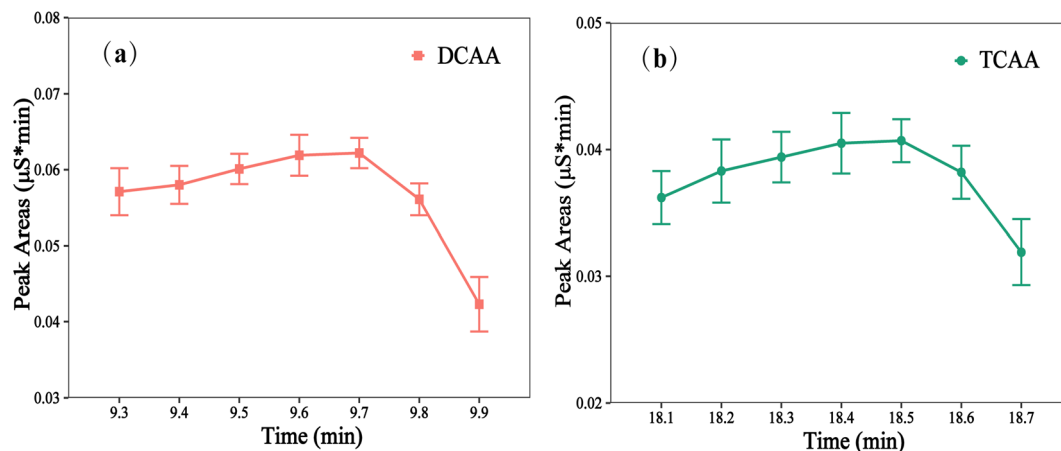


Fig. 3 Effect of the switching time of valve 2 on the peak areas of target substances using the cyclic IC method ($n = 6$). (a) DCAA, $100 \mu\text{g L}^{-1}$; (b) TCAA, $100 \mu\text{g L}^{-1}$. Conditions: eluent, 12 mmol per L KOH; flow rate, 1.0 mL min^{-1} ; suppressor current, 115 mV; analytical column, IonPac AG19 + AS19; enrichment column, IonPac AG19; temperature of the detector cell, $35 \text{ }^\circ\text{C}$; temperature of the analytical column, $26 \text{ }^\circ\text{C}$; sampling volume, 1.0 mL.

than that of the DCAA. However, after 9.7 min, some of the DCAA could not be entirely collected, resulting in a sharp decrease in peak area (Fig. 3a). As a result, the optimum switching cut window of valve 2 was established at 9.7–12.5 min. Additionally, 18.5–20.1 min was selected as the third cut windows of valve 2. At this point, the DCAA, a small amount of chloride, and nitrite ions concentrated on the enrichment column in the previous stage have been completely eluted out and analyzed for the second time by the analytical column before being discharged into the waste. As shown in Fig. 3b, 18.5 min was the optimal start time for the third cut window.

Under the optimized cut window of 18.5–20.1 min, the TCAA was completely concentrated on the enrichment column while minimizing the presence of nitrate matrix as much as possible.

Fig. 4 displays the representative chromatogram of actual tap water samples spiked with 5 DBPs standards. As shown in Fig. 4, Chlorite (peak a), bromate (peak b), and chlorate (peak d) were not affected by the coexisting inorganic anions, and they could be directly quantified by the first separation of analytical column. Nevertheless, DCAA (peak c) and TCAA (peak e) were obviously interfered by the tail peaks of chloride and nitrate, respectively. Under the optimized switching windows, the above interferences were eliminated, and baseline separation was achieved (peak c' and e') by cycle analysis.

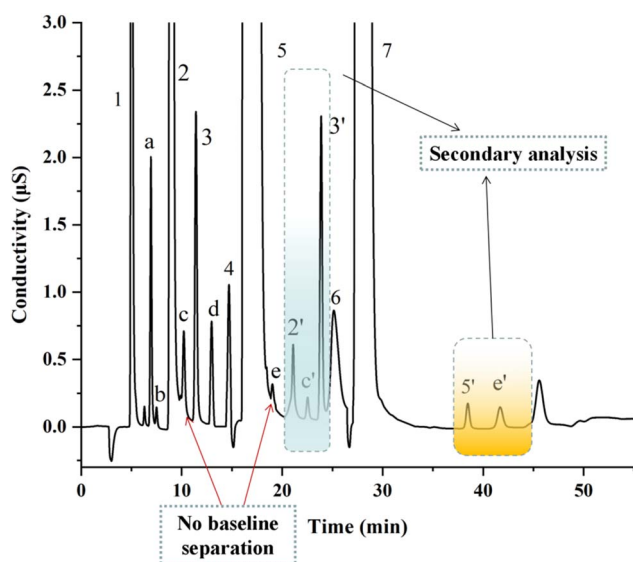


Fig. 4 Chromatogram of actual tap water samples spiked with 5 DBPs standards. Peaks for first analysis (add levels): 1 = fluoride; 2 = chloride; 3 = nitrite; 4 = bromide; 5 = nitrate; 6 = carbonate; 7 = sulfate; a = chlorite (0.1 mg L^{-1}); b = bromate (0.02 mg L^{-1}); c = DCAA (0.1 mg L^{-1}); d = chlorate (0.1 mg L^{-1}); e = TCAA (0.1 mg L^{-1}); peaks for secondary analysis: 2' = chloride; c' = DCAA (0.1 mg L^{-1}); 3' = nitrite; 5' = nitrate; e' = TCAA (0.1 mg L^{-1}).

3.5 Analytical performances

Under the above optimized conditions, five standard solutions containing DBPs at various concentrations ranging from 5.00 – $100 \mu\text{g L}^{-1}$ (1.0 – 20 for bromate) were analyzed. Each target DBPs exhibited satisfactory linearity within the studied range, with all determination coefficients $R \geq 0.9991$. The limits of detection (LODs) and limits of quantification (LOQs), calculated by injecting a 1.0 mL volume of a standard solution with a concentration of $5.0 \mu\text{g L}^{-1}$ (bromate: $1.0 \mu\text{g L}^{-1}$) and based on signal-to-noise ratios (S/N) of 3 and 10, were calculated to be in the range of 0.18 – $1.91 \mu\text{g L}^{-1}$ and 0.60 – $6.37 \mu\text{g L}^{-1}$, respectively. The precision results of the cyclic IC method were obtained by calculating the relative standard deviation (RSD) values for 6 repetitive injections of $5.0 \mu\text{g L}^{-1}$ ($1.0 \mu\text{g L}^{-1}$ for bromate) standard solutions. The RSD for peak area and retention time ranged from 0.13 – 1.03% and 1.24 – 4.29% , respectively. All analytical performances of the proposed method are listed in Table 2.

This method was applied for the simultaneous determination of five DBPs in actual drinking water. The anion matrix in the samples has no interference with the determination of target analytes by using the cyclic IC system. Spiked-recovery

Table 2 Calibration parameters (five points) for the DBPs in standard solutions ($n = 6$)

Analytes	Linear range ($\mu\text{g L}^{-1}$)	Determination coefficient (R)	LODs ^a ($\mu\text{g L}^{-1}$)	LOQs ^b ($\mu\text{g L}^{-1}$)	RSD (%)	
					Retention time	Peak area
Chlorite	5.00–100	0.9992	0.18	0.60	0.13	1.24
Bromate	1.00–20.0	0.9991	0.38	1.27	0.25	2.76
DCAA	5.00–100	0.9991	0.59	1.97	0.54	3.05
Chlorate	5.00–100	0.9995	0.43	1.43	0.22	2.17
TCAA	5.00–100	0.9990	1.91	6.37	1.03	4.29

^a LODs: limits of detection. ^b LOQs: limit of quantification.

experiments with three concentration levels were also performed using three typical samples (two tap water and one mineral water) to determine the accuracy of the method. As shown in Table 3, the method had spiking recovery rates of 92.3–105.3% with an RSD of 1.80–3.92% at the low concentration level, 94.8–106.4% with an RSD of 0.95–3.54% at the medium concentration level, and 95.3–102.7% with an RSD of 0.61–3.77% at the high concentration level. These results were satisfactory for trace analysis. Therefore, the complete resolution of chromatographic peaks and accurate quantification of five DBPs with high concentration of anion matrix in drinking water were achieved by the cyclic IC method.

3.6 Methods comparison

To evaluate the applicability of the cyclic IC method for the determination of trace DBPs, we compared the method used in this study with IC methods reported in the literature in terms of method performance and the greenness level. As

shown in Table 4, the LODs of the cyclic IC and the literature methods were both in the $\mu\text{g L}^{-1}$ level. The mobile phase used in the cyclic IC was a KOH solution, which resulted in a lower background conductivity value of the chromatogram baseline than an IC system using Na_2CO_3 solution as the eluent. Consequently, the LODs of the cyclic IC system were relatively lower. Additionally, the cyclic IC method demonstrated better quantification precision than the literature methods. This is due to the elimination of matrix ions through cyclic analysis, enabling accurate quantification of the target analytes. It should be noted that the retention time precisions of DCAA and TCAA were slightly reduced in the cyclic IC system. In terms of analysis time, the cyclic IC method required a longer duration than the literature methods. Thus, by using two assessment tools (analytical eco-scale and GAPI) to evaluate the level of greenness of the developed method^{27,28} (Table 5), the cyclic IC system consumed more solvents, reagents and energy than the conventional methods. However, due to the

Table 3 Data on analysis of real samples and spiked recoveries of five DBPs

Analytes	Original ($\mu\text{g L}^{-1}$)	Low level			Medium level			High level		
		Add level ($\mu\text{g L}^{-1}$)	Recovery (%)	RSD (%)	Add level ($\mu\text{g L}^{-1}$)	Recovery (%)	RSD (%)	Add level ($\mu\text{g L}^{-1}$)	Recovery (%)	RSD (%)
Sample 1 (tap water)										
Chlorite	ND ^a	5.00	97.4	2.13	20.0	98.3	1.22	50.0	100.3	2.42
Bromate	ND	1.00	98.3	3.04	4.00	97.6	1.74	10.0	98.5	1.83
DCAA	10.1	5.00	96.6	3.47	20.0	100.2	0.96	50.0	99.7	1.65
Chlorate	ND	5.00	105.3	1.91	20.0	99.4	2.41	50.0	101.4	0.61
TCAA	15.2	5.00	94.7	3.29	20.0	95.2	3.54	50.0	96.2	2.76
Sample 2 (tap water)										
Chlorite	12.6	5.00	97.8	1.80	20.0	99.4	1.44	50.0	102.7	0.80
Bromate	ND	1.00	97.6	2.43	4.00	100.6	1.26	10.0	99.3	2.62
DCAA	ND	5.00	102.1	2.46	20.0	98.3	1.78	50.0	98.1	1.14
Chlorate	9.26	5.00	99.4	2.29	20.0	106.4	2.61	50.0	97.4	2.35
TCAA	ND	5.00	94.7	2.72	20.0	96.1	3.10	50.0	95.9	3.77
Sample 3 (mineral water)										
Chlorite	ND	5.00	96.4	2.41	20.0	99.4	2.33	50.0	100.4	1.46
Bromate	2.41	1.00	97.0	1.93	4.00	98.9	2.12	10.0	98.6	0.82
DCAA	ND	5.00	93.6	2.75	20.0	95.6	0.95	50.0	97.9	1.84
Chlorate	ND	5.00	96.1	3.17	20.0	99.4	1.53	50.0	101.6	2.64
TCAA	ND	5.00	92.3	3.92	20.0	97.5	2.39	50.0	95.3	3.69

^a ND: not detected (lower than the limit of detection).

Table 4 Comparative data for the determination of DBPs by ion chromatography methods

Analytes	Column(s)	Eluent	Flow rate (mL min ⁻¹)	Analysis time (min)	Detector	Quantification precision (RSD, %)	LODs (µg L ⁻¹)	Ref.
BrO ₃ ⁻ , ClO ₃ ⁻	Metosep A Dual 1	1 mmol per L <i>ortho</i> -phthalic acid, 2% MeCN	1.0	15	UV/Vis	1.31–2.06	5.2–10	21
BrO ₃ ⁻ , ClO ₂ ⁻ , ClO ₃ ⁻ , Br ⁻	IonPac AS 19-HC + AG 19-HC	9 mmol per L Na ₂ CO ₃	1.3	25	Conductivity UV/Vis	0.54–8.81	µg L ⁻¹ levels	22
ClO ₂ ⁻ , BrO ₃ ⁻ , ClO ₃ ⁻ , ClO ₄ ⁻	IonPac AS 20 + AG 20	5–100 mmol per L NaOH	0.375	18	Conductivity	3.49–6.78	2–27	23
ClO ₃ ⁻ , NO ₂ ⁻	IonPac AS 19 + AG 19	KOH gradient	1	>30	Conductivity	<2	2.2	24
BrO ₃ ⁻ , ClO ₂ ⁻ , ClO ₃ ⁻ , Br ⁻	IonPac AS 19-HC + AG 19-HC	9 mmol per L Na ₂ CO ₃	0.4	25	Conductivity	0.10–3.66	1.32–2.55	25
BrO ₃ ⁻ , ClO ₂ ⁻ , I ⁻	IonPac AS 19-HC	9 mmol per L Na ₂ CO ₃	1.1	6.5	UV/Vis	0.66–4.60	µg L ⁻¹ levels	26
ClO ₂ ⁻ , BrO ₃ ⁻ , DCAA, ClO ₃ ⁻ , TCAA	IonPac AS 19 + AG 19	12 mmol per L KOH	1.0	60	Conductivity	0.13–1.03	0.18–1.91	This study

Table 5 Greenness assessment of the proposed method and traditional method according to analytical eco-scale and GAPI

Eco-scale assessment			GAPI assessment		
Category	Description (per sample)		Category	Description (per sample)	
	Cyclic IC system	Traditional IC method ^{21–26}		Cyclic IC system	Traditional IC method ^{21–26}
Reagents			Sample preparation		
Reagents (g)	28.8 mg NaOH	6.20–23.9 mg Na ₂ CO ₃ /3.6–72 mg NaOH	(1) Collection; (2) preservation; (3) transport; (4) storage	(1) Off line; (2)—; (3)—; (4) normal conditions	(1) Off line; (2)—; (3)—; (4) normal conditions
Water (mL)	60	15–30	(5) Type of method: direct or indirect; (6) scale of extraction; (7) solvents/reagents used; (8) additional treatments	(5) Direct; (6) no; (7) no; (8) no	(5) Indirect; (6) no; (7) no; (8) pretreatment
Instrumentation			Reagents and solvents		
Energy (W h)	150	37.5–75	(9) Amount; (10) health hazard; (11) safety hazard	(9) 28.8 mg NaOH + 60 mL water; (10) low; (11) safe	(9) 6.20–23.9 mg Na ₂ CO ₃ /3.6–72 mg NaOH + 15–30 mL water; (10) low; (11) safe
Occupational safety	Safe	Safe	Instrumentation		
Hazard	Low	Low	(12) Energy (W h)	(12) 150	(12) 37.5–75
Waste (mL)	60	15–30	(13) Occupational hazard	(13) Safe	(13) Safe
Total comment	Green method	Green method	(14) Waste; (15) waste treatments	(14) 60 mL; (15) no treatment	(14) 15–30 mL; (15) no treatment

use of a low concentration of KOH solution as the mobile phase instead of organic solvents, the waste generated by the cyclic IC system was relatively less hazardous to the health of the operator and the environment. As a result, the eco-scale assessment shows that both cyclic ion chromatography and conventional IC methods are environmentally friendly. The main advantage of the cyclic IC method, as assessed by GAPI, is that the samples do not require complex pretreatment and

can be injected directly into the system for automated analysis. This reduces the time and cost associated with sample pretreatment and manual operation. Overall, the cyclic IC method outperforms traditional IC methods in terms of performance indicators and level of automation. Therefore, this method can be utilized as a green routine approach for the daily detection of water samples.

4 Conclusions

In this study, a novel cyclic IC method has been proposed based on valve switching technology. This method achieved the simultaneous determination of five trace DBPs (chlorite, bromate, DCAA, chlorate, and TCAA) in drinking water through large-volume injection. Meanwhile, interferences from chloride and nitrate in the drinking water samples were eliminated online by the cyclic determination of DCAA and TCAA, respectively. Under optimal conditions, the proposed method showed good accuracy, precision, and linearity over a wide range of concentrations. Compared to traditional IC methods, drinking water samples can be injected directly into the cyclic IC system for analysis without pretreatment. Therefore, the cyclic IC method can be a promising alternative for the determination of trace DBPs in drinking water. Additionally, the method can be applied as an online matrix elimination technique to determine trace substances in various samples containing high concentrations of salt matrices.

Author contributions

Haibao Zhu: writing – original draft, methodology, formal analysis. Zheng Ruan: data curation, formal analysis, investigation. Han Wang: methodology, project administration, writing – review and editing. Danhua Liu: supervision, writing – review and editing. Hongfang Tang: writing – review and editing. Jiahong Wang: methodology, writing – review and editing, supervision.

Conflicts of interest

The authors declare that they have no conflicts of interest.

Acknowledgements

This work was supported by the Basic Scientific Research Project of Hangzhou Medical College (YS2021006), Medical and Health Projects of Zhejiang Province, China (2022PY049), and Basic Public Welfare Research Project of Zhejiang Province, China (LGC20B050001).

References

- 1 J. Wei, B. Ye, W. Wang, L. Yang, J. Tao and Z. Hang, *Sci. Total Environ.*, 2010, **408**, 4600–4606.
- 2 F. Dong, Z. Pang, J. Yu, J. Deng, X. Li, X. Ma, A. M. Dietrich and Y. Deng, *J. Hazard. Mater.*, 2022, **423**, 127113.
- 3 M. R. Khan, M. S. Samdani, M. Azam and M. Ouladsmame, *J. King Saud Univ., Sci.*, 2021, **33**, 101408.
- 4 Z. Li, G. Song, Y. Bi, W. Gao, A. He, Y. Lu, Y. Wang and G. Jiang, *Environ. Sci. Technol.*, 2021, **55**, 4103–4114.
- 5 U. von Gunten, *Water Res.*, 2003, **37**, 1469–1487.
- 6 D. Tao, R. Wang, S. Shi, L. Yun, R. Tong, Y. e. Peng, W. Guo, Y. Liu and S. Hu, *Sci. Total Environ.*, 2020, **740**, 139888.
- 7 M. Ye, P. N. Nesterenko, Y. Lu, X. Huang, X. Jin and M. Chen, *J. Chromatogr. Sci.*, 2021, **59**, 217–222.
- 8 E. E. Chang, Y. P. Lin and P. C. Chiang, *Chemosphere*, 2001, **43**, 1029–1034.
- 9 C. Y. Yang, Y. P. Hang and X. L. Zhong, *Chin. J. Anal. Chem.*, 2007, **35**, 1647–1650.
- 10 USEPA, *Method 552*, Environmental Monitoring and System Laboratory, Cincinnati, OH, 1990.
- 11 E. S. Gilchrist, D. A. Healy, V. N. Morris and J. D. Glennon, *Anal. Chim. Acta*, 2016, **942**, 12–22.
- 12 D. Martínez, J. Farré, F. Borrull, M. Calull, J. Ruana and A. Colom, *J. Chromatogr.*, 1998, **808**, 229–236.
- 13 S. Cheng, Y.-P. Wu, T. R. Young, M. C. Dodd, J. Wu, H. Zhang, Z.-L. Huo, Y.-T. Qian, Y. Li, W.-T. Li and A.-M. Li, *Sci. Total Environ.*, 2021, **754**, 142297.
- 14 H. B. Teh and S. F. Y. Li, *J. Chromatogr.*, 2015, **1383**, 112–120.
- 15 Y. Liu and S. Mou, *Microchem. J.*, 2003, **75**, 79–86.
- 16 R. Michalski, *LC-GC Eur.*, 2011, **24**, 244–250.
- 17 R. Michalski, *Pol. J. Environ. Stud.*, 2005, **14**, 257–268.
- 18 H. Dong, K. Xiao, Y. Xian, Y. Wu and L. Zhu, *Food Chem.*, 2019, **270**, 196–203.
- 19 S. A. Snyder, B. J. Vanderford and D. J. Rexing, *Environ. Sci. Technol.*, 2005, **39**, 4586–4593.
- 20 J. Fu, C.-H. Huang, C. Dang and Q. Wang, *Chin. Chem. Lett.*, 2022, **33**, 4495–4504.
- 21 M. El Haddad, R. Mamouni, M. Ridaoui and S. Lazar, *J. Saudi Chem. Soc.*, 2015, **19**, 108–111.
- 22 H. P. Wagner, B. V. Pepich, D. P. Hautman and D. J. Munch, *US EPA Method 317.0*, 2001.
- 23 J. P. Hutchinson, C. Johns, M. C. Breadmore, E. F. Hilder, R. M. Guijt, C. Lennard, G. Dicinoski and P. R. Haddad, *Electrophoresis*, 2008, **29**, 4593–4602.
- 24 N. Wang, R. Q. Wang and Y. Zhu, *J. Hazard. Mater.*, 2012, **235–236**, 123–127.
- 25 J. D. Pfaff, D. P. Hautman and D. J. Munch, *US EPA Method 300.1*, 1997.
- 26 V. M. Matsis and E. C. Nikolaou, *US EPA Method 326.0, Desalination*, 2008, **224**, 231e239.
- 27 D. Moema, T. A. Makwakwa, B. E. Gebreyohannes, S. Dube and M. M. Nindi, *J. Food Compos. Anal.*, 2023, **117**, 105131.
- 28 H. M. Hafez, S. El Deeb, M. Mahmoud Swaif, R. Ismail Ibrahim, R. Ali Kamil, A. Salman Abdelwahed and A. Ehab Ibrahim, *Microchem. J.*, 2023, **185**, 108262.