







OPEN

Author Correction: Hypothermic Oxygenated New Machine Perfusion System in Liver and Kidney Transplantation of Extended Criteria Donors: First Italian Clinical Trial

Matteo Ravaioli , Vanessa De Pace, Andrea Angeletti , Giorgia Comai, Francesco Vasuri, Maurizio Baldassarre, Lorenzo Maroni , Federica Odaldi, Guido Fallani , Paolo Caraceni, Giuliana Germinario, Chiara Donadei, Deborah Malvi, Massimo Del Gaudio, Valentina Rosa Bertuzzo, Antonio Siniscalchi, Vito Marco Ranieri, Antonietta D'Errico, Gianandrea Pasquinelli, Maria Cristina Morelli, Antonio Daniele Pinna, Matteo Cescon & Gaetano La Manna

Correction to: *Scientific Reports* <https://doi.org/10.1038/s41598-020-62979-9>, published online 08 April 2020

This Article contains an error in the order of the Figures. Figures 1, 2 and 3 were published as Figures 2, 3 and 1 respectively. The correct Figures appear below as Figures 1, 2 and 3. The Figure legends are correct.

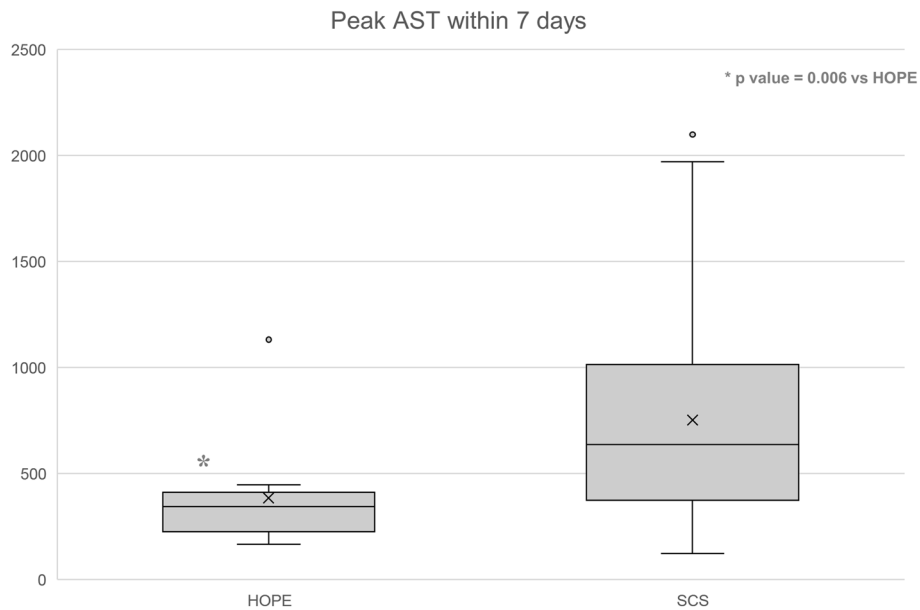


Figure 1.

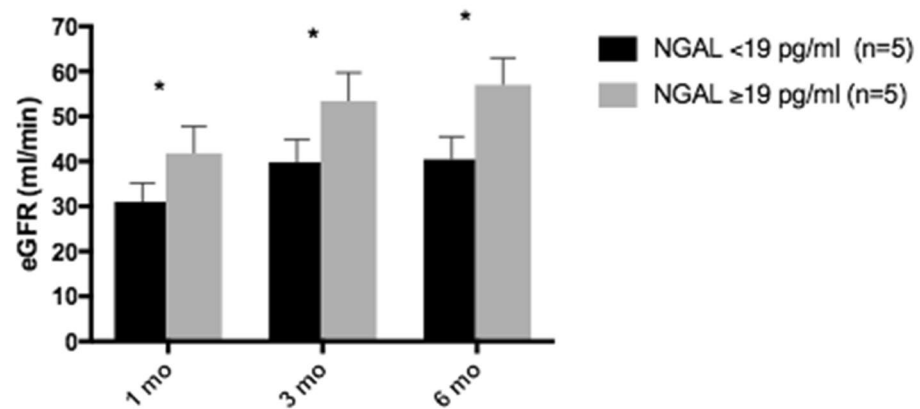


Figure 2.

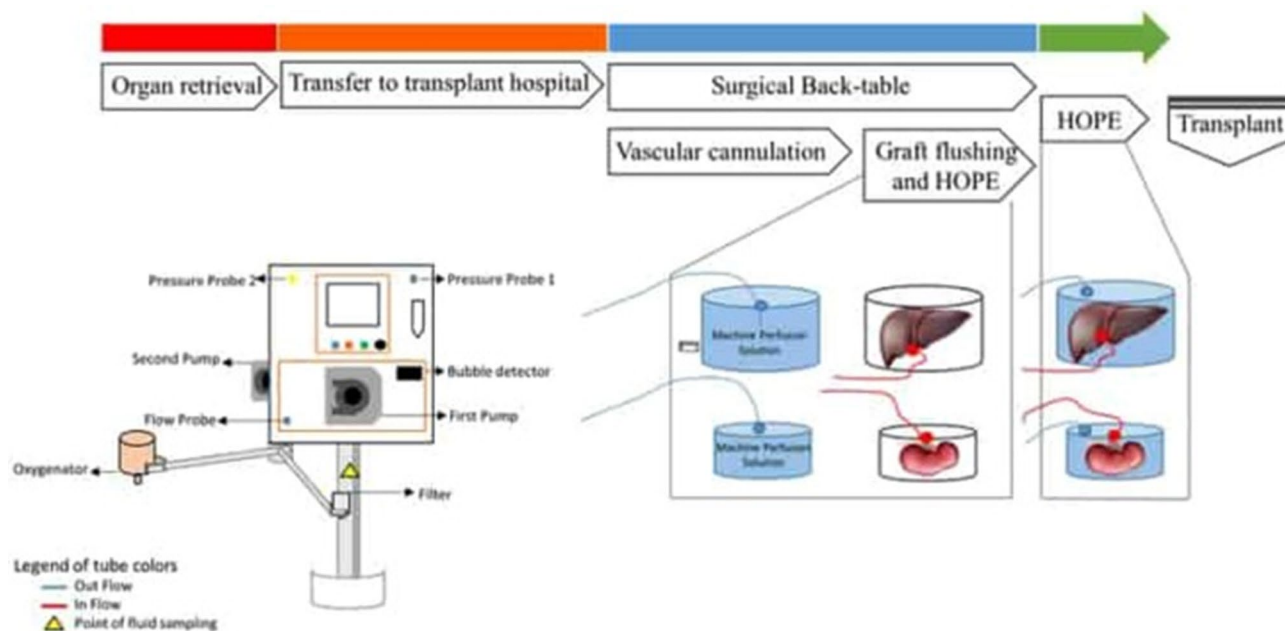


Figure 3.

Open Access This article is licensed under a Creative Commons Attribution 4.0 International License, which permits use, sharing, adaptation, distribution and reproduction in any medium or format, as long as you give appropriate credit to the original author(s) and the source, provide a link to the Creative Commons license, and indicate if changes were made. The images or other third party material in this article are included in the article's Creative Commons license, unless indicated otherwise in a credit line to the material. If material is not included in the article's Creative Commons license and your intended use is not permitted by statutory regulation or exceeds the permitted use, you will need to obtain permission directly from the copyright holder. To view a copy of this license, visit <http://creativecommons.org/licenses/by/4.0/>.

© The Author(s) 2020