




Novel physiological analysis using blood flow velocity for colonic polyps: Pilot study

OPEN
ACCESS



Authors

Eiji Kamba¹, Takashi Murakami¹, Naoki Tsugawa¹, Kei Nomura¹, Keiichi Haga¹, Yoichi Akazawa¹, Hirofumi Fukushima¹, Hiroya Ueyama¹, Kenshi Matsumoto², Tomoyoshi Shibuya¹, Takeshi Terai³, Takashi Yao⁴, Akihito Nagahara¹

Institutions

- 1 Department of Gastroenterology, Juntendo University, Bunkyo-ku, Japan
- 2 Department of Gastroenterology, Nihonbashi Muromachi Mitsui Tower Midtown Clinic, Tokyo, Japan
- 3 Department of Gastroenterology, Terai Clinic, Tokyo, Japan
- 4 Department of Human Pathology, Juntendo University, Bunkyo-ku, Japan

Keywords

Endoscopy Lower GI Tract, Polyps/adenomas/..., Diagnosis and imaging (inc chromoendoscopy, NBI, iSCAN, FICE, CLE...), Tissue diagnosis

received 12.11.2023

accepted after revision 27.3.2024

accepted manuscript online 15.4.2024

Bibliography

Endosc Int Open 2024; 12: E781–E787

DOI 10.1055/a-2306-9218

ISSN 2364-3722

© 2024. The Author(s).

This is an open access article published by Thieme under the terms of the Creative Commons Attribution-NonDerivative-NonCommercial License, permitting copying and reproduction so long as the original work is given appropriate credit. Contents may not be used for commercial purposes, or adapted, remixed, transformed or built upon. (<https://creativecommons.org/licenses/by-nc-nd/4.0/>)

Georg Thieme Verlag KG, Rüdigerstraße 14,
70469 Stuttgart, Germany

Corresponding author

Dr. Takashi Murakami, Juntendo University, Department of Gastroenterology, 2-1-1 Hongo, 113-8421 Bunkyo-ku, Japan
t-murakm@juntendo.ac.jp

ABSTRACT

Real-time visualization of red blood cell flow inside subepithelial microvessels is performed with magnifying endoscopy. However, microvascular blood flow velocity in the colorectum has not been investigated. Here, we aimed to evaluate the blood flow velocity of microvessels of colonic polyps and to compare it with that of surrounding mucosa. We examined 50 lesions, including 30 adenomas (ADs) and 20 hyperplastic polyps (HPs). Blood flow velocities of lesions and their surrounding mucosa were evaluated using magnifying blue laser imaging (BLI) prior to endoscopic resection. Calculation of mean blood flow velocities was based on mean movement distance of one tagged red blood cell using split video images of magnifying BLI. Mean microvascular blood flow velocity was significantly lower in ADs (1.65 ± 0.66 mm/sec; range 0.46–2.90) than in HPs (2.83 ± 1.10 mm/sec; 1.07–4.50) or the surrounding mucosa (3.73 ± 1.11 mm/sec; 1.80–6.20; $P < 0.001$). The blood flow velocity rate compared with the surrounding mucosa was significantly lower in ADs (0.41 ± 0.16 ; 0.10–0.82) than in HPs (0.89 ± 0.25 ; 0.46–1.51; $P < 0.001$). We found that mean microvascular blood flow velocity was significantly lower in ADs than in HPs and the surrounding non-neoplastic mucosa. These findings indicate that a novel dynamic approach with microvascular blood flow velocity using magnifying endoscopy may be useful in assessing physiological differences between ADs and HPs.

Introduction

Colorectal polyps are classified as neoplastic (adenomatous) or non-neoplastic (hyperplastic, hamartomatous, or inflammatory) based on their histology. Adenomas (ADs) are recognized

as precursor lesions of colorectal cancer (CRC) in the traditional colorectal carcinogenesis theory: the adenoma-carcinoma sequence. As a cornerstone of effective prevention, colonoscopy with polypectomy has led to a reduction in incidence of, and mortality from, CRC [1,2]. In contrast to ADs, hyperplastic

VIDEO



► **Video 1** Dynamic blood flow within subepithelial microvessels on magnifying blue laser imaging. The first half of the video shows a magnified blue laser imaging video of normal mucosa in the colon. When fully zoomed in, the movement of red blood cells can be clearly seen. The second half of the video shows distinct blood flow in colorectal adenomas (left) and hyperplastic polyps (right). It can be seen that the blood flow of the adenoma is slower than that of the hyperplastic polyp.

450-nm laser that supply white light by excitation. BLI is useful for a detailed observation of microvascular architecture for differential diagnosis and yields a unique image that emphasizes the capillary pattern and surface structure [4].


Microvascular density in colorectal tumors can be determined by magnifying BLI. The endoscopic microvascular density in a carcinoma is significantly higher than that in an adenoma [5]. Furthermore, magnifying BLI not only enables clear visualization of microvascular structures of the colorectum but also allows real-time visualization of red blood cell (RBC) flow within subepithelial microvessels (► **Video 1**). Mean microvascular blood flow velocity was reported as significantly lower in an early gastric neoplasm than in the surrounding non-neoplastic mucosa [6]. However, microvascular blood flow velocity in the colorectum has not been investigated. Here, we evaluated blood flow velocity of colonic polyps, including ADs and HPs, compared with that of the surrounding mucosa in a pathophysiological analysis.

polyps (HPs) are usually regarded as harmless, non-neoplastic lesions with no malignant potential.

Recently, image-enhanced endoscopies (IEEs), such as blue laser imaging (BLI) and narrow-band imaging (NBI), have been developed. Many studies have highlighted the usefulness of IEEs in detection and diagnosis of colorectal lesions [3]. BLI uses two monochromatic lasers (410 and 450 nm) rather than xenon light. Vascular microarchitecture is visualized by a 410-nm laser and a

Patients and methods

Patients who underwent colonoscopy for screening at our hospital between March 2019 and January 2023 were included. When colorectal polyps were found, we performed video recordings and retrospectively reviewed the videos. Of these, the lesions that could not be assessed due to the poor quality of images were excluded. Only lesions in which the movement of RBCs could be clearly observed were extracted. Finally, 50 lesions, including 30 ADs (from 20 patients) and 20 HPs (from 13 patients), were assessed.



► **Fig. 1** Method for measuring microvascular blood flow velocity. All magnifying blue laser imaging (BLI) video images were split into 30 fps. The distance covered by one tagged red blood cell was measured manually at continuing split images (Distance A) on a large screen, and 1-mm increments (Distance B) were also measured manually on the same screen. Subsequently, mean microvascular blood flow velocity was calculated by Distance A, Distance B, and the number of frames N (mean blood flow velocity [mm/s] = Distance A [mm]/Distance B [mm] × 30 [frames]/number of frames N [frames]).

► **Table 1** Baseline characteristics of lesions studied.

Lesions, n = 50 (Patients, n = 33)	ADs n = 30 (n = 20)	HPs n = 20 (n = 13)	P value
Gender (%) (male/female)	13 (65)/7 (35)	9 (69)/4 (31)	>0.999
Age (range)	68 (45–83)	66 (49–76)	0.416
Location (%)			0.188
▪ Right colon	19 (63)	8 (40)	
▪ Left colon	9 (30)	8 (40)	
▪ Rectum	2 (7)	4 (20)	
Size (mm) median	3.5 (2–16)	3.5 (2–12)	0.908
Macroscopic type (%)			0.682
▪ Ip	0	0	
▪ lsp	1 (3)	0	
▪ ls	20 (67)	13 (65)	
▪ lla	9 (30)	7 (35)	

ADs, adenomas; HPs, hyperplastic polyps.
Age is represented as median (range).


Endoscopic system and examination

We used high-resolution optical magnifying endoscopes (EC-L600ZP; Fujifilm Corporation, Tokyo, Japan) and an endoscope video system (LASEREO 7000 series; Fujifilm Corporation). Blood flow velocities were evaluated using magnifying BLI. The structure enhancement function and color mode in BLI were set at B8 and C2, respectively. Endoscopy examinations were performed by six endoscopy specialists (E.K., T.M., K.N., K.H., Y. A., H.F.), each with experience in at least 1000 prior colonoscopic procedures. Lesions were carefully evaluated using BLI prior to endoscopic resection. Careful examination with conventional endoscopy was followed by BLI magnification endoscopy. We evaluated magnifying BLI endoscopic findings using a Japan NBI Expert Team (JNET) system [7].

Microvascular blood flow rate measurement

The method used for measuring microvascular blood flow velocity is illustrated in ► **Fig. 1**. Measurements and analysis were conducted by E.K. and T.M. Magnifying BLI video images were split into 30 frames per second, and mean blood flow velocities were calculated from the average distance of a single tagged RBC. Before each examination, the endoscope and marker were attached and adjusted for focusing using full zoom. The examination was subsequently conducted. During video recording of lesions, full zoom was used to adjust magnification in all cases.

Initially, the segmented images were continuously captured on a large screen. A single tagged RBC, identifiable in each lesion, was manually identified by E.K. and T.M. The distance tra-

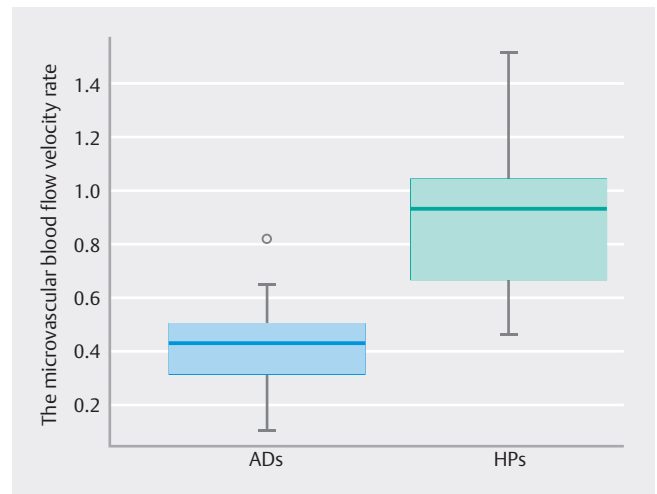

► **Fig. 2** Microvascular blood flow velocity rates of ADs and HPs. ADs (median, 0.43; range, 0.10–0.82) vs. HPs (median, 0.93; range, 0.46–1.51), ****P* < 0.001. AD, adenoma; HP, hyperplastic polyp.

veled by this RBC (Distance A) was manually measured. The distances in 1-mm increments (Distance B) were also manually measured on the same screen. Subsequently, mean microvascular blood flow velocity was calculated based on Distance A, Distance B, and the number of frames (mean blood flow [$\mu\text{m}/\text{s}$] = Distance A [μm]/Distance B [μm] \times 30 [frames]/Frame Number [frames]). Microvascular blood flow velocity in the lesion and surrounding mucosa was evaluated. Furthermore, because of the possible existence of individual differences, such as, for example, in blood pressure, microvascular blood flow velocity in the lesion was compared with the surrounding mucosa for both ADs and HPs.

Histopathological diagnosis

After appropriate BLI video imaging, each lesion was endoscopically resected and pathologically diagnosed. The histological diagnosis of each excised lesion was conducted at the Department of Human Pathology at Juntendo University.

Statistical analysis

Statistical analyses were undertaken using EZR (Easy R; Saitama Medical Center, Jichi Medical University, Saitama, Japan), a graphical user interface for R (The R Foundation for Statistical Computing, Vienna, Austria). A Mann-Whitney U-test was used to compare continuous data. Fisher's exact test was used in the categorical analysis of variables. Statistical significance was set as *P* < 0.05.

Ethics approval

The Institutional Review Board and the Ethical Committee of Juntendo University Hospital (#20–219) approved this study. The study was performed in accordance with the principles of the Declaration of Helsinki. This was also an opt-out study. Because the study was conducted using pre-existing data, informed consent from registered patients was not required.

► **Table 2** Microvascular blood flow velocity of lesions studied.

Adenomas	(A) Lesions	(B) Surrounding mucosa	Hyperplastic polyps	(C) Lesions	(D) Surrounding mucosa
1	1.16	3.69	31	3.97	3.72
2	1.59	3.42	32	3.18	3.19
3	2.3	3.81	33	3.44	3.32
4	1.8	3.81	34	3.44	3.32
5	2.2	3.83	35	4.24	4.09
6	2.12	5.11	36	4.5	4.26
7	2.01	6.2	37	3.44	3.71
8	2.3	3.52	38	3.28	3.07
9	2.2	6.03	39	3.71	2.46
10	2.6	5.15	40	3.97	4.29
11	1.85	5.37	41	3.22	3.55
12	2.65	5.96	42	1.38	2.3
13	1.32	3.83	43	1.38	2.3
14	2.12	4.77	44	1.07	2.3
15	1.59	3.22	45	1.84	2.3
16	1.48	1.8	46	2.3	2.3
17	1.06	2.1	47	3.23	5.07
18	2.12	4.77	48	1.09	2.31
19	1.5	4.98	49	1.63	2.31
20	2.1	4.98	50	2.3	2.53
21	2.9	4.88			
22	0.69	2.53			
23	1.38	2.53			
24	0.57	3.69			
25	0.69	3.69			
26	1.84	3.69			
27	0.92	3.69			
28	1.38	3.69			
29	0.46	4.38			
30	0.75	4.48			
Median	1.69	3.82	Median	3.22	3.13
(range)	0.46–2.90	1.80–6.20	(range)	1.07–4.50	2.30–5.07


(A) Adenomas vs (B) surrounding mucosa, $P < 0.001$. (A) Adenomas vs (C) hyperplastic polyps, $P < 0.001$. (C) Hyperplastic polyps vs (D) surrounding mucosa, $P = 0.408$.

Results

Baseline characteristics

► **Table 1** outlines baseline characteristics of the polyps studied. A higher proportion of males was evident in both the AD and HP groups (AD, 13 males vs. 7 females; HP, 9 vs. 4) and

the median age was 68 and 66 years in the AD and HP groups, respectively. HPs were predominantly located in the distal colon (left-side colon and rectum) rather than in the proximal colon, whereas ADs were more frequently located in the right-side colon. Median sizes for ADs and HPs were 3.5 mm and 3.5 mm, respectively.



► **Fig. 3** Blue laser imaging and pathological images of a representative adenoma and hyperplastic polyp cases. **a** Blue laser imaging (BLI) in an adenoma (Case 13). **b** BLI image of a hyperplastic polyp (Case 35). **c** Pathological image of an adenoma (Case 13). **d** Pathological image of a hyperplastic polyp (Case 35). Microvessels in adenomas are larger, denser, and more tortuous than those in hyperplastic polyps. Green arrows indicate dilated and tortuous microvessels.

Macroscopically, both ADs and HPs were predominantly sessile (0-I) or superficial (0-IIa) types. No significant differences in patient age and sex, tumor location, size, or macroscopic type were found between lesion groups. Regarding the JNET classification, all cases of ADs were classified as Type 2A, while all cases of HPs were classified as Type 1. All excised ADs exhibited low-grade dysplasia and were classified as tubular adenomas.

Microvascular blood flow velocity

► **Table 2** shows microvascular blood flow velocity of each lesion and the surrounding non-neoplastic mucosa. Mean microvascular blood flow velocity was found to be significantly lower for AD lesions (median 1.69 mm/sec; range 0.46–2.90) than for HP lesions (median 3.22 mm/sec; 1.07–4.50) or the surrounding mucosa (median 3.82 mm/sec; 1.80–6.20; $P < 0.001$, respectively). However, mean velocity was not significantly different

between HPs and the surrounding mucosa. shows actual blood flow in AD and HP cases. In addition, no significant differences in mean velocity were observed with respect to age or sex.

Microvascular blood flow velocity rate

Mean microvascular blood flow velocity rates of ADs and HPs are also presented in ► **Fig. 2** The mean velocity rate of the lesion compared with the surrounding mucosa was significantly lower for ADs (median 0.43; 0.10–0.82) than for HPs (median 0.93; 0.46–1.51; $P < 0.001$).

Discussion

In this study, mean microvascular blood flow velocity was calculated for both colorectal lesions (ADs and HPs) and the surrounding non-neoplastic mucosa. We found that the mean microvascular blood flow velocity rate of lesions compared

with the surrounding mucosa was significantly lower in ADs than in HPs. To our knowledge, no studies have analyzed microvascular blood flow velocity of colonic subepithelial microvascular vessels using magnifying BLI. This is the first study to compare the microvascular blood flow velocity of colorectal polyps. Endoscopically, subepithelial microvessels in ADs are thicker and more tortuous than those in HPs [5, 7]. In addition, in this study, blood flow velocity was significantly lower in ADs than in normal mucosa, whereas HPs showed no significant difference with regard to blood flow velocity of microvessels compared with those of normal mucosa.

As shown in ► **Fig. 3**, in ADs, tumor gland density around the microvasculature was higher compared with that in HPs. The structure of tumor glands was irregular and the stromal architecture surrounding the tumor glands, where microvessels coursed, appeared to be complex and narrow. Therefore, it is hypothesized that differences in tortuosity of microvessel diameters and variations in tumor gland density around the microvessels may be associated with a decrease in microvascular blood flow. However, further research is needed to elucidate the factors that regulate microvascular blood flow in the colonic mucosa.

The JNET classification evaluates lesion surface and vascular structure using magnifying NBI [7]. The pit pattern classification by Kudo et al. (1996) assesses the form of pits on the tumor surface according to staining patterns [8]. Both classifications are useful for qualitatively and quantitatively diagnosing colorectal tumors because they are highly reproducible and show good diagnostic accuracy with respect to pathology and invasion depth [9, 10]. However, these classifications are performed using still images. To date, no diagnostic system that uses moving images has been available for colorectal polyps. This analysis remains limited to pathophysiological insights at this stage. However, in the future, if the blood flow velocity in subepithelial microvessels can be measured automatically, that may contribute to establishment of a new diagnostic system of colorectal lesions using moving images.

In this analysis, lesions were found in which the movement of RBCs could not be captured by magnifying endoscopy. Possible reasons include: 1) the effect of large vessel diameter and high density; 2) bleeding with scope contact when observing the surface structures of lesions; and 3) few flat areas to visualize subepithelial microvessels and ensure a stable view. Therefore, although we attempted to capture blood flow in subepithelial microvessels in some colorectal cancers by magnifying endoscopy, it was difficult to observe blood flow and measure blood flow velocity.

This study has several limitations. First, it was retrospective in nature and used a small cohort of patients at a single institution. Second, this study was exploratory and focused only on ADs and HPs. Future prospective, multicenter, comparative studies with larger sample sizes should be conducted. Third, we did not specify in which area of a lesion to measure microvascular blood flow rate and at what moment microvascular blood flow was to be measured. Fourth, because microvessels within the mucosa usually have a disorganized, three-dimensional, microvascular architecture, if they run vertically, blood

flow as measured on the surface in two dimensions may become slow. For example, comparing the size of an RBC when initially tagged with that when it is finally tagged may offer a simple estimation of depth. However, this remains a task for future investigation. Fifth, the presence of irregularities in the lesion itself and the observation not necessarily being perpendicular to the mucosa suggests that the distances depicted in ► **Fig. 1** may lack reproducibility. Achieving reproducibility might be possible by placing an actual scale on a lesion and recording it in the video footage for distance measurement. Sixth, in this study, the physiological characteristics of two types of lesions were not evaluated. To investigate the relationship between blood flow velocity and physiological differences, it is necessary to compare blood flow velocity under different physiological conditions within the same lesion. And finally, because the researchers who conducted the analysis were not blinded to the data, a potential for bias exists in the measurements. In future, we intend to investigate microvascular blood flow velocity in several types of lesions, including colorectal cancer. We also intend to elucidate the pathophysiological processes that underlie lower microvascular blood flow velocity in colorectal lesions and compare it to that of normal mucosa.

Conclusions

In conclusion, we evaluated subepithelial microvascular blood flow velocity of colorectal lesions using magnifying endoscopy. We found that mean microvascular blood flow velocity was significantly lower in ADs than in HPs and the surrounding non-neoplastic mucosa. Assessment of the dynamic function of the colonic mucosa by magnifying endoscopy may offer a new approach to elucidating the pathophysiology of colonic tumors. Additional validation is necessary to ascertain the potential applicability of this analysis in future clinical diagnostic practice.

Conflict of Interest

The authors declare that they have no conflict of interest.

References

- [1] Zauber AG, Winawer SJ, O'Brien MJ et al. Colonoscopic polypectomy and long-term prevention of colorectal-cancer deaths. *N Engl J Med* 2012; 366: 687–696 doi:10.1056/NEJMoa1100370
- [2] Winawer SJ, Zauber AG, Ho MN et al. Prevention of colorectal cancer by colonoscopic polypectomy. The National Polyp Study Workgroup. *N Engl J Med* 1993; 329: 1977–1981 doi:10.1056/NEJM199312303292701
- [3] Gono K, Obi T, Yamaguchi M et al. Appearance of enhanced tissue features in narrow-band endoscopic imaging. *J Biomed Opt* 2004; 9: 568–577 doi:10.1117/1.1695563
- [4] Yoshida N, Yagi N, Inada Y et al. Ability of a novel blue laser imaging system for the diagnosis of colorectal polyps. *Dig Endosc* 2014; 26: 250–258 doi:10.1111/den.12127
- [5] Gonai T, Kawasaki K, Nakamura S et al. Microvascular density under magnifying narrow-band imaging endoscopy in colorectal epithelial neoplasms. *Intest Res* 2020; 18: 107–114 doi:10.5217/ir.2019.00061

- [6] Ueyama H, Yatagai N, Ikeda A et al. Dynamic diagnosis of early gastric cancer with microvascular blood flow rate using magnifying endoscopy (with video): A pilot study. *J Gastroenterol Hepatol* 2021; 36: 1927–1934
- [7] Sano Y, Tanaka S, Kudo SE et al. Narrow-band imaging (NBI) magnifying endoscopic classification of colorectal tumors proposed by the Japan NBI Expert Team. *Dig Endosc* 2016; 28: 526–533 doi:10.1111/den.12644
- [8] Kudo S, Tamura S, Nakajima T et al. Diagnosis of colorectal tumorous lesions by magnifying endoscopy. *Gastrointest Endosc* 1996; 44: 8–14 doi:10.1016/s0016-5107(96)70222-5
- [9] Li M, Ali SM, Umm-a-OmarahGilani S et al. Kudo's pit pattern classification for colorectal neoplasms: a meta-analysis. *World J Gastroenterol* 2014; 20: 12649–12656 doi:10.3748/wjg.v20.i35.12649
- [10] Kobayashi S, Yamada M, Takamaru H et al. Diagnostic yield of the Japan NBI Expert Team (JNET) classification for endoscopic diagnosis of superficial colorectal neoplasms in a large-scale clinical practice database. *United European Gastroenterol J* 2019; 7: 914–923 doi:10.1177/2050640619845987