

Available online at www.sciencedirect.com

SciVerse ScienceDirect

journal homepage: www.jfda-online.com

Original Article

Sensitivity and specificity of *in vitro* diagnostic device used for influenza rapid test in Taiwan



Kun-Teng Wang^a, Chia-Pei Lin^a, Yi-Ya Fang^a, Ming-Hui Kao^a,
Daniel Yang-Chih Shih^b, Chi-Fang Lo^c, Der-Yuan Wang^{a,*}

^a Section of Biologics, Division of Research and Analysis, Food and Drug Administration, Ministry of Health and Welfare, Taiwan, ROC

^b Division of Research and Analysis, Food and Drug Administration, Ministry of Health and Welfare, Taiwan, ROC

^c Food and Drug Administration, Ministry of Health and Welfare, Taiwan, ROC

ARTICLE INFO

Article history:

Received 3 April 2013

Received in revised form

17 May 2013

Accepted 28 June 2013

Available online 6 October 2013

Keywords:

In vitro diagnostic device

Pandemic influenza A (H1N1) virus

Sensitivity

Specificity

ABSTRACT

The pandemic influenza A/H1N1 outbreak resulted in 18,449 deaths in over 214 countries. In Taiwan, the influenza rapid test, an *in vitro* diagnostic device (Flu-IVD), only requires documented reviews for market approval by the Taiwan Food and Drug Administration. The purpose of this study was to investigate the analytical sensitivity and specificity of Flu-IVDs used in Taiwan. Analytical sensitivity and specificity tests were performed for influenza antigens A/California/7/2009 (H1N1) virus, A/Victoria/210/2009 (H3N2) virus, B/Brisbane/60/08 virus, and human coronavirus OC43. A total of seven domestic and 31 imported Flu-IVD samples were collected, of which, 20 samples had inadequate labeling, including those with removed package inserts or incorrect insert information. The analytical sensitivity of Flu-IVDs for A/H1N1, A/H3N2, and Flu B was 500–1000 ng/mL, 1000 ng/mL, and 1000 ng/mL, respectively. For the 50% cell culture infective dose (CCID₅₀) label, the average A/H1N1 and A/H3N2 sensitivity for Flu-IVDs was $\log_{10} 5.8 \pm 0.5$ and $\log_{10} 6.6 \pm 0.5$ CCID₅₀/mL, respectively. As to the specificity test, no product cross-reacted with human coronavirus OC43. This study provides important information on the Flu-IVD regulation status and can thus help the government formulate policies for the regulation of *in vitro* diagnostic devices in Taiwan.

Copyright © 2013, Food and Drug Administration, Taiwan. Published by Elsevier Taiwan

LLC. Open access under [CC BY-NC-ND license](https://creativecommons.org/licenses/by-nc-nd/4.0/).

1. Introduction

In 1998, a triple-reassortant swine influenza virus from human, swine, and avian genomes was identified in the USA [1]. Ten years later, humans were found to be infected with

these influenza viruses [2]. A novel human influenza A (H1N1) virus caused a worldwide respiratory disease outbreak in April 2009. The major transmission route for influenza virus is via respiratory droplets released while coughing [3–5]. Influenza virus replicates in the epithelial cells of the upper respiratory

* Corresponding author. Section of Biologics, Division of Research and Analysis, Food and Drug Administration, Ministry of Health and Welfare, Taiwan, ROC.

E-mail address: dywang@fda.gov.tw (D.-Y. Wang).

1021-9498 Copyright © 2013, Food and Drug Administration, Taiwan. Published by Elsevier Taiwan LLC. Open access under [CC BY-NC-ND license](https://creativecommons.org/licenses/by-nc-nd/4.0/).

<http://dx.doi.org/10.1016/j.jfda.2013.09.011>

tract, which destroys the host cells, further spreading to infect other cells. The clinical manifestations of influenza are fever, headache, myalgia, fatigue, rhinorrhea, sore throat, and cough. The impact of influenza outbreaks is much higher in children than in adults. Most healthy adults will recover after 3–7 days [6–8]. Influenza A/H3N2 was the predominant serotype during the 2010–2011 season, whereas the A/H1N1 2009 virus still cocirculated with the A/H3N2 and influenza B strains [9]. The pandemic influenza A/H1N1 outbreak resulted in over 18,449 deaths in over 214 countries until 2012 [10,11].

Conventional diagnostic testing of influenza virus included virus incubation and nucleic acid amplification test. Virus incubation is the first method used to diagnose virus infections, while it takes about 7 days to amplify the virus in the host cells. A nucleic acid amplification test is the most sensitive method to detect virus infection, but pretreatment of the sample, including virus isolation and nucleic extraction, still requires about 1 day. The above methods are not suitable for the rapid screening of influenza virus [12]. *In vitro* diagnostic devices (IVDs) play crucial roles in disease diagnosis because of their rapid and convenient properties. Diagnostic accuracy of IVDs is dependent on their sensitivity and specificity. A previous study evaluated the 3M rapid detection test for the respiratory syncytial virus, and found the sensitivity and specificity of the device to be 74% and 100%, respectively [13]. In April 2011, a study conducted by Iregbu et al [14] on the performance of Dual Path Platform testing kits revealed a sensitivity of 100% and specificity of 99.5%. By contrast, a study by Shrivastava et al [15] reported that the commercial Dengue NS1 antigen kit had a sensitivity of 26% against 91 clinical samples. Few studies have reported the sensitivity of influenza IVDs (Flu-IVDs) in detecting influenza A. These previous studies used four commercialized rapid test kits [16–20].

Flu-IVD rapid test kits are based on immunochromatographic tests. This type of IVD is designed for easy and fast operation, which enables physicians to obtain results at the primary influenza screening sites. The Flu-IVD rapid test kits have been classified into a low-risk class I device according to the medical device regulation and risk assessment in Taiwan. They are applied and approved by the Taiwan Food and Drug Administration (FDA) for pre-market approvals via the fast track pathway, that is, they are exempt from the substantial performance review.

In this study, we collected Taiwan-FDA-approved Flu-IVDs from the Taiwanese market and evaluated their performance. The standard antigens prepared from viral cultures and purified hemagglutinins (HAs) were used to evaluate the analytical sensitivity and specificity of the Flu-IVDs. The results represent the actual responses of these rapid test kits and provided references for future amendments in regulations.

2. Methods

2.1. Analytical standard

The international standards for HA and influenza virus were used as the analytical standards for the Flu-IVDs sensitivity

test. For HA standards, the Influenza Antigen A/California/7/2009 (H1N1, NYMCX-179A, Egg derived, NIBSC code: 09/146), A/Victoria/210/2009 (H3N2, NYMCX-187, NIBSC code: 10/102), and Influenza B/Brisbane/60/08 Antigen Reagent (NIBSC code: 08/352) were obtained from the National Institute for Biological Standards and Control (Potters Bar, Herts, UK). The influenza A/Taiwan/9042/2008 (H1N1) virus with 108.23 50% cell culture infective doses (CCID₅₀)/mL and A/Taiwan/439/2009 (H3N2) virus with 106.3 CCID₅₀/mL from Chang Geng University were used as influenza viral particle standards. The human coronavirus OC43 (HCoV-OC43, ATCC VR-759) was obtained from American Type Culture Collection (Manassas, VA, USA).

2.2. Specimen collection

Flu-IVDs were purchased directly from the manufacturers and local distributors in 1–3 different lots. The product name, lot number, and manufacturing country of each Flu-IVD are listed in Tables 1 and 2.

2.3. Appearances and label survey

The appearance of the products and the labels on the Flu-IVDs were compared with information on their licenses, including Chinese and English names, license numbers, name of manufacturer, address of manufacturer, and expiration dates.

2.4. Sensitivity analysis

Sensitivity was assayed as described previously, with modifications [21]. The sensitivity of the collected Flu-IVDs was specified as HA concentrations or CCID₅₀. The HA standards consisting of Influenza Antigens A/California/7/2009 (H1N1), A/Victoria/210/2009 (H3N2) and B/Brisbane/60/08 were diluted individually to 0.25–50,000 ng/mL, 0.25–13,000 ng/mL, and 0.25–13,500 ng/mL, respectively, with the dilution buffer provided in the Flu-IVDs. Additionally, the influenza A/Taiwan/9042/2008 (H1N1) and A/Taiwan/439/2009 (H3N2) viruses were prepared from infected rhabdomyosarcoma (RD) cells and diluted to concentrations of 101.3–105.3 CCID₅₀/mL and 101.23–107.23 CCID₅₀/mL, respectively, with minimum essential medium (Gibco, Grand Island, NY, USA). The sensitivity assay of each Flu-IVD, including the positive and negative controls, was carried out by following the instructions in

Table 1 – List of domestic influenza *in vitro* diagnostic devices collected in Taiwan.

Product name	Lot no.	Manufacturing country
Firststep Influenza A&B Test Card	10072609	Taiwan
Formosa One Sure Flu A/B Rapid Test Kit	MS19A21 MS19A71 MS19A81	Taiwan
Long TERM Influenza A&B	990510-06 990629-01 990928-07	Taiwan

Table 2 – List of imported influenza in vitro diagnostic devices collected in Taiwan.

Product name	Lot no.	Manufacturing country
DIAQUICK influenza Ag Dipstick	1301/069039-U	Austria
BD Directigen EZ Flu A + B	9341551	China
Feng Chi Kaibilia Influenza A + Influenza B nucleoprotein antigen Rapid Test Kit	AB091102 AB100501 AB100502	China
On-call Influenza A&B Rapid Test Strip	FLU00880002	China
Actim Influenza A&B Test Kit	0021825 0021888 0081929	Finland
“Jolex” BioTracer Influenza A&B	11321910 11321911 11321912	Korea
Bioland NanoSign Influenza A/B Antigen	INF101109	Korea
“SD” Influenza Ag	069041 069042 069043	Korea
EZ-TRUST Influenza A&B Rapid Screen Test	W7100401 W7100402 W7100403	Singapore
Linear Influenza A + B rapid test Kit	Z-031 Z-036 Z-037	Spain
VEGAL Influenza A + B	Z031	Spain
Binax NOW Influenza A&B	43842	USA
Genzyme Influenza A&B Test	091511A	USA
Meridian TRU FLU Test	731230.075 731230.082	USA
Applied Biotech Influenza A + B test	911067 912150 1008156	USA
Unipath Clearview Exact Influenza A&B	FLU9090087	UK

the operation manuals. Two independent and well-trained technicians performed the experiments.

2.5. Specificity analysis

HCoV-OC43 was prepared from infected MRC-5 cells. The extract containing 1×10^7 CCID₅₀/mL of virus was used to evaluate the specificity of Flu-IVDs. The experimental protocol was carried out in accordance with the operation manuals of each Flu-IVDs. Two independent and well-training researchers carried out the experiments.

3. Results and discussion

Flu-IVDs are classified as class 1 medical devices, indicating that the license could be easily obtained through document reviews. Therefore, the quality of Flu-IVDs needs to be investigated and monitored. In Taiwan, suspected influenza patients are immediately tested with Flu-IVDs at the primary screening site in epidemics areas. The therapeutic strategies are divided into two parts based on the test results. If the test

result is positive and the patient exhibits influenza-like symptoms, the patient is immediately administered antiviral drugs such as oseltamivir (Tamiflu) and continuously monitored with Flu PCR test kits. However, negative test results indicate that the patient only has a common cold, and no antiviral drug treatment is given. The use of Flu-IVDs plays a crucial role in controlling influenza epidemics. Hence, false-positive outcomes may cause inappropriate administration of oseltamivir, which could lead to future challenges in the prevention of influenza. Prior to 2009, several commercial Flu-IVD rapid test kits were approved in Taiwan. However, after the influenza A/H1N1 pandemics in 2009, the Taiwan FDA issued many licenses for similar products. We thus aimed to examine the analytical sensitivity and specificity of Flu A-IVDs used in Taiwan.

3.1. Specimen collection

A total of 38 products with 19 Flu-IVD licenses were collected, of which seven were domestic and 31 were imported Flu-IVDs. Product labels of 20 samples did not comply with the regulations in Taiwan FDA. For example, those with unsatisfactory product labels lacked a product name and/or license number on the packaging or buffer containers. Some products had no package insert in them, and some package inserts did not indicate the sensitivity of the product. The percentage of unsatisfactory product labels in domestic and imported kits was 43% (3/7) and 55% (17/31), respectively.

3.2. Analytical sensitivity

Based on the reaction principles, the detecting targets of the collected samples were grouped as HA and viral particles. The Flu-IVDs belonging to the HA group were evaluated for their analytical sensitivity with the World Health Organization (WHO) international standard Influenza Antigens A/California/7/2009 (H1N1), A/Victoria/210/2009 (H3N2), and B/Brisbane/60/08. As shown in Table 3, seven products of three Flu-IVD licenses (A–C) that were manufactured in the USA and Spain used HA concentrations as their sensitivity label. The analytical sensitivity of these Flu-IVDs against A/H1N1, A/H3N2, and Flu B was 500–1000 ng/mL, 1000 ng/mL, and 1000 ng/mL, respectively. For A/H1N1 detection, products A

Table 3 – Evaluation of sensitivity of Flu-IVDs for hemagglutinin concentrations.

Source	Standard type	Product code ^a	Sensitivity results (ng/mL)	
			H1N1	H3N2
Import	Flu A	A	500	1000
		B	500	1000
		C	1000	1000
	Flu B	A		1000
		B		1000
		C		1000

^a Seven products of three Flu-IVD licenses (code A–C) were analyzed.

and B displayed higher analytical sensitivity than product C. The sensitivity results for A/H3N2 and Flu B were identical in these samples. We obtained seven products from three domestic Flu-IVDs (D–F) and 17 products from eight Flu-IVDs (G–N) imported from China, the UK, Finland, Singapore, USA, and Korea with CCID₅₀ labels. In the past 5 years, type A/Taiwan/439/2009 (H3N2) and type A/Taiwan/9042/2008 (H1N1) were the two main strains of influenza outbreak in Taiwan. Hence, these two virus strains were used as influenza viral particle standards for CCID₅₀ test [22]. The averages of A/H1N1 and A/H3N2 sensitivity were log₁₀ 5.8 ± 0.5 CCID₅₀/mL and log₁₀ 6.6 ± 0.5 CCID₅₀/mL, respectively. In Fig. 1, the unbroken, broken, and dotted lines represent the mean, mean ± 1 standard deviation (SD) and mean ± 2 SD in the sensitivity

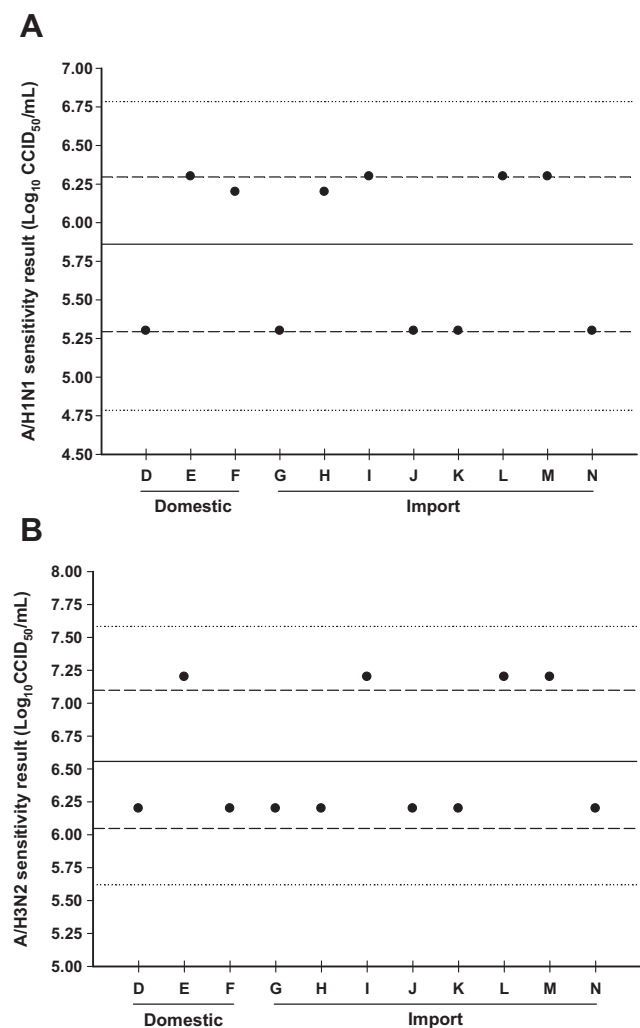


Fig. 1 – Evaluation of the sensitivity of Flu-IVDs for H1N1 (A) and H3N2 (B) in 50% cell culture infective dose. Unbroken (—), broken (—), and dotted lines (.....) indicate the mean, mean ± SD values, and mean ± 2 SD values, respectively. Product codes are designated by a letter from D to N. Seven products of three domestic Flu-IVD licenses (code D–F) and 17 products of eight imported Flu-IVD licenses (from code G–N) were analyzed. Flu-IVD = influenza *in vitro* diagnostic device; SD = standard deviation.

tests, respectively. For A/H1N1, the sensitivity of all products was within mean ± 1 SD (Fig. 1A). As to A/H3N2 sensitivity, however, the products E, I, L, and M fell into the mean ± 2 SD range (Fig. 1B). Seven products from five imported Flu-IVDs did not have test sensitivity labeling. Therefore, HA concentrations were used to determine their sensitivities. In Table 4, the sensitivities of these seven samples against H1N1, H3N2, and Flu B were 500–1000 ng/mL, 500–3250 ng/mL, and 1000–6750 ng/mL, respectively.

Previous researchers have used clinical specimens to monitor the clinical performance of Flu-IVDs. A study by Drexler et al [17] found that BinaxNow Influenza A&B Rapid Test Kits had a poor clinical sensitivity; the sensitivity was 11.1% for the pandemic (H1N1) 2009 virus (16 positive cases against 144 polymerase-chain-reaction-confirmed cases). A study by Uyeki et al [20] also showed that the QuickVue Influenza A + B Test had a low sensitivity (27%) for the detection of both influenza A and B viruses. The Center for Disease Control and Prevention screened 45 specimens with positive results for novel influenza A (H1N1) using Directigen EZ Flu A + B and obtained a sensitivity of 49% [23].

We assumed that one of the reasons for the discrepancies was that the human epidemic strains of influenza viruses used in the Flu-IVDs did not match the current influenza virus outbreak strains. Pandemic influenza virus strains varied from year to year and from country to country. For example, the influenza A/Texas/1/77 strain was used as the master influenza virus strain to develop the monoclonal antibodies in the BinaxNow Influenza A&B Rapid Test; however, the major virus strain that caused the influenza outbreak in Taiwan was the type A/Taiwan/439/2009 (H3N2) and type A/Taiwan/9042/2008 (H1N1). Other Flu-IVDs failed to mention the master influenza virus strain used in their preparations. Therefore, inappropriate master influenza virus strains used in the Flu-IVD preparations may contribute to the low detection sensitivity. Moreover, studies have shown that analytical sensitivity did not directly reflect the clinical sensitivity on patient specimens. The analytical sensitivity of influenza H5N1 detection and seasonal influenza was the same, although their clinical performances were poor [23,24]. Manufacturers

Table 4 – Unlabeled sensitivity of Flu-IVDs.

Source	Standard type	Product code ^a	Results (ng/mL)	
			H1N1	H3N2
Import	Flu A	O	500	500
		P	1000	6500
		Q	500	3250
		R	500	500
		S	500	500
	Flu B	O		1000
		P		1000
		Q		ND
		R		1000
		S		6750

ND = not detected.

^a Seven products of five Flu-IVD licenses (code O–S) were analyzed.

Table 5 – Specificity results of all influenza in vitro diagnostic devices.

Test virus	Cross-reactivity	Specificity rate
Human coronavir-OC43	0/38	100%

should follow WHO recommendations for the annually pandemic influenza virus strains to be used in their preparation of the Flu-IVDs in order to improve the quality. We also suggest that the class level for Flu-IVDs in Taiwan for government regulations be elevated so that the government can monitor the quality of IVDs using a lot release system. Furthermore, Taiwan FDA should establish a reference or proficiency panel to evaluate in vitro Flu-IVDs in the near future.

3.3. Analytical specificity

Patients suffering from respiratory illness such as cough, asthma, and emphysema are usually diagnosed with acute respiratory tract infections. Viruses such as influenza virus, coronavirus, and respiratory syncytial virus commonly cause respiratory tract infections [25]. Several studies have conducted a specificity test by real-time polymerase chain reaction analysis for different respiratory-tract-infection-related viruses [26,27]. The specificity of Flu-IVDs played an important role in the selective interaction of influenza A and B viruses. According to the epidemiological studies, HCoV caused >15% of common colds in adults, of which OC43 was the most common [28]. Hence, we used the common HCoV-OC43 to determine the specificity of Flu-IVDs in this study and the result showed that not all Flu-IVDs cross-reacted with HCoV-OC43, suggesting good specificity (Table 5).

In conclusion, seven domestic and 31 imported Flu-IVDs were collected to analyze the sensitivity and specificity. Analytical sensitivity of Flu-IVDs for A/H1N1, A/H3N2, and Flu B was 500–1000 ng/mL, 1000 ng/mL, and 1000 ng/mL, respectively. Average sensitivity of A/H1N1 and A/H3N2 for Flu-IVDs was $\log_{10} 5.8 \pm 0.5$ CCID₅₀/mL and $\log_{10} 6.6 \pm 0.5$ CCID₅₀/mL, respectively. No products cross-reacted with HCoV-OC43. Our results could provide more information for future policy-making strategies and preparedness against seasonal and pandemic influenza.

Acknowledgments

This work was supported by grants from the Department of Health, Executive Yuan, Taiwan (grant no. DOH99-FDA-72020).

REFERENCES

- [1] Olsen CW. The emergence of novel swine influenza viruses in North America. *Virus Res* 2002;85:199–210.
- [2] Dawood FS, Jain S, Finelli L, et al. Emergence of a novel swine-origin influenza A (H1N1) virus in humans. *N Engl J Med* 2009;360:2605–15.
- [3] Blachere FM, Lindsley WG, Pearce TA, et al. Measurement of airborne influenza virus in a hospital emergency department. *Clin Infect Dis* 2009;48:438–40.
- [4] Bean B, Moore BM, Sterner B, et al. Survival of influenza viruses on environmental surfaces. *J Infect Dis* 1982;146:47–51.
- [5] Ryu YB, Jeong HJ, Yoon SY, et al. Influenza virus neuraminidase inhibitory activity of phlorotannins from the edible brown alga *Ecklonia cava*. *J Agric Food Chem* 2011;59:6467–73.
- [6] Kaji M, Watanabe A, Aizawa H. Differences in clinical features between influenza A H1N1, A H3N2, and B in adult patients. *Respirology* 2003;8:231–3.
- [7] Lanari M, Capretti MG, Decembrino L, et al. Focus on pandemic 2009 H1N1 influenza (swine flu). *Minerva Pediatr* 2010;62:39–40.
- [8] Chung EY, Chiang VW. Influenza vaccination, diagnosis, and treatment in children. *Pediatr Emerg Care* 2011;27:760–9.
- [9] LaRossa P. Pandemic novel 2009 H1N1 influenza: what have we learned? *Semin Respir Crit Care Med* 2011;32:393–9.
- [10] McCullers JA, Huber VC. Correlates of vaccine protection from influenza and its complications. *Hum Vaccin Immunother* 2012;8:34–44.
- [11] Cheng VC, To KK, Tse H, et al. Two years after pandemic influenza A/2009/H1N1: what have we learned? *Clin Microbiol Rev* 2012;25:223–63.
- [12] Mahony JB, Petrich A, Smieja M. Molecular diagnosis of respiratory virus infections. *Crit Rev Clin Lab Sci* 2011;48:217–49.
- [13] Munjal I, Gialanella P, Goss C, et al. Evaluation of the 3M rapid detection test for respiratory syncytial virus (RSV) in children during the early stages of the 2009 RSV season. *J Clin Microbiol* 2011;49:1151–3.
- [14] Iregbu KC, Esfandiari J, Nnorom J, et al. Dual Path Platform HIV 1/2 assay: evaluation of a novel rapid test using oral fluids for HIV screening at the National Hospital in Abuja, Nigeria. *Diagn Microbiol Infect Dis* 2011;69:405–9.
- [15] Shrivastava A, Dash PK, Tripathi NK, et al. Evaluation of a commercial Dengue NS1 enzyme-linked immunosorbent assay for early diagnosis of dengue infection. *Indian J Med Microbiol* 2011;29:51–5.
- [16] Grijalva CG, Poehling KA, Edwards KM, et al. Accuracy and interpretation of rapid influenza tests in children. *Pediatrics* 2007;119:e6–11.
- [17] Drexler JF, Helmer A, Kirberg H, et al. Poor clinical sensitivity of rapid antigen test for influenza A pandemic (H1N1) 2009 virus. *Emerg Infect Dis* 2009;15:1662–4.
- [18] Faix DJ, Sherman SS, Waterman SH. Rapid-test sensitivity for novel swine-origin influenza A (H1N1) virus in humans. *N Engl J Med* 2009;361:728–9.
- [19] Hurt AC, Baas C, Deng YM, et al. Performance of influenza rapid point-of-care tests in the detection of swine lineage A (H1N1) influenza viruses. *Influenza Other Respi Viruses* 2009;3:171–6.
- [20] Uyeki TM, Prasad R, Vukotich C, et al. Low sensitivity of rapid diagnostic test for influenza. *Clin Infect Dis* 2009;48:e89–92.
- [21] Wang DY, Wang KT, Wang YC, et al. Establishment of a serological panel for in vitro diagnostics of severe acute respiratory syndrome. *J Food Drug Anal* 2012;20:938–46.
- [22] Chen YW, Huang YC, Ho TH, et al. Viral etiology of bronchiolitis among pediatric inpatients in northern Taiwan with emphasis on newly identified respiratory viruses. *J Microbiol Immunol Infect* 2012. <http://dx.doi.org/10.1016/j.jmii.2012.08.012>.

-
- [23] Evaluation of rapid influenza diagnostic tests for detection of novel influenza A [H1N1] Virus – United States. 2009. *Morb Mortal Wkly Rep* 2009;58:826–9.
- [24] Chan KH, Lam SY, Puthavathana P, et al. Comparative analytical sensitivities of six rapid influenza A antigen detection test kits for detection of influenza A subtypes H1N1 H3N2 and H5N1. *J Clin Virol* 2007;38:169–71.
- [25] Abdel-Ghafar AN, Chotpitayasunondh T, Gao Z, et al. Update on avian influenza A (H5N1) virus infection in humans. *N Engl J Med* 2008;358:261–73.
- [26] Sails AD, Saunders D, Airs S, et al. Evaluation of the Cepheid respiratory syncytial virus and influenza virus A/B real-time PCR analyte specific reagent. *J Virol Methods* 2009;162:88–90.
- [27] Bellau-Pujol S, Vabret A, Legrand L, et al. Development of three multiplex RT-PCR assays for the detection of 12 respiratory RNA viruses. *J Virol Methods* 2005;126:53–63.
- [28] Yu X, Lu R, Wang Z, et al. Etiology and clinical characterization of respiratory virus infections in adult patients attending an emergency department in Beijing. *PLoS One* 2012;7:e32174.