

The effects of different lighting conditions on the accuracy of intraoral scanning

Mehmet Karakuzu^{1*}, Caner Öztürk², Züleyha Başar Karakuzu³, Mustafa Zortuk¹

¹Department of Prosthodontics, Faculty of Dentistry, Hatay Mustafa Kemal University, Hatay, Turkey

²Department of Prosthodontics, Faculty of Dentistry, Ankara Medipol University, Ankara, Turkey

³Department of Oral and Maxillofacial Surgery, Faculty of Dentistry, Hatay Mustafa Kemal University, Hatay, Turkey

ORCID

Mehmet Karakuzu

<https://orcid.org/0009-0008-8452-3736>

Caner Öztürk

<https://orcid.org/0000-0001-9549-2770>

Züleyha Başar Karakuzu

<https://orcid.org/0009-0001-6995-1360>

Mustafa Zortuk

<https://orcid.org/0000-0003-4924-608X>

PURPOSE. This study aimed to investigate the extent to which intraoral scanning are affected by clinical conditions, and whether ambient lighting and different color temperatures have an impact on the accuracy of intraoral scanner, as well as to evaluate scanning time. **MATERIALS AND METHODS.** Twelve different environments were created using various ambient lighting conditions (0, 500, 1000 and 1500 lux) and color temperatures (white, blue and yellow). A partially edentulous mandibular model with two implants and a three-unit bridge was scanned under each environment until 10 digital models were obtained, and scanning times were recorded using a virtual stopwatch. A 3D analysis was performed on the obtained digital models, and the data were analyzed using a software. The generalized linear model analysis and Tukey multiple comparison test were used to analyse the data ($P < .05$). **RESULTS.** The effect of lux, color temperature, and scanning times on RMS data was found to be significant ($P < .001$). The mean RMS value was the highest in the 0 lux group and the lowest in the 500 lux group. Regarding the color temperature, the highest RMS value was in the white color group and the lowest in the yellow color group. Scanning times were similar among the 0, 500 and 1000 lux groups, with a significant increase in the 1500 lux group. **CONCLUSION.** Different ambient lighting conditions and color temperatures have significant effect on the accuracy of intraoral scanning. [J Adv Prosthodont 2024;16:311-8]

KEYWORDS

Ambient light; Color temperature; Intraoral scanning

INTRODUCTION

In contemporary clinical dental practice, the utilization of computer-aided design and computer-aided manufacturing (CAD-CAM) technologies has rapidly increased.¹ The initial step involves surface scanning of teeth and related tissues using an intraoral scanner (IOS). In the CAD-CAM digital workflow,

Corresponding author

Mehmet Karakuzu

Department of Prosthodontics,
Faculty of Dentistry, Hatay Mustafa
Kemal University, Tayfur Sökmen
Kampüsü Alahan-Antakya, Hatay
31060, Turkey

Tel +90 507 016 70 80

E-mail dt.mhmtkrkz@gmail.com

Received August 3, 2024 /

Last Revision September 25, 2024 /

Accepted October 22, 2024

© 2024 The Korean Academy of Prosthodontics

© This is an Open Access article distributed under the terms of the Creative Commons Attribution Non-Commercial License (<https://creativecommons.org/licenses/by-nc/4.0>) which permits unrestricted non-commercial use, distribution, and reproduction in any medium, provided the original work is properly cited.

digital scanning technologies offer high accuracy for both implant- and tooth-supported restorations when compared to traditional impression techniques.¹⁻³

Digital impression has numerous advantages such as improving patient acceptance, reducing distortion of impression materials, and visualizing preparation in three dimensions beforehand, all while being cost-effective and time-efficient.⁴ Moreover, digital impression, devoid of harmful stimuli, ensures high patient satisfaction by eliminating the risk of choking, gagging, and taste irritation,⁵ thereby reducing the treatment time.⁶⁻¹⁰ With the advancement of intraoral scanners, there has been rapid progress in the accuracy of digital impression. The accuracy of digital impression is determined by its trueness and precision.¹¹ Trueness refers to the deviation of the scanned data from the original geometry, while precision refers to the deviation between repeated scans of the same data.¹²⁻¹⁴ Minimizing adaptation problems in prostheses is the focus of many current studies to ensure prosthetic restorations are made with minimal errors independently of the dentist and technician.¹⁵

While there are studies comparing intraoral scanners internally,^{2,3,7,9} research on environmental factors affecting the digital workflow is scarce. Various factors such as user experience and learning process affect the sensitivity of digital scanning.^{16,17} Additionally, factors such as calibration,¹⁸ scanning protocol,¹⁹ ambient lighting conditions,²⁰ surface characteristics,²¹⁻²⁴ presence of mobile tissues,²⁵ presence of reflective restorations, and presence of saliva also influence the accuracy. Revilla-Leon *et al.*²⁶ reported that ambient lighting conditions significantly affect the geometry replication capability of an intraoral scanner. Therefore, this study was aimed to investigate the extent to which intraoral scanning is influenced by environmental conditions in clinical settings, as well as to determine whether the intensity of ambient lighting and different color temperatures have an impact on the accuracy of intraoral scanner. The null hypothesis of the study was that varying ambient lighting conditions and color temperatures would have no effect on the accuracy of intraoral scanning.

MATERIALS AND METHODS

As a reference model, a fully dentate mandibular model (Frasaco Study Model ANA 4; Frasaco GmbH, Tett nang, Germany), produced for multipurpose in dentistry, was used in this study. In the preparation of the implant area on the reference model, teeth 44, 45, and 46 were removed from the model, and digital implant analogs (Osstem TS; Osstem Implant Co. Ltd., Seoul, Korea) were placed in the areas of teeth 44 and 46.

In the preparation of the teeth, teeth 34 and 36 were removed from the model, and teeth 33, 35, and 37 were prepared with a chamfer bur according to preparation principles, including a convergence angle of 6 – 10 degrees, circumferential reduction of 1.2 – 1.5 mm, a step width of 1 mm, and occlusal reduction of 2 mm. Pink silicone (Gingifast Rigid; Zhermack GmbH, Badia Polesine, Italy) was applied to mimic the periodontal tissue around the analogs and in the socket areas of teeth 45, 36, and 34 until it reached the level of the gingival line. All analogs and prepared tooth were positioned to the same level, assumed to be the gingival line level.

A laboratory scanner (3Shape E3; 3Shape, GmbH, Copenhagen, Denmark) was used for the reference model acquisition. The scan bodies (Osstem TS; Osstem Implant Co. Ltd., Seoul, Korea) were placed on the prepared model, and the scanning process was initiated using the laboratory scanner. The scanning process was repeated 10 times, and the obtained scanning data were overlapped using reverse engineering software, (Geomagic Design X 3D System Inc., Rock Hill, SC, USA), to ensure the accuracy of the data.

To mimic clinical lighting conditions, 4 different ambient lightings (0 lux (dark), 500 lux, 1000 lux, 1500 lux), and 3 different light sources (white light (7500 K), blue light (19000 K), yellow light (3900 K)) were used in this study.

For ambient lighting, a setup with 12 white LED bulbs (Panasonic LED E27 860 lumens 6500 K White; Panasonic Corporation, Osaka, Japan) was prepared with 12 sensors, overlooking the scanning area. The ambient lighting was measured and adjusted to 0 lux, 500 lux, 1000 lux, and 1500 lux using a light meter (DT-3809 Led Light Meter; Shenzhen Everbest Machinery Industry Co. Ltd., Shenzhen, China) (Fig. 1). Three dif-



Fig. 1. Lux measurements of lighting environments.



Fig. 2. Color filters: White (7500 K), Blue (19000 K), and Yellow (3900 K).

ferent color temperatures were obtained by adding a conversion filter to the tip of a portable reflector, resulting in desired colors: white (7500 K), blue (19000 K), and yellow (3900 K) (Fig. 2). Thus, a total of 12 possible lighting conditions were created. All environments were created in a windowless, naturally lit (NL), and dark room.

In this study, an intraoral scanner (YOUJOY 3DS 2.0; Youjoy Co. Ltd., Ningbo, China) was used. The scanning process was performed according to the scanning recommendation protocol of the manufacturer. The scanning process was repeated 10 times for each environment, and after each scan, the scanned surfaces were examined, areas with artifacts were identified and cut by cleaning, and scanning times were recorded in seconds using a virtual stopwatch of intraoral scanner. Finally, the scans were saved and stored as standard tessellation language (STL) files.

To compare the measurements, all STL files ob-

tained from the scanner were transferred to a reverse engineering software (Geomagic Design X 3D System Inc., Rock Hill, SC, USA). The transferred data were standardized by performing initial alignment and best alignment according to the reference-accepted regions through the program (Fig. 3). Subsequently, the obtained data were saved as RMS data. The data were analyzed using a software (IBM SPSS V23; SPSS Inc., Chicago, IL, USA). Normal distribution compliance was examined with the Shapiro Wilk test. Generalized Linear Models were used for the comparison of parameters conforming to normal distribution by color and lux, and multiple comparisons were made using the Tukey Test. The significance level was set at $P < .05$.

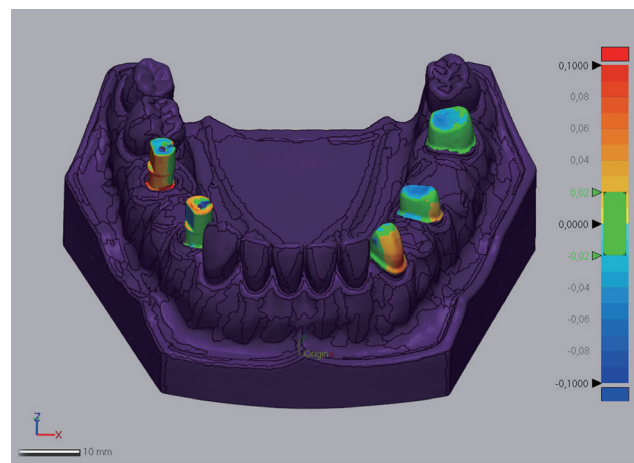


Fig. 3. Image of superimposed STL files.

RESULTS

The main effect of color groups and lux was found to be statistically significant on the RMS data ($P < .05$). The interaction between color groups and lux did not have a statistically significant effect on the mean RMS values ($P = .348$). The mean RMS value was 0.0658 in the white color group, 0.0599 in the blue color group, and 0.0544 in the yellow color group. The mean RMS value was 0.0852 in the 0 lux group, 0.0393 in the 500 lux group, 0.0419 in the 1000 lux group, and 0.0736 in the 1500 lux group. Independent of lux value, the mean RMS value obtained from the white color was significantly higher than those from other colors ($P < .001$). The mean RMS value obtained from the blue color was also significantly higher than that from the yellow color ($P < .001$). In the 0 lux group, the mean RMS value was significantly higher compared to all other lux values ($P < .05$). While there was no statistically significant difference between the 500 and 1000 lux values ($P > .05$), both values showed significantly lower RMS values compared to the 1500 lux value ($P < .05$). In the 0 lux group, similar RMS values were ob-

tained in the white and blue colors ($P > .05$), while a significantly lower RMS value was found in the yellow color ($P < .05$) (Table 1).

The main effect of color groups was not statistically significant on time ($P = .431$). The mean time was 265.4 seconds in the white color, 268.7 seconds in the blue color, and 266.1 seconds in the yellow color. The main effect of lux was statistically significant on time ($P < .001$). The mean time was 260.5 seconds in the 0 lux group, 259.4 seconds in the 500 lux group, 263.3 seconds in the 1000 lux group, and 283.6 seconds in the 1500 lux group. The mean time in the 1500 lux group was the highest and differed from the other groups. The 0, 500, and 1000 lux groups showed similarity in terms of time. The interaction between color groups and lux was not statistically significant on time ($P = .388$) (Table 2).

DISCUSSION

In this study, the accuracy of digital impression of implant-supported and fixed prosthetic restorations under different ambient lighting conditions and color

Table 1. Descriptive statistics and multiple comparison results of RMS (mm) values according to Color and Lux

Lux	Color			
	White	Blue	Yellow	Total
0	0.0907 ± 0.006	0.0876 ± 0.005	0.0774 ± 0.0045	0.0852 ± 0.0077 ^a
500	0.0457 ± 0.0051	0.0383 ± 0.0048	0.0341 ± 0.0057	0.0393 ± 0.007 ^c
1000	0.0475 ± 0.0054	0.0421 ± 0.0051	0.0363 ± 0.0058	0.0419 ± 0.007 ^c
1500	0.0792 ± 0.0059	0.0716 ± 0.0056	0.07 ± 0.0062	0.0736 ± 0.007 ^b
Total	0.0658 ± 0.0206 ^a	0.0599 ± 0.0214 ^b	0.0544 ± 0.0204 ^c	0.06 ± 0.0212

Mean ± standard deviation, a-c: There is no significant difference between main effects with the same letter.

Table 2. Descriptive statistics and multiple comparison results of times values (sec) in seconds according to Color and Lux

Lux	Color			
	White	Blue	Yellow	Total
0	262 ± 12.8	261.6 ± 14	257.8 ± 12.9	260.5 ± 12.9 ^b
500	257.4 ± 9.7	265.4 ± 16.2	255.5 ± 9.9	259.4 ± 12.6 ^b
1000	257.6 ± 13.2	264.7 ± 15.1	267.5 ± 10.7	263.3 ± 13.4 ^b
1500	284.4 ± 7.9	283.1 ± 10.4	283.4 ± 9.9	283.6 ± 9.2 ^a
Total	265.4 ± 15.5	268.7 ± 16	266.1 ± 15.3	266.7 ± 15.6

Mean ± standard deviation, a-b: There is no significant difference between main effects with the same letter.

temperatures has been evaluated. This study refused the null hypothesis that varying ambient lighting conditions and color temperatures have no effect on the accuracy of intraoral scanning.

When the results of this study were examined in terms of lux values, within each color group, the 0 lux values showed significantly higher RMS values compared to all other lux values. Similarly, ambient values of 1500 lux also showed significantly higher RMS values compared to 500 lux and 1000 lux values. There was no statistically significant difference between 500 and 1000 lux values. Lux values were determined in our study considering clinical conditions. The 500 lux value represents classic room lighting in a dental clinic, while values of 1500 lux and above represent dental unit reflector lighting.²⁷ Furthermore, the 500 lux value was seen as a value measured in average room light and was added as a parameter. Examination of the data concluded that clinical lighting conditions (500 and 1000 lux) were appropriate for the scanner to perform optimally. In a similar study, digital scans were performed under 0 lux and 1003 lux ambient illuminations, where the 1003 lux condition yielded the lowest deviation values, while 0 lux resulted in higher RMS values.²⁸ In another study, illuminations of 0 lux, 500 lux, and 2500 lux were used, and an average deviation value was found significantly lower at 500 lux compared to 0 and 2500 lux. These findings are consistent with the results of the present study.

In a previous study that evaluated the impact of various lighting conditions on the mesh qualities of different IOS devices, three different IOS devices were evaluated under four different lighting conditions.²⁶ Scans were conducted in environments created with operating room light at 10000 lux, room light at 1003 lux, natural light at 500 lux, and no light at 0 lux. The different IOS devices showed significant differences in mesh quality values in scans conducted under different lighting conditions but with the same illumination conditions and using the same IOS.²⁶ The findings of this study were similar to a previous study,²⁶ with the highest RMS values obtained in the 0 lux environment. In another study conducted by Revilla-Leon *et al.*,²⁹ environmental lighting conditions were tested up to 10000 lux in increments of 1000 lux, forming ten groups based on different brightness levels. The

1000 lux lighting condition was found to be ideal for maximizing the scanning accuracy of the tested IOS, and it was recommended to avoid dental unit light. In another study examining ambient illuminations of various intensities (100, 500, 1000, 5000, and 10000 lux) for different intraoral scanners in full-arch implant scans, seven different IOSs were evaluated. It was concluded that changes in ambient lighting conditions had a significant effect on scanning accuracy and scanning time, but this effect varied for all IOSs used.³⁰

When the results of the present study were examined in terms of color values, within each lux group, the RMS value obtained from the white color was significantly higher than those from other colors. The RMS value obtained from the blue color was also significantly higher than that from the yellow color. The mean RMS values differed across all color groups. Overall, the lowest RMS data were obtained at 3900 K (yellow), followed by 19000 K (blue), and finally 7500 K (white). In the dark ambient group, statistically similar RMS values were obtained at 7500 K (white) and 19000 K (blue), while significantly less RMS data were obtained at 3900 K (yellow). In this study, when determining color temperatures, 3900 K (yellow) was chosen to mimic daylight in a windowed clinic. The 7500 K (white) color temperature was added as a parameter to mimic the color of the dental reflector light found in contemporary dental units and the 19000 K (blue) light was selected as a third parameter. In a study conducted by Köseoğlu *et al.*, digital scans were performed using two different scanning light modes, blue and white, under different ambient illuminations. The blue mode condition had the lowest deviation values, while the white mode condition yielded higher deviation data.²⁸ In a similar study, scans were performed at different lux values under color temperatures of 3900 K (yellow), 4100 K (orange), 7500 K (white), and 19000 K (blue), and it was found that the 3900 K (yellow) color temperature was optimal for obtaining digital impressions. The 4100 K (orange) color temperature was found to be superior to 7500 K (white) and 19000 K (blue).²⁰ Although the optimal color temperature of 3900 K (yellow) aligns with the present study, the similarity of the 7500 K (white) and 19000 K (blue) color temperature data does not corre-

spond to the present study. These differences may be associated with the different intraoral scanner used in the other study.

When the results of the present study were examined in terms of scanning times, within each lux group, the primary effect of lux was found to be statistically significant on scanning time. The average time in the 1500 lux group was the highest and differed from the other groups. The 0 lux, 500 lux, and 1000 lux groups showed similarity in terms of time. There was no statistically significant interaction between color and lux on time.

Parallel to the present study, in a study by Wese-mann *et al.*,³¹ six intraoral scanners were used, and scans were performed at different lighting levels with each IOS. In all scans, scanning times were recorded and it was observed that scanning time increased for all IOSs except iTero Element in scans performed above 500 lux. Additionally, the shortest scanning time for each scanner varied. In another study by Arakida *et al.*, scanning times were examined under ambient illuminations of 0 lux, 500 lux, and 2500 lux, and it was found that scanning time was significantly longer at 2500 lux compared to the other scans.²⁰ This longer scanning time is associated with the effect of ambient light on the accuracy of digital impression, related to the three-dimensional (3D) data acquisition process.³² Most optical scanners obtain 3D data by reflecting laser light onto the surface of the original geometry and capturing this reflected light in a high-speed circuit. However, when the brightness of the laser light is too high, the sensor becomes saturated, resulting in the system being unable to calculate the positions of points. Moreover, a laser with high brightness may cause partial errors at points and delay the capture of data.³³

In terms of ambient lighting conditions and color temperatures, the lowest RMS values were obtained at 500 lux and 3900 K (yellow), which are the closest to clinical conditions. This was followed by data obtained at 1000 lux. The highest average RMS values were obtained in a 0 lux (dark) environment and at a 7500 K (white) color temperature. Therefore, it was concluded that appropriate clinical lighting conditions and yellow color temperature were necessary for the scanner to perform optimally.

Although efforts were made to create a scenario close to clinical conditions in this study, there were some limitations. Factors such as the moist and warm environment inside the oral cavity, as well as patient-related factors such as saliva and tongue, may increase deviation in a similar *in vivo* study. Additionally, mobile mucosal areas in edentulous areas may lead to significant errors in processing data and affect the scanning time. All these factors can negatively affect the measurement quality of a scanner. Although the RMS values obtained were carried out by a single clinician, errors related to the clinician can be considered as a limitation. Thus, further researches are needed.

CONCLUSION

Within the limitations of this study, the following conclusions were drawn:

A higher RMS value was obtained at 0 lux compared to all other lux values. While there was no statistical difference between the 500 and 1000 lux values, both values showed significantly lower RMS values than the 1500 lux value. Regardless of the lux value, the RMS value obtained from 7500 K (white) color was significantly higher than other colors. The RMS value obtained from 19000 K (blue) color was also significantly higher than the RMS value obtained from 3900 K (yellow) color. The time average in the 1500 lux group was found to be the highest and differed from other groups. The 0, 500, and 1000 lux groups showed similarity in terms of time. The color groups had no effect on the scanning time.

REFERENCES

1. Abduo J, Elseyoufi M. Accuracy of intraoral scanners: a systematic review of influencing factors. *Eur J Prosthodont Restor Dent* 2018;26:101-21.
2. Rutkūnas V, Gečiauskaitė A, Jегelevičius D, Vaitiekūnas M. Accuracy of digital implant impressions with intraoral scanners. A systematic review. *Eur J Oral Implantol* 2017;10 Suppl 1:101-20.
3. Michelinakis G, Apostolakis D, Tsagarakis A, Kourakis G, Pavlakis E. A comparison of accuracy of 3 intraoral scanners: a single-blinded in vitro study. *J Prosthet*

- Dent 2020;124:581-8.
4. Christensen GJ. Impressions are changing: deciding on conventional, digital or digital plus in-office milling. *J Am Dent Assoc* 2009;140:1301-4.
 5. Akarslan ZZ, Yıldırım Biçer AZ. Influence of gag reflex on dental attendance, dental anxiety, self-reported temporomandibular disorders and prosthetic restorations. *J Oral Rehabil* 2013;40:932-9.
 6. Grünheid T, McCarthy SD, Larson BE. Clinical use of a direct chairside oral scanner: an assessment of accuracy, time, and patient acceptance. *Am J Orthod Dentofacial Orthop* 2014;146:673-82.
 7. Yuzbasioglu E, Kurt H, Turunc R, Bilir H. Comparison of digital and conventional impression techniques: evaluation of patients' perception, treatment comfort, effectiveness and clinical outcomes. *BMC Oral Health* 2014;14:10.
 8. Schepke U, Meijer HJ, Kerdijk W, Cune MS. Digital versus analog complete-arch impressions for single-unit premolar implant crowns: Operating time and patient preference. *J Prosthet Dent* 2015;114:403-6.e1.
 9. Joda T, Brägger U. Patient-centered outcomes comparing digital and conventional implant impression procedures: a randomized crossover trial. *Clin Oral Implants Res* 2016;27:e185-9.
 10. Gjølvd B, Chrcanovic BR, Korduner EK, Collin-Bagewitz I, Kisch J. Intraoral digital impression technique compared to conventional impression technique: a randomized clinical trial. *J Prosthodont* 2016;25:282-7.
 11. Chandran DT, Jagger DC, Jagger RG, Barbour ME. Two- and three-dimensional accuracy of dental impression materials: effects of storage time and moisture contamination. *Biomed Mater Eng* 2010;20:243-9.
 12. Ziegler M. Digital impression taking with reproducibly high precision. *Int J Comput Dent* 2009;12:159-63.
 13. Ender A, Mehl A. In-vitro evaluation of the accuracy of conventional and digital methods of obtaining full-arch dental impressions. *Quintessence Int* 2015;46:9-17.
 14. Ender A, Mehl A. Accuracy of complete-arch dental impressions: a new method of measuring trueness and precision. *J Prosthet Dent* 2013;109:121-8.
 15. Menini M, Setti P, Pera F, Pera P, Pesce P. Accuracy of multi-unit implant impression: traditional techniques versus a digital procedure. *Clin Oral Investig* 2018;22:1253-62.
 16. Kim J, Park JM, Kim M, Heo SJ, Shin IH, Kim M. Comparison of experience curves between two 3-dimensional intraoral scanners. *J Prosthet Dent* 2016;116:221-30.
 17. Lim JH, Park JM, Kim M, Heo SJ, Myung JY. Comparison of digital intraoral scanner reproducibility and image trueness considering repetitive experience. *J Prosthet Dent* 2018;119:225-32.
 18. Richert R, Goujat A, Venet L, Viguie G, Viennot S, Robinson P, Farges JC, Fages M, Ducret M. Intraoral scanner technologies: a review to make a successful impression. *J Healthc Eng* 2017;2017:8427595.
 19. Müller P, Ender A, Joda T, Katsoulis J. Impact of digital intraoral scan strategies on the impression accuracy using the TRIOS pod scanner. *Quintessence Int* 2016;47:343-9.
 20. Arakida T, Kanazawa M, Iwaki M, Suzuki T, Minakuchi S. Evaluating the influence of ambient light on scanning trueness, precision, and time of intra oral scanner. *J Prosthodont Res* 2018;62:324-9.
 21. Cuesta E, Rico JC, Fernández P, Blanco D, Valiño G. Influence of roughness on surface scanning by means of a laser stripe system. *Int J Adv Manuf Technol* 2009;43:1157-66.
 22. Vukašinović N, Možina J, Duhovnik J. Correlation between incident angle, measurement distance, object colour and the number of acquired points at CNC laser scanning. *J Mech Eng* 2012;58:23-8.
 23. Anh JW, Park JM, Chun YS, Kim M, Kim M. A comparison of the precision of three-dimensional images acquired by 2 digital intraoral scanners: effects of tooth irregularity and scanning direction. *Korean J Orthod* 2016;46:3-12.
 24. Park JM. Comparative analysis on reproducibility among 5 intraoral scanners: sectional analysis according to restoration type and preparation outline form. *J Adv Prosthodont* 2016;8:354-62.
 25. Patzelt SB, Vonau S, Stampf S, Att W. Assessing the feasibility and accuracy of digitizing edentulous jaws. *J Am Dent Assoc* 2013;144:914-20.
 26. Revilla-León M, Jiang P, Sadeghpour M, Piedra-Cascón W, Zandinejad A, Özcan M, Krishnamurthy VR. Intraoral digital scans: part 2-influence of ambient scanning light conditions on the mesh quality of different intraoral scanners. *J Prosthet Dent* 2020;124:575-80.

27. Viohl J. Dental operating lights and illumination of the dental surgery. *Int Dent J* 1979;29:148-63.
28. Koseoglu M, Kahramanoglu E, Akin H. Evaluating the effect of ambient and scanning lights on the trueness of the intraoral scanner. *J Prosthodont* 2021;30:811-6.
29. Revilla-León M, Subramanian SG, Att W, Krishnamurthy VR. Analysis of different illuminance of the room lighting condition on the accuracy (trueness and precision) of an intraoral scanner. *J Prosthodont* 2021;30:157-62.
30. Ochoa-López G, Cascos R, Antonaya-Martín JL, Revilla-León M, Gómez-Polo M. Influence of ambient light conditions on the accuracy and scanning time of seven intraoral scanners in complete-arch implant scans. *J Dent* 2022;121:104138.
31. Wesemann C, Kienbaum H, Thun M, Spies BC, Beuer F, Bumann A. Does ambient light affect the accuracy and scanning time of intraoral scans? *J Prosthet Dent* 2021;125:924-31.
32. Ma Y, Guo YQ, Saleh MQ, Yu H. Influence of ambient light conditions on intraoral scanning: a systematic review. *J Prosthodont Res* 2024;68:237-45.
33. Blanco D, Fernández E, Cuesta E, Suárez M. Influence of ambient light on the quality of laser digitized surfaces. In: *International Conference of Computational Intelligence and Intelligent Systems. World Congress on Engineering*. Vol. 1. London: Conference proceedings; July 2-4, 2008. p. 32-7.