



CT-scan vs. 3D surface scanning of a skull: first considerations regarding reproducibility issues

Stella Fahrni^{a,b}, Lorenzo Campana^b, Alejandro Dominguez^c, Tanya Uldin ^b, Fabrice Dedouit^b, Olivier Delémont^a and Silke Grabherr^b

^aSchool of Criminal Justice, University of Lausanne, Lausanne-Dorigny, Switzerland; ^bDepartment of Forensic Imaging, University Centre for Legal Medicine Lausanne-Geneva, Lausanne, Switzerland; ^cDepartment of Technological Radiology, Health School of Sciences Vaud - HESAV, Lausanne, Switzerland

ABSTRACT

Three-dimensional surface scanning (3DSS) and multi-detector computed tomography (MDCT) are two techniques that are used in legal medicine for digitalizing objects, a body or body parts such as bones. While these techniques are more and more commonly employed, surprisingly little information is known about the quality rendering of digitalized three-dimensional (3D) models provided by each of them. This paper presents findings related to the measurement precision of 3D models obtained through observation of a study case, where a fractured skull reconstructed by an anthropologist was digitalized using both post-mortem imaging methods. Computed tomography (CT) scans were performed using an 8-row MDCT unit with two different slice thicknesses. The variability of 3D CT models superimposition allowed to assess the reproducibility and robustness of this digitalization technique. Furthermore, two 3D surface scans were done using a professional high resolution 3D digitizer. The comparison of 3D CT-scans with 3D surface scans by superimposition demonstrated several regions with significant differences in topology (average difference between +1.45 and −1.22 mm). When comparing the reproducibility between these two digitalizing techniques, it appeared that MDCT 3D models led in general to greater variability for measurement precision between scanned surfaces. Also, the reproducibility was better achieved with the 3D surface digitizer, showing 3D models with fewer and less pronounced differences (from +0.32 to −0.31 mm). These experiments suggest that MDCT provides less reproducible body models than 3D surface scanning. But further studies must be undertaken in order to corroborate this first impression, and possibly explain the reason for these findings.

ARTICLE HISTORY

Received 28 February 2017
Accepted 22 May 2017

KEYWORDS

Forensic imaging; multi-detector computed tomography (MDCT); 3D surface scanning; anthropology

Introduction

Forensic imaging tends to be more and more used in legal medicine and forensic sciences [1–6]. Many different techniques exist and some of them are currently available and routinely employed in different forensic centres [1–4,6].

The most commonly used technique is post-mortem computed tomography (PMCT) [4,7]. This technique provides a rapid documentation of a body, allowing to store it digitally and to view the interior of it [3]. Although it is not the preferred method used for viewing internal organs [8], it gives a first glimpse at major malformations, presence of blood or bone fractures etc. [9–11]. Additionally, it allows performing three-dimensional (3D) reconstruction showing the surface of the scanned body as well as the internal organs [3,12,13]. This possibility to represent the body, and especially the skeletal system in 3D, is an advantage often used for example to show fracture systems [14], ballistic trauma or to perform so-called “virtual anthropology” by investigating the virtual

skeletons obtained using 3D volume rendering methods [15–23].

Another method of 3D imaging is three-dimensional surface scanning (3DSS). This technique was adapted for use from the industry [24] and is employed today for medico-legal purposes especially in Switzerland [25–29]. The three main fields of application of this technique are traffic accident reconstructions [25,26], correlation between a wound and an injury causing instrument [28], and the comparison of bite marks with the suspect’s dentition [27]. It has also been employed by anthropologists and anatomists to digitally document bones [30]. Concerning 3DSS, different technical systems exist. Today, the most commonly used methods for scanning are fringe-pattern technology [26] or other patterned light systems such as mobile hand scanners [31].

Although much literature exists on different techniques about how to obtain “virtual skeletons”, to our knowledge there is no information available on the quality of digitized 3D models in terms of repeatability,

reproducibility and robustness of the digitalization process [30,32]. The objective of this technical note is to provide a first overview on data comparison between digital 3D models obtained by MDCT-scanning and 3DSS. Thus, we will discuss the influence of technical parameters on the resulting models looking at experience-based specific cases.

Material and methods

MDCT is routinely performed on all human bodies admitted for medico-legal examination at our centre of expertise. This technique is also employed on the bones examined by the anthropologist [15,30]. The present case study analysis and discussion was performed on a skull after maceration. The victim suffered blunt force trauma located on the left frontal bone, which was most likely to be the individual's cause of death. The skull was reconstructed including all fragments by a board-certified anthropologist using white glue. All the following investigations were performed once these procedures were done.

MDCT-scanning

Three MDCT-scans were performed by a board-certified radiographer using an 8-row MDCT unit (LightSpeed, General Electric Healthcare). The three scans were performed with an interval of 48 days between the first and the second one, and only a day between the second and the third one. The acquisition protocols used differed from one scan to another, especially concerning the slice thickness. It varied from 1.25 mm (Scan 1) to 0.625 mm (Scan 3). The detailed acquisition parameters can be found in Table 1.

In order to generate 3D models for computed tomography (CT) raw data, we used the OsiriX MD imaging software (Free version 5.6). Volume rendering was done followed by surface rendering (high resolution and pixel value 200; Figure 1(A,B)). The file was then exported to STL format (STereoLithography, Standard Tessellation Language) in order to compare CT-data with 3D surface scan data.

3DSS

For the 3D surface scanning, a GOM ATOS Compact Scan 5M was employed by a trained operator. Measuring Volume of 300 (300 mm × 230 mm × 230 mm) and 1.5 mm reference point (white diameter) were chosen in order to obtain a reachable resolution of 0.124 mm. The two different 3D surface scans were performed with the same parameters, the same instrumentation and by the same trained operator. The first 3DSS was performed on 19 September 2014 (Figure 1(C,D)) and the second 40 days later on 29 October 2014.

Comparison between 3D models

Superimposition and comparison between both 3D models were done with a GOM ATOS software 7.5. A pre-alignment was performed using three identical points, and then a "Best fit alignment" was used over the surface as to obtain the best possible superimposition. All comparisons were made by the same experienced operator.

When using the surface comparison function of the GOM ATOS software 7.5, colours are mapped on the models. They provide an indication of the spatial correlation of the models, and allow a quick and efficient visual appreciation of the qualitative colour matching of the models. Regions, in which the surface is displayed in green colour, indicate almost no deviation between the two models. The red colour shows that there is a positive deviation as the borders of the first model are overlapping those of the second one. Blue colour indicates a negative deviation as the borders of the first model are not reaching the borders of the second one. A punctual value for the deviation can be highlighted by clicking on an area.

Results and discussion

If we only focus on the single aspect of 3D modelling, all of them seem to represent the object in details. The only visualization problem that could appear would be the 3D rendering of MDCT, when inlay dental material creates some types of artefacts on the model that do not allow the exact representation of the tooth's shape. These

Table 1. Scan parameters of CT-scans 1-3 (Ge HealthCare LightSpeed - 8 rows).

| CT-scan | Scan type | Thickness slice Table speed Pitch | Interval spacing | Scan Field of view (FOV) | Kilo Volts (kV) | Milli Amperage (mA) | Algorithm of reconstruction | Position of acquisition |
|------------------------------------------------|------------------|-----------------------------------|------------------|--------------------------|-----------------|---------------------|-----------------------------|-------------------------|
| CT-scan 1 Date 11.09.2014 | Helical 1.0 s | 1.25 mm 6.25 0.625:1 | 0.6 | Head 25 | 140 | 140 | Bone + | Axial |
| CT-scan 2 Date 29.10.2014 (+ 48 days) | Helical 1.0 s | 1.25 mm 6.25 0.625:1 | 0.6 | Head 25 | 140 | 140 | Bone + | Coronal |
| CT-scan 3 Date 30.10.2014 (+ 49 days) | Helical 1.0 s | 0.625 mm 1.25 1:1 | 0.3 | Head 25 | 140 | 140 | Bone + | Coronal |

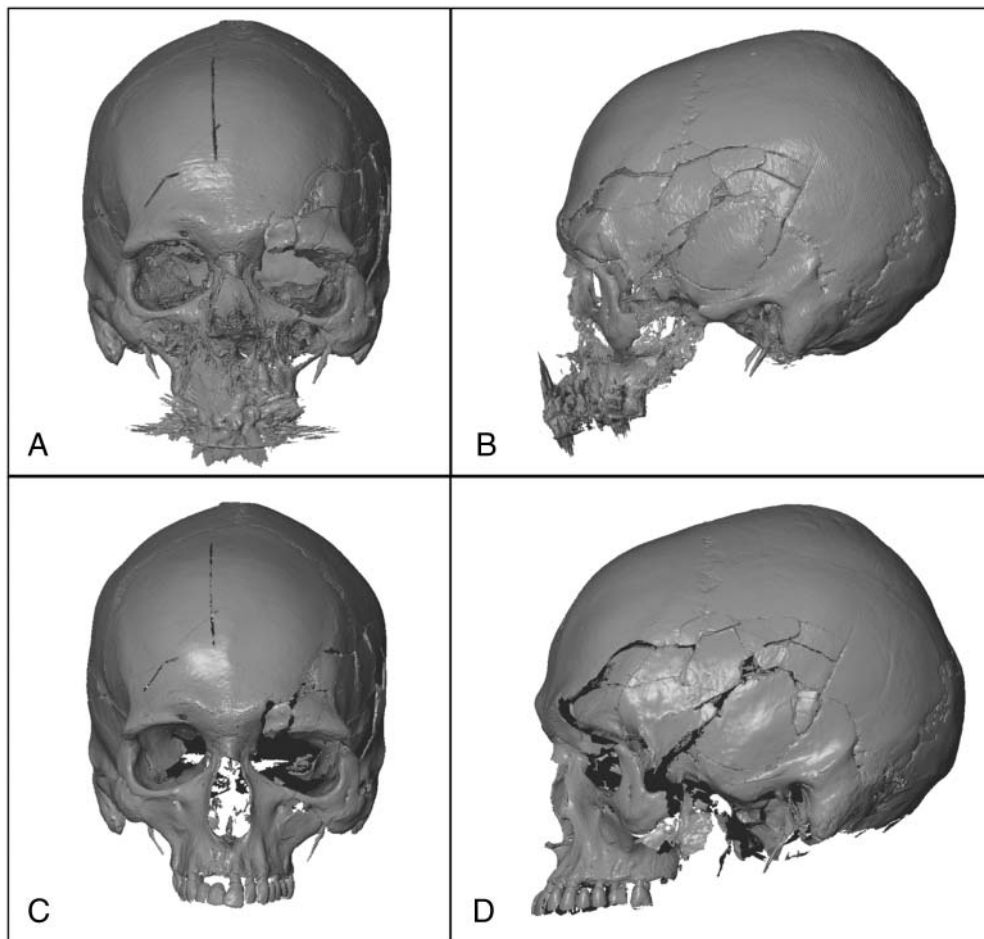


Figure 1. 3D Model obtained with the CT-scan 1: (A) front view; (B) profile view. 3D Model obtained with the 3D surface scanner 1: (C) front view; (D) profile view.

hardening artefacts are due to the interaction of X-rays with some metallic component of the treated tooth [33].

To evaluate the precision of the obtained images, it is important to compare on one hand scans performed at different time lags with the same technique, and on the other hand to compare the results obtained with the different methods. A thorough examination of the accuracy would definitely require to perform a set of scans for each of the considered techniques. In this regard, our study does not claim to provide such a complete assessment, but it shed lights on possible issues that would require further clarifications.

Comparison between MDCT models obtained at different time lags

This comparison shows generally a great difference in some areas of the 3D model going from +1.58 to -1.64 mm in average. For example, in the occipital region, difference of -1.12 mm can be observed (Figure 2 (A,B)). The comparison between model of the second and the third CT scan shows slightly better results with intervals of values from +0.76 to -0.67 mm (Figure 2(C,D)). This may be due to a thinner slice thickness of the third scan. In fact, as Dalrymple and collaborators explained in their article, the thinner the slice, the better the spatial

resolution [34]. This means that employing a slice thickness of 0.625 mm improves precision and reduces differences observed between MDCT-scans.


Although significant differences are observed between 3D models from MDCT-scans, they are still better than values obtained for dry bones in other research. In some studies like the one of Stull and collaborators [35], authors demonstrated high accuracy between measurements taken from a dry element and measurements taken from the 3D-MDCT image of the same dry element. They compared morphological measurements performed manually from dry-bones with those performed by measuring the same parameters on 3D models obtained by MDCT-scan of the same bones. They found that measurement differences were in acceptable range for anthropologist (<2 mm). Therefore, they assessed that CT images are accurate representations of the true objects' dimensions [35]. They also claim that differences were rather resulting from human error than from imaging technology. However, they did not compare MDCT-scan of the same dry bone. In our case, the variations observed were too high for the same bone measured. And as the measurements are calculated by the software, this eliminates the human error from the hypothesis. We do not think that such differences between MDCT-scans

This first impression would require further studies on a more extensive set of samples, taking into account different acquisition parameters.

Disclosure statement

The authors did not have any conflicts of interest to declare.

ORCID

Tanya Uldin  <http://orcid.org/0000-0001-7958-232X>

References

- Grabherr S, Grimm J, Baumann P, et al. Application of contrast media in post-mortem imaging (CT and MRI). *Radiol Med*. 2015;120:824–834.
- Krentz BV, Alamo L, Grimm J, et al. Performance of post-mortem CT compared to autopsy in children. *Int J Legal Med*. 2016;130:1089–1099.
- Ljung P, Winskog C, Persson A, et al. Full body virtual autopsies using a state-of-the-art volume rendering pipeline. *IEEE Trans Vis Comput Graph*. 2006;12:869–876.
- Okuda T, Shiotani S, Sakamoto N, et al. Background and current status of postmortem imaging in Japan: short history of “Autopsy imaging (Ai).” *Forensic Sci Int*. 2013;225:3–8.
- Persson A, Jackowski C, Engström E, et al. Advances of dual source, dual-energy imaging in postmortem CT. *Eur J Radiol*. 2008;68:446–455.
- Ruder TD, Thali MJ, Hatch GM. Essentials of forensic post-mortem MR imaging in adults. *Br J Radiol*. 2014;87:20130567.
- Dirnhofer R, Jackowski C, Vock P, et al. VIRTOPSY: minimally invasive, imaging-guided virtual autopsy. *Radiographics*. 2006;26:1305–1333.
- Chevallier C, Doenz F, Vaucher P, et al. Postmortem computed tomography angiography vs. conventional autopsy: advantages and inconveniences of each method. *Int J Legal Med*. 2013;127:981–989.
- Dedouit F, Otal P, Costagliola R, et al. [Role of modern cross-sectional imaging in thanatology: a pictorial essay]. *J Radiol*. 2006;87:619–638.
- Donchin Y, Rivkind AI, Bar-Ziv J, et al. Utility of post-mortem computed tomography in trauma victims. *J Trauma Acute Care Surg*. 1994;37:552–556.
- Iwase H, Yajima D, Hayakawa M, et al. Evaluation of computed tomography as a screening test for death inquest. *J Forensic Sci*. 2010;55:1509–1515.
- Campana L, Breitbeck R, Bauer-Kreuz R, et al. 3D documentation and visualization of external injury findings by integration of simple photography in CT/MRI data sets (IprojeCT). *Int J Legal Med*. 2016;130:787–797.
- Shimofusa R, Yamamoto S, Horikoshi T, et al. Applicability of facial soft tissue thickness measurements in 3-dimensionally reconstructed multidetector-row CT images for forensic anthropological examination. *Leg Med*. 2009;11:S256–S259.
- Thali MJ, Yen K, Schweitzer W, et al. Virtopsy, a new imaging horizon in forensic pathology: virtual autopsy by postmortem multislice computed tomography (MSCT) and magnetic resonance imaging (MRI)-a feasibility study. *J Forensic Sci*. 2003;48:386–403.
- de Froidmont S, Grabherr S, Vaucher P, et al. Virtual anthropology: a comparison between the performance of conventional X-ray and MDCT in investigating the trabecular structure of long bones. *Forensic Sci Int*. 2013;225:53–59.
- Dedouit F, Guilbeau-Frugier C, Telmon N, et al. Virtual autopsy and forensic anthropology of a mummified fetus: a report of one case. *J Forensic Sci*. 2008;53:208–212.
- Dedouit F, Telmon N, Costagliola R, et al. New identification possibilities with postmortem multislice computed tomography. *Int J Legal Med*. 2007;121:507–510.
- Grabherr S, Cooper C, Ulrich-Bochsler S, et al. Estimation of sex and age of “virtual skeletons”—a feasibility study. *Eur Radiol*. 2009;19:419–429.
- Weber GW. Virtual anthropology (VA): a call for glasnost in paleoanthropology. *Anat Rec*. 2001;265:193–201.
- Weber GW. Virtual anthropology. *Am J Phys Anthropol*. 2015;156:22–42.
- Zollikofer CPE, Ponce De León MS, Martin RD. Computer-assisted paleoanthropology. *Evol Anthropol Issues News Rev*. 1998;6:41–54.
- zur Nedden D, Knapp R, Wicke K, et al. Skull of a 5,300-year-old mummy: reproduction and investigation with CT-guided stereolithography. *Radiology*. 1994;193:269–272.
- Dedouit F, Telmon N, Costagliola R, et al. Virtual anthropology and forensic identification: report of one case. *Forensic Sci Int*. 2007;173:182–187.
- Grabherr S, Baumann P, Fahrni S, et al. Virtuelle vs. reale forensische bildgebende Verfahren [Virtual versus real forensic imaging procedures]. *Rechtsmedizin*. 2015;25:493–509.
- Buck U, Naether S, Braun M, et al. Application of 3D documentation and geometric reconstruction methods in traffic accident analysis: with high resolution surface scanning, radiological MSCT/MRI scanning and real data based animation. *Forensic Sci Int*. 2007;170:20–28.
- Buck U, Naether S, Räss B, et al. Accident or homicide—virtual crime scene reconstruction using 3D methods. *Forensic Sci Int*. 2013;225:75–84.
- Naether S, Buck U, Campana L, et al. The examination and identification of bite marks in foods using 3D scanning and 3D comparison methods. *Int J Legal Med*. 2012;126:89–95.
- Thali MJ, Braun M, Brueschweiler W, et al. ‘Morphological imprint’: determination of the injury-causing weapon from the wound morphology using forensic 3D/CAD-supported photogrammetry. *Forensic Sci Int*. 2003;132:177–181.
- Thali MJ, Braun M, Dirnhofer R. Optical 3D surface digitizing in forensic medicine: 3D documentation of skin and bone injuries. *Forensic Sci Int*. 2003;137:203–208.
- Fasel JH, Uldin T, Vaucher P, et al. Evaluating preoperative models: a methodologic contribution. *World Neurosur*. 2016;89:681–685.
- Kersten T, Przybilla H, Lindstaedt M, et al. Comparative geometrical investigations of hand-held scanning systems. *ISPRS-Int Archives Photogram Remote Sens Spatial Inf Sci*. 2016;XLI-B5:507–514.
- Verhoff MA, Ramsthaler F, Krähahn J, et al. Digital forensic osteology—possibilities in cooperation with the Virtopsy® project. *Forensic Sci Int*. 2008;174:152–156.

- [33] Boas FE, Fleischmann D. CT artifacts: causes and reduction techniques. *Imag Med.* 2012;4:229–240.
- [34] Dalrymple NC, Prasad SR, El-Merhi FM, et al. Price of isotropy in multidetector CT 1. *Radiographics.* 2007;27:49–62.
- [35] Stull KE, Tise ML, Ali Z, et al. Accuracy and reliability of measurements obtained from computed tomography 3D volume rendered images. *Forensic Sci Int.* 2014;238:133–140.
- [36] Fishman EK, Ney DR, Heath DG, et al. Volume rendering versus maximum intensity projection in CT angiography: what works best, when, and why. *Radiographics.* 2006;26:905–922.