


ORIGINAL ARTICLE

COVID-19 and breast fine needle aspiration cytology method: What should we change?

Luca Nicosia¹ | Anna Carla Bozzini¹ | Antuono Latronico¹ | Francesca Addante² |
 Mauro Giuseppe Mastropasqua²  | Lorenza Meneghetti¹ | Giovanni Mauri³ |
 Elvio De Fiori⁴ | Marta Montesano¹ | Clementina Di Tonno⁵ | Valeria Midolo De Luca⁵ |
 Chiara Casadio⁵ | Enrico Cassano¹

¹Department of Breast Radiology, IEO, European Institute of Oncology IRCCS, Milan, Italy

²Department of Emergency and Organ Transplants, School of Medicine, Section of Anatomic Pathology, University of Bari "Aldo Moro", Bari, Italy

³Division of Interventional Radiology, IEO, European Institute of Oncology IRCCS, Milan, Italy

⁴Department of Radiology, IEO, European Institute of Oncology IRCCS, Milan, Italy

⁵Division of Pathology and Laboratory Medicine, IEO, European Institute of Oncology IRCCS, Milan, Italy

Correspondence

Mauro Giuseppe Mastropasqua, Department of Emergency and Organ Transplants, Section of Anatomic Pathology, School of Medicine, University of Bari, Bari 70124, Italy.
 Email: mauro.mastropasqua@uniba.it

Abstract

Introduction: Air-dried slide preparation for fine needle aspiration cytology procedures is currently considered unsafe because of the risk of infectious aerosols of coronavirus 19. This study compares the safety and accuracy of two different protocols, one with and one without air-dried slides.

Methods: Starting from 3 March 2020, we discontinued the use of air-dried slides during breast fine needle aspiration procedures. We selected cases collected during two periods: 2 months before and 2 months after 3 March. In both groups, the number of procedures was recorded together with the distribution of the diagnostic categories and the concordance between cytological and histological results on surgical specimens for lesions suggestive of malignancy, using the chi-squared test.

Results: Of the 100 procedures performed during the pre-COVID-19 period, 55% were negative (C2), 3% were non-diagnostic (C1) and 40% were positive (C4 or C5). Of the 75 procedures obtained during the COVID-19 period, 44% were negative (C2), 2.7% were non-diagnostic (C1) and 52% were positive (C4 or C5). Despite the use of a new protocol during the COVID-19 period, we observed concordance between cytological and histological results for lesions suggestive of malignancy. There was no statistically significant difference concerning the distribution of the diagnostic categories in the two groups.

Conclusions: Taking into account the slightly lower number of procedures being analysed during the COVID-19 period, the introduction of a new protocol that does not include air-dried slides is safe and reliable.

KEYWORDS

breast, COVID 19, cytology, fine needle aspiration, surgery

1 | INTRODUCTION

Fine needle aspiration cytology (FNAC) has been an essential step in the evaluation of breast lesions since 1968, when Franzen and Zajicek published the first series of cytology results based on 2111 patients, obtaining excellent results.¹

FNAC has been confirmed as an excellent method for the diagnosis of both palpable and non-palpable lesions, under ultrasound guidance, with satisfactory levels of sensitivity and specificity.^{2,3}

In comparison to other breast diagnostic procedures, FNAC has many advantages: it can be performed in the outward clinic, most of the equipment needed for a high-quality product is low-priced and

readily available, results are generally available in a few hours with a low rate of complications and good patient tolerability.^{4,5}

In most breast oncology centres, standard FNAC slide production consists of preparing a thin smear of aspirated material, avoiding crush artefacts. The slides are rapidly air-dried and quickly fixed in 95% ethanol.⁶ However, since the outbreak and dramatic spread in the north of Italy of coronavirus disease 2019 (COVID-19),^{7,8} the preparation of air-dried slides has become a risky procedure due to the aerosols of potentially infectious material. Specimen processing should follow biosafety level 2 guidelines with personal protective equipment at all times.⁹⁻¹¹

Further, the risk of infection of mucous membranes of the nose, eyes or mouth from potential COVID-19 contamination of dry surfaces is also a complication.^{12,13}

In contrast, alcohol-fixed smears significantly reduce coronavirus infectivity¹⁴ and so are preferred over air-dried smears.

In accordance with this, our Breast Unit at the European Institute of Oncology (Milan, Lombardy, the epicentre of the pandemic area), decided to change the FNAC protocol avoiding air-dried slides, in favour of an alcohol-based method. Samples were ethanol fixed to avoid the production of potentially infectious aerosols during the expulsion of material onto slides for air drying.

However, to ensure diagnostic accuracy of the procedure, we aimed to verify the efficacy of this new protocol compared to the standard one.

2 | METHODS

We have retrospectively analysed all breast ultrasound-guided FNACs for suspicious lesions performed between January 2020 and May 2020 in our Breast unit.

The cut-off between the old and the new protocols was 3 March.

Selected cases were from routine screening and follow-up programmes or symptomatic patients, provided they presented visible lesions on ultrasonography, either palpable or not palpable.

Lesions were morphologically classified according to the Breast Imaging Reporting and Data System¹⁶ (Table 1).

Cytological characterisation of samples was recorded and classified into five categories (C1-C5) according to European Guidelines for Quality Assurance in Breast Cancer Screening¹⁷ (Table 2).

Surgery was performed when high-risk or malignant lesions (C4 and C5) were detected and the final pathological diagnosis was recorded.

All FNAC procedures were ultrasound guided and performed by two operators using personal protective equipment, specifically FFP2 or FFP3 masks, protective glasses and gloves.

All operators used the aspiration technique with a 23-gauge needle connected to a 20 mL syringe with extension tubing.

Following identification of the lesion by ultrasonography and alcohol disinfection of the skin, the needle was inserted into the suspected lesion. The syringe plunger was pulled back by the second operator, creating negative pressure, and cells were collected

into the cutting edge of the needle. The needle was then withdrawn from the lesion, and its content expelled onto previously labelled slides. This is the first risky moment that may lead to aerosol/droplet formation.

Smears were prepared by gently spreading the aspirated material, avoiding crush artefacts, using a second slide. The standard procedure prior to COVID-19 involved fixing one slide in 95% alcohol (Figure 1) while the other was air-dried (Figure 2). The rest of the specimen was put into a ready-to-use ThinPrep CytoLyt[®] solution for subsequent automated processing with ThinPrep 5000 Processor[®] (according to manufacturer's instruction; Hologic Corporation). The entire procedure was repeated twice. The slide containers, labelled with the patient data, were sent to the cytology laboratory for analysis along with a complete Cytopathology Requisition Form, including all the pertinent patient history.

During the COVID-19 period, air-dried slides were no longer used due to the high risk of infectious aerosol formation while performing all the cyto-preparatory steps.

TABLE 1 Clinico-radiological features

	Pre COVID 19 period	COVID 19 period
Patients (n)	100	75
Age at VABB, mean (y)	50 (25-80)	50 (35-65)
Mean diameter of the lesion (mm)	12 (5-24)	10 (4-25)
Non palpable lesion	91 (91%)	68 (90.6%)
Palpable lesion	9 (9%)	9.3%
Side and location of the lesion		
Right breast	48 (48%)	49 (65.3%)
Left breast	52 (52%)	26 (34.7%)
Upper quadrants	69 (69%)	44 (58.6%)
Lower quadrants	31 (31%)	31 (41.4%)
BI-RADS ¹⁶		
BI-RADS 3	4 (4%)	1 (1.3%)
BI-RADS 4a	59 (59%)	40 (53.3%)
BI-RADS 4b	9 (9%)	9 (12%)
BI-RADS 4c	24 (%)	6 (8%)
BI-RADS 5	4 (%)	19 (25.4%)

BI-RADS, Breast Imaging-Reporting and Data System; VABB, vacuum-assisted breast biopsy.

TABLE 2 Cytological characterisation of samples¹⁷

Cytological results		
C1	3 (3%)	2 (2.7%)
C2	55 (55%)	33 (44%)
C3	2 (2%)	1 (1.4%)
C4	10 (10%)	7 (9.3%)
C5	30 (30%)	32 (42.6%)



FIGURE 1 Slide fixing in 95% alcohol solution



FIGURE 2 Air-dried slide

For C4 and C5 lesions, we evaluated the accuracy and reliability of the protocols used in the pre-COVID-19 and during COVID-19 periods using subsequent diagnosis on surgical specimens as a reference point.

We also compared the number of cytological procedures performed 2 months before and 2 months after the cut-off point (3 March). In particular, we compared the percentage of inadequate (C1) results obtained by the COVID-19 protocol, with the percentage of inadequate results obtained with the pre-COVID-19 standard procedure.

Continuous data are reported as median and ranges. Categorical data are reported as counts and percentages.

The Pearson's chi-square test assessed the concordance between cytological and histological results on surgical specimens in case of lesions suggestive of malignancy. *P* values less than .05 were considered statistically significant.

3 | RESULTS

During the pre-COVID-19 period (2 January-2 March), 100 FNAC breast procedures were performed compared to 75 procedures made during the COVID-19 period (3 March-3 May).

Patients' average age was 50 years for both groups (range 25-80 years and 35-65 years).

For the pre-COVID-19 period, 55 out of 100 cases (55%) were negative (C2) on FNAC, 3/100 (3%) were non-diagnostic (C1) and 2/100 (2%) were probably benign (C3), subsequently confirmed histologically. The remaining 40/100 (40%) were positive (C4 or C5), in detail: 30/100 were C5 and 10/100 were C4. All these patients underwent surgery, and only one (previously diagnosed as C4) resulted negative on histology (Figure 3).

For the COVID-19 period, 33 out of 75 cases (44%) were negative (C2) on FNAC, 2/75 (2.7%) were non-diagnostic (C1) and 1/75 (1.4%) was probably benign (C3), subsequently confirmed histologically. The remaining 39/75 (52%) patients were positive (C4 or C5), in detail: 32/75 were C5 and 7/75 were C4. All these patients underwent surgery, and only one (initially diagnosed as C4) resulted negative on histology (Figure 3).

By comparing the two groups, we observed no statistically significant differences in terms of distribution of the diagnostic categories or agreement between cytological and histological diagnoses of potentially malignant lesions (Table 3).

4 | DISCUSSION

FNAC is an essential tool for breast cancer diagnosis: its availability, rapidity, cost-effectiveness and low associated risks are the main strengths of this procedure.

Generally speaking, air-dried slides offer optimal definition of cytoplasmic and nuclear features in terms of quality, clear evidence of nuclear shape and dimension, providing useful details for a definite diagnosis of malignancy.¹⁸ This depends on the distention of cells on smears unopposed by the immediate alcohol fixation. In many challenging cases, comparing the morphological features provided by air-dried and alcohol-fixed specimens could be of paramount importance in establishing the diagnosis (Figure 4).

However, the extraordinary COVID-19 emergency forced us to rethink the organisation and practices of FNAC considering the new World Health Organisation laboratory biosafety guidelines.¹⁰ The preparation of fixed smears could be probably safer lowering the potential risk of operator contamination with infectious

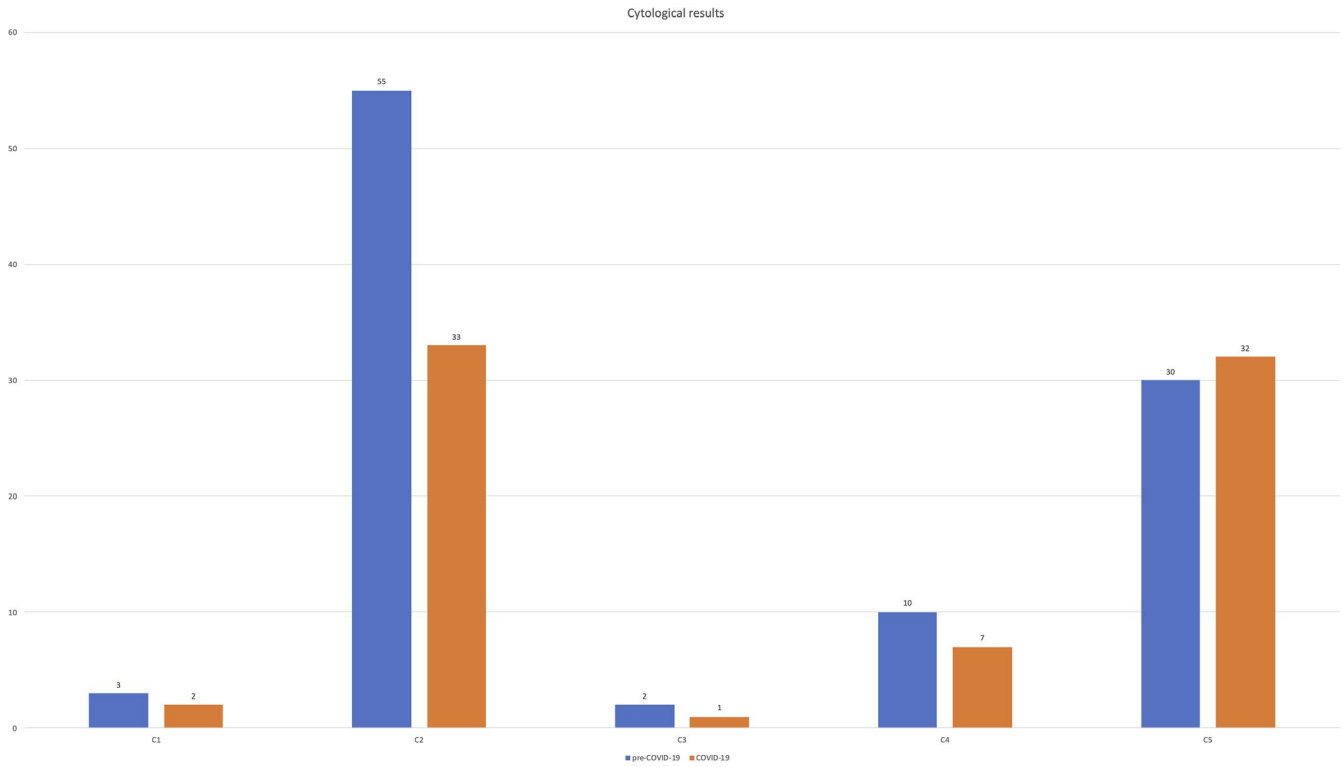


FIGURE 3 Distribution of C categories in pre-COVID and COVID periods

TABLE 3 Comparison between fine needle aspiration cytology (FNAC) and histopathological final surgical results

Histology				
FNAC	Benign	Carcinoma	Total	
A). Pre-COVID 19 period				
C4	1	9	10	Observed agreement = 97.5% (39/40) Diagnostic overestimation rate: 2.5%
C5	0	30	30	
Total	1	39	40	
B). COVID 19 period				
C4	1	6	7	Observed agreement = 97.4% (38/39) Diagnostic overestimation rate: 2.5%
C5	0	32	32	
Total	1	36	39	

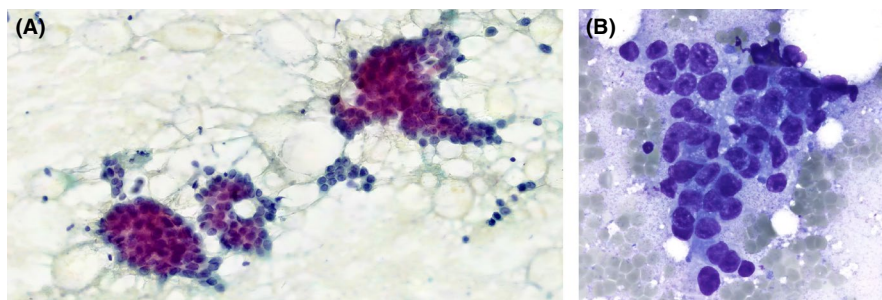


FIGURE 4 Details of monomorphic large cell population in three-dimensional clusters with pleomorphic nuclei and prominent nucleoli offered by air-dried slides and useful for a definite diagnosis of malignancy (A: Papanicolaou stain, original magnification 20x; B: May-Grünwald Giemsa stain, original magnification 40x)

material. The aim of our work was to show the preliminary results of FNAC performed using an exclusively alcohol-based protocol in comparison to the traditional one based on the preparation of air-dried slides.

Our results showed no significant difference between the two procedures. Specifically, we found no differences in the number of diagnoses classified as C1 and quality or quantity of cells. Importantly, for lesions suggestive of malignancy (C4 and C5), the concordance between cytological and histological results was excellent in both protocols.

Therefore, at least in our initial experience, these results suggested the reliability of alcohol-based procedures in terms of diagnosis and safeness.

Moreover, the overall number of breast FNAC procedures during the COVID-19 period was slightly lower compared to that of the pre-COVID-19 period (75 vs 100, respectively), and this was clearly related to the restrictions imposed by the Italian Government. In fact, the percentage of malignant results was higher during the COVID-19 period than that in the pre-COVID-19 period (52% vs 40%, respectively). Such restrictions ended in decreasing number of diagnostic procedures for both screening and follow-up programmes, favouring those dedicated to symptomatic patients.

A still safer opportunity is given by liquid-based cytology. In this case, the specimen is directly collected in the fixative, which is warranted as it inactivates the virus and is processed in a closed system. Furthermore, centrifugation of aspirates allows cell blocks to be obtained, which can be submitted to histological evaluation and also immunohistochemical studies.

This is the only procedure we still use for head and neck and lung specimens. The limitation is related to the need of having the instruments and experience in interpreting the slides.

5 | CONCLUSIONS

Given the risks associated with air-dried slide production, our results showed that this new protocol provided safe FNAC procedures during COVID-19 pandemic without compromising diagnostic conclusions.

Emergency management and infection-control measures performed with FNAC in our hospital protected both patients and operators, making this experience useful for other departments dealing with pandemic.

CONFLICT OF INTEREST

The authors declare that there is no conflict of interest.

AUTHOR CONTRIBUTIONS

Conceptualisation: Nicosia L. and Cassano E. Methodology: Bozzini A., Latronico A., Meneghetti L. and Casadio C. Investigation: Montesano M., Di Tonno C. and Midolo V. Formal analysis: Mauri G. and De Fiori E. Data curation: Nicosia L., Addante F. and Mastropasqua M.G. Software: Montesano M. Validation: Mastropasqua M.G.,

Casadio C. and Cassano E. Resources: Montesano M., De Fiori E. and Cassano E. Original draft preparation: Nicosia L. and Cassano E. Writing, review and editing: Addante F., Mastropasqua M.G. and Casadio C. Supervision: Casadio C. and Cassano E. All authors have read and agreed to the published version of the manuscript.

ETHICAL APPROVAL

Approval by the Ethics Committee was obtained for this retrospective study.

PATIENT CONSENT

Patients' informed consent was obtained for this retrospective study.

DATA AVAILABILITY STATEMENT

Data sharing is not applicable to this article as no new data were created or analysed in this study.

ORCID

Mauro Giuseppe Mastropasqua  <https://orcid.org/0000-0002-8306-0839>

REFERENCES

- Zajicek J, Franzén S, Jakobsson P, Rubio C, Unsgaard B. Aspiration biopsy of mammary tumors in diagnosis and research—a critical review of 2,200 cases. *Acta Cytol.* 1967;11(3):169-175.
- Masood S. *Cytopathology of the breast. ASCP theory and practice of cytopathology.* Chicago, IL: ASCP Press; 1996.
- Chauhan V, Pujani M, Agarwal C, et al. IAC standardized reporting of breast fine-needle aspiration cytology, Yokohama 2016: a critical appraisal over a 2 year period. *Breast Dis.* 2019;38(3-4):109-115.
- Sheikh FA, Tinkoff GH, Kline TS, Neal HS. Final diagnosis by fine-needle aspiration biopsy for definitive operation in breast cancer. *Am J Surg.* 1987;154(5):470-474.
- Berner A, Davidson B, Sigstad E, Risberg B. Fine-needle aspiration cytology vs. core biopsy in the diagnosis of breast lesions. *Diagn Cytopathol.* 2003;29(6):344-348.
- Kocjan G, Chandra A, Cross P, et al. BSCC Code of practice—fine needle aspiration cytology. *Cytopathology.* 2009;20(5):283-296.
- Tuite AR, Ng V, Rees E, Fisman D. Estimation of COVID-19 outbreak size in Italy. *Lancet Infect Dis.* 2020;20(5):537.
- Livingston E, Bucher K. Coronavirus Disease 2019 (COVID-19) in Italy. *JAMA.* 2020;323(14):1335.
- Centers for Disease Control and Prevention. Laboratory biosafety guidelines for handling and processing specimens associated with SARS-CoV. <https://www.cdc.gov/sars/guidance/f-lab/app5.html>
- World Health Organization. Laboratory biosafety guidance related to the novel coronavirus (2019-nCoV). Interim guidance. https://www.who.int/docs/default-source/coronaviruse/laboratory-biosafety-novel-coronavirus-version-1-1.pdf?sfvrsn=Z912a9847_2
- Barbareschi M, Ascoli V, Bonoldi E, et al. Biosafety in surgical pathology in the era of SARS-Cov2 pandemia. A statement of the Italian Society of Surgical Pathology and Cytology. *Pathologica.* 2020;112(2):59-63.
- Otter JA, Donskey C, Yezli S, Douthwaite S, Goldenberg SD, Weber DJ. Transmission of SARS and MERS coronaviruses and influenza virus in healthcare settings: the possible role of dry surface contamination. *J Hosp Infect.* 2016;92(3):235-250.
- van Doremalen N, Bushmaker T, Morris DH, et al. Aerosol and surface stability of SARS-CoV-2 as compared with SARS-CoV-1. *N Engl J Med.* 2020;382(16):1564-1567.

14. Kratzel A, Todt D, V'kovski P, et al. Inactivation of Severe acute respiratory syndrome coronavirus 2 by WHO-recommended hand rub formulations and alcohols. *Emerg Infect Dis*. 2020;26(7):1592-1595.
15. Hulkower RL, Casanova LM, Rutala WA, Weber DJ, Sobsey MD. Inactivation of surrogate coronaviruses on hard surfaces by health care germicides. *Am J Infect Control*. 2011;39(5):401-407.
16. D'Orsi CJ, Sickles EA, Mendelson EB, et al. *ACR BI-RADS® Atlas, Breast Imaging Reporting and Data System*. Reston, VA: American College of Radiology; 2013.
17. Perry N, Broeders M, de Wolf C, Tornberg S, Holland R, von Karsa L. *European Guidelines for quality assurance in breast cancer screening and diagnosis*, 4th edn. Luxembourg: Office for Official Publications of the European Communities; 2006.
18. Fulciniti F, Frangella C, Staiano M, et al. Air-dried smears for optimal diagnostic immunocytochemistry. *Acta Cytol*. 2008;52(2):178-186.

How to cite this article: Nicosia L, Bozzini AC, Latronico A, et al. COVID-19 and breast fine needle aspiration cytology method: What should we change?. *Cytopathology*. 2021;32:312–317. <https://doi.org/10.1111/cyt.12959>