

Comparative Effectiveness of 3-Dimensional vs 2-Dimensional and High-Definition vs Standard-Definition Neuroendoscopy: A Preclinical Randomized Crossover Study

Hani J. Marcus, MRCS*‡
 Archie Hughes-Hallett, MRCS‡
 Thomas P. Cundy, MBBS‡
 Aimee Di Marco, MRCS‡
 Philip Pratt, PhD‡
 Dipankar Nandi, DPhil*
 Ara Darzi, FRS‡
 Guang-Zhong Yang, FEng‡

*Department of Neurosurgery, Imperial College Healthcare NHS Trust, London, United Kingdom; ‡The Hamlyn Centre, Institute of Global Health Innovation, Imperial College London, London, United Kingdom

Correspondence:

Hani J. Marcus, MRCS,
 Clinical Research Fellow and
 Specialty Registrar in Neurosurgery,
 Imperial College London and
 Imperial College Healthcare NHS Trust,
 Hamlyn Centre,
 Paterson Bldg (Level 3),
 Praed Street,
 London W2 1NY, UK.
 E-mail: hani.marcus10@imperial.ac.uk

Received, August 29, 2013.

Accepted, November 1, 2013.

Published Online, November 11, 2013.

Copyright © 2013 by the Congress of Neurological Surgeons. This is an open-access article distributed under the terms of the Creative Commons Attribution-NonCommercial-NoDerivatives 3.0 License, where it is permissible to download and share the work provided it is properly cited. The work cannot be changed in any way or used commercially.

BACKGROUND: Although the potential benefits of 3-dimensional (3-D) vs 2-dimensional (2-D) and high-definition (HD) vs standard-definition (SD) endoscopic visualization have long been recognized in other surgical fields, such endoscopes are generally considered too large and bulky for use within the brain. The recent development of 3-D and HD neuroendoscopes may therefore herald improved depth perception, better appreciation of anatomic details, and improved overall surgical performance.

OBJECTIVE: To compare simultaneously the effectiveness of 3-D vs 2-D and HD vs SD neuroendoscopy.

METHODS: Ten novice neuroendoscopic surgeons were recruited from a university hospital. A preclinical randomized crossover study design was adopted to compare 3-D vs 2-D and HD vs SD neuroendoscopy. The primary outcomes were time to task completion and accuracy. The secondary outcomes were perceived task workload using the NASA (National Aeronautics and Space Administration) Task Load Index and subjective impressions of the endoscopes using a 5-point Likert scale.

RESULTS: Time to task completion was significantly shorter when using the 3-D vs the 2-D neuroendoscopy ($P = .001$), and accuracy of probe placement was significantly greater when using the HD vs the SD neuroendoscopy ($P = .009$). We found that 3-D endoscopy significantly improved perceived depth perception ($P < .001$), HD endoscopy significantly improved perceived image quality ($P < .001$), and both improved participants' overall impression ($P < .001$).

CONCLUSION: Three-dimensional neuroendoscopy and HD neuroendoscopy have differing but complementary effects on surgical performance, suggesting that neither alone can completely compensate for the lack of the other. There is therefore strong preclinical evidence to justify 3-D HD neuroendoscopy.

KEY WORDS: Endoscopy, HD, High definition, Minimally invasive neurosurgery, 3D, 3-dimensional

Neurosurgery 74:375–381, 2014

DOI: 10.1227/NEU.0000000000000249

www.neurosurgery-online.com

Endoscopes and endoscope-assisted approaches have been used within the field of neurosurgery since the work of pioneers such as Walter Dandy almost a century ago.¹ Although the potential benefits of 3-dimensional (3-D) vs 2-dimensional (2-D) and high-definition (HD) vs standard-definition (SD) endoscopic visualization have long been recognized in other

surgical fields, such endoscopes are generally considered too large and bulky for use in the brain.^{2–6} The recent development of 3-D and HD neuroendoscopes may therefore bring improved depth perception, better appreciation of anatomic details, and improved surgical performance compared with conventional neuroendoscopy.^{7–10} These benefits must be balanced, however, against the higher cost, larger size, and greater weight of HD endoscopes. Moreover, the human visual system is exquisitely sensitive to stereoscopic cues, and although stereo fusion can tolerate quite major

ABBREVIATIONS: HD, high definition; SD, standard definition

artifacts, symptoms such as diplopia and nausea have been described with prolonged use of 3-D endoscopy systems.¹¹

Previous studies have sought to assess the impact of either 3-D or HD neuroendoscopy on surgical performance, with mixed findings.^{7-9,11-15} A major limitation of all these studies is that they do not allow comparison of the effectiveness of 3-D and HD neuroendoscopy. It remains unclear whether, for example, HD neuroendoscopy provides sufficient monocular cues to obviate the need for true 3-D endoscopy. The aim of this study was therefore to compare simultaneously the effectiveness of 3-D vs 2-D and HD vs SD neuroendoscopy.

PATIENTS AND METHODS

The trial protocol was approved by the Imperial College Joint Research Compliance Office. The Consolidated Standards of Reporting Trials statement was used in the preparation of this manuscript.

Participants and Study Settings

Ten novice neuroendoscopic surgeons were recruited from a university hospital. Participants were deemed suitable for inclusion if they had no earlier experience with endoscopic or endoscope-assisted neurosurgery (performed zero). Informed consent was obtained from all participants.

Trial Design

A preclinical randomized crossover study design was adopted comparing 3-D against 2-D and HD against SD neuroendoscopy.

A Sawbones skull and brain (Pacific Research Laboratories, Inc, Vashon Island, Washington) with an accompanying circle of Willis including an anterior communicating artery aneurysm was used. A 25 × 15-mm left supraorbital craniotomy was fashioned, and 5 colored targets were placed around the surgical field approximately 30 mm in diameter and 30 to 60 mm in depth.

A VisionSense III neuroendoscopy system (VisionSense, Petach Tikva, Israel) was used for visualization. The SD 0° rigid VisionSense endoscope was 4.9 mm in diameter and 20 cm in length, providing a resolution of 640 × 480 pixels. The HD 0° rigid VisionSense endoscope was 4 mm in diameter and 18 cm in length, providing a resolution of 1920 × 1200 pixels. Images were displayed using a 24-in stereoscopic flat-screen system and switched between 3-D and 2-D (left eye) using the system's toggle.

Participants were randomly allocated using a computer-generated sequence into groups to determine the order in which 2-D SD, 3-D SD, 2-D HD, or 3-D HD neuroendoscopy was used. Blocked randomization was used to ensure that an equal number of participants began with 3-D vs 2-D and HD vs SD neuroendoscopy.

Each participant was asked to place a probe on targets in a predetermined random sequence of 10 colors (see Figure 1). Participants were instructed to be both quick and accurate, placing the probe as close to the center of the colored targets as possible. This process was repeated on 3 occasions with each endoscope configuration.

Outcomes

The primary outcomes were time to task completion (seconds) and accuracy with which probes were placed on targets (score). To determine accuracy, all recorded videos were reviewed and scored independently by 2 observers (H.J.M. and A.H.H.) on how closely each probe was to the center of the colored targets; participants were scored 3 points if they directly made contact

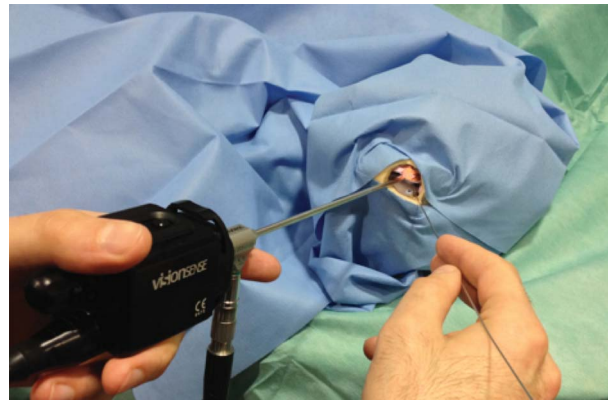


FIGURE 1. Photograph illustrating the experimental setup, with the neuroendoscope (left hand) used to guide the probe (right hand) to colored targets through a left supraorbital keyhole craniotomy (draped with only surgical field exposed).

with the 1-mm colored target, 2 points if they made contact with the surrounding 1-mm black line, 1 point if they made contact with the surrounding 2-mm white line, and zero points if they missed the target entirely (see Figure 2). Whereas participants were aware of the endoscope they were using, the data analysts were partially blinded to the allocation (to 3-D vs 2-D but not HD vs SD).

The secondary outcomes were perceived task workload using the NASA (National Aeronautics and Space Administration) Task Load Index¹⁶ and subjective impressions of the endoscopes using a 5-point Likert scale. Participants were asked after using each endoscope to what extent they considered the system provided high-quality images, if it allowed high-fidelity depth perception, and if they would like to use the visualization modality again.

Statistical Analysis

The sample size was calculated on the basis of recently published work.¹⁷ We estimated that to detect a reduction in time to task

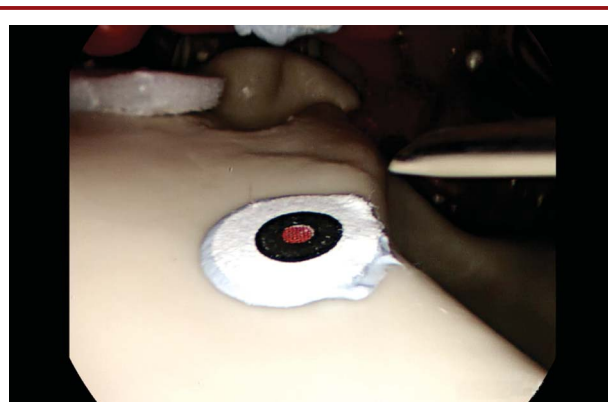


FIGURE 2. Endoscope image illustrating a typical target. Participants were scored 3 points if they contacted the 1-mm colored target, 2 points if they made contact with the surrounding 1-mm black line, 1 point if they made contact with the surrounding 2-mm white line, and zero points if they missed the target entirely.

TABLE 1. Demographics of Participants

Sex, male:female	7:3
Age, median (range), y	29.5 (25-43)
Handedness, R:L	8:2

completion from 90 to 66 seconds (standard deviation, 30 seconds), with a 2-sided 5% significance level and a power of 80%, a sample size of 10 participants was necessary.

Data were analyzed with SPSS version 20.0 (Chicago, Illinois). The Cronbach α was used to assess the interrater reliability of accuracy scores. The medians and interquartile ranges were calculated for all outcome measures and nonparametric tests performed, with a value of $P < .05$ considered statistically significant. We compared 2-D SD, 3-D SD, 2-D HD, and 3-D HD neuroendoscopy using the Kruskal-Wallis 1-way analysis of variance. Subsequently, if a significant difference was identified, the Mann-Whitney U test was used to compare 3-D vs 2-D and HD vs SD neuroendoscopy with the Bonferroni correction. We also performed a post hoc analysis comparing the data from the 2 novice neuroendoscopic surgeons with extensive laparoscopic experience against the other participants to determine whether there was a significant difference in performance.

RESULTS

Baseline Demographic Data

The demographics of the 10 participants are summarized in Table 1. All participants completed the study, and no losses occurred after randomization. Two of the subjects had considerable experience with laparoscopic surgery (performed > 50 cases) but had no experience with neuroendoscopy and thus were included. Post hoc analysis confirmed no significant difference in performance.

Primary Outcomes

The Cronbach α demonstrated excellent interrater reliability when scoring the accuracy of probe placement ($\alpha = 0.925$). The medians and interquartile ranges of the primary outcomes are summarized in Table 2. The time to task completion and

accuracy of probe placement with different neuroendoscopes were significantly different ($P = .005$ and $P = 0.021$, respectively); they are illustrated in Figures 3 and 4.

The medians and interquartile ranges of the primary outcome data stratified according to 3-D vs 2-D and HD vs SD neuroendoscopy are summarized in Tables 3 and 4, respectively. Post hoc statistical analysis suggested that time to completion was significantly shorter when using 3-D vs 2-D neuroendoscopy ($P = .001$) and that the accuracy of probe placement was significantly greater when using HD vs SD neuroendoscopy ($P = .009$).

Secondary Outcomes

The medians and interquartile ranges of the secondary outcome data are summarized in Table 2. The subjective impressions of the endoscopes using a 5-point Likert scale varied significantly ($P < .001$), but the perceived task workload according to the Task Load Index did not reach statistical significance ($P = 0.161$).

The medians and interquartile ranges of the secondary outcome data stratified according to 3-D vs 2-D and HD vs SD neuroendoscopy are summarized in Tables 2 and 3, respectively. Post hoc statistical analysis suggested that 3-D neuroendoscopy significantly improved perceived depth perception ($P < .001$), HD neuroendoscopy significantly improved perceived image quality ($P < .001$), and both improved the overall likelihood that participants would use the modality again ($P < .001$). Because the Kruskal-Wallis analysis failed to demonstrate a significant difference in the cognitive workload with different endoscopes, no further analysis was performed.

DISCUSSION

The advantages of 3-D and HD endoscopy have been demonstrated in other surgical fields, but until recently, the large sizes of such endoscopes restricted their use in the brain.²⁻⁶ This preclinical randomized crossover study is the first to compare simultaneously the effectiveness of 3-D vs 2-D and HD vs SD neuroendoscopy. Interestingly, the effects of 3-D and HD neuroendoscopy appear to be distinct and complementary; the use of 3-D vs 2-D neuroendoscopy led to a significant reduction

TABLE 2. Summary of Results According to Neuroendoscope Used^a

	2-D SD	3-D SD	2-D HD	3-D HD	P
Time, s ^b	69.5 (59.3-80.5)	53.5 (42.0-73.5)	58.5 (50.0-84)	51 (43.3-65.8)	.005 ^b
Accuracy ^b	14.5 (12.1-17.1)	15.3 (14.0-18.5)	16.3 (14.1-20.5)	18.0 (14.9-23.0)	0.021 ^b
NASA-TLX	42.9 (36.4-62.0)	32.0 (26.5-43.3)	35.0 (29.1-52.8)	26.8 (22.4-37.9)	0.161
Likert scale					
Quality ^b	2.0 (1.3-2.0)	3.0 (2.3-4.0)	4.0 (4.0-5.0)	5.0 (5.0-5.0)	<.001 ^b
Depth ^b	2.0 (2.0-2.0)	4.0 (4.0-4.0)	3.0 (2.3-3.0)	4.0 (4.0-5.0)	<.001 ^b
Overall ^b	2.5 (2.0-3.0)	3.0 (3.0-4.0)	4.0 (3.3-4.0)	5.0 (5.0-5.0)	<.001 ^b

^aHD, high definition; NASA-TLX, National Aeronautics and Space Administration Task Load Index; SD, standard definition; 2-D, 2-dimensional; 3-D, 3-dimensional.

^bLikert scale: 5 = high quality, excellent depth perception, and overall would use again; 1 = low quality, poor depth perception, and overall would not use again. Values are median (interquartile range) reported.

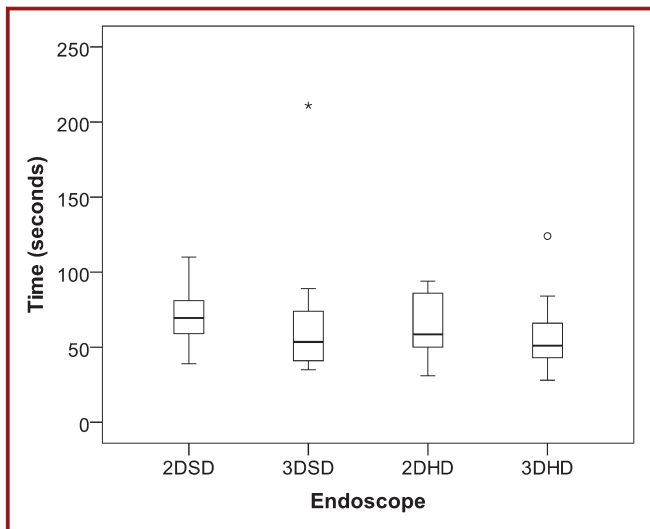


FIGURE 3. Graph illustrating the time to completion with different neuroendoscopes. Points represent outliers (circle greater than 1.5 times the IQR; star greater than 3 times the IQR). HD, high definition; SD, standard definition; 2D, 2-dimensional; 3D, 3-dimensional.

in the time to task completion and a subjective improvement in depth perception, whereas the use of HD vs SD neuroendoscopy led to a significant increase in the accuracy of probe placement and a subjective improvement in image quality.

Although no previous studies have addressed the influence of both 3-D and HD neuroendoscopy, similar studies have assessed their impact individually with varying results. Fraser et al⁸ used the VisionSense II system to compare 3-D and 2-D neuroendoscopy

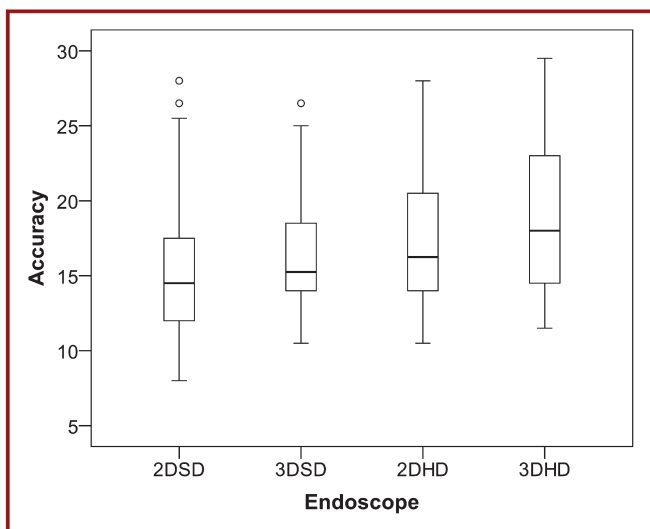


FIGURE 4. Graph illustrating the accuracy of probe placement with different neuroendoscopes. Points represent outliers (circle greater than 1.5 times the IQR). HD, high definition; SD, standard definition; 2D, 2-dimensional; 3D, 3-dimensional.

TABLE 3. Summary of Results Stratified Into 3- vs 2-Dimensional^a

	2-D (2-D SD and 2-D HD)	3-D (3-D SD and 3-D HD)	P
Time, s	67.5 (52.0-81.3)	52.0 (42.5-68.3)	.001 ^b
Accuracy	15.5 (12.9-19.4)	17.0 (14.0-21.3)	0.085
NASA-TLX	39.7 (31.2-53.4)	28.9 (24.2-43.3)	NA
Likert scale			
Quality	3.5 (2.0-4.0)	4.0 (3.0-5.0)	0.460
Depth	2.0 (2.0-3.0)	4.0 (4.0-4.0)	<.001 ^b
Overall	3.0 (2.8-4.0)	4.0 (4.0-5.0)	.001 ^b

^aHD, high definition; NASA-TLX, National Aeronautics and Space Administration Task Load Index; SD, standard definition; 2-D, 2-dimensional; 3-D, 3-dimensional.
^bLikert scale: 5 = high quality, excellent depth perception, and overall would use again; 1 = low quality, poor depth perception, and overall would not use again. Values are median (interquartile range).

in a model simulating the transnasal transsphenoidal approach to the pituitary. In all, 33 participants with varying levels of experience were asked to use a rongeur to remove the sellar floor and then take 4 small pituitary biopsies. Although 3-D neuroendoscopy resulted in improved cutting efficiency ($P = .04$) and was subjectively the user preference, it was not associated with a significant difference in other primary outcomes such as time to completion or error rates. Thus far, only limited clinical studies have directly compared 3-D and 2-D neuroendoscopy, and most have failed to demonstrate any significant differences.^{11,15} In a recent retrospective cohort study, Barkhoudarian et al¹⁸ analyzed 160 transnasal transsphenoidal procedures, of which 65 were performed with a 3-D neuroendoscope and 95 with a 2-D neuroendoscope. Although there was no significant difference in overall operating time, within the disease-specific comparison, pituitary adenoma resection was shorter with 3-D vs 2-D neuroendoscopy (174 vs 147 minutes; $P = .03$); there was no difference in the rate of gross total resection or complications.

TABLE 4. Summary of Results Stratified Into Standard Definition vs High Definition^a

	SD (2-D SD and 3-D SD)	HD (2-D HD and 3-D HD)	P
Time, s	63.0 (49.0-76.5)	54.0 (45.8-69.5)	0.110
Accuracy	14.8 (13.0-18.1)	17.5 (14.5-22.6)	.009 ^b
NASA-TLX	39.7 (27.5-47.8)	31.5 (22.6-45.5)	NA
Likert scale			
Quality	2.0 (2.0-3.0)	5.0 (4.0-5.0)	<.001 ^b
Depth	3.0 (2.0-4.0)	4.0 (3.0-4.3)	0.060
Overall	3.0 (2.8-4.0)	4.0 (4.0-5.0)	<.001 ^b

^aHD, high definition; NASA-TLX, National Aeronautics and Space Administration Task Load Index; SD, standard definition; 2-D, 2-dimensional; 3-D, 3-dimensional.
^bLikert scale: 5 = high quality, excellent depth perception, and overall would use again; 1 = low quality, poor depth perception, and overall would not use again. Values are median (interquartile range).

Studies have also assessed the impact of HD vs SD neuroendoscopy on surgical performance. Schroeder and Nehlsen⁷ reported higher image resolution and color fidelity with HD neuroendoscopy, particularly when discriminating tumor from neighboring tissue during transnasal transsphenoidal approaches. Conrad et al⁹ captured a series of images during endoscopic approaches and found significantly improved recognition of anatomic landmarks by surgeons when using HD vs SD cameras (84.4% vs 63.0%; $P = .01$). The clinical significance of HD visualization has not yet been ascertained, although it is commonly assumed.

The major limitation of all the above studies is that they address the effects of either 3-D or HD neuroendoscopy, rather than both, making it difficult to tease apart their relative importance and the extent to which each can compensate for the other. It is well recognized, for example, that a number of monocular cues can contribute to depth perception such as motion parallax, the kinetic depth effect, and pictorial cues (eg, size, perspective, texture, interposition, lighting, and shadow).¹⁹⁻²³ It has been suggested that HD endoscopy, by allowing improved recognition of these monocular cues, might obviate the need for stereoscopy.²⁴ The present study provides firm evidence that although 3-D and HD neuroendoscopy individually improve surgical performance, they do so in different ways, and neither can fully compensate for the lack of the other.

Limitations

It should be noted that this study has a number of limitations. First, although all participants were novices in neuroendoscopy, 2 had substantial experience in laparoscopic surgery. Post hoc analysis failed to demonstrate a significant difference between these 2 surgeons and the remaining participants, but it remains likely that this influenced their performance (albeit with a trend toward reduced time to task completion and improved accuracy of probe placement). Second, although the task was based on similar externally validated measures of surgical performance, it has not itself been validated.²⁵ Moreover, the duration of the task may not have been long enough for participants to experience symptoms such as diplopia and nausea that have been described with prolonged use of 3-D endoscopy. Third, although the use of 3-D neuroendoscopes that were toggled to 2-D, rather than dedicated 2-D neuroendoscopes, allowed control of the video capture and display hardware, it might have led to a somewhat lower image quality. Finally, an inherent limitation of the methodology was that video was captured with the endoscope being assessed and the accuracy of probe placement was therefore only partially blinded, with researchers able to distinguish HD vs SD but not 3-D vs 2-D. Unfortunately, the small size of the keyhole supraorbital craniotomy made it difficult to place a further endoscope or camera without obstructing access.

Generalizability

Clearly, the generalizability of these findings is likely to depend on several factors. In this study, only novice neuroendoscopists were

included, in part because of the difficulty in recruiting sufficient numbers of experienced neurosurgeons (particularly because the sample size would have to be substantially larger to detect a presumably smaller effect on performance). The general surgical literature suggests that the influence of 3-D vs 2-D endoscopy on surgical performance is reduced or negated with experience as surgeons learn to use monocular cues to judge distance.²⁶ The relative influence of 3-D and HD neuroendoscopy is also likely to vary depending on the nature of the surgical task performed. We speculate that complex procedures such as neurovascular dissection would be far more influenced by the nature of the endoscope used than relatively straightforward procedures.

CONCLUSION

The results of this study may have considerable implications on endoscopic and endoscope-assisted neurosurgical approaches. Importantly, the fact that 3-D vs 2-D and HD vs SD neuroendoscopy had differing but complementary effects suggests that neither 3-D nor HD alone can completely compensate for the lack of the other. There is therefore strong preclinical evidence for the development and use of next-generation 3-D HD neuroendoscopes, particularly for inexperienced surgeons or when complex surgery is performed. Further studies are merited to confirm that no side effects or adverse reactions occur with prolonged use and that these findings are translated into improved surgical performance in a clinical setting.

Disclosures

Dr Marcus is supported by an Imperial College Wellcome Trust Clinical Fellowship. The authors have no personal, financial, or institutional interest in any of the drugs, materials, or devices described in this article.

REFERENCES

1. Hsu W, Li KW, Bookland M, Jallo GI. Keyhole to the brain: Walter Dandy and neuroendoscopy. *J Neurosurg Pediatr.* 2009;3(5):439-442.
2. Buess GF, van Bergen P, Kunert W, Schurr MO. Comparative study of various 2-D and 3-D vision systems in minimally invasive surgery [in German]. *Chirurg.* 1996;67(10):1041-1046.
3. LaGrange CA, Clark CJ, Gerber EW, Strup SE. Evaluation of three laparoscopic modalities: robotics versus three-dimensional vision laparoscopy versus standard laparoscopy. *J Endourol.* 2008;22(3):511-516.
4. Taffinder N, Smith SG, Huber J, Russell RC, Darzi A. The effect of a second-generation 3D endoscope on the laparoscopic precision of novices and experienced surgeons. *Surg Endosc.* 1999;13(11):1087-1092.
5. Kong SH, Oh BM, Yoon H, et al. Comparison of two- and three-dimensional camera systems in laparoscopic performance: a novel 3D system with one camera. *Surg Endosc.* 2010;24(5):1132-1143.
6. Blavier A, Gaudissart Q, Cadiere GB, Nyssen AS. Impact of 2D and 3D vision on performance of novice subjects using da Vinci robotic system. *Acta Chir Belg.* 2006;106(6):662-664.
7. Schroeder HW, Nehlsen M. Value of high-definition imaging in neuroendoscopy. *Neurosurg Rev.* 2009;32(3):303-308; discussion 308.
8. Fraser JF, Allen B, Anand VK, Schwartz TH. Three-dimensional neurostereoscopy: subjective and objective comparison to 2D. *Minim Invasive Neurosurg.* 2009;52(1):25-31.
9. Conrad J, Philipps M, Oertel J. High-definition imaging in endoscopic transsphenoidal pituitary surgery. *Am J Rhinol Allergy.* 2011;25(1):e13-e17.

10. Marcus HJ, Seneci CA, Payne CJ, Nandi D, Darzi A, Yang GZ. Robotics in keyhole transcranial endoscope-assisted microsurgery: a critical review of existing systems and proposed specifications for new robotic platforms [published August 5, 2013]. *Neurosurgery*. doi:10.1227/NEU.000000000000123.
11. Tabaei A, Anand VK, Fraser JF, Brown SM, Singh A, Schwartz TH. Three-dimensional endoscopic pituitary surgery. *Neurosurgery*. 2009;64(5 suppl 2):288-293; discussion 294-295.
12. Roth J, Fraser JF, Singh A, Bernardo A, Anand VK, Schwartz TH. Surgical approaches to the orbital apex: comparison of endoscopic endonasal and transcranial approaches using a novel 3D endoscope. *Orbit*. 2011;30(1):43-48.
13. Roth J, Singh A, Nyquist G, et al. Three-dimensional and 2-dimensional endoscopic exposure of midline cranial base targets using expanded endonasal and transcranial approaches. *Neurosurgery*. 2009;65(6):1116-1128; discussion 1128-1130.
14. Castelnovo P, Battaglia P, Bignami M, et al. Endoscopic transnasal resection of anterior skull base malignancy with a novel 3D endoscope and neuronavigation. *Acta Otorhinolaryngol Ital*. 2012;32(3):189-191.
15. Kari E, Oyesiku NM, Dadashev V, Wise SK. Comparison of traditional 2-dimensional endoscopic pituitary surgery with new 3-dimensional endoscopic technology: intraoperative and early postoperative factors. *Int Forum Allergy Rhinol*. 2012;2(1):2-8.
16. Hart SG, Staveland LE. Development of NASA-TLX (Task Load Index): results of empirical and theoretical research. In: Peter AH, Najmedin M, eds. *Advances in Psychology*. Vol 52. Amsterdam, the Netherlands: North-Holland; 1988:139-183.
17. Storz P, Buess GF, Kunert W, Kirschniak A. 3D HD versus 2D HD: surgical task efficiency in standardised phantom tasks. *Surg Endosc*. 2012;26(5):1454-1460.
18. Barkhoudarian G, Romero AD, Laws ER. Evaluation of the three-dimensional endoscope in transphenoidal surgery. *Neurosurgery*. 2013;73(1 suppl Operative):ons74-ons78; discussion ons78-ons79.
19. Steele KM, Brigner WL, Adkins A. Perceived depth from simultaneous changes in length and direction of a single line. *Percept Mot Skills*. 1995;80(2):579-584.
20. Mather G, Smith DR. Depth cue integration: stereopsis and image blur. *Vision Res*. 2000;40(25):3501-3506.
21. O'Shea RP, Blackburn SG, Ono H. Contrast as a depth cue. *Vision Res*. 1994;34(12):1595-1604.
22. Rogers B. Motion parallax as an independent cue for depth perception: a retrospective. *Perception*. 2009;38(6):907-911.
23. Voorhorst FA, Overbeeke KJ, Smets GJ. Using movement parallax for 3D laparoscopy. *Med Prog Through Technol*. 1996;21(4):211-218.
24. van Bergen P, Kunert W, Buess GF. The effect of high-definition imaging on surgical task efficiency in minimally invasive surgery: an experimental comparison between three-dimensional imaging and direct vision through a stereoscopic TEM rectoscope. *Surg Endosc*. 2000;14(1):71-74.
25. Derossis AM, Fried GM, Abrahamowicz M, Sigman HH, Barkun JS, Meakins JL. Development of a model for training and evaluation of laparoscopic skills. *Am J Surg*. 1998;175(6):482-487.
26. Shah J, Buckley D, Frisby J, Darzi A. Depth cue reliance in surgeons and medical students. *Surg Endosc*. 2003;17(9):1472-1474.

COMMENTS

The authors should be congratulated for this important study. 3-Dimensional (3-D) endoscopy will certainly become more important in endoscopy and endoscopic neurosurgery. Most promising here is indeed the VisionSense principle¹ with “chip in the tip” using bee’s eye technology (“compound eye”) and with LED illumination (avoiding the heat of xenon light²), which is now also available in full high-definition (HD) resolution (VisionSense III, “a single sensor divided into hundreds of thousands of tiny eyes”). This scope now has even a decreased outer diameter of <4 mm (actual, 3.3 mm). It corresponds to a rigid HOPKINS scope required for effective 3-D imaging (should also not be below 3.5 mm in diameter; otherwise, the available 3-D minicameras will not provide an adequate resolution and brightness).

This study is of special interest and value because it is a randomized crossover study in which 10 novice neurosurgeons without neuroendoscopic experience performed endoscopic surgery in an anatomic

model with a supraorbital craniotomy (2 participants had experience with laparoscopy). The randomization was quite complex and skillful; blocked randomization ensured that equal numbers of participants started with 3-D vs 2-dimensional (2-D) and HD vs standard-definition (SD) endoscopy.

As could be expected (but was not yet demonstrated in such a statistical setup), the accuracy of the task performed (probe placement) was significantly better with HD vs SD endoscopy. More interesting is the result that time to completion was significantly shorter with 3-D vs 2-D endoscopic imaging; without longer training in 3-D endoscopy, one would expect a steeper learning curve with a 3-D screen. This result shows the advanced performance of the VisionSense III system. The task work loading was not different, and the overall likelihood of the participants was greatest when 3-D neuroendoscopy was combined with HD resolution. In a clinical pilot study,¹ which is not cited by the authors, otolaryngologists found a better depth perception and orientation and an improved completeness of surgery in sinonasal surgery comparing 2-D conventional endoscopy with an earlier version of the VisionSense 3D system.

The authors also provide an adequate, restrictive Discussion, pointing to the limitations of the study regarding the short duration of the task, which would not exclude the occurrence of discomfort with prolonged 3-D endoscopy like diplopia and nausea. The conclusion that neither 3-D nor HD alone can compensate for the lack of the other is convincing; therefore, we should encourage the industry to provide fully autoclavable 3-D HD neuroendoscopes with diameters not exceeding 4 mm in diameter. However, we have to remember that the human eye has a higher resolution than HD video—one advantage of using the operation microscope. Therefore, the next step—the ultra-HD-resolution—is already being considered and will be available in the next years in the clinical setup.

Michael R. Gaab
Hannover, Germany

-
1. Manes RP, Barnett S, Batra PS. Utility of novel 3-dimensional stereoscopic vision system for endoscopic sinonasal and skull-base surgery. *Int Forum Allergy Rhinol*. 2011;1(3):191-197.
 2. Tomazic PV, Hammer GP, Gerstenberger C, Koele W, Stammberger H. Heat development at nasal endoscopes’ tips: danger of tissue damage? A laboratory study. *Laryngoscope*. 2012;122(8):1670-1673.


The authors have completed an innovative assessment of 3-dimensional (3-D) and high-definition (HD) vs 2-dimensional (2-D) neuroendoscopy in a preclinical randomized crossover study design with 10 neuroendoscopy-novice participants using a standardized model. Previous assessments have usually compared 3-D and HD neuroendoscopy but not against the common 2-D standard. They determined that time to task completion and perceived depth perception were greater with 3-D vs 2-D neuroendoscopy whereas accuracy of probe placement and perceived image quality were improved with HD vs 2-D neuroendoscopy. Overall, each neuroendoscopic enhancement had benefits in different aspect of the study assessment, and the authors conclude that this provides strong evidence to justify the combination of the 2 modalities (3-D HD neuroendoscopy).

There is a reasonable assumption that improved image quality and migration from 2-D to 3-D images will ultimately improve the ease with which a surgeon can maintain intraoperative orientation, decrease the

learning curve for neuroendoscopic trainees, and ultimately decrease morbidity for neuroendoscopic procedures. The 3-D neuroendoscopes require further improvements to further reduce their size and to allow the addition of working ports for instruments and irrigation. This study provides the justification to further develop these relatively new tech-

nologies with the proviso that we continue to assess them both in similar preclinical models but also in clinical situations.

Mark Hamilton
Calgary Alberta, Canada



Discuss.

NEUROSURGERY® Journal Club.

This new feature capitalizes on and extends the existing practice of Journal Club common to all neurosurgical training programs where resident and fellows critically review published articles under the guidance of faculty.

For more information, please contact the Neurosurgery Editorial Office by phone at 404.712.5930; or email managingeditor@1cns.org

