

WORKSHOP PRESENTATION

Open Access

Optimized saturation pulse trains for SASHA T_1 mapping at 3T

Kelvin Chow^{1*}, Peter Kellman², Bruce S Spottiswoode³, Sonia NIELLES-Vallespin², Richard B Thompson¹

From 18th Annual SCMR Scientific Sessions
Nice, France. 4-7 February 2015

Background

SASHA and MOLLI T_1 mapping sequences can have errors in calculated T_1 values when their magnetization preparation pulses do not fully saturate/invert magnetization [1,2]. The commonly used 90° - 90° - 90° saturation pulse train [3] has poor performance at 3T due to large B_1 field inhomogeneities. We propose that a new hard RF pulse train with numerically optimized flip angles [4] will offer superior performance and reduce errors in SASHA T_1 values due to incomplete saturation.

Methods

Flip angles for a 6-pulse train were optimized by minimizing the maximum residual longitudinal magnetization in Bloch equation simulations performed over ranges of values expected at 3T: 40-120% B_1 scaling, -240-240 Hz off-resonance, 200-2000 ms T_1 , and 14 μ T B_1 strength. Complete spoiling of transverse magnetization was assumed during spoilers. Optimization code is available at <https://bitbucket.org/kelvinc/pulsetrainopt>.

Saturation performance for the 90° - 90° - 90° and the 6-pulse train was measured in a phantom with saturation recovery GRE. B_0 and B_1 maps were calculated using multi-TE and multiple flip angle GRE respectively. A magnetic field gradient was used to produce a range of off-resonance and experiments were repeated with the prescribed pulse train flip angles scaled by 40-120% to emulate B_1 inhomogeneity.

SASHA and MOLLI T_1 mapping were performed using investigational prototype sequences on a 66 kg swine in a 3T system (MAGNETOM Skyra, Siemens AG, Germany). SASHA was acquired using both the 90° - 90° - 90° and proposed pulse train with a 45° imaging flip angle. MOLLI used an optimized inversion pulse (2) with a 20° flip angle. A B_1 map was acquired using a

saturated double angle method with single-shot EPI readouts.

Results

The optimized 6-pulse train flip angles were 115 - 90 - 125 - 85 - 176 - 223° with a 33 ms duration. The 6-pulse train had excellent performance (Fig. 1), with an average and maximum absolute residual longitudinal magnetization over the optimization range of 0.27% and 0.87% respectively. Experimental data had excellent agreement with simulations.

In the swine study, the B_1 varied from 30-95% across the left ventricle (LV) profile (Fig. 2). MOLLI and 90° - 90° - 90° SASHA T_1 maps show a >50% artifactual decrease in T_1 values with reduced B_1 values in the lateral wall. SASHA T_1 values using the 6-pulse train are more spatially homogeneous (1386 ± 70 ms across the entire LV profile).

Conclusions

A saturation pulse train optimized for B_0 , B_1 , and T_1 ranges expected at 3T was shown to have residual longitudinal magnetization of <1%. In-vivo swine MOLLI and SASHA data with the commonly used 90° - 90° - 90° pulses had >50% T_1 variation due to B_1 inhomogeneity while 6-pulse train SASHA had a 5% coefficient of variation.

Funding

Canadian Institutes of Health Research, Alberta Innovates - Health Solutions, NIH/NHLBI Intramural Research Program.

Authors' details

¹University of Alberta, Edmonton, AB, Canada. ²NIH, Bethesda, MD, USA. ³Siemens Healthcare, Chicago, IL, USA.

Published: 3 February 2015

¹University of Alberta, Edmonton, AB, Canada
Full list of author information is available at the end of the article


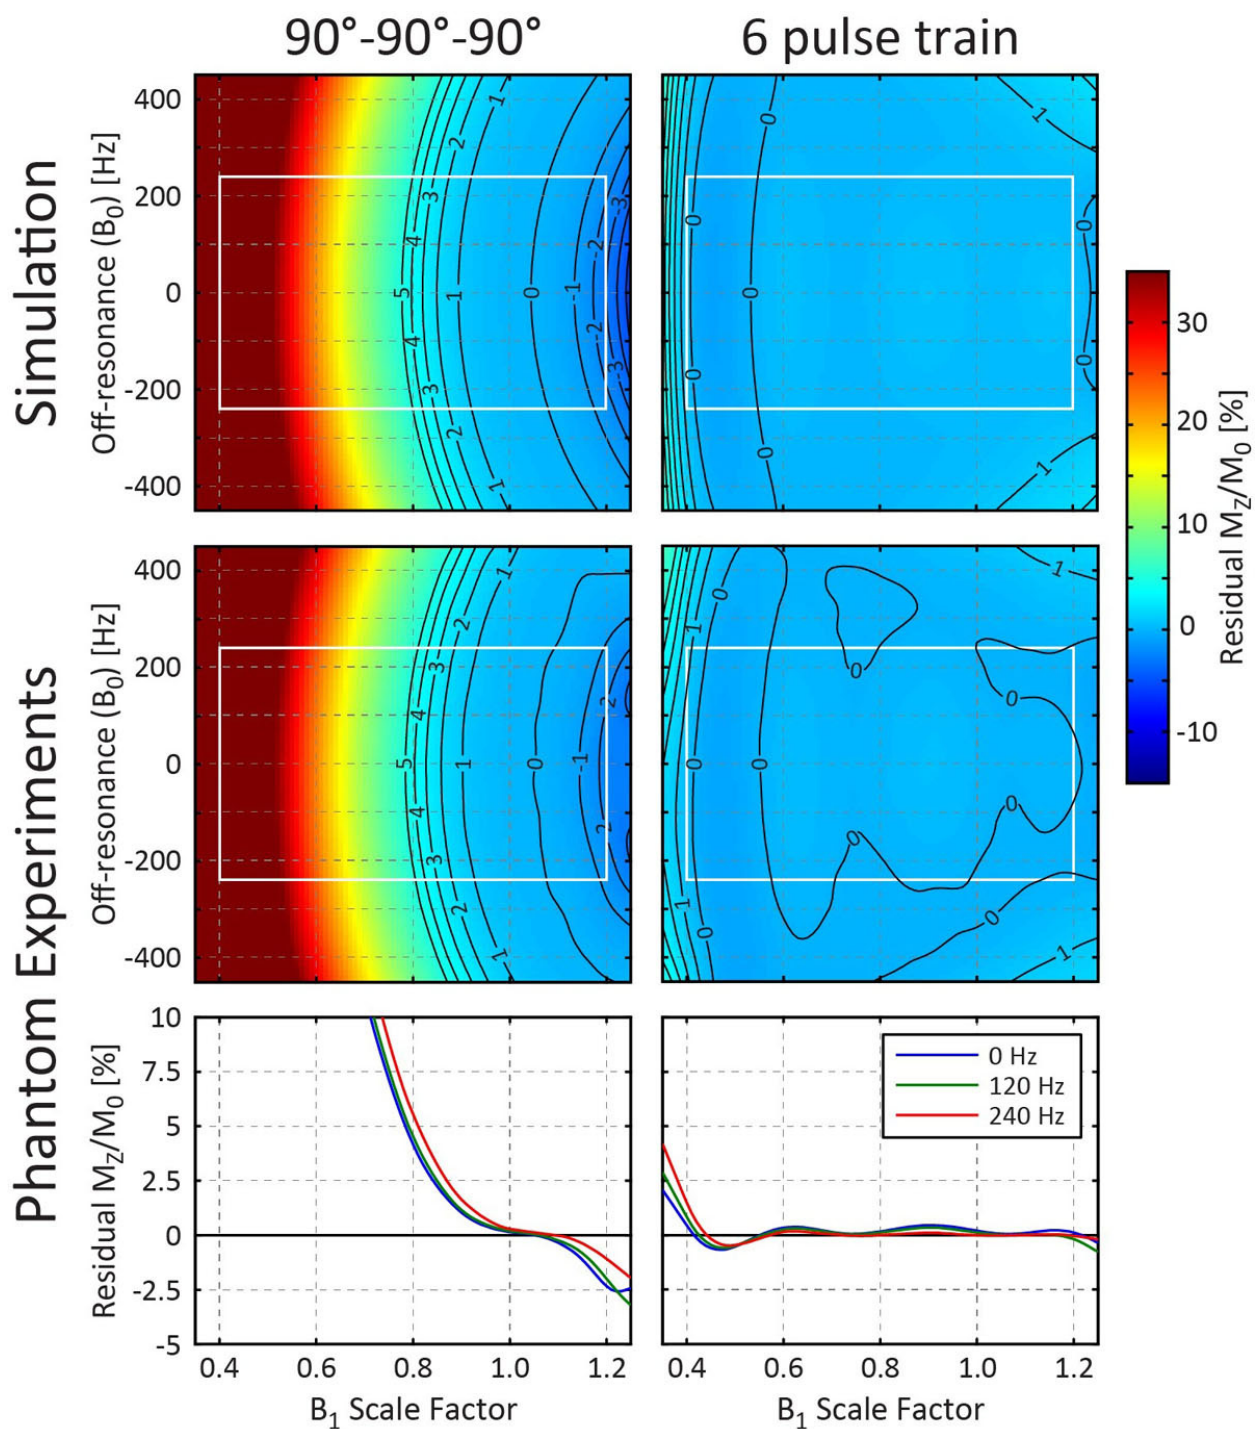


Figure 1 Simulated and experimentally measured residual longitudinal magnetization for a commonly used $90^\circ-90^\circ-90^\circ$ saturation pulse train and a proposed 6 pulse train. White boxes denote the 3T optimization range.

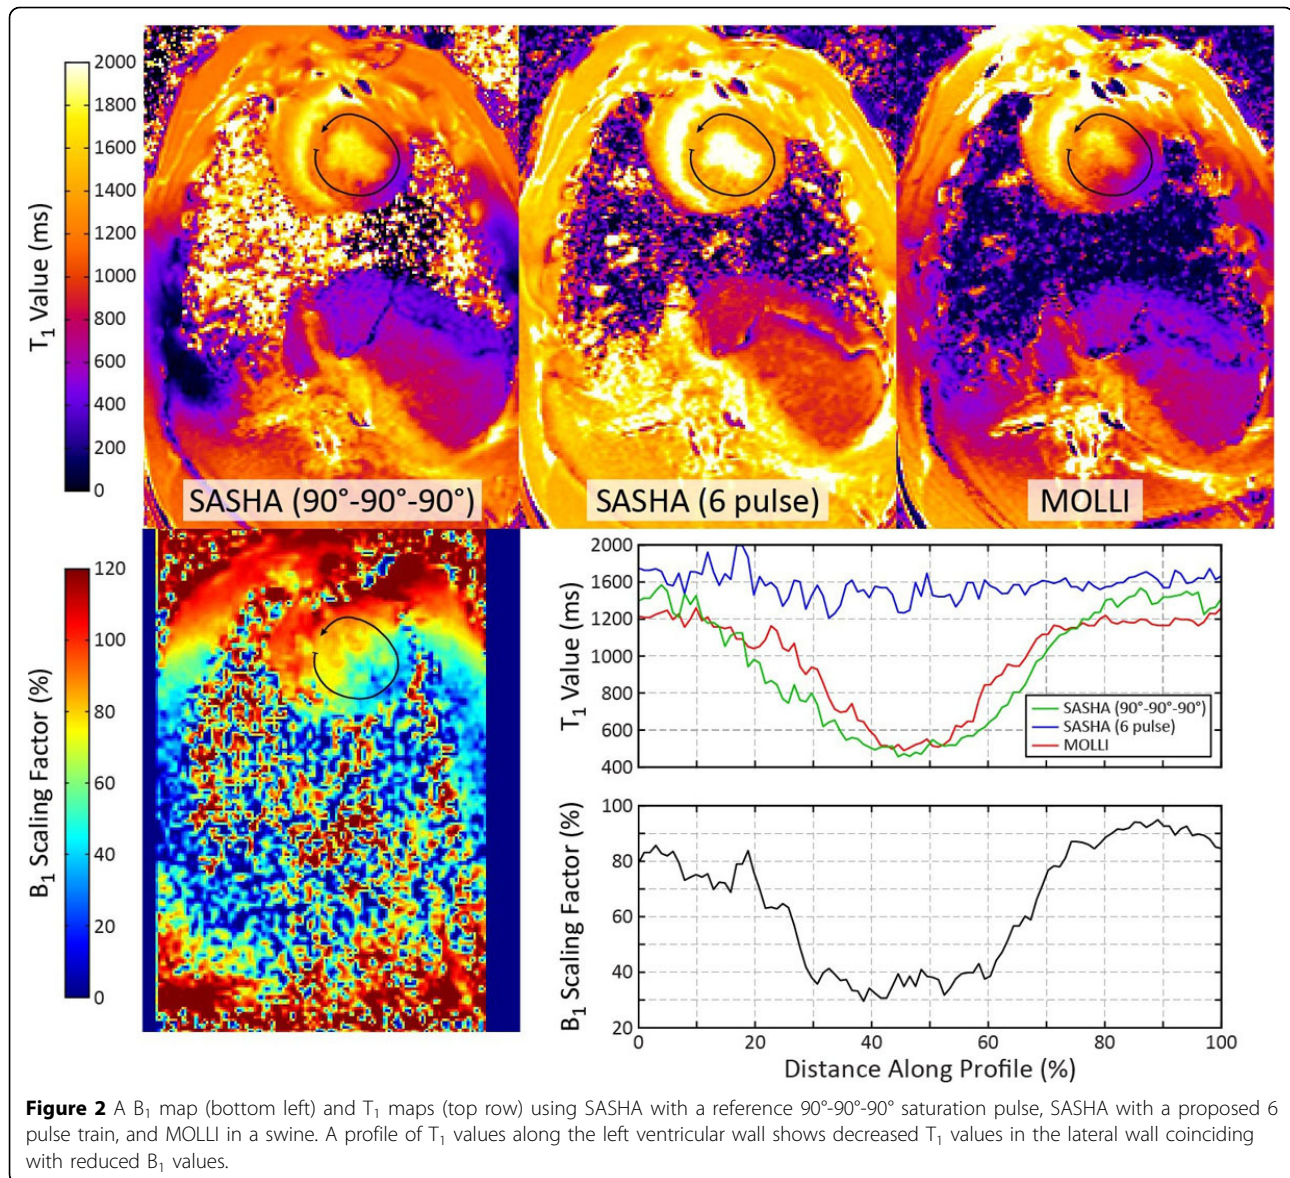

References

1. Chow K, et al: *MRM* 2014, **71**:2082.
2. Kellman P, et al: *MRM* 2014, **71**:1428.
3. Oesingmann N, et al: *JCMR* 2004, **6**:373.
4. Sung K, et al: *MRM* 2008, **60**:997.

doi:10.1186/1532-429X-17-S1-W20

Cite this article as: Chow et al.: Optimized saturation pulse trains for SASHA T₁ mapping at 3T. *Journal of Cardiovascular Magnetic Resonance* 2015 **17**(Suppl 1):W20.

Submit your next manuscript to BioMed Central and take full advantage of:

- Convenient online submission
- Thorough peer review
- No space constraints or color figure charges
- Immediate publication on acceptance
- Inclusion in PubMed, CAS, Scopus and Google Scholar
- Research which is freely available for redistribution

Submit your manuscript at
www.biomedcentral.com/submit

