

RESEARCH ARTICLE

Open Access

Evaluation of *Entamoeba histolytica* recombinant phosphoglucomutase protein for serodiagnosis of amoebic liver abscess

Tan Zi Ning^{1†}, Wong Weng Kin^{1†}, Rahmah Noordin^{2†}, See Too Wei Cun^{1†}, Foo Phiaw Chong^{1†}, Zeehaida Mohamed^{3†}, Alfonso Olivos-Garcia^{4†} and Lim Boon Huat^{1*}

Abstract

Background: Amoebic liver abscess (ALA) is the most frequent clinical presentation of extra-intestinal amoebiasis. The diagnosis of ALA is typically based on the developing clinical symptoms, characteristic changes on radiological imaging and serology. Numerous serological tests have been introduced for the diagnosis of ALA, either detecting circulating amoebic antigens or antibodies. However those tests show some pitfalls in their efficacy and/or the preparation of the tests are costly and tedious. The commercial IHA kit that used crude antigen was reported to be useful in diagnosis of ALA, however high antibody background in endemic areas may cause problems in its interpretation. Thus, discovery of well-defined antigen(s) is urgently needed to improve the weaknesses of current serodiagnostic tests.

Methods: Crude antigen of *E. histolytica* was analysed by 2-DE and Western blot to identify a protein of diagnostic potential for ALA. The corresponding gene of the antigenic protein was then cloned, expressed and the purified recombinant protein was subsequently evaluated for serodiagnosis of ALA in an indirect ELISA format.

Results: Analysis of crude antigen showed that phosphoglucomutase (PGM) has the diagnostic potential. Recombinant PGM (rPGM) showed 79.17% (19/24) sensitivity and 86.67% (195/225) specificity in diagnosis of ALA based on the COV of mean +1SD. There was no significant difference between rPGM-ELISA and IHA diagnostic kit in the diagnosis of ALA in terms of sensitivity and specificity at p-value < 0.05.

Conclusion: In conclusion, rPGM-ELISA is found to be useful for serodiagnosis of ALA. Future studies will determine whether rPGM-ELISA also detects antibodies produced in amoebic dysentery and asymptomatic cases.

Keywords: *Entamoeba histolytica*, Amoebic liver abscess, 2-DE, Western blot, Phosphoglucomutase, Diagnosis, rPGM-ELISA

Background

Liver abscess is commonly detected by radiological imaging technique, but it cannot differentiate between amoebic and pyogenic liver abscesses. Differential diagnosis depends on clinical grounds and amoebic serology [1]. The serological tests revealed varied sensitivity levels, depending on the presence or absence of invasive disease and the types of invasive disease. Interestingly, more than

90% of patients with amoebic liver abscess (ALA) developed detectable anti-amoebic antibodies at 7 – 10 days after onset of symptoms. This augurs well for the development of serodiagnosis against the infection [2-4].

Numerous studies indicated high sensitivity and specificity of crude amoebic antigen *e.g.* crude soluble antigen and excretory-secretory antigens in capturing amoebic antibodies for diagnosis of ALA [5-8]. However, the pitfalls of crude antigen are the need to maintain *E. histolytica* cultures and the mass production of the antigen, which are costly and tedious. Occasionally, this cocktail antigen preparation reveals false positivity [9]. IHA Cellognost[®] Amoebiasis Kit (Dade Behring Marburg

* Correspondence: limbh493@gmail.com

†Equal contributors

¹School of Health Sciences, Universiti Sains Malaysia, Kubang Kerian, Kelantan 16150, Malaysia

Full list of author information is available at the end of the article

GmbH, Germany) that uses crude antigen was reported to be useful in diagnosis of ALA, yet due to the high background in endemic areas, the diagnostic validity varied between 70% and 90% among different geographical locations [10-12]. Hence, a standardised serological test based on well-defined antigen(s) is needed to overcome the weaknesses.

Recombinant DNA technology offers large-scale production of defined antigens through prokaryotic expression system. Serodiagnosis of invasive amoebiasis using defined recombinant *E. histolytica* antigens of serine-rich protein (SREHP), Gal/GalNAc-specific lectin and 29 kDa cysteine-rich surface protein has been reported since 1990s [13]. The recombinant protein of SREHP showed sensitivity of 79% and specificity of 87% in diagnosis of ALA, yet its overall diagnostic validity was lower than the conventional tests that utilized crude antigen [14]. Even though both recombinant Gal/GalNAc-specific lectin and 29 kDa cysteine-rich surface proteins showed high validity of $\geq 90\%$ sensitivity and specificity in serodiagnosis of amoebic dysentery and asymptomatic amoebiasis, they were not specific in the diagnosis of ALA [15,16].

Therefore, this study attempted to identify and analyse potential new antigenic protein(s) from crude antigen of *E. histolytica* using human ALA serum samples. The corresponding gene of the antigenic protein(s) was then cloned and expressed, followed by the diagnostic potential evaluation of the purified recombinant protein in an indirect ELISA format.

Methods

Human serum

Positive serum samples were obtained from 24 patients warded in Hospital Universiti Sains Malaysia (HUSM) who were diagnosed with ALA based on clinical symptoms; detectable abscess by ultrasound imaging; and positive serology with a commercial indirect haemagglutination kit, IHA (Celognost[®] Amoebiasis Kit, Dade Behring Marburg GmbH, Germany). On the other hand, non-ALA serum samples with IHA seronegative were obtained from 33 patients, in which four serum samples were obtained from patients with pyogenic liver abscess ($n = 4$) whereas the others were obtained from patients infected with pathogens other than *E. histolytica*, which include enteropathogenic *Escherichia coli* ($n = 1$), *Shigella sonnei* Group D ($n = 1$), *Salmonella* spp. ($n = 5$), *Klebsiella pneumoniae* ($n = 1$), *Staphylococcus aureus* ($n = 1$), *Ascaris lumbricoides* ($n = 1$), *Escherichia coli* ($n = 2$), Coagulase-negative *Staphylococcus* ($n = 1$), *Stenotrophomonas maltophilia* ($n = 1$), *Toxoplasma gondii* ($n = 9$) and *Helicobacter pylori* ($n = 6$). In this study, all the six *H. pylori* sera were pooled into a single tube because the individual volumes were too little. In addition, a total of 197 blood donor serum samples were obtained

from Department of Haematology & Blood Transfusion Unit at HUSM. All the human serum samples were collected and checked with IHA from the year 2008 onwards and kept at -20°C until used. This study was conducted in accordance with the requirement of Universiti Sains Malaysia Human Research Ethics Committee, USM/KK/PPP/JEPeM (213.3. [10]).

Maintenance of *E. histolytica* and preparation of crude soluble antigen (CSA)

E. histolytica HM-1:IMSS was axenically cultured and maintained in Diamond's TYI-S-33 medium [17]. For CSA preparation, 10×10^6 of *E. histolytica* trophozoites were mixed with 500 μL complete Lysis-M buffer supplemented with protease inhibitor cocktail (Roche, Germany) and 20 μL of 0.5 M iodoacetamide (Sigma, USA). The mixture was then sonicated (Branson, Mexico) at 10% amplitude for three cycles of 1 min sonication with 0.5 sec pulse-on and 0.5 sec pulse-off. The lysate was centrifuged at $10\,000 \times g$ for 10 min at 4°C to collect the CSA in the supernatant. Subsequently, the protein concentration was estimated using Bradford protein assay [18].

Analysis of CSA antigenic protein profile via SDS-PAGE and Western blotting

Twenty micrograms of CSA per well was separated by 9% sodium dodecyl sulfate polyacrylamide gel electrophoresis (SDS-PAGE) using Bio-Rad Mini-Protean III Electrophoresis Cell (Bio-Rad, USA) at a constant current of 25 mA per gel for about 1 h and the separated proteins were electroblotted onto a 0.45 μm -pore-size nitrocellulose (NC) membrane via a semidry transblot apparatus (Bio-Rad, USA) at constant voltage of 15 V for 45 min. The NC membrane was blocked for 1 h at RT with 5% skim milk with 10 mM Tris-buffered saline (TBS), pH 7.2 as the diluent. Subsequently, the NC membrane was cut into multiple strips and incubated with human sera at a dilution of 1:200 in TBS containing 0.1% Tween 20 (TBST) for 2 h at RT. The excess serum was removed by washing (3×5 min) the strips with TBST. Next, the strips were incubated with a monoclonal mouse anti-human IgG conjugated with horseradish peroxidase (HRP) (Invitrogen, USA) at a dilution of 1:6000 for 1 h at RT. The unbound secondary antibodies were removed by washing (3×5 min) with 0.1% TBST. The Western blot signal was detected by enhanced chemiluminescence (ECL) reagent (Roche Diagnostics, Germany), captured using X-ray film (Kodak, USA). The sensitivity and specificity of the antigenic protein was then evaluated based on serum samples collected from ALA cases ($n = 24$), patients with infections other than amoebiasis ($n = 33$) and blood donors ($n = 30$).

Identification of the antigenic protein via 2-DE and Western blotting

A 2-DE gel electrophoresis was performed to further separate the antigenic protein band. Proteins of CSA were first fractionated based on their isoelectric point (pI) using 3100 OFFGEL Fractionator (Agilent Technologies, Germany). The Immobiline™ Dry Strip (GE Healthcare, UK) with linear pH range 3–10 with a 12-well setup was used. The fractionation of CSA was performed according to the manual provided by the manufacturer. In brief, the protein sample was prepared by gently mixing 1600 µL of OFFGEL stock solution (1.25X) with 400 µL of the CSA sample with total protein mass of 2 mg. A volume of 150 µL of OFFGEL sample was loaded into each well of IPG strip after gel rehydration with 40 µL of IPG strip rehydration buffer. Mineral oil used as cover fluid was pipetted onto the gel strip ends. The sample was focused with a maximum power of 200 mW, maximum current of 50 µA and typical voltages ranging from 500 to 4500 V until 50 kWh was reached in ~24 h. The typical starting voltages used were from 200 to 1500 V. A volume of 20 µL of the fractionated protein sample was mixed with 5 µL of 5X SDS sample buffer without boiling, and subsequently separated by SDS-PAGE. The separated proteins were then transferred onto NC membrane followed by Western blot analysis using pooled and individual ALA or IHA seronegative serum samples at 1:200 dilution.

Mass spectrometry analysis and protein identification

The antigenic protein band was excised from the 2-D SDS-PAGE gel and sent to Australian Proteomic Service for peptide sequencing by mass-spectrometry. At the proteomic facility, protein sample was digested with trypsin and the peptides were extracted and analysed by electrospray ionisation mass spectrometry (ESI-TRAP) using the Ultimate 3000 nano HPLC system (Dionex) coupled to a 4000 Q TRAP mass spectrometer (Applied Biosystems). The mass-spectrometry analysis was performed with two different gel slice samples to ensure reproducibility.

Cloning of selected gene

Based on the amino acid sequence of the ~70 kDa antigenic protein, the encoding gene was identified. PCR primers were then designed based on the protein coding sequence retrieved from the GenBank (accession number XM_643579) to amplify the gene of interest from *E. histolytica* genomic DNA isolated from 3×10^6 of *E. histolytica* trophozoites using a QIAamp DNA mini kit (QIAGEN GmbH, Germany). The optimum annealing temperature was 52°C. For cloning into pET-14b vector, *XhoI* (CTCGAG) and *BamHI* (GGATCC) recognition sequences were added to the forward and reverse primers, respectively. The primers sequences used to generate a 1785 bp PCR product were 5'- CCG CTC

GAG ATG GCA CTG AAT AAT TAT ATT AAG-3' forward primer; and 5'- CGC GGA TCC TTA CTC AGC TTT TGG TGG-3' reverse primer. The amplified product with the expected size was cut and extracted from the 1% agarose gel using QIAGEN gel extraction kit (QIAGEN GmbH, Germany). Before ligation, both the PCR amplified product and pET-14b vector were digested with *XhoI* and *BamHI* (Fermentas Life Sciences, USA). The digested products were then purified by PCR purification kit (QIAGEN GmbH, Germany).

Ligation was performed by mixing the digested plasmid and PCR amplified product in the ratio of 1:3 in a final volume of 10 µL containing 1X T4 DNA Ligase buffer, 5 U of T4 DNA Ligase and dH₂O. The ligation mixture was incubated overnight at 4 °C. Next, *E. coli* XL 1-Blue competent cells were transformed with the ligation mixture by heat-shock method. Colony PCR using T7 promoter primer (5'-TAATACGACTCACTATAGG-3') and T7 terminator primer (5'-GCTAGTTATTGCTCAGCGG-3) was performed to screen for positive transformants, and the positive clones were confirmed by DNA sequencing.

Expression and purification of recombinant antigenic protein

Recombinant plasmid carrying the open reading frame for the antigenic protein was transformed into expression host (*E. coli* BL-21 AI strain). The bacteria was grown at 37°C until OD_{600 nm} reached 1.2 and protein expression was induced with 0.2% (w/v) L-arabinose at 22°C for overnight. The recombinant protein was purified using nickel-nitrilotriacetic acid (Ni-NTA) affinity purification method. In brief, 800 mL of culture were harvested by centrifugation at 1800 × g, 20 min, at 4°C. The supernatant was discarded and the cell pellet was mixed and resuspended in 10 mL of lysis buffer [50 mM Tris-HCl (pH 7.5), 300 mM NaCl, 10 mM Imidazole and 1% Triton X-100] supplemented with 7.8 µL of β-mercaptoethanol. The suspension was then sonicated and centrifuged at 1800 × g, 30 min, at 4°C. The supernatant was transferred into a clean 15 mL centrifuge tube. A volume of 100 µL of Ni-NTA agarose (QIAGEN, Germany) was mixed with the supernatant and the suspension was then rotated at 4°C for 2 h. After that, the suspension was centrifuged at 450 × g, 2 min, at 4°C. The supernatant was discarded and the Ni-NTA agarose was washed with 10 mL of ice-cooled His-Tag washing buffer [50 mM Tris-HCl (pH 7.5), 300 mM NaCl and 20 mM Imidazole]. The suspension was rotated at 4°C for 30 min. The supernatant was discarded and the washing step on Ni-NTA agarose was repeated for another 5 times. In the final washing step, the suspension was centrifuged at 450 × g, 2 min, at 4°C and the supernatant was discarded. The recombinant protein that bound to the Ni-NTA agarose was eluted by 120 µL of

ice-cooled His-Tag elution buffer [50 mM Tris-HCl (pH 7.5), 300 mM NaCl and 200 mM Imidazole] and rotated at 4°C for 3 h. The suspension was then centrifuged at 450 × g, 5 min, at 4°C and the concentration of the supernatant (eluted protein) collected in a clean 1.5 mL micro-centrifuge tube was determined by Bradford protein assay.

Development and evaluation of indirect recombinant antigen based ELISA

Indirect-ELISA was performed on the human serum samples using the purified recombinant protein based on modifications of method described by Reen [19]. The coating concentration of the antigen for each well of a microtiter plate was 1 µg/mL; and the primary and secondary antibody dilutions were 1:50 and 1:250, respectively. In brief, each well of a 96-well flat-bottom microtiter plate (NUNC, Denmark) was coated with 100 µL of antigen diluted in 0.1 M bicarbonate buffer (pH 9.6). The plate was then covered and incubated overnight in a humid box at 4°C. Prior to the blocking step, coated plate was equilibrated for 1 h at room temperature and then each well was rinsed (5 × 5 min) with 200 µL phosphate buffered saline added with 0.05% Tween-20 (PBST). The plate was blotted against a piece of paper towel after every round of rinsing. After 1 h in blocking reagent (Roche, Germany), each well was washed with 0.05% PBST (5 × 5 min), followed by another hour of incubation with 100 µL of diluted serum samples, performed in duplicate. After another round of washing, 100 µL of PBS diluted HRP-conjugated mouse monoclonal anti-human IgG (Invitrogen, USA) was added into the well and incubated for 1 h. Following a final round of washing, 100 µL of TMB substrate was added and the plate was incubated in the dark at room temperature for 15 min. The optical densities (OD) were finally read at 450 nm VersaMax™ Microplate Reader (Sunnyvale, USA). The and specificity of the recombinant antigen in an indirect ELISA format was then evaluated against the IHA kit using the different categories of serum samples collected. The COV for the indirect ELISA was set at either mean OD value plus one or two standard deviations (SD) from the OD values obtained from 113 IHA seronegative blood donor serum samples.

Statistical analysis

Statistical analysis was performed with SPSS for Windows version 18.0. The association between the indirect ELISA and IHA in clinical diagnosis of ALA was analysed using chi-square test; if indicated Fisher's exact test was used instead.

Results

IgG blots of CSA

Immunoblotting results showed that there were three antigenic proteins *i.e.* ~170 kDa, ~100 kDa and ~70 kDa,

recognized by individual human ALA serum samples (Figure 1). Based on the 24 human ALA serum samples, the sensitivities of these three antigenic proteins were 70.83%, 62.5% and 70.83%, respectively; while their specificities were 100%, 100% and 96.83%, respectively, when tested against a total of 63 negative control serum samples. The results on the sensitivity and specificity are summarised in Table 1.

2-DE Western blot analysis and protein identification

Both the ~170 kDa and ~70 kDa proteins revealed almost similar sensitivity and specificity. Since the ~170 kDa was most probably the previously studied lectin antigen [16] and ~100 kDa showed lower sensitivity, hence here, only the ~70 kDa protein was further studied. In 2D-Western blotting analysis, the 70 kDa protein was presented in fraction 7 with pH between 6.5 and 7.08. Western blot in fraction 7 using two individual human ALA serum samples revealed positive reactivity against the targeted antigenic protein (Figure 2). Mass-spectrometry analysis identified the ~70 kDa antigenic protein as phosphoglucosyltransferase (PGM) of *E. histolytica* (accession number C4M3Z6) with the protein score of 793 and 19 peptide sequences matched to the amino acid sequence. The score > 55 indicates identity or extensive homology at a significant level of $p < 0.05$. The total sequence coverage of the protein was reported as 25%.

Expression and purification of the recombinant PGM (rPGM) protein

The rPGM protein tagged with six consecutive histidine residues was purified using Ni-NTA affinity purification and was evaluated by 9% SDS-PAGE (Figure 3). The result showed that about 50% of the expressed PGM was present in the soluble fraction (lane 3). In lane 4, it revealed the soluble recombinant protein was successfully purified to apparent homogeneity.

Efficacy of rPGM-ELISA

The COVs of rPGM-ELISA at mean OD value + 1SD and mean OD value + 2D were determined to be 0.25 and 0.32, respectively. The sensitivity was calculated based on results of 24 human ALA serum samples; while a total of 225 human sera from other infections and blood donors were used for specificity test. Based on the COV of mean + 1SD and mean + 2SD, the sensitivities of rPGM-ELISA were 79.17% (19/24) and 45.83% (11/24), respectively; while the specificities of the tests were 86.67% (195/225) and 93.78% (211/225), respectively (Table 2). Thus the COV based on mean + 1SD was selected over the COV of mean + 2SD as it showed better sensitivity and specificity in diagnosis of ALA. In comparison with IHA kit, statistical analysis showed that there was no significant difference between rPGM-

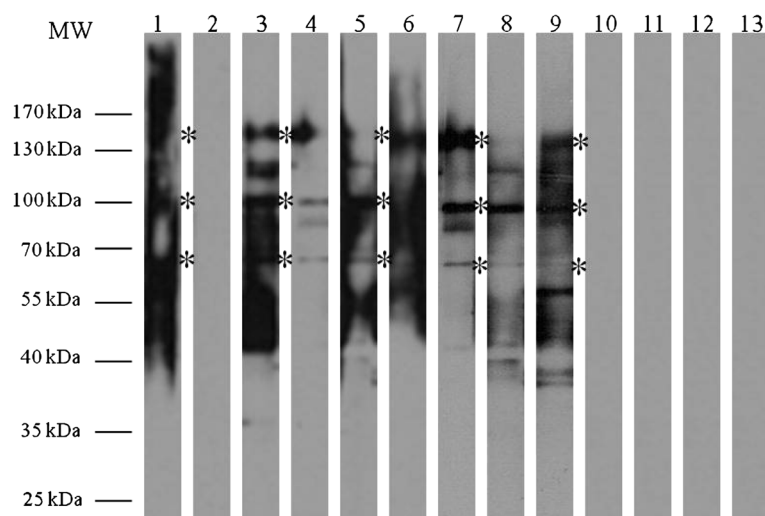


Figure 1 Western blot profile of CSA probed with representative individual human serum. Lane MW: Molecular weight standard (PageRuler™ Prestained Protein Ladder); Lane 1: Pooled human ALA serum; Lane 2: Pooled human IHA seronegative serum; Lanes 3 to 9: Individual human ALA serum; Lanes 10–12: Individual human IHA seronegative serum; Lane 13: TBS control. (*) indicates the estimated molecular weight of proteins (~170 kDa, ~100 kDa and ~70 kDa).

ELISA and IHA in terms of sensitivity and specificity at p -value < 0.05 (Table 3).

Discussion

Conventionally, diagnosis of ALA is confirmed by finding the *E. histolytica* trophozoites in liver pus aspirate obtained *via* ultrasound guided percutaneous aspiration biopsy, but the parasites are often absent as most of them are located at the margin on the peripheral of the abscess [20,21]. Therefore, serodiagnosis is widely adopted for diagnosis of ALA, detecting either amoebic antigens or antibodies from serum samples. Although numerous commercial antigen detection kits have been developed *i.e.* TechLab *E. histolytica* II ELISA (TechLab, Blacksburg, VA), *Entamoeba* CELISA-PATH (Cellabs Pty Ltd., Brookvale, Australia), Optimum S *Entamoeba histolytica* antigen ELISA (Merlin Diagnostika, Berheim-Hersel, Germany), Triage parasite panel BIOSATE (diagnostic, San Diego, CA), and ProSpecT *Entamoeba histolytica* microplate assay (REMEL Inc., Lenexa, KS), only TechLab *E. histolytica* II ELISA was evaluated for the detection of circulating antigen in ALA patient serum samples [22]. Haque *et al.* [23] reported that the kit detected Gal/GalNAc lectin in the ALA patient serum samples with a


sensitivity of 96%. However, reports by Parija and Khairnar [24] and Zeehaida *et al.* [25] revealed lower sensitivities at 50% and 8.6%, respectively.

Instead of antigen detection, diagnosis of ALA can be performed by detecting circulating antibodies because hepatic amoebiasis raises a strong humoral response, especially immunoglobulin G [26]. Although a variety of serological assays was reported in diagnosis of ALA based on detecting circulating antibodies *i.e.* IHA, latex agglutination, indirect immunofluorescence, counter-immunoelectrophoresis, gel diffusion, complement fixation and ELISA; IHA and ELISA are still the preferred choices [22]. ELISA is commonly used as the routine diagnostic assay in diagnosis of ALA because it can be developed for in-house use based on different amoebic antigen preparations such as CSA, excretory-secretory antigens, plasma membrane antigens, purified antigenic proteins or recombinant proteins.

The CSA-based ELISA technique has either been used in routine diagnosis of ALA or field screening of amoebiasis [8,10,27,28]. In the diagnosis of ALA, CSA-based ELISA was reported to be 100% sensitive and $> 90\%$ specific [8,29]. Excretory-secretory antigens have been reported to be useful in diagnosis of ALA, which

Table 1 Sensitivity and specificity of each potential antigenic protein bands of CSA

Molecular weight of antigenic protein band (kDa)	Clinically confirmed human ALA serum (n = 24)	Human IHA seronegative serum (n = 63)	Sensitivity (%)	Specificity (%)
170	17	0	70.83	100
100	15	0	62.5	100
70	17	2	70.83	96.83

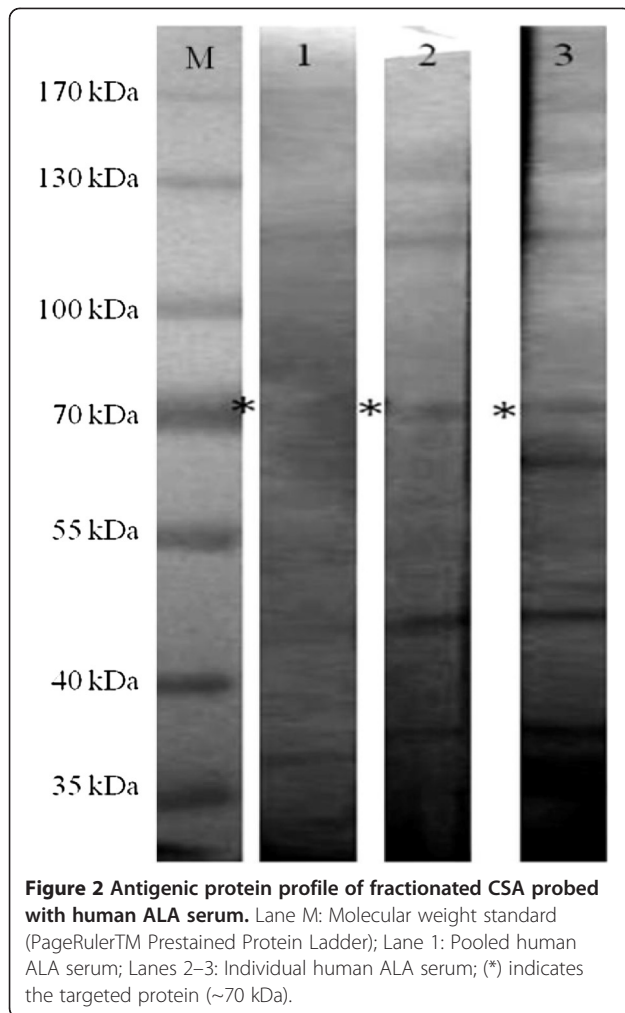

showed sensitivity of ~80% in Western blot analysis [7,30]. Another ELISA using amoebic plasma membrane antigen for diagnosis of ALA was reported to be 95% sensitive and 91% specific against anti-amoebic IgG; while detection of anti-amoebic IgM was 91% sensitive and 95% specific [31].

Nonetheless, crude preparations of amoebic antigens produced variable diagnostic efficacies, which may lead to false positive in the diagnosis of ALA. These antigen preparations require maintenance of *E. histolytica* cultures, which is costly and tedious. Moreover, the proteins are not well-defined; hence the interpretation of results may vary from batch to batch. In this study, analysis of the CSA protein profile showed that most of the antigenic proteins recognized by the human ALA serum antibodies ranged from 25 kDa to 170 kDa. Lower percentage (9%) polyacrylamide gel revealed that the ~170 kDa, ~100 kDa and ~70 kDa protein bands were well recognized by human ALA serum samples. Here, the ~70 kDa protein with 70.83% sensitivity and 96.83% specificity was selected for cloning and production of

recombinant protein. The ~170 kDa protein also revealed almost similar sensitivity and specificity, but was not selected because it was most probably similar to the previously described lectin surface antigen of *E. histolytica* [16].

Prior to elucidating the identity of the ~70 kDa protein, it was further separated using 2-DE electrophoresis, a widely used technique in biomarker discoveries [32]. Proteins of CSA were fractionated *via* OFFGEL approach based on pI separation. This approach is advantageous when serum sample is limited. Multiple individual serum samples can be applied on the selected pI protein fraction containing the protein of interest in NC strip blot format, instead of using the whole gel NC membrane format in the conventional 2D-Western blot.

The ~70 kDa protein in this study was identified as *E. histolytica* PGM by mass-spectrometry analysis. This protein is reported to be involved in the glycolytic pathway of *E. histolytica*, which catalyses the inter-conversion of glucose 6-phosphate and glucose 1-phosphate. Previously, PGM was used as the gold standard for differentiation between *E. histolytica* and *E. dispar* *via* isoenzyme electrophoresis together with hexokinase [33]. Interestingly, there is no report on the value of this protein in diagnosis of invasive amoebiasis.

Well-defined antigens such as purified antigenic proteins and recombinant proteins of *E. histolytica* can overcome some of the setbacks posed by utilization of crude soluble preparations. For instance, purified lectin antigen and purified 29 kDa cysteine-rich surface protein in an ELISA format were reported to be useful for diagnosis of ALA [34,35]. According to Flores *et al.* (1993), the purified native 29 kDa cysteine-rich surface protein showed 79% sensitivity and 98% specificity in the diagnosis of ALA [34]. Several recombinant proteins have been produced such as SREHP, Gal/GalNAc-specific lectin, 29 kDa cysteine-rich surface protein and 40 kDa NADP⁺-dependent alcohol dehydrogenase (EhADH1) [13,36]. Recombinant proteins of SREHP, Gal/GalNAc-specific lectin and 29 kDa cysteine-rich surface protein have been evaluated for diagnosis of ALA. SREHP/MBP fusion protein, which was among the first recombinant proteins used in serodiagnosis of ALA was reported to have a sensitivity and specificity of 74% and 55%, respectively. Interestingly, its diagnostic validity increased to 79% and 87%, respectively, after the removal of its MBP component [14]. The validity is almost similar with rPGM protein in the current study, which is 79.17% sensitive and 86.67% specific. Recombinant full-length 170 kDa Gal/GalNAc-specific lectin protein has been produced and its validity in diagnosis of ALA was about 91% sensitivity [16]. Besides, several recombinant fragments of the Gal/GalNAc-specific lectin protein have also been investigated for the diagnosis of ALA. For

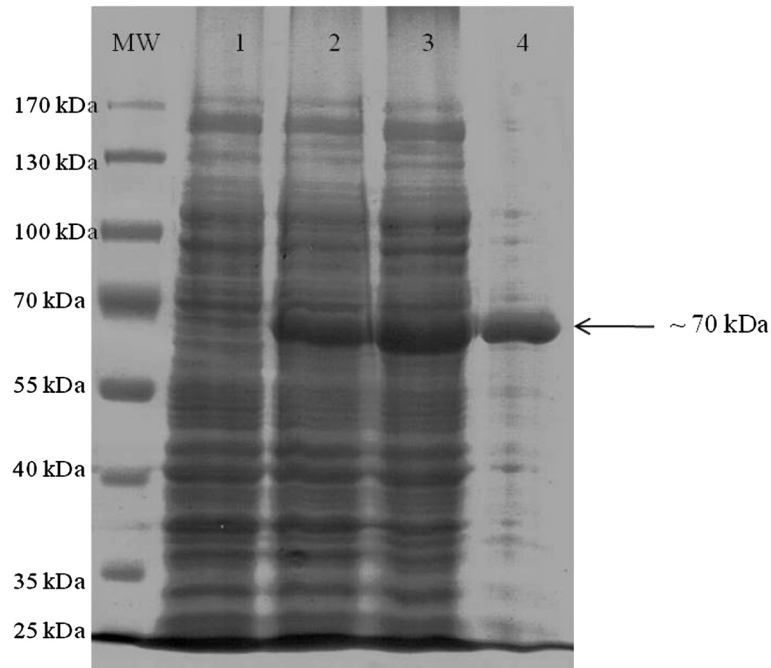


Figure 3 Purified recombinant PGM protein. Lane MW: PageRuler™ Prestained Protein Ladder; Lane 1: Non-induced cell pellet; Lane 2: Induced cell pellet; Lane 3: Induced cell supernatant; Lane 4: Purified protein; Arrow indicates the recombinant PGM protein (~70 kD).

example, recombinant protein of a truncated immunodominant domain of the Gal/GalNAc-specific lectin protein with 1.85 kbp cDNA insert showed more than 90% for both sensitivity and specificity [28]. Another study using recombinant Gal/GalNAc-specific lectin-derived protein (LC3) showed 100% sensitivity in diagnosis of ALA [37]. A study carried out by Tachibana *et al.* [29] reported that the 150 kDa recombinant intermediate subunit (IgI) of the Gal/GalNAc-specific lectin protein used in diagnosis of ALA was only 8.6% sensitive. A recombinant 29 kDa cysteine-rich surface protein was also

developed and evaluated as its purified form showed moderate validity in diagnosis of ALA. The evaluation of this recombinant protein in the diagnosis of ALA showed increment of sensitivity (90%) compared to its purified native form protein (79%) [34].

Although several recombinant proteins have been evaluated, they were not specific for diagnosis of ALA because several studies have reported that those recombinant proteins were immunoreactive with serum samples for amoebic dysentery and asymptomatic cases [15,16,29,38,39]. In the current study, the novel rPGM protein showed diagnostic validity of ~80% sensitivity and ~90% specificity in diagnosis of ALA. The efficacy

Table 2 Number of serum sample at different COV settings from different serum test groups using rPGM-ELISA

rPGM-ELISA (COV = mean + 1SD)	Number of Serum samples		Total
	< 0.25	≥ 0.25	
Human ALA serum	5	19	24
Other infections human serum	21	7	28
Blood donors' serum	174	23	197
Total	200	49	249
rPGM-ELISA (COV = mean + 2SD)	< 0.32	≥ 0.32	
Human ALA serum	13	11	24
Other infections human serum	26	2	28
Blood donors' serum	185	12	197
Total	224	25	249

Table 3 Comparison between rPGM-ELISA and IHA in terms of sensitivity and specificity in diagnosis of ALA using statistical analysis

	Sensitivity	IHA		Total	Fisher's Exact Test (p-value)
		.00	1.00		
rPGM-ELISA	.00	0	5	5	0.620
	1.00	2	17	19	
Total		2	22	24	
	Specificity	IHA		Total	Fisher's Exact Test (p-value)
		.00	1.00		
rPGM-ELISA	.00	181	14	195	0.638
	1.00	28	2	30	
Total		209	16	225	

Note: (.00): Negative; (1.00): Positive.

of rPGM-ELISA was almost comparable to previously reported recombinant proteins such as SREHP, Gal/GalNAc-specific lectin and 29 kDa cysteine-rich surface protein, which showed both sensitivity and specificity ranging from 80% to 100% [16,34,39].

Conclusion

In conclusion, the novel rPGM protein used in an indirect ELISA format developed in this study could be useful for in-house routine diagnosis of ALA. Future studies will determine whether rPGM-ELISA also detects antibodies produced in amoebic dysentery and asymptomatic cases.

Consent

Written informed consents were obtained from the patients for publication of this report.

Competing interests

The authors hereby declare that they have no competing interests.

Authors' contributions

All authors contributed to this work. First author, TZN carried out the experiments and drafted the manuscript. All authors were involved in the manuscript preparation. All authors read and approved the final version of the manuscript.

Acknowledgements

This study was funded by Universiti Sains Malaysia Research University Grant: 1001/PPSK/813044. The first two authors (TZN and WWK) received financial support through the university fellowship and the fifth author (FPC) is a graduate assistant at School of Health Sciences. Besides, we would like to thank the Dean of School of Health Sciences and also the Director of Institute for Research in Molecular Medicine (INFORMM), Universiti Sains Malaysia for the facilities made available.

Author details

¹School of Health Sciences, Universiti Sains Malaysia, Kubang Kerian, Kelantan 16150, Malaysia. ²Institute for Research in Molecular Medicine, Universiti Sains Malaysia, Penang 11800, Malaysia. ³Department of Medical Microbiology and Parasitology, School of Medical Sciences, Universiti Sains Malaysia, Kubang Kerian, Kelantan 16150, Malaysia. ⁴Departamento de Medicina Experimental, Facultad de Medicina, Universidad Nacional Autónoma de México, México D. F. 04510, México.

Received: 25 December 2012 Accepted: 13 March 2013

Published: 21 March 2013

References

1. Pitt HA: Surgical management of hepatic abscesses. *World J Surg* 1990, **14**:498–504.
2. Mathur S, Gehlot RS, Mohta A, Bhargava N: Clinical profile of amoebic liver abscess. *JACM* 2002, **3**:367–373.
3. Sharma MP, Ahuja V: Amoebic liver abscess. *JACM* 2003, **4**:107–111.
4. Wells CD, Arguedas M: Amebic liver abscess. *South Med J* 2004, **97**:673–682.
5. Knappik M, Borner U, Jelinek T: Sensitivity and specificity of a new commercial enzyme-linked immunoassay kit for detecting *Entamoeba histolytica* IgG antibodies in serum samples. *Eur J Clin Microbiol Infect Dis* 2005, **24**:701–703.
6. Robert R, Mahaza C, Bernard C, Buffard C, Senet JM: Evaluation of a new bicolored latex agglutination test for immunological diagnosis of hepatic amoebiasis. *J Clin Microbiol* 1990, **28**:1422–1424.
7. Wong WK, Tan ZN, Othman N, Lim BH, Mohamed Z, Olivos Garcia A, Noordin R: Analysis of *Entamoeba histolytica* excretory-secretory antigen and identification of a new potential diagnostic marker. *Clin Vaccine Immunol* 2011, **18**:1913–1917.
8. Yang J, Kennedy MT: Evaluation of enzyme-linked immunosorbent assay for the serodiagnosis of amoebiasis. *J Clin Microbiol* 1979, **10**:778–785.
9. Lotter H, Mannweiler E, Schreiber M, Tannich E: Sensitive and specific serodiagnosis of invasive amoebiasis by using a recombinant surface protein of pathogenic *Entamoeba histolytica*. *J Clin Microbiol* 1992, **30**:3163–3167.
10. del Carmen S-GM, Velazquez-Rojas M, Salgado-Rosas H, Torres-Rasgado E, Perez-Fuentes R, Martinez-Munguia J, Talamas-Rohana P: Seroprevalence of anti-*Entamoeba histolytica* antibodies by IHA and ELISA assays in blood donors from Puebla. Mexico. *Arch Med Res* 2000, **31**:S53–S54.
11. Kraoul L, Adjmi H, Lavarde V, Pays JF, Tourte-Schaefer C, Hennequin C: Evaluation of a rapid enzyme immunoassay for diagnosis of hepatic amoebiasis. *J Clin Microbiol* 1997, **35**:1530–1532.
12. Zeehaida M, Bachok N, Hasan H: Analysis of indirect hemagglutination assay results among patients with amoebic liver abscess. *Int Med J* 2009, **16**:195–199.
13. Stanley SL Jr: Progress towards development of a vaccine for amoebiasis. *Clin Microbiol Rev* 1997, **10**:637–649.
14. Myung K, Burch D, Jackson TF, Stanley SL Jr: Serodiagnosis of invasive amoebiasis using a recombinant *Entamoeba histolytica* antigen-based ELISA. *Arch Med Res* 1992, **23**:285–288.
15. Ravdin JI, Jackson TF, Petri WA Jr, Murphy CF, Ungar BL, Gathiram V, Skilogiannis J, Simjee AE: Association of serum antibodies to adherence lectin with invasive amoebiasis and asymptomatic infection with pathogenic *Entamoeba histolytica*. *J Infect Dis* 1990, **162**:768–772.
16. Zhang Y, Li E, Jackson TF, Zhang T, Gathiram V, Stanley SL Jr: Use of a recombinant 170-kilodalton surface antigen of *Entamoeba histolytica* for serodiagnosis of amoebiasis and identification of immunodominant domains of the native molecule. *J Clin Microbiol* 1992, **30**:2788–2792.
17. Diamond LS, Harlow DR, Cunnick CC: A new medium for the axenic cultivation of *Entamoeba histolytica* and other *Entamoeba*. *Trans R Soc Trop Med Hyg* 1978, **72**:431–432.
18. Bradford MM: A rapid and sensitive method for the quantitation of microgram quantities of protein utilizing the principle of protein-dye binding. *Anal Biochem* 1976, **72**:248–254.
19. Reen DJ: *Basic Protein and Peptide Protocols: CHAPTER 47 Enzyme-Linked Immunosorbent Assay (ELISA)*. Totowa, NJ: Humana Press Inc.; 1994.
20. Keeley KJ, Schmaman A, Scott A: Definitive diagnosis of amoebic liver abscess: value of liver biopsy. *Br Med J* 1962, **1**:375–376.
21. Tsutsumi V, Mena-Lopez R, Anaya-Velazquez F, Martinez-Palomo A: Cellular bases of experimental amoebic liver abscess formation. *Am J Pathol* 1984, **117**:81–91.
22. Fotedar R, Stark D, Beebe N, Marriott D, Ellis J, Harkness J: Laboratory diagnostic techniques for *Entamoeba* species. *Clin Microbiol Rev* 2007, **20**:511–532. table of contents.
23. Haque R, Mollah NU, Ali IK, Alam K, Eubanks A, Lyerly D, Petri WA Jr: Diagnosis of amoebic liver abscess and intestinal infection with the TechLab *Entamoeba histolytica* II antigen detection and antibody tests. *J Clin Microbiol* 2000, **38**:3235–3239.
24. Parija SC, Khairnar K: Detection of excretory *Entamoeba histolytica* DNA in the urine, and detection of *E. histolytica* DNA and lectin antigen in the liver abscess pus for the diagnosis of amoebic liver abscess. *BMC Microbiol* 2007, **7**:41.
25. Zeehaida M, Wan Nor Amilah WA, Amry AR, Hassan S, Sarimah A, Rahmah N: A study on the usefulness of Techlab *Entamoeba histolytica* II antigen detection ELISA in the diagnosis of amoebic liver abscess (ALA) at Hospital Universiti Sains Malaysia (HUSM), Kelantan, Malaysia. *Trop Biomed* 2008, **25**:209–216.
26. Valenzuela O, Ramos F, Morán P, González E, Valadez A, Gómez A, Melendro EI, Ramiro M, Muñoz O, Ximénez C: Persistence of secretory anti-amoebic antibodies in patients with past invasive intestinal or hepatic amoebiasis. *Parasitol Res* 2001, **87**:849–852.
27. Haghighi A, Rezaeian M: Detection of serum antibody to *Entamoeba histolytica* in various population samples of amoebic infection using an enzyme-linked immunosorbent assay. *Parasitol Res* 2005, **97**:209–212.
28. Shenai BR, Komalam BL, Arvind AS, Krishnaswamy PR, Rao PV: Recombinant antigen-based avidin-biotin microtiter enzyme-linked immunosorbent assay for serodiagnosis of invasive amoebiasis. *J Clin Microbiol* 1996, **34**:828–833.
29. Tachibana H, Cheng XJ, Masuda G, Horiki N, Takeuchi T: Evaluation of recombinant fragments of *Entamoeba histolytica* Gal/GalNAc lectin

- intermediate subunit for serodiagnosis of amebiasis. *J Clin Microbiol* 2004, **42**:1069–1074.
30. Pal S, Sengupta K, Manna B, Sarkar S, Bhattacharya S, Das P: **Comparative evaluation of somatic & excretory-secretory antigens of *Entamoeba histolytica* in serodiagnosis of human amoebiasis by ELISA.** *Indian J Med Res* 1996, **104**:152–156.
 31. Sathar MA, Bredenkamp BL, Gathiram V, Simjee AE, Jackson TF: **Detection of *Entamoeba histolytica* immunoglobulins G and M to plasma membrane antigen by enzyme-linked immunosorbent assay.** *J Clin Microbiol* 1990, **28**:332–335.
 32. Zhou M, Conrads TP, Veenstra TD: **Proteomics approaches to biomarker detection.** *Brief Funct Genomic Proteomic* 2005, **4**:69–75.
 33. Ortner S, Binder M, Scheiner O, Wiedermann G, Duchene M: **Molecular and biochemical characterization of phosphoglucomutases from *Entamoeba histolytica* and *Entamoeba dispar*.** *Mol Biochem Parasitol* 1997, **90**:121–129.
 34. Flores BM, Reed SL, Ravdin JI, Torian BE: **Serologic reactivity to purified recombinant and native 29-kilodalton peripheral membrane protein of pathogenic *Entamoeba histolytica*.** *J Clin Microbiol* 1993, **31**:1403–1407.
 35. Kaur U, Sharma AK, Sharma M, Vohra H: **Distribution of *Entamoeba histolytica* Gal/GalNAc lectin-specific antibody response in an endemic area.** *Scand J Immunol* 2004, **60**:524–528.
 36. Sanuki J, Nakano K, Tokoro M, Nozaki T, Okuzawa E, Kobayashi S, Asai T: **Purification and identification of major soluble 40-kDa antigenic protein from *Entamoeba histolytica*: its application for serodiagnosis of asymptomatic amebiasis.** *Parasitol Int* 2001, **50**:73–80.
 37. Abd-Alla MD, Jackson TF, Reddy S, Ravdin JI: **Diagnosis of invasive amebiasis by enzyme-linked immunosorbent assay of saliva to detect amebic lectin antigen and anti-lectin immunoglobulin G antibodies.** *J Clin Microbiol* 2000, **38**:2344–2347.
 38. Lee J, Park SJ, Yong TS: **Serodiagnosis of amoebiasis using a recombinant protein fragment of the 29 kDa surface antigen of *Entamoeba histolytica*.** *Int J Parasitol* 2000, **30**:1487–1491.
 39. Stanley SL Jr, Jackson TF, Reed SL, Calderon J, Kunz-Jenkins C, Gathiram V, Li E: **Serodiagnosis of invasive amebiasis using a recombinant *Entamoeba histolytica* protein.** *JAMA* 1991, **266**:1984–1986.

doi:10.1186/1471-2334-13-144

Cite this article as: Ning et al.: Evaluation of *Entamoeba histolytica* recombinant phosphoglucomutase protein for serodiagnosis of amoebic liver abscess. *BMC Infectious Diseases* 2013 **13**:144.

Submit your next manuscript to BioMed Central and take full advantage of:

- Convenient online submission
- Thorough peer review
- No space constraints or color figure charges
- Immediate publication on acceptance
- Inclusion in PubMed, CAS, Scopus and Google Scholar
- Research which is freely available for redistribution

Submit your manuscript at
www.biomedcentral.com/submit

