




Time scale performance of rapid antigen testing for SARS-CoV-2: Evaluation of 10 rapid antigen assays

Zakarya Abusrewil¹  | Inas M. Alhudiri²  | Hamza H. Kaal³ |
 Salah Eldin El Meshri⁴ | Fawzi O. Ebrahim⁵ | Tarek Dalyoum² |
 Abdussamee A. Efrefer² | Khaled Ibrahim² | Mohammed B. Elfghi³ |
 Suleiman Abusrewil⁶ | Adam Elzagheid² 

¹Forensic Medicine and Toxicology Department, University of Tripoli, Tripoli, Libya

²Genetic Engineering Department, Biotechnology Research Center, Tripoli, Libya

³Hospital Universitario Principe de Asturias, Alcala De Henares, Madrid, Spain

⁴Microbiology Department, Biotechnology Research Center, Tripoli, Libya

⁵Cell Biology Department, Biotechnology Research Center, Tripoli, Libya

⁶Pediatric Department, University of Tripoli, Tripoli, Libya

Correspondence

Adam Elzagheid, Genetic Engineering Department, Biotechnology Research Center, Tripoli, Libya.
 Email: elzagheid@yahoo.com

Abstract

There is a great demand for more rapid tests for SARS-CoV-2 detection to reduce waiting time, boost public health strategies for combating disease, decrease costs, and prevent overwhelming laboratory capacities. This study was conducted to assess the performance of 10 lateral flow device viral antigen immunoassays for the detection of SARS-CoV-2 in nasopharyngeal swab specimens. We analyzed 231 nasopharyngeal samples collected from October 2020 to December 2020, from suspected COVID-19 cases and contacts of positive cases at Biotechnology Research Center laboratories, Tripoli, Libya. The performance of 10 COVID-19 Antigen (Ag) rapid test devices for the detection of SARS-CoV-2 antigen was compared to a quantitative reverse transcription-polymerase chain reaction (RT-qPCR). In this study, 161 cases had symptoms consistent with COVID-19. The mean duration from symptom onset was 6.6 ± 4.3 days. The median cycle threshold (C_t) of positive samples was 25. Among the 108 positive samples detected by RT-qPCR, the COVID-19 antigen (Ag) tests detected 83 cases correctly. All rapid Ag test devices used in this study showed 100% specificity. While tests from six manufacturers had an overall sensitivity range from 75% to 100%, the remaining four tests had a sensitivity of 50%–71.43%. Sensitivity during the first 6 days of symptoms and in samples with high viral loads ($C_t < 25$), was 100% in all but two of the test platforms. False-negative samples had a median C_t of 34 and an average duration of onset of symptoms of 11.3 days (range = 5–20 days). Antigen test diagnosis has high sensitivity and specificity in early disease when patients present less than 7 days of symptom onset. Patients are encouraged to test as soon as they get COVID-19-related symptoms within 1 week and to seek medical advice within 24 h if they develop disturbed smell/taste. The use of rapid antigen tests is important for controlling the COVID-19 pandemic and reducing the burden on molecular diagnostic laboratories.

KEYWORDS

COVID-19 diagnosis, rapid antigen tests, SARS-CoV-2, surveillance

1 | INTRODUCTION

Nucleic acid amplification test using quantitative reverse transcription-polymerase chain reaction (RT-qPCR) assay is currently the mainstay diagnostic test for COVID-19 in most laboratories. However, results of RT-qPCR assays can take several days to deliver, hampering the disease containment efforts. Consequently, there is an emerging demand for more rapid and easier tests to reduce waiting time, boost public health strategies for combating disease, decrease costs, and prevent overwhelming laboratory capacities.

SARS-CoV-2-rapid antigen tests have been largely developed and many countries have adopted them for diagnosis in triage and hospital settings and at points of entry.¹ However, many of these tests have not been independently validated. The World Health Organization (WHO) encourages laboratories to evaluate the performance of commercial rapid antigen assays to update the current evidence and recommend specific test kits.²

According to previous studies, rapid antigen tests could be used in high-risk populations to quickly identify patients with infection and prevent disease transmission by repeat testing.³ Evaluation of these tests showed also diagnostic performance in screening mass population.⁴

Libyan health authorities have approved the use of rapid antigen tests in triage, isolation centers, and hospitals.⁵ This study was conducted to assess the performance of 10 antigen-based rapid assays for the detection of SARS-CoV-2 in nasopharyngeal swab specimens from suspected COVID-19 cases and contacts.

2 | MATERIALS AND METHODS

2.1 | Study population

This was a prospective single-center study. A total of 231 patients with clinical features suggestive of COVID-19 or a history of close contact with COVID-19 positive patients were enrolled in this study from October 10 to December 31, 2020. However, there were financial difficulties to obtain adequate quantities of the antigen test device to study a larger sample size for each type during the pandemic, and hence the number of samples tested was between 15 and 39 depending on the kit contents. The majority of patients were having symptoms suggestive of COVID-19 (70%). A quarter of participants were asymptomatic and were in contact with the COVID-19 positive case. Few patients were asymptomatic but had no history of contact. Duration since symptom onset was variable among the cases with an average of 7 days (Table 1).

2.2 | Antigen test procedure

We evaluated the performance of 10 rapid antigen tests for SARS-CoV-2. These lateral flow tests are a qualitative membrane-based colloidal gold chromatography immunoassay (Fluorecare SARS-CoV-2 spike protein

test, Shenzhen Microprofit Biotech Co; ESPLINE SARS-CoV-2, Fujirbio; RapiGen Covid-19 Ag Detection Kit, Biocredit; Abbott Panbio™ COVID-19 Ag Rapid Test; Flowflex™ SARS-CoV-2 Antigen Rapid Test, Acon; Assut Europe antigen testing COVID-19; Coronavirus antigen rapid test cassette, Orient Gene; CerTest SARS-CoV-2 one step card test; CerTest Biotech, Bioperfectus SARS-CoV-2 Antigen Rapid Test Kit; Bioperfectus technologies; AMP Rapid Test SARS-CoV-2 Ag; AMP Diagnostics). All assays detect SARS-CoV-2 nucleoprotein except Fluorecare assay which detects spike protein. Tests were performed according to the manufacturer's protocol; briefly, nasopharyngeal swabs were placed in extraction solution, swirled 10 times, and squeezed against the collection tube wall. Extracted sample was applied on a cassette with an appropriate time allowed for a monoclonal anti-SARS-CoV-2 antibody reaction. The required duration for the test to be interpreted is between 15- and 30-min depending on the test manufacturer. There are two lines on the cassette, control line (C) which should always appear as a colored line after adding a proper sample volume. A positive result was defined by the clear colored intense band at the T (test) mark on the cassette, weak positive was defined by faint to the moderately intense band. Negative results indicate no visible band. If the control reaction failed the test was considered invalid test and repeated. The results were read by two independent observers.

2.3 | RT-qPCR assay

RNA was extracted from viral transport media (VTM) using magnetic bead NuActor Automatic Extractor (Boditech Med). Patient samples were also analyzed by RT-qPCR within 24 h after collection to determine false negatives and positives (Xpert Xpress SARS-CoV-2 GeneXpert or DAAN GENE RT-PCR COVID-19 detection kit). Both assays target nucleocapsid (N) gene for which cycle threshold (C_t) was considered in this study.

We had also analyzed 31 samples out of the total number of 231 to evaluate the reliability of reusing swabs after rapid Ag testing for RT-qPCR. There is an additional step in rapid Ag testing in which

TABLE 1 Characteristics of study patients

Characteristics	No. (%)
Gender	
Male	130 (56.2)
Female	101 (43.7)
Age (mean ± SD)	40.8 ± 15.23
Asymptomatic patients with close contact	58 (25)
Days since close contact (mean ± SD)	7.1 ± 3
Asymptomatic no contact	12 (5)
Symptomatic patients	161 (69.6)
Days from symptom onset (mean ± SD)	7 ± 6

swabs are placed in lysis buffer before being transported into VTM. Results were compared to those obtained from swabs used directly for the standard RT-qPCR procedure.

2.4 | Statistical analysis

Sensitivity, specificity, positive, and negative predictive values and accuracy were calculated using MedCalc online statistical software.⁶ Laboratory COVID-19 prevalence data were obtained from the Biotechnology Research Center case registry for the study period (unpublished).

Sensitivity was calculated as: (true positives)/(true positives + false negatives) × 100. Specificity was calculated as: (true negatives)/(true negatives + false positives) × 100.

Positive predictive value:

$$\text{Sensitivity} \times \text{prevalence} / (\text{sensitivity} \times \text{prevalence} + (1 - \text{specificity}) \times (1 - \text{prevalence}))$$

Negative predictive value:

$$\text{Specificity} \times (1 - \text{prevalence}) / ((1 - \text{sensitivity}) \times \text{prevalence} + (\text{specificity}) \times (1 - \text{prevalence}))$$

Accuracy: $\text{Sensitivity} \times \text{prevalence} + \text{specificity} \times (1 - \text{Prevalence})$.

3 | RESULTS

A total of 108 nasopharyngeal samples tested positive for SARS-CoV-2 by RT-PCR accounting for 46.75% of cases. The mean duration from symptom onset was 6.6 ± 4.3 . In this study, 161 cases had symptoms consistent with COVID-19. The median cycle threshold (C_t) of positive samples was 25. Among the 108 positive samples detected by RT-qPCR, the COVID-19 Ag tests detected 83 cases correctly. Among negative samples, the COVID-19 Ag test detected all 123 samples as negative. All rapid Ag test devices used in this study showed 100% specificity. While tests from six manufacturers had an overall sensitivity range from 75% to 100%, the remaining four tests had a sensitivity of 50%–71.43% (Table 2). False-negative samples had a median C_t of 34 and an average duration of onset of symptoms of 11.3 days (range = 5–20 days).

The prevalence of positive samples calculated from the Biotechnology Research Center lab database during the study period was 27%. At this prevalence rate, estimated positive predictive values were 100% and the negative predictive value ranged between 84.39% and 100% for the different rapid antigen test devices.

We evaluated the sensitivity of each antigen test from the first day of symptoms up to 6, >7, 7–9, 10–12, and >12 days (Figure 1). Sensitivity during the first 6 days of symptoms and in samples with high viral loads ($C_t < 25$), was 100% in all but two (Assut and AMP) of the test platforms (Table 3). The median RT-qPCR cycle threshold value of positive samples was 25. The majority of antigen test platforms had excellent performance during the first 6 days of symptoms with sensitivity ranging between 75% and 100% (Table 3).

It is worth mentioning that three participants (3/58, 5.2%) who were asymptomatic at the time of testing with a history of close

contact with a confirmed SARS-CoV-2 case tested positive by antigen test (Espline & Rapigen rapid Ag tests). The C_t s of their RT-qPCR assay were 23, 24, and 25, and the duration since contact was 5, 6, and 10 days, respectively. All other asymptomatic cases with exposure were correctly diagnosed as negative. All asymptomatic cases with no history of exposure were also tested negative by the Ag test. Among symptomatic patients, the sensitivity was 77%.

Patients who experienced a change in smell/taste were 41. More than a third of them (15/41, 36.5%) were not detected by rapid Ag tests; Abbott (no = 3, mean C_t = 36), Assut (no = 1, C_t = 29), Bio-perfectus (no = 1, C_t = 33), CerTest (no = 2, mean C_t = 34.5), Orient Gene (no = 3, mean C_t = 32.3), Espline (no = 1, C_t = 36), and Rapigen (no = 4, mean C_t = 35). In this subgroup, the mean duration since symptoms onset was 12 days and the mean C_t was 34. However, those who had altered smell/taste and tested positive had a mean of 6.6 days since symptoms onset, and the mean C_t was 25. Loss of smell/taste was the only symptom in few patients (3/41, 7.3%).

Although the recommended time for interpretation ranges between 10 and 30 min, in all samples with $C_t < 25$ the test line was clearly visible within 2 min of application which gave a rough estimation of viral load. When interpreting results after or before the time set by the manufacturer, it was observed that the positive test line either faded or became unreadable in most cassette assays. Also, the result interpretation before the end of recommended time was unreliable in cases with low viral load ($C_t > 25$).

The cycle threshold for nasopharyngeal swab positive samples used for antigen testing and then transferred to VTM for RT-qPCR was increased three to six cycles in comparison with other direct swabs.

4 | DISCUSSION

Rapid antigen testing is cost-effective, easy to use, and can be manufactured in large quantities. The timeliness of the results they provided will reduce the load on the diagnostic laboratories. The FDA has authorized 14 SARS-CoV-2 antigen diagnostic tests for emergency use as of March 19, 2021.⁷ Most of these tests are lateral flow assays that can be visually read. We aimed to study rapid antigen tests from different manufacturers to evaluate their performance using time since the onset of symptoms as criteria for testing. This study was also part of preimplementation evaluation to confirm the performance of the tests by RT-qPCR.

Our study showed that most Ag rapid tests examined were reliable to diagnose SARS-CoV-2 infection. They demonstrated excellent performance in samples with high viral load $C_t \leq 25$ which are usually samples taken within the first 6 days after the onset of symptoms. CerTest Biotech, Panbio, Rapigen, Acon Ag rapid tests demonstrated similar results to studies reported by other authors during the first week.^{8–10} The WHO recommended the use of SARS-CoV-2 Ag rapid tests that meet a minimum sensitivity of $\geq 80\%$ and $\geq 97\%$ specificity compared to a nucleic acid amplification test reference assay.² All tests showed a specificity of 100% and sensitivity

TABLE 2 Diagnostic performance of SARS-COV-2 rapid antigen detection tests

Type of antigen (No. of cases)	Detected by RT-qPCR (%) ^a	Not-detected by RT-qPCR (%) ^b	False negatives	Median C _t (range)	Symptom's duration (days), mean ± SD	Sensitivity, % (confidence interval)	Specificity, % (confidence interval)	PPV, %	NPV, %	Accuracy, %
FLUORECARE (21)	11 (52.4)	9 (47.6)	1	27.5 (21–34)	5.3 ± 3.3	91.67 (61.52–99.79)	100	100	97.01	97.75
ESPLINE (17)	8 (47)	7 (53)	2	29.5 (20–37)	6.8 ± 3.5	80.00 (44.39–97.48)	100	100	93.11	94.6
RAPIGEN (39)	10 (25.6)	23(74.4)	6	25 (20–36)	6.4 ± 3.1	62.50 (35.4–84.80)	100	100	87.82	89.88
ASSUT (31)	5 (16.1)	24 (84)	2	21 (15–29)	5 ± 3	71.43 (29.04–96.33)	100	100	90.44	92.29
Orient GENE (22)	5 (23)	12 (77.3)	5	31 (16–39)	7.3 ± 4	50.00 (18.71–81.29)	100	100	84.39	86.5
AMP (15)	6 (40)	8 (60)	1	24 (18–37)	6.3 ± 3.2	85.71 (42.13–99.64)	100	100	94.98	96.14
ACON (25)	15 (52.4)	10 (47.6)	0	23 (18–37)	6.7 ± 4.4	100.00 (78.20–100)	100	100	100	100
ABBOTT (23)	10 (43.48)	10 (56.5)	3	29 (13–38)	9.6 ± 7	76.92 (46.19–94.96)	100	100	91.61	93.45
CERTEST BIOTEC (17)	5 (29.4)	9 (70.6)	3	22.7 (19–35)	7 ± 5	62.50 (24.49–91.48)	100	100	87.82	89.88
BIOPERFECTUS (21)	8 (38.1)	11 (62)	2	21 (14–34)	6.3 ± 4.5	80.00 (44.39–97.48)	100	100	93.11	94.6

Abbreviations: NPV, negative predictive value; PPV, positive predictive value; RT-qPCR, quantitative reverse transcription-polymerase chain reaction.

^aDetected by RT-qPCR denotes true positives.

^bNot detected by RT-qPCR denotes true negatives.

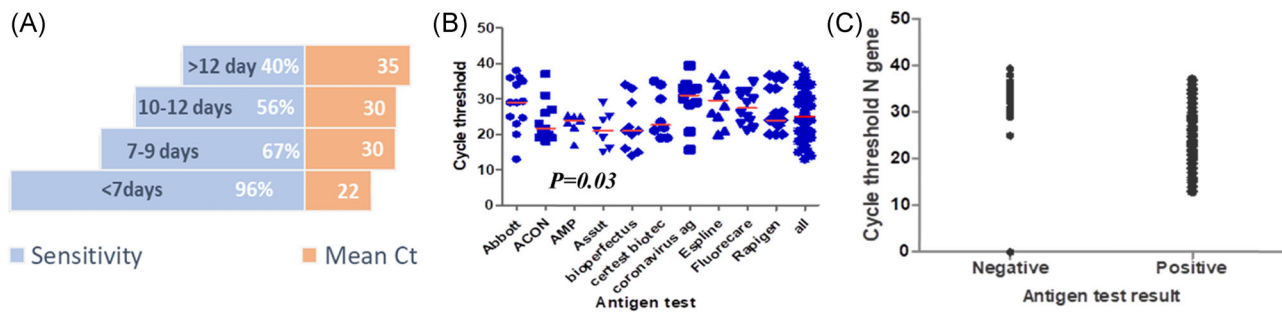


FIGURE 1 (A) Mirror chart showing percentage sensitivity of rapid antigen tests by symptoms onset against corresponding mean C_t . (B) Scatter plot of C_t values of samples in each commercial test (red line = median). (C) SARS-CoV-2 antigen test results according to viral load

TABLE 3 Diagnostic performance of SARS-COV-2 rapid antigen detection tests according to symptoms duration and cycle threshold

Antigen test	Sensitivity, % (<7 days)	Sensitivity, % ($C_t \leq 25$)
Fluorecare	100	100
Esplina	100	100
Rapigen	100	100
Assut	80	83.3
Orient gene	100	100
AMP	75	85.7
Acon	100	100
Abbott	100	100
Certest biotec	100	100
Bioperfectus	100	100

over 90% for high viral load samples, with excellent levels of agreement with PCR in 8 of 10 tests (Fluorecare, Esplina, Rapigen, Orient Gene, Acon, Abbott, CerTest Biotec, and Bioperfectus). Two rapid Ag tests showed sensitivity below the WHO recommended value namely, Assut and AMP; 80% and 75%, respectively.

It is worth emphasizing that interpretation time should not succeed nor exceed the manufacturer's recommended time to avoid false interpretation of the test result. The intensity of test line color is proportionally correlated with viral load. The test line in low viral load samples may appear weak or faint which may not be clearly visible to the reader. Therefore, an additional independent reader is recommended when low viral loads are expected to reduce subjectivity and confirm the diagnosis but for most cases, one reader is sufficient for interpreting the results. We also do not recommend placing the same nasopharyngeal swab used for antigen test in VTM for RT-qPCR analysis as the viral material will be diluted and may give false-negative results.

Since SARS-CoV-2 cases have been increasing with the emergence of new variants,¹¹ and numerous antigen tests were manufactured, it is important to evaluate them before implementation. Although there is more risk of developing false-negative results after 7 days of symptom onset, this is largely counterbalanced by the

rapidity of the test especially when used in the targeted population. Our study shows that all COVID-19 Ag tests had good specificity for SARS-CoV-2 detection in nasopharyngeal swab samples but had a good sensitivity only for cases within 7 days of developing symptoms (higher viral loads).

We proposed a strategy for use of rapid antigen tests in symptomatic patients according to our results and experience as shown in the flowcharts (Figure 2A,B). Although the procedure is relatively easy to perform, testing with Ag rapid tests should be conducted by trained operators following the manufacturer's instructions. Interpretation of the results of rapid Ag tests should consider the prevalence of the disease in the community because positive and negative predictive value of any diagnostic test is affected by disease prevalence in the population tested.²

In our medical departments, triage, and isolation centers, we have trained medical staff on how to use the antigen test properly, developed criteria for testing (Figure 2), and audited the procedure. It is important to note that the use of rapid antigen tests requires careful respiratory sample management, waste disposal, and biosafety considerations.

The incubation period of SARS-CoV-2 infection was estimated between 3 and 6 days with a median incubation of 4 days.^{12,13} Patients may only present to the hospital 6–10 days following symptom onset,¹⁴ therefore, missing the opportunity for rapid detection using antigen tests. We consequently emphasize the importance of encouraging patients to seek medical advice and immediate testing as soon as they develop any COVID-19-related symptoms. In particular, when patients lose the sense of smell, they should be tested immediately, preferably within 24 h. because this symptom usually occurs after the onset of other COVID-19 symptoms.^{15,16} We also observed in our study that most patients present with loss of smell a few days after symptoms onset and in some patients, it was the sole symptom (12 patients with loss of smell came late). We believe that Ag testing would encourage patients to come earlier for testing because of a reduction in waiting time.

Viral culture studies in cell lines showed that samples with C_t value ≥ 34 , ≥ 24 , or ≥ 38 , and more than 8 days of symptoms onset had no growth and thus might indicate the person is less infectious.^{17–19} Thus, there is no agreement about the cut-off C_t value. A positive

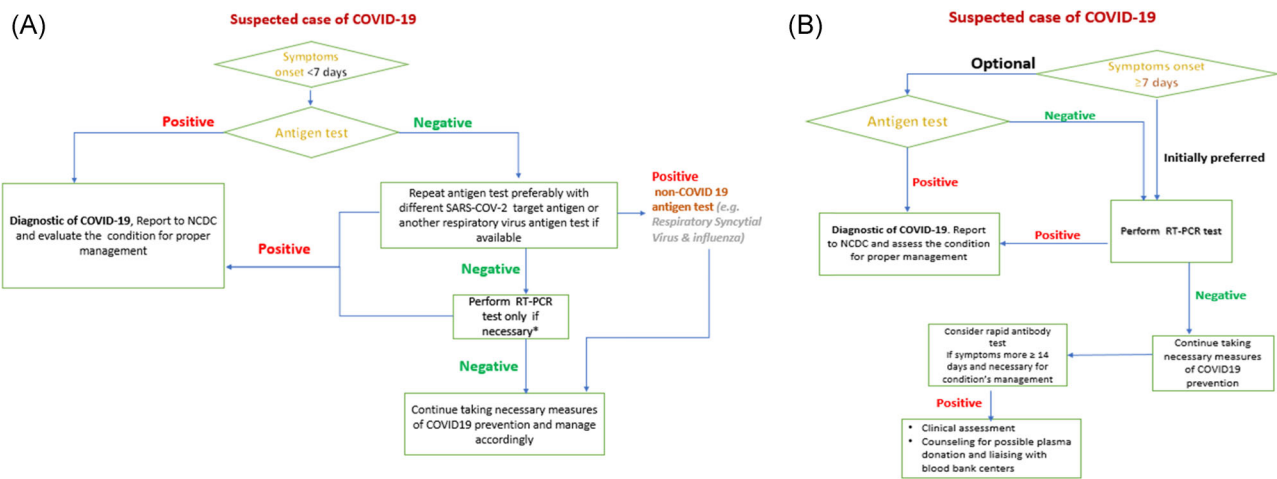


FIGURE 2 (A) Flowchart of the proposed use of rapid antigen tests in suspected COVID-19 cases with symptoms duration less than 7 days. *Vulnerable cases and elderly. (B) Flowchart of the proposed use of rapid antigen tests in suspected COVID-19 cases with symptoms duration of more than 7 days

PCR result reflects only the detection of viral RNA and does not necessarily indicate the presence of the viable viruses. Therefore, false-negative results could potentially be noninfectious, increasing the safety margin in the utility of rapid antigen test in cases more than 7 days after the start of symptoms and asymptomatic patients.

This study has some limitations. First, the sample size was small for each individual antigen rapid test kit. Second, because the data was collected prospectively based on the presence of symptoms or history of contact with an infected patient, it was difficult to select patients with different C_t values in enough size. However, if we assumed that the performance of all antigen rapid test devices was similar, the data would be reliable enough to give credible results.

Rapid Ag testing performance is mostly affected by symptoms duration, viral load, manufacturing company, operator experience, and qualification. In addition, new SARS-COV-2 variants may alter the performance especially with spike proteins targeted rapid ag tests.^{20,21}

In conclusion, rapid Ag tests have high sensitivity and specificity in early disease when patients present before 7 days of symptom onset. Patients are encouraged to test as soon as they get COVID-19-related symptoms within 1 week and to seek medical advice within 24 h if they develop disturbed smell/taste. The use of rapid antigen tests is important for controlling the COVID-19 pandemic and reducing the burden on molecular diagnostic laboratories.

ACKNOWLEDGMENT

The authors gratefully acknowledge the support of the Libyan authority for research, science, and technology and all lab researchers at the Biotechnology Research Center COVID-19 detection team.

CONFLICT OF INTERESTS

The authors declare that there are no conflict of interests.

ETHICS STATEMENT

All procedures performed in studies involving human participants were in accordance with the ethical standards of the institutional and/or national research committee and with the 1964 Helsinki declaration and its later amendments or comparable ethical standards. This study was approved by the Biotechnology Research Center Bioethics Committee. Informed consent was obtained from all individual participants included in the study.

AUTHOR CONTRIBUTIONS

The corresponding authors had full access to all the data in the study and have final responsibility for the decision to submit for publication. Zakarya Abusrewil and Inas M. Alhudiri contributed equally and share the first authorship. *Concept and design:* Zakarya Abusrewil and Inas M. Alhudiri. *Acquisition, analysis, or interpretation of data:* Zakarya Abusrewil, Inas M. Alhudiri, Hamza H. Kaal, Salah E. El Meshri, and Fawzi O. Ebrahim. *Drafting and revising the manuscript:* Zakarya Abusrewil, Inas M. Alhudiri, Khaled Ibrahim, and Tarek Dalyoum. *Statistical analysis:* Tarek Dalyoum, A. Abdussamee Efrefer, and Mohammed B. Elfgi. *Administrative, technical, or material support:* Salah E. El Meshri, Hamza H. Kaal, and Fawzi O. Ebrahim. *Supervision:* Suleiman Abusrewil and Adam Elzagheid.

ORCID

Zakarya Abusrewil <https://orcid.org/0000-0003-2356-6528>
 Inas M. Alhudiri <https://orcid.org/0000-0002-3371-0215>
 Adam Elzagheid <https://orcid.org/0000-0002-7086-5937>

REFERENCES

1. Rapid Antigen test. 2020. https://ec.europa.eu/commission/presscorner/detail/en/ip_20_2483. Accessed March 28, 2021.
2. World Health Organization (WHO). Antigen-detection in the diagnosis of SARS-CoV-2 infection using rapid immunoassays. Interim guidance. 2020. <https://www.who.int/publications/i/item/antigen->

- detection-in-the-diagnosis-of-sars-cov-2infection-using-rapid-immunoassays. Accessed March 28, 2021.
3. Linares M, Pérez-Tanoira R, Carrero A, et al. Panbio antigen rapid test is reliable to diagnose SARS-CoV-2 infection in the first 7 days after the onset of symptoms. *J Clin Virol.* 2020;133:104659. <https://doi.org/10.1016/j.jcv.2020.104659>
 4. Peto T, On behalf of the UK COVID-19 Lateral Flow Oversight Team. COVID-19: rapid antigen detection for SARS-CoV-2 by lateral flow assay: a national systematic evaluation of sensitivity and specificity for mass-testing. *EClinicalMedicine.* 2021;36:100924. <https://doi.org/10.1016/j.eclinm.2021.100924>
 5. Press conference for scientific consultancy committee for coronavirus epidemic in Libya. 2020. <https://www.youtube.com/watch?v=C16TxEReuU>. Accessed March 28, 2021.
 6. MedCalc's Diagnostic test evaluation calculator. 2020. https://www.medcalc.org/calc/diagnostic_test.php. Accessed January 22, 2021.
 7. In Vitro Diagnostics EUAs | FDA. <https://www.fda.gov/medical-devices/coronavirus-disease-2019-covid-19-emergency-use-authorizations-medical-devices/vitro-diagnostics-euas>. Accessed December 24, 2020.
 8. Pérez-García F, Romanyk J, Gómez-Herruz P, et al. Diagnostic performance of CerTest and Panbio antigen rapid diagnostic tests to diagnose SARS-CoV-2 infection. *J Clin Virol.* 2021;137:104781. <https://doi.org/10.1016/j.jcv.2021.104781>
 9. Linares M, Pérez-Tanoira R, Carrero A, et al. Panbio antigen rapid test is reliable to diagnose SARS-CoV-2 infection in the first 7 days after the onset of symptoms. *J Clin Virol.* 2020;133:104659. <https://doi.org/10.1016/j.jcv.2020.104659>
 10. Aoki K, Nagasawa T, Ishii Y, et al. Evaluation of clinical utility of novel coronavirus antigen detection reagent, Espline® SARS-CoV-2. *J Infect Chemother.* 2021;27(2):319-322. <https://doi.org/10.1016/j.jiac.2020.11.015>
 11. Luring AS, Hodcroft EB. Genetic variants of SARS-CoV-2—what do they mean? *JAMA.* 2021;325(6):529-531. <https://doi.org/10.1001/jama.2020.27124>
 12. Guan W, Ni Z, Hu Y, et al. Clinical characteristics of coronavirus disease 2019 in China. *N Engl J Med.* 2020. 382(18):1708-1720. <https://doi.org/10.1056/NEJMoa2002032>
 13. Meo SA, Alhowikan AM, Al-Khlaiwi T, et al. Novel coronavirus 2019-nCoV: prevalence, biological and clinical characteristics comparison with SARS-CoV and MERS-CoV. *Eur Rev Med Pharmacol Sci.* 2020; 24(4):2012-2019. https://doi.org/10.26355/eurrev_202002_20379
 14. Chan JF, Yuan S, Kok KH, et al. A familial cluster of pneumonia associated with the 2019 novel coronavirus indicating person-to-person transmission: a study of a family cluster. *Lancet.* 2020;395(10223):514-523. [https://doi.org/10.1016/S0140-6736\(20\)30154-9](https://doi.org/10.1016/S0140-6736(20)30154-9)
 15. Chetrit A, Lechien JR, Ammar A, et al. Magnetic resonance imaging of COVID-19 anosmic patients reveals abnormalities of the olfactory bulb: preliminary prospective study. *J Infect.* 2020;81(5):816-846. <https://doi.org/10.1016/j.jinf.2020.07.028>
 16. Salmon Ceron D, Bartier S, Hautefort C, et al. Self-reported loss of smell without nasal obstruction to identify COVID-19. The multicenter Coranosmia cohort study. *J Infect.* 2020;81(4):614-620. <https://doi.org/10.1016/j.jinf.2020.07.005>
 17. Bullard J, Dust K, Funk D, et al. Predicting infectious SARS-CoV-2 from diagnostic samples. *Clin Infect Dis.* 2020;71:2663-2666. <https://doi.org/10.1093/cid/ciaa638>
 18. Wölfel R, Corman VM, Guggemos W, et al. Virological assessment of hospitalized patients with COVID-2019. *Nature.* 2020;581(7809):465-469. <https://doi.org/10.1038/s41586-020-2196-x>
 19. La Scola B, Le Bideau M, Andreani J, et al. Viral RNA load as determined by cell culture as a management tool for discharge of SARS-CoV-2 patients from infectious disease wards. *Eur J Clin Microbiol Infect Dis.* 2020;39(6):1059-1061. <https://doi.org/10.1007/s10096-020-03913-9>
 20. Mahase E. Covid-19: innova lateral flow test is not fit for "test and release" strategy, say experts. *BMJ.* 2020;371:m4469-m4521. <https://doi.org/10.1136/bmj.m4469>
 21. Li Q, Wu J, Nie J, et al. The impact of mutations in SARS-CoV-2 spike on viral infectivity and antigenicity. *Cell.* 2020;182(5):1284-1294.e9. <https://doi.org/10.1016/j.cell.2020.07.012>

How to cite this article: Abusrewil Z, Alhudiri IM, Kaal HH, et al. Time scale performance of rapid antigen testing for SARS-CoV-2: Evaluation of 10 rapid antigen assays. *J Med Virol.* 2021;93:6512-6518. <https://doi.org/10.1002/jmv.27186>